

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048978.D
 Acq On : 09 Jun 2022 14:43
 Operator : SY/MD
 Sample : VIBLK073
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK073

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048978.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	135743	153063	13.04%	1.610%
2	1.893	164	172	188	rBV	94707	129084	11.00%	1.358%
3	2.562	367	380	396	rBV	216838	352259	30.01%	3.705%
4	2.764	437	443	444	rBV2	652	519	0.04%	0.005%
5	2.877	475	478	481	rBV	392	295	0.03%	0.003%
6	3.044	520	530	539	rVB4	2819	5394	0.46%	0.057%
7	3.086	539	543	547	rVB2	546	519	0.04%	0.005%
8	3.128	552	556	559	rBV2	389	399	0.03%	0.004%
9	3.182	559	573	591	rBV	20801	48416	4.12%	0.509%
10	3.353	621	626	629	rBV3	494	493	0.04%	0.005%
11	3.475	661	664	669	rBV2	302	310	0.03%	0.003%
12	3.542	678	685	690	rBV2	401	505	0.04%	0.005%
13	3.626	708	711	718	rVB2	354	338	0.03%	0.004%
14	3.742	741	747	750	rBV	324	282	0.02%	0.003%
15	3.864	783	785	789	rVB2	641	274	0.02%	0.003%
16	3.948	807	811	819	rBV2	362	432	0.04%	0.005%
17	3.989	819	824	827	rVV2	315	311	0.03%	0.003%
18	4.092	852	856	861	rBV2	371	339	0.03%	0.004%
19	4.198	886	889	893	rBV	506	352	0.03%	0.004%
20	4.372	940	943	948	rVB2	459	419	0.04%	0.004%
21	4.465	968	972	975	rBV	452	422	0.04%	0.004%
22	4.620	1004	1020	1046	rBV2	159226	390065	33.23%	4.103%
23	4.851	1086	1092	1094	rBV4	401	389	0.03%	0.004%
24	5.060	1141	1157	1178	rBV	223996	495898	42.25%	5.216%
25	5.224	1205	1208	1212	rVB	577	390	0.03%	0.004%
26	5.247	1212	1215	1218	rBV	446	330	0.03%	0.003%
27	5.311	1222	1235	1241	rBV6	3401	7137	0.61%	0.075%
28	5.375	1253	1255	1263	rVB2	783	751	0.06%	0.008%
29	5.417	1263	1268	1271	rBV2	328	310	0.03%	0.003%
30	5.452	1276	1279	1284	rVB	493	337	0.03%	0.004%
31	5.722	1341	1363	1388	rBV2	427016	1173826	100.00%	12.347%
32	5.967	1433	1439	1445	rVB5	746	1114	0.09%	0.012%
33	6.054	1463	1466	1470	rVB2	400	304	0.03%	0.003%
34	6.118	1484	1486	1490	rVB	630	367	0.03%	0.004%
35	6.166	1497	1501	1503	rBV	415	337	0.03%	0.004%
36	6.247	1510	1526	1555	rBV	375594	706309	60.17%	7.430%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048978.D
 Acq On : 09 Jun 2022 14:43
 Operator : SY/MD
 Sample : VIBLK073
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK073

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.533	1605	1615	1625	rVB8	4574	8915	0.76%	0.094%
38	6.591	1629	1633	1636	rBV2	859	767	0.07%	0.008%
39	6.690	1649	1664	1682	rBV	277390	541972	46.17%	5.701%
40	6.790	1689	1695	1696	rBV3	501	400	0.03%	0.004%
41	6.828	1705	1707	1713	rVB2	539	471	0.04%	0.005%
42	6.996	1757	1759	1765	rVB3	467	370	0.03%	0.004%
43	7.166	1808	1812	1813	rBV2	1353	880	0.07%	0.009%
44	7.565	1920	1936	1958	rBV	161523	285089	24.29%	2.999%
45	7.790	1999	2006	2011	rBV5	1399	1932	0.16%	0.020%
46	7.896	2021	2039	2057	rBV	522824	912125	77.71%	9.594%
47	8.050	2086	2087	2093	rVB2	636	326	0.03%	0.003%
48	8.082	2093	2097	2101	rBV	535	432	0.04%	0.005%
49	8.179	2116	2127	2143	rBV2	118214	195224	16.63%	2.054%
50	8.314	2166	2169	2172	rBV3	563	424	0.04%	0.004%
51	8.529	2231	2236	2237	rBV2	361	336	0.03%	0.004%
52	8.552	2237	2243	2253	rVB5	3810	5744	0.49%	0.060%
53	8.632	2255	2268	2302	rBV	466136	851852	72.57%	8.960%
54	8.812	2320	2324	2329	rBV4	670	658	0.06%	0.007%
55	9.047	2394	2397	2402	rVB2	508	387	0.03%	0.004%
56	9.073	2402	2405	2408	rBV	392	274	0.02%	0.003%
57	9.259	2456	2463	2467	rBV	391	407	0.03%	0.004%
58	9.320	2479	2482	2486	rVB2	400	296	0.03%	0.003%
59	9.346	2486	2490	2495	rBV2	367	410	0.03%	0.004%
60	9.417	2499	2512	2530	rBV	513140	846917	72.15%	8.909%
61	9.571	2558	2560	2566	rVB2	486	390	0.03%	0.004%
62	9.632	2576	2579	2581	rBV	387	280	0.02%	0.003%
63	9.693	2596	2598	2603	rVB3	413	271	0.02%	0.003%
64	9.751	2613	2616	2621	rVB2	474	320	0.03%	0.003%
65	10.227	2761	2764	2768	rBV	564	440	0.04%	0.005%
66	10.346	2795	2801	2803	rBV2	507	461	0.04%	0.005%
67	10.526	2853	2857	2860	rBV	433	344	0.03%	0.004%
68	10.700	2905	2911	2915	rVB2	281	281	0.02%	0.003%
69	10.758	2915	2929	2946	rBV	438368	706032	60.15%	7.427%
70	10.867	2959	2963	2965	rBV2	425	325	0.03%	0.003%
71	10.896	2965	2972	2981	rVB3	1753	2554	0.22%	0.027%
72	11.057	3019	3022	3026	rBV	413	303	0.03%	0.003%
73	11.095	3030	3034	3038	rVV3	251	284	0.02%	0.003%
74	11.121	3038	3042	3046	rVV4	527	450	0.04%	0.005%
75	11.269	3082	3088	3094	rBV2	426	610	0.05%	0.006%
76	11.346	3110	3112	3117	rVB	404	274	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048978.D
 Acq On : 09 Jun 2022 14:43
 Operator : SY/MD
 Sample : VIBLK073
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK073

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	11.394	3122	3127	3131	rBV3	485	512	0.04%	0.005%
78	11.455	3141	3146	3148	rBV	451	375	0.03%	0.004%
79	11.651	3203	3207	3210	rBV3	360	288	0.02%	0.003%
80	11.703	3220	3223	3225	rBV	596	357	0.03%	0.004%
81	11.725	3225	3230	3233	rVV2	455	307	0.03%	0.003%
82	11.812	3244	3257	3276	rBV	496066	790766	67.37%	8.318%
83	12.047	3325	3330	3335	rBV	359	498	0.04%	0.005%
84	12.192	3358	3375	3400	rBV	522563	860910	73.34%	9.056%
85	12.555	3485	3488	3492	rBV2	356	359	0.03%	0.004%
86	12.655	3516	3519	3522	rVB	659	402	0.03%	0.004%
87	12.674	3522	3525	3527	rBV2	335	268	0.02%	0.003%
88	12.709	3532	3536	3542	rBV2	508	492	0.04%	0.005%
89	12.767	3546	3554	3568	rVB5	1805	3139	0.27%	0.033%
90	12.938	3603	3607	3611	rBV2	480	430	0.04%	0.005%
91	13.057	3641	3644	3648	rBV2	428	375	0.03%	0.004%
92	13.664	3827	3833	3837	rBV3	519	655	0.06%	0.007%
93	14.519	4097	4099	4103	rBV	439	362	0.03%	0.004%
94	14.732	4162	4165	4170	rBV3	516	616	0.05%	0.006%
95	15.056	4263	4266	4270	rBV2	663	586	0.05%	0.006%
96	15.105	4278	4281	4284	rBV2	607	415	0.04%	0.004%
97	15.143	4290	4293	4295	rBV2	527	393	0.03%	0.004%
98	15.262	4328	4330	4333	rVB	654	334	0.03%	0.004%
99	15.439	4382	4385	4388	rBV2	906	612	0.05%	0.006%
100	15.925	4533	4536	4540	rBV6	955	801	0.07%	0.008%




Sum of corrected areas: 9506768

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048978.D
Acq On : 09 Jun 2022 14:43
Operator : SY/MD
Sample : VIBLK073
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK073

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

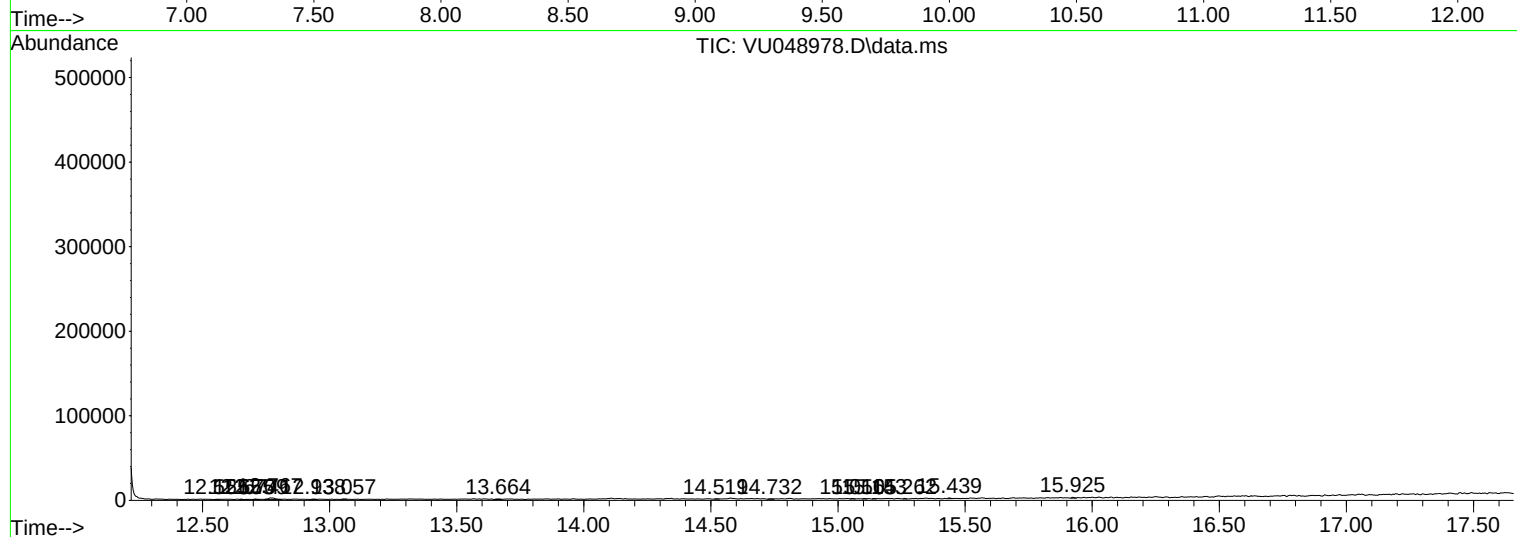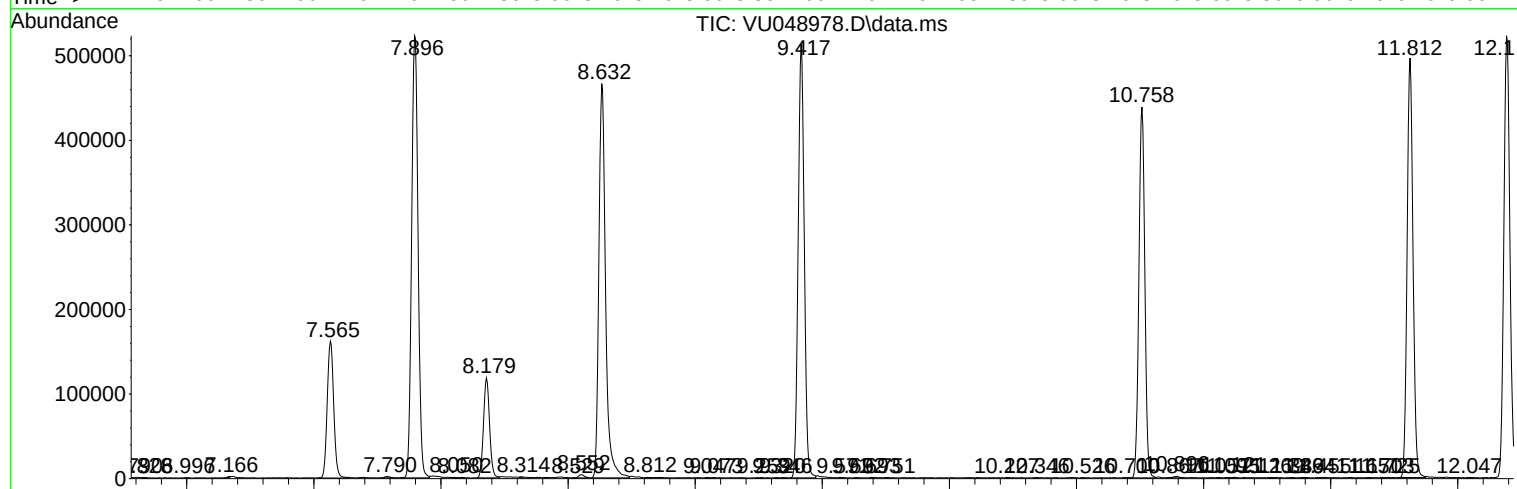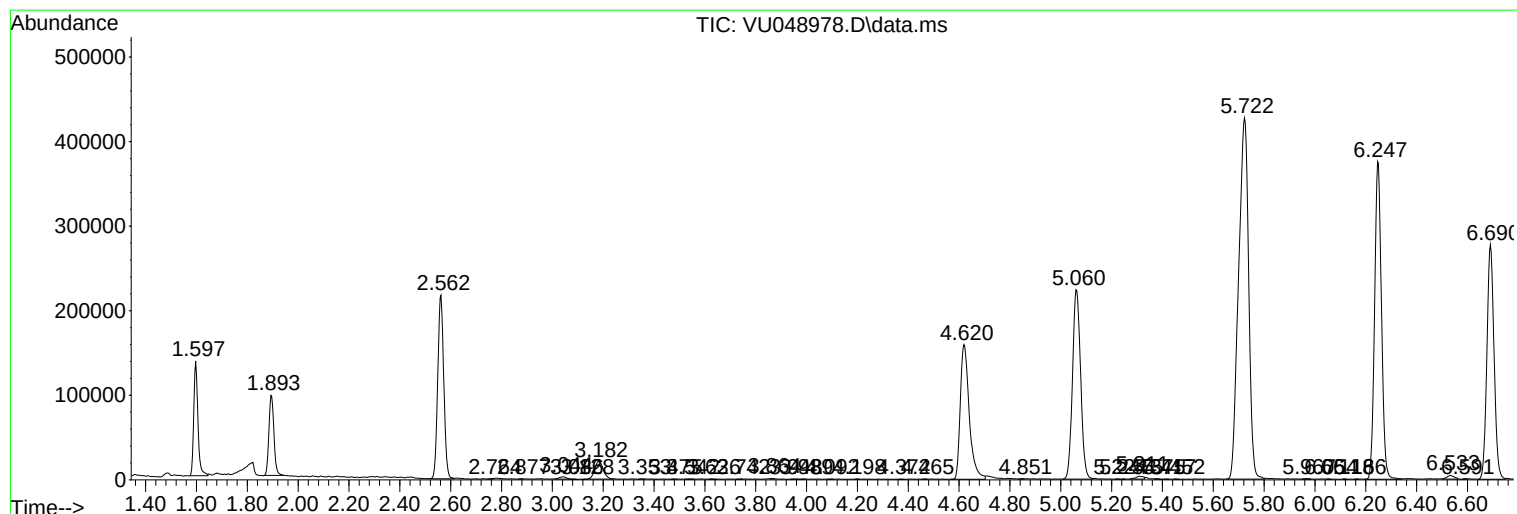

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048978.D
Acq On : 09 Jun 2022 14:43
Operator : SY/MD
Sample : VIBLK073
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK073

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048978.D
Acq On : 09 Jun 2022 14:43
Operator : SY/MD
Sample : VIBLK073
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK073

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------