

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048979.D
 Acq On : 09 Jun 2022 15:07
 Operator : SY/MD
 Sample : N3248-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048979.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	101	rBV	138852	167576	3.62%	0.788%
2	1.887	162	170	187	rVB	96180	135337	2.92%	0.636%
3	2.070	222	227	235	rVB	6623	7655	0.17%	0.036%
4	2.125	237	244	249	rBV	14188	18963	0.41%	0.089%
5	2.568	367	382	417	rVV4	948973	1735051	37.47%	8.160%
6	3.041	518	529	536	rVB4	2069	3264	0.07%	0.015%
7	3.176	560	571	591	rVB5	2717	6001	0.13%	0.028%
8	3.350	609	625	640	rBV	18848	37728	0.81%	0.177%
9	3.475	659	664	668	rBV2	419	398	0.01%	0.002%
10	3.594	697	701	704	rBV	614	483	0.01%	0.002%
11	3.697	730	733	736	rBV2	439	304	0.01%	0.001%
12	3.864	764	785	817	rBV	481204	1141792	24.66%	5.370%
13	4.224	891	897	900	rBV2	436	364	0.01%	0.002%
14	4.263	906	909	915	rVB2	358	390	0.01%	0.002%
15	4.298	915	920	922	rBV2	380	318	0.01%	0.001%
16	4.366	936	941	943	rBV2	347	303	0.01%	0.001%
17	4.468	968	973	978	rBV2	307	417	0.01%	0.002%
18	4.661	1001	1033	1068	rBV2	702880	1918062	41.42%	9.021%
19	5.063	1140	1158	1181	rBV	227222	538251	11.62%	2.531%
20	5.314	1215	1236	1259	rBV	2075273	4630990	100.00%	21.779%
21	5.517	1292	1299	1314	rVB4	3599	8498	0.18%	0.040%
22	5.722	1341	1363	1383	rBV2	426964	1155067	24.94%	5.432%
23	5.970	1435	1440	1443	rBV2	1105	1143	0.02%	0.005%
24	6.034	1454	1460	1463	rBV3	371	361	0.01%	0.002%
25	6.111	1478	1484	1487	rBV3	583	518	0.01%	0.002%
26	6.247	1511	1526	1546	rBV	383059	721420	15.58%	3.393%
27	6.314	1546	1547	1553	rVB3	1230	722	0.02%	0.003%
28	6.346	1555	1557	1567	rVB4	763	738	0.02%	0.003%
29	6.398	1567	1573	1577	rVB2	422	514	0.01%	0.002%
30	6.423	1577	1581	1583	rBV3	399	317	0.01%	0.001%
31	6.436	1583	1585	1590	rVB3	699	386	0.01%	0.002%
32	6.539	1602	1617	1639	rBV	889861	1654962	35.74%	7.783%
33	6.690	1649	1664	1685	rBV	274919	534244	11.54%	2.513%
34	6.790	1690	1695	1698	rBV5	1027	1047	0.02%	0.005%
35	6.925	1735	1737	1741	rVB2	448	340	0.01%	0.002%
36	6.973	1743	1752	1755	rBV4	1938	2570	0.06%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048979.D
 Acq On : 09 Jun 2022 15:07
 Operator : SY/MD
 Sample : N3248-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	7.047	1768	1775	1776	rBV3	410	327	0.01%	0.002%
38	7.173	1803	1814	1816	rBV3	2571	3117	0.07%	0.015%
39	7.275	1842	1846	1852	rBV2	461	523	0.01%	0.002%
40	7.565	1923	1936	1952	rBV	163960	282842	6.11%	1.330%
41	7.697	1969	1977	1982	rBV5	1029	1421	0.03%	0.007%
42	7.735	1984	1989	1992	rVB4	543	495	0.01%	0.002%
43	7.793	2002	2007	2012	rVV3	429	595	0.01%	0.003%
44	7.896	2025	2039	2057	rBV	525753	908852	19.63%	4.274%
45	7.973	2060	2063	2068	rVB5	636	588	0.01%	0.003%
46	8.179	2115	2127	2141	rBV	117735	192989	4.17%	0.908%
47	8.230	2141	2143	2150	rVB6	816	817	0.02%	0.004%
48	8.263	2150	2153	2157	rBV2	762	616	0.01%	0.003%
49	8.401	2186	2196	2206	rBV3	24325	40366	0.87%	0.190%
50	8.472	2210	2218	2230	rVB2	3707	6376	0.14%	0.030%
51	8.552	2230	2243	2257	rBV	733611	1234522	26.66%	5.806%
52	8.635	2257	2269	2302	rVB	438899	804985	17.38%	3.786%
53	8.980	2372	2376	2382	rBV2	373	490	0.01%	0.002%
54	9.021	2385	2389	2392	rBV3	452	294	0.01%	0.001%
55	9.111	2413	2417	2421	rBV	442	341	0.01%	0.002%
56	9.349	2488	2491	2496	rVB2	517	493	0.01%	0.002%
57	9.417	2496	2512	2536	rBV	530432	871446	18.82%	4.098%
58	9.758	2612	2618	2621	rBV2	403	395	0.01%	0.002%
59	9.989	2686	2690	2694	rVB	344	292	0.01%	0.001%
60	10.015	2694	2698	2703	rBV2	298	292	0.01%	0.001%
61	10.060	2707	2712	2715	rBV	417	376	0.01%	0.002%
62	10.314	2787	2791	2795	rVB2	335	291	0.01%	0.001%
63	10.414	2816	2822	2825	rBV2	502	510	0.01%	0.002%
64	10.523	2851	2856	2859	rVB3	422	386	0.01%	0.002%
65	10.606	2878	2882	2886	rBV2	277	290	0.01%	0.001%
66	10.758	2916	2929	2949	rVV2	442351	723481	15.62%	3.402%
67	10.893	2963	2971	2980	rVB2	5525	8095	0.17%	0.038%
68	10.934	2980	2984	2988	rBV2	341	323	0.01%	0.002%
69	11.118	3038	3041	3045	rVB2	568	415	0.01%	0.002%
70	11.169	3052	3057	3062	rVB2	484	547	0.01%	0.003%
71	11.198	3062	3066	3070	rBV2	588	393	0.01%	0.002%
72	11.266	3083	3087	3094	rVB2	373	425	0.01%	0.002%
73	11.365	3113	3118	3123	rBV2	311	297	0.01%	0.001%
74	11.417	3130	3134	3136	rBV2	569	387	0.01%	0.002%
75	11.471	3149	3151	3154	rVV2	448	295	0.01%	0.001%
76	11.568	3177	3181	3186	rBV2	505	556	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048979.D
 Acq On : 09 Jun 2022 15:07
 Operator : SY/MD
 Sample : N3248-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	11.751	3233	3238	3242	rBV2	625	487	0.01%	0.002%
78	11.812	3242	3257	3277	rBV	539316	852791	18.41%	4.011%
79	11.963	3301	3304	3307	rVB	449	322	0.01%	0.002%
80	12.031	3322	3325	3330	rVV2	431	328	0.01%	0.002%
81	12.195	3362	3376	3402	rBV	535852	879281	18.99%	4.135%
82	12.410	3440	3443	3448	rVB2	563	508	0.01%	0.002%
83	12.439	3448	3452	3455	rBV	573	504	0.01%	0.002%
84	12.475	3460	3463	3465	rBV	451	290	0.01%	0.001%
85	12.774	3543	3556	3567	rBV2	2335	3898	0.08%	0.018%
86	12.844	3573	3578	3582	rBV2	555	497	0.01%	0.002%
87	12.963	3612	3615	3618	rBV2	562	386	0.01%	0.002%
88	13.385	3743	3746	3749	rBV2	577	485	0.01%	0.002%
89	13.757	3859	3862	3869	rBV2	280	341	0.01%	0.002%
90	13.848	3886	3890	3892	rBV3	514	442	0.01%	0.002%
91	14.140	3979	3981	3987	rVB	710	488	0.01%	0.002%
92	14.204	3998	4001	4005	rVB	606	386	0.01%	0.002%
93	14.320	4032	4037	4039	rBV3	566	530	0.01%	0.002%
94	15.066	4267	4269	4272	rVB2	689	348	0.01%	0.002%
95	15.423	4377	4380	4384	rBV3	728	679	0.01%	0.003%
96	15.468	4391	4394	4396	rBV3	580	348	0.01%	0.002%
97	15.648	4448	4450	4454	rBV5	722	605	0.01%	0.003%
98	15.966	4546	4549	4551	rBV	769	577	0.01%	0.003%
99	15.995	4556	4558	4565	rVV4	1145	1004	0.02%	0.005%
100	16.156	4606	4608	4611	rBV4	1067	768	0.02%	0.004%




Sum of corrected areas: 21263328

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048979.D
Acq On : 09 Jun 2022 15:07
Operator : SY/MD
Sample : N3248-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

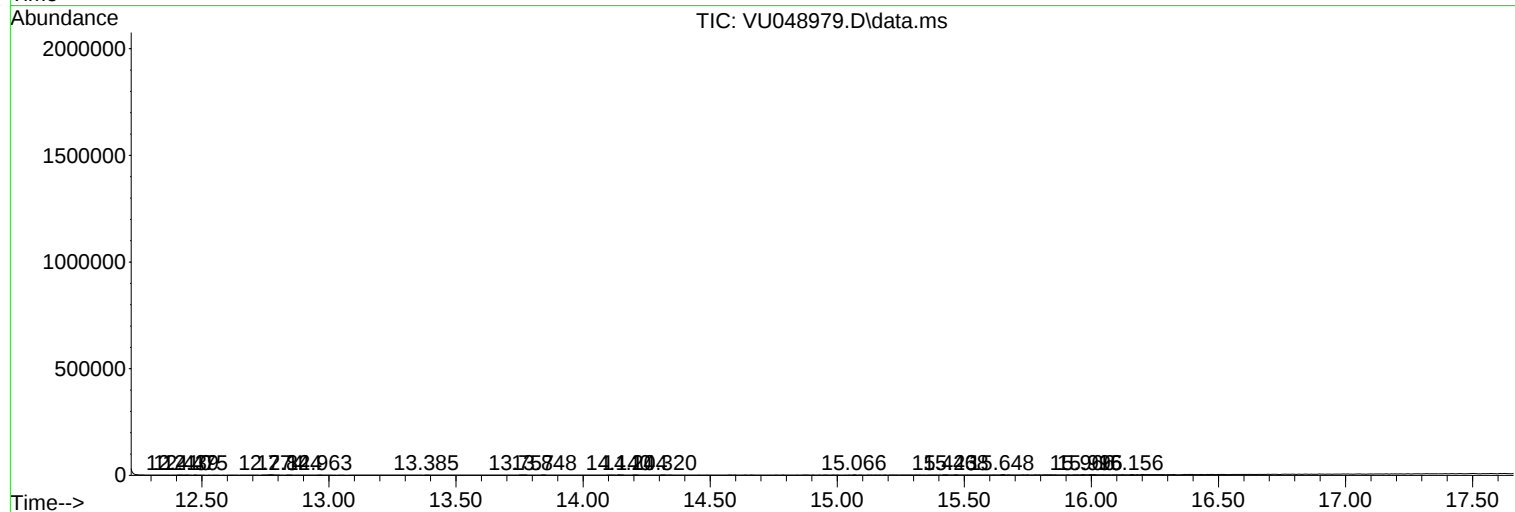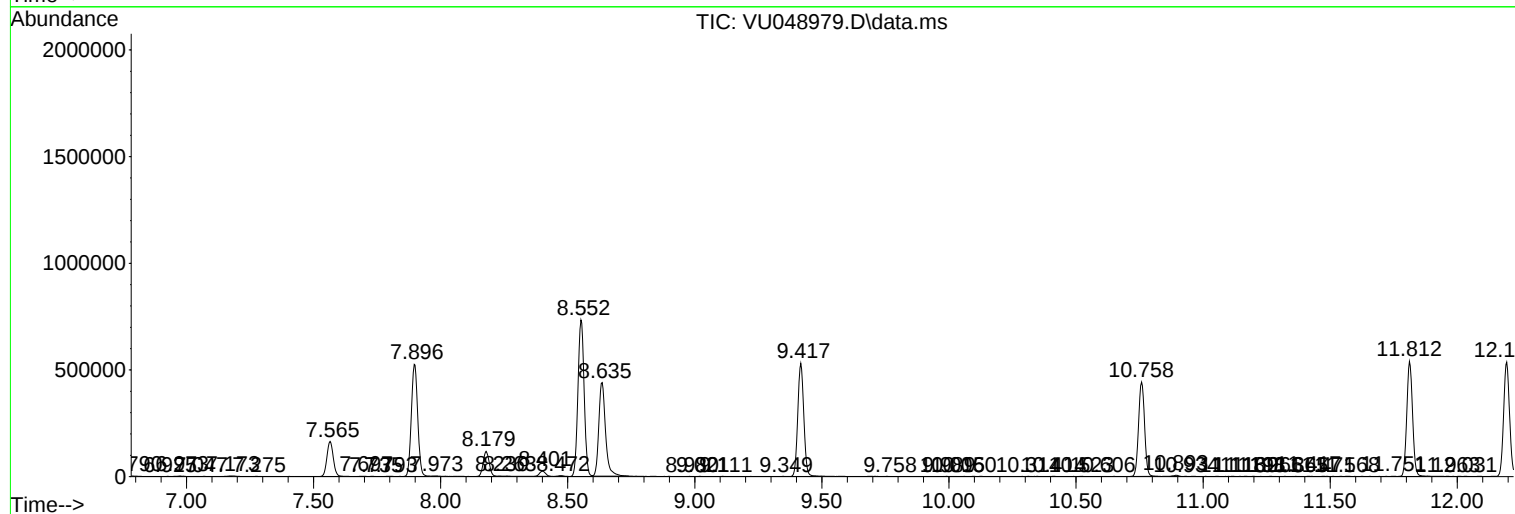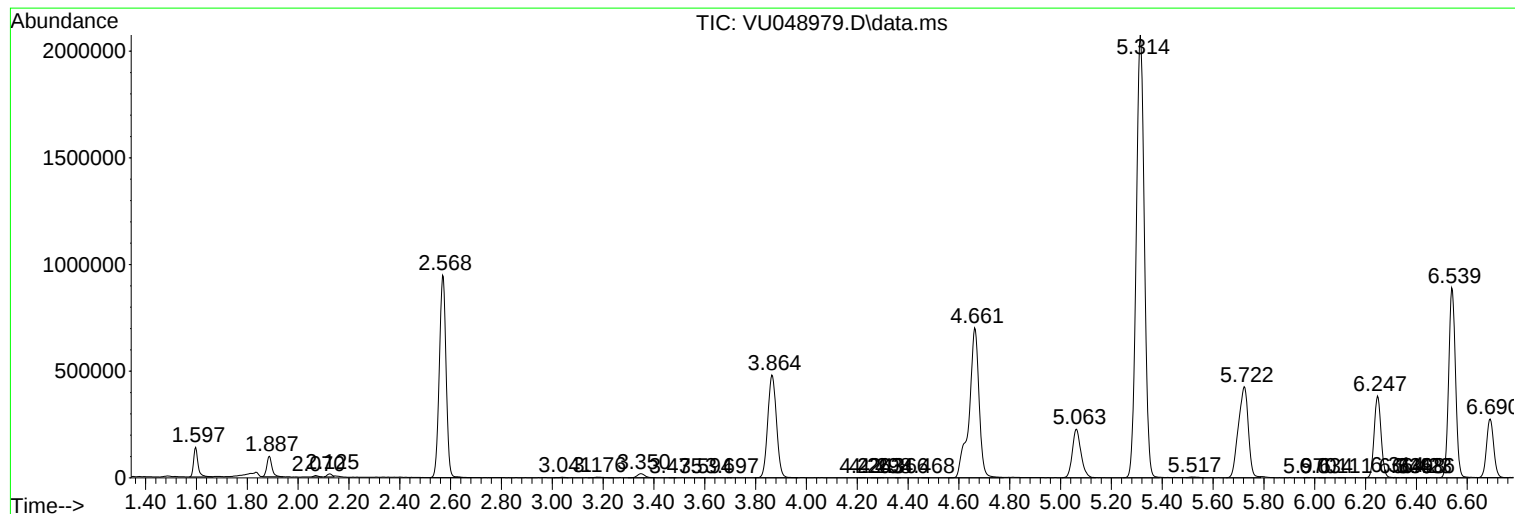

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048979.D
Acq On : 09 Jun 2022 15:07
Operator : SY/MD
Sample : N3248-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048979.D
Acq On : 09 Jun 2022 15:07
Operator : SY/MD
Sample : N3248-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc