

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048980.D
 Acq On : 09 Jun 2022 15:30
 Operator : SY/MD
 Sample : N3248-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	136743	156178	13.34%	1.571%
2	1.893	164	172	186	rVB	98110	129778	11.09%	1.305%
3	2.562	367	380	396	rBV	231453	381355	32.57%	3.835%
4	2.626	396	400	409	rVV6	2055	3086	0.26%	0.031%
5	2.662	409	411	415	rVB4	778	480	0.04%	0.005%
6	2.755	437	440	442	rBV	348	255	0.02%	0.003%
7	2.771	442	445	447	rBV	566	452	0.04%	0.005%
8	2.819	457	460	461	rBV2	486	264	0.02%	0.003%
9	3.041	525	529	537	rVB4	814	1043	0.09%	0.010%
10	3.080	538	541	548	rVB2	381	344	0.03%	0.003%
11	3.186	559	574	581	rBV4	2060	4194	0.36%	0.042%
12	3.350	613	625	640	rBV3	16883	33338	2.85%	0.335%
13	3.449	654	656	660	rVB	424	241	0.02%	0.002%
14	3.723	738	741	744	rBV2	339	255	0.02%	0.003%
15	3.867	771	786	801	rVV3	24546	57771	4.93%	0.581%
16	3.922	801	803	810	rVB2	325	282	0.02%	0.003%
17	3.974	815	819	822	rBV	391	338	0.03%	0.003%
18	4.041	835	840	843	rBV2	311	295	0.03%	0.003%
19	4.089	853	855	860	rVB2	298	267	0.02%	0.003%
20	4.121	860	865	869	rBV2	406	419	0.04%	0.004%
21	4.250	903	905	911	rVV	387	369	0.03%	0.004%
22	4.292	915	918	924	rVB	347	277	0.02%	0.003%
23	4.465	969	972	978	rVB	317	260	0.02%	0.003%
24	4.494	978	981	986	rBV2	276	250	0.02%	0.003%
25	4.536	990	994	997	rBV2	260	242	0.02%	0.002%
26	4.620	1007	1020	1028	rBV	148287	336389	28.73%	3.383%
27	4.787	1069	1072	1075	rVB2	380	300	0.03%	0.003%
28	5.063	1137	1158	1180	rBV	220414	489196	41.79%	4.920%
29	5.227	1207	1209	1216	rVB2	335	278	0.02%	0.003%
30	5.314	1220	1236	1258	rBV	73316	166313	14.21%	1.673%
31	5.723	1342	1363	1382	rBV2	432797	1170743	100.00%	11.774%
32	5.970	1436	1440	1441	rBV	977	580	0.05%	0.006%
33	6.022	1451	1456	1457	rBV2	354	263	0.02%	0.003%
34	6.144	1490	1494	1497	rBV	306	233	0.02%	0.002%
35	6.247	1512	1526	1543	rBV	371842	705683	60.28%	7.097%
36	6.330	1550	1552	1557	rVB3	774	538	0.05%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048980.D
 Acq On : 09 Jun 2022 15:30
 Operator : SY/MD
 Sample : N3248-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.417	1575	1579	1586	rVB4	621	896	0.08%	0.009%
38	6.469	1591	1595	1597	rBV	546	359	0.03%	0.004%
39	6.539	1605	1617	1633	rBV2	70119	133822	11.43%	1.346%
40	6.690	1648	1664	1685	rBV	283516	546984	46.72%	5.501%
41	6.803	1693	1699	1700	rBV5	841	730	0.06%	0.007%
42	6.854	1713	1715	1720	rVB	384	251	0.02%	0.003%
43	6.980	1751	1754	1758	rVB3	678	391	0.03%	0.004%
44	7.015	1762	1765	1772	rBV2	278	297	0.03%	0.003%
45	7.079	1781	1785	1787	rBV2	413	321	0.03%	0.003%
46	7.105	1790	1793	1796	rVB3	414	304	0.03%	0.003%
47	7.134	1799	1802	1805	rBV2	381	311	0.03%	0.003%
48	7.176	1805	1815	1822	rBV5	1548	2876	0.25%	0.029%
49	7.260	1836	1841	1844	rVB	538	336	0.03%	0.003%
50	7.501	1913	1916	1919	rBV	384	237	0.02%	0.002%
51	7.565	1919	1936	1952	rBV	158357	275922	23.57%	2.775%
52	7.797	2003	2008	2010	rVB2	471	411	0.04%	0.004%
53	7.816	2010	2014	2022	rVB3	599	735	0.06%	0.007%
54	7.896	2022	2039	2061	rBV	536173	921041	78.67%	9.263%
55	8.179	2111	2127	2143	rBV2	120308	222772	19.03%	2.240%
56	8.469	2207	2217	2230	rBV4	3209	5681	0.49%	0.057%
57	8.552	2230	2243	2256	rBV	82453	136248	11.64%	1.370%
58	8.632	2256	2268	2297	rBV2	439425	802354	68.53%	8.070%
59	8.816	2323	2325	2328	rBV2	379	258	0.02%	0.003%
60	9.015	2381	2387	2389	rBV2	313	297	0.03%	0.003%
61	9.134	2418	2424	2426	rBV2	456	504	0.04%	0.005%
62	9.417	2499	2512	2533	rBV	505645	845812	72.25%	8.507%
63	9.558	2554	2556	2560	rBV	393	324	0.03%	0.003%
64	9.610	2570	2572	2579	rVB	372	259	0.02%	0.003%
65	9.694	2594	2598	2602	rVB3	397	386	0.03%	0.004%
66	9.784	2624	2626	2632	rVB3	466	375	0.03%	0.004%
67	9.822	2632	2638	2640	rBV2	353	343	0.03%	0.003%
68	9.909	2662	2665	2671	rVB2	383	293	0.03%	0.003%
69	9.980	2684	2687	2691	rBV	415	357	0.03%	0.004%
70	10.028	2697	2702	2705	rVV	314	270	0.02%	0.003%
71	10.105	2721	2726	2729	rBV3	608	562	0.05%	0.006%
72	10.465	2833	2838	2841	rVB2	327	296	0.03%	0.003%
73	10.488	2841	2845	2846	rBV	318	245	0.02%	0.002%
74	10.555	2863	2866	2870	rBV2	287	261	0.02%	0.003%
75	10.636	2886	2891	2893	rBV2	520	465	0.04%	0.005%
76	10.758	2916	2929	2952	rBV	438382	706052	60.31%	7.101%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048980.D
 Acq On : 09 Jun 2022 15:30
 Operator : SY/MD
 Sample : N3248-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	10.893	2961	2971	2988	rVB3	5088	8556	0.73%	0.086%
78	11.185	3055	3062	3065	rBV2	296	409	0.03%	0.004%
79	11.414	3131	3133	3137	rBV2	507	301	0.03%	0.003%
80	11.549	3170	3175	3177	rBV2	261	238	0.02%	0.002%
81	11.742	3232	3235	3239	rBV2	387	343	0.03%	0.003%
82	11.812	3244	3257	3276	rBV	509264	807088	68.94%	8.117%
83	11.980	3306	3309	3312	rVB3	368	251	0.02%	0.003%
84	12.025	3319	3323	3326	rVB2	374	275	0.02%	0.003%
85	12.192	3362	3375	3399	rBV	532933	863287	73.74%	8.682%
86	12.523	3473	3478	3483	rVB2	498	611	0.05%	0.006%
87	12.777	3545	3557	3564	rBV5	1985	2958	0.25%	0.030%
88	12.825	3569	3572	3575	rBV3	406	241	0.02%	0.002%
89	12.870	3583	3586	3590	rBV2	301	323	0.03%	0.003%
90	13.324	3723	3727	3729	rBV	508	396	0.03%	0.004%
91	13.340	3729	3732	3738	rVB3	649	702	0.06%	0.007%
92	13.507	3780	3784	3787	rBV2	501	399	0.03%	0.004%
93	13.632	3819	3823	3826	rBV2	532	414	0.04%	0.004%
94	13.738	3854	3856	3863	rVB3	562	445	0.04%	0.004%
95	13.983	3929	3932	3934	rBV	431	294	0.03%	0.003%
96	14.192	3994	3997	4000	rBV3	571	352	0.03%	0.004%
97	14.340	4040	4043	4049	rVB3	742	717	0.06%	0.007%
98	14.648	4137	4139	4145	rVB3	642	438	0.04%	0.004%
99	15.256	4325	4328	4329	rBV	445	247	0.02%	0.002%
100	15.414	4374	4377	4380	rBV2	810	566	0.05%	0.006%




Sum of corrected areas: 9943038

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048980.D
Acq On : 09 Jun 2022 15:30
Operator : SY/MD
Sample : N3248-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

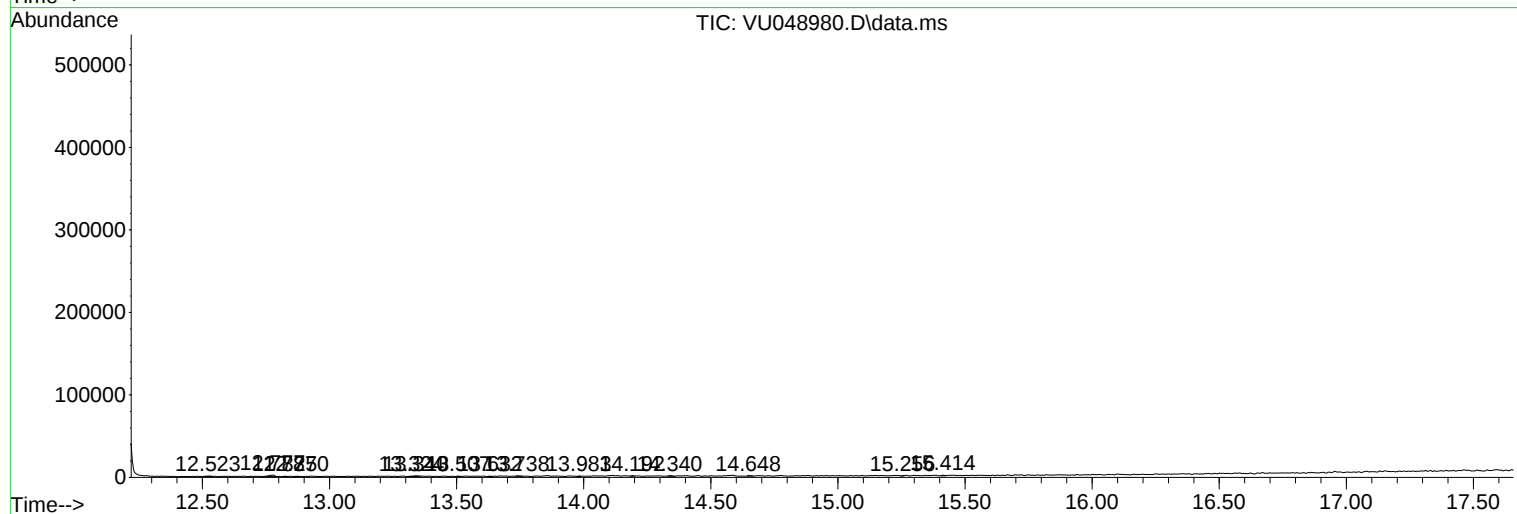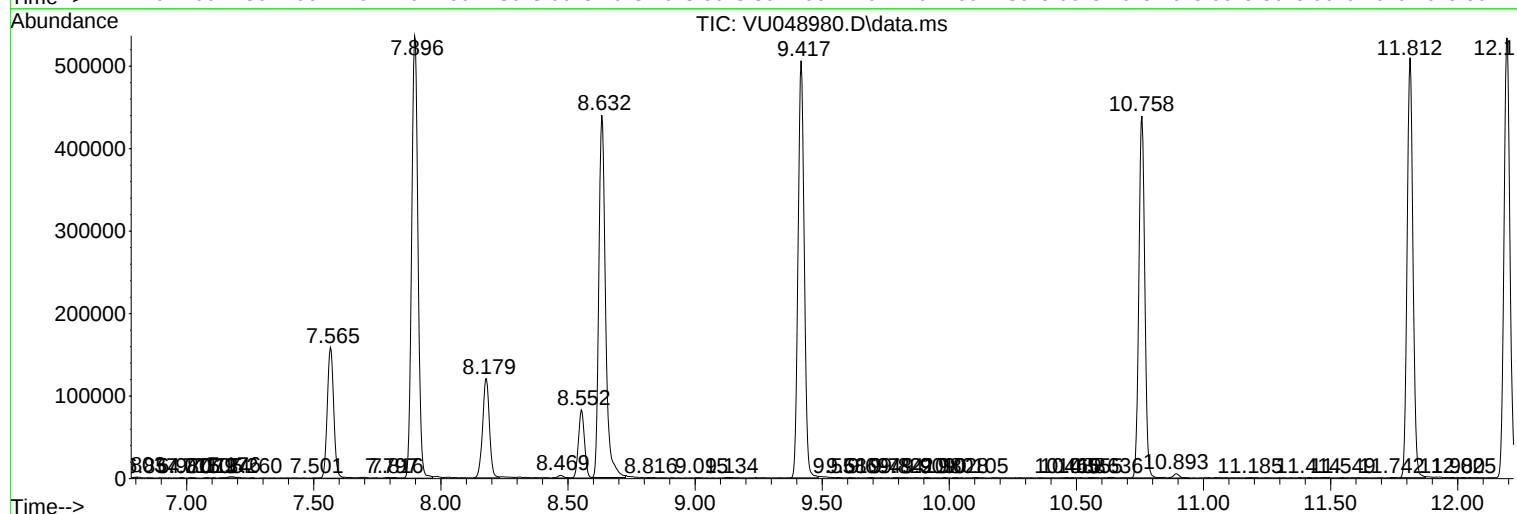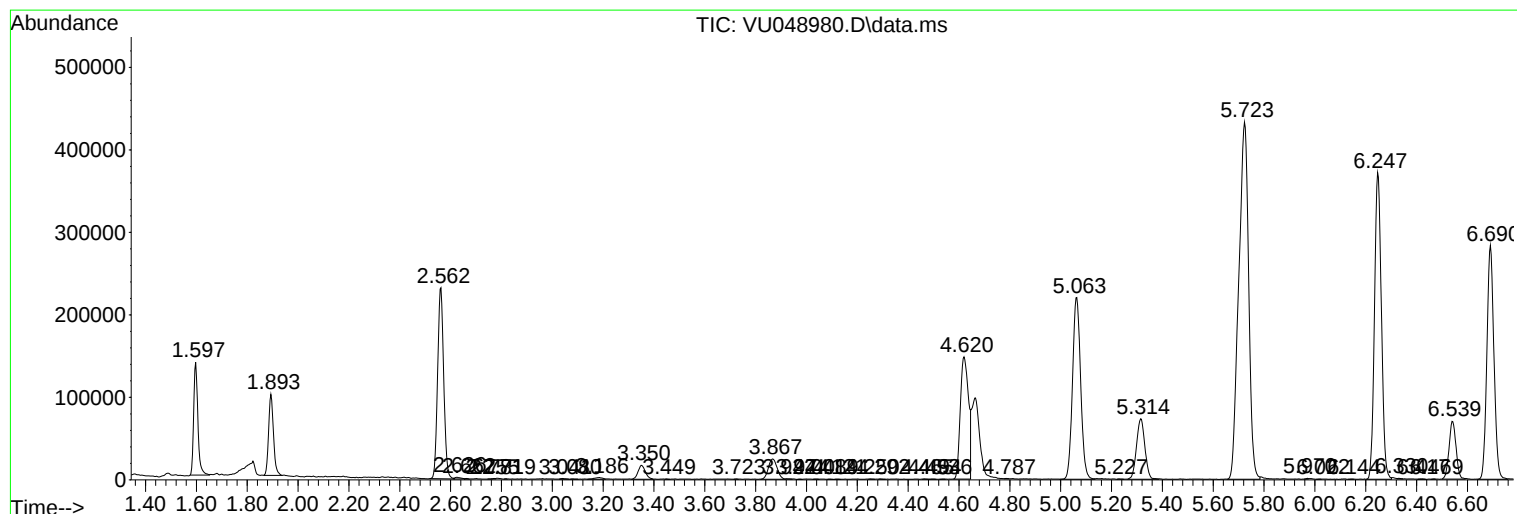

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048980.D
Acq On : 09 Jun 2022 15:30
Operator : SY/MD
Sample : N3248-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048980.D
Acq On : 09 Jun 2022 15:30
Operator : SY/MD
Sample : N3248-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc