

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048987.D
 Acq On : 09 Jun 2022 19:39
 Operator : SY/MD
 Sample : N3248-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048987.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	96	rVB	141306	159072	13.19%	1.478%
2	1.897	166	173	199	rVB	100414	140572	11.66%	1.306%
3	2.562	368	380	396	rBV2	244278	414555	34.38%	3.852%
4	2.739	433	435	436	rBV2	346	155	0.01%	0.001%
5	3.038	525	528	539	rVB4	964	1320	0.11%	0.012%
6	3.099	544	547	550	rBV	295	181	0.02%	0.002%
7	3.118	550	553	559	rBV2	207	248	0.02%	0.002%
8	3.186	563	574	576	rBV3	2061	3323	0.28%	0.031%
9	3.350	619	625	638	rVB5	3675	6732	0.56%	0.063%
10	3.594	698	701	705	rBV2	196	140	0.01%	0.001%
11	3.868	769	786	809	rBV	72571	167465	13.89%	1.556%
12	4.012	828	831	835	rBV2	297	185	0.02%	0.002%
13	4.083	852	853	854	rBV	128	33	0.00%	0.000%
14	4.327	926	929	930	rBV	222	130	0.01%	0.001%
15	4.401	950	952	956	rBV2	243	203	0.02%	0.002%
16	4.446	960	966	971	rVB2	342	406	0.03%	0.004%
17	4.472	971	974	975	rBV2	306	218	0.02%	0.002%
18	4.514	986	987	990	rBV2	254	108	0.01%	0.001%
19	4.533	990	993	997	rBV	151	136	0.01%	0.001%
20	4.620	1007	1020	1051	rBV	150148	415912	34.49%	3.865%
21	4.925	1111	1115	1120	rBV2	290	269	0.02%	0.002%
22	4.983	1128	1133	1139	rVB2	662	691	0.06%	0.006%
23	5.064	1139	1158	1181	rBV	225356	502720	41.69%	4.671%
24	5.160	1186	1188	1190	rBV	451	225	0.02%	0.002%
25	5.208	1201	1203	1204	rBV	121	41	0.00%	0.000%
26	5.224	1206	1208	1212	rVV2	245	164	0.01%	0.002%
27	5.314	1218	1236	1258	rBV	433960	974709	80.82%	9.057%
28	5.469	1282	1284	1286	rBV	310	195	0.02%	0.002%
29	5.520	1298	1300	1301	rBV	323	144	0.01%	0.001%
30	5.723	1341	1363	1386	rBV2	448760	1205962	100.00%	11.206%
31	5.977	1436	1442	1450	rVB5	843	1299	0.11%	0.012%
32	6.028	1455	1458	1459	rBV2	160	84	0.01%	0.001%
33	6.093	1476	1478	1480	rBV	163	85	0.01%	0.001%
34	6.115	1483	1485	1491	rVB2	397	291	0.02%	0.003%
35	6.247	1511	1526	1544	rBV	374967	704658	58.43%	6.548%
36	6.469	1593	1595	1597	rBV2	307	134	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048987.D
 Acq On : 09 Jun 2022 19:39
 Operator : SY/MD
 Sample : N3248-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.485	1597	1600	1605	rVB2	270	257	0.02%	0.002%
38	6.543	1605	1618	1632	rBV4	18328	35760	2.97%	0.332%
39	6.633	1643	1646	1649	rBV	494	337	0.03%	0.003%
40	6.691	1649	1664	1682	rBV	289647	559882	46.43%	5.202%
41	6.861	1714	1717	1719	rBV	202	116	0.01%	0.001%
42	6.896	1725	1728	1731	rBV2	306	202	0.02%	0.002%
43	7.070	1779	1782	1784	rBV	238	121	0.01%	0.001%
44	7.138	1798	1803	1806	rBV3	513	522	0.04%	0.005%
45	7.173	1806	1814	1820	rBV5	1459	2212	0.18%	0.021%
46	7.292	1849	1851	1854	rBV2	298	193	0.02%	0.002%
47	7.314	1855	1858	1862	rVV2	298	226	0.02%	0.002%
48	7.359	1868	1872	1877	rBV2	365	346	0.03%	0.003%
49	7.408	1885	1887	1890	rVB2	270	123	0.01%	0.001%
50	7.498	1909	1915	1916	rBV2	375	329	0.03%	0.003%
51	7.565	1923	1936	1953	rBV	161304	278116	23.06%	2.584%
52	7.790	2003	2006	2012	rBV3	522	567	0.05%	0.005%
53	7.835	2017	2020	2022	rBV	165	81	0.01%	0.001%
54	7.896	2026	2039	2057	rBV	526368	908572	75.34%	8.442%
55	8.083	2091	2097	2098	rBV2	394	341	0.03%	0.003%
56	8.121	2106	2109	2114	rBV2	257	247	0.02%	0.002%
57	8.179	2115	2127	2145	rBV2	114905	192019	15.92%	1.784%
58	8.552	2232	2243	2255	rBV2	43076	71724	5.95%	0.666%
59	8.633	2255	2268	2299	rBV2	443052	812931	67.41%	7.554%
60	8.867	2339	2341	2344	rBV	310	227	0.02%	0.002%
61	8.906	2351	2353	2357	rVB2	422	216	0.02%	0.002%
62	8.983	2375	2377	2382	rVB2	411	282	0.02%	0.003%
63	9.186	2436	2440	2443	rBV2	216	191	0.02%	0.002%
64	9.221	2447	2451	2454	rBV	359	360	0.03%	0.003%
65	9.266	2462	2465	2467	rBV2	344	216	0.02%	0.002%
66	9.337	2483	2487	2491	rBV2	225	157	0.01%	0.001%
67	9.359	2491	2494	2495	rBV	222	110	0.01%	0.001%
68	9.417	2498	2512	2529	rBV	512423	836123	69.33%	7.769%
69	9.613	2572	2573	2576	rBV	198	82	0.01%	0.001%
70	9.633	2576	2579	2586	rVB2	290	269	0.02%	0.002%
71	9.742	2610	2613	2615	rBV	384	243	0.02%	0.002%
72	9.867	2647	2652	2655	rBV	291	288	0.02%	0.003%
73	9.935	2670	2673	2675	rBV	309	196	0.02%	0.002%
74	10.006	2692	2695	2701	rBV2	291	251	0.02%	0.002%
75	10.105	2718	2726	2735	rBV8	1252	1907	0.16%	0.018%
76	10.478	2839	2842	2847	rBV2	491	424	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048987.D
 Acq On : 09 Jun 2022 19:39
 Operator : SY/MD
 Sample : N3248-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	10.501	2847	2849	2851	rBV	268	127	0.01%	0.001%
78	10.639	2890	2892	2896	rBV3	405	284	0.02%	0.003%
79	10.758	2916	2929	2953	rBV	421123	682067	56.56%	6.338%
80	10.932	2980	2983	2989	rVB2	422	419	0.03%	0.004%
81	10.964	2989	2993	2998	rBV2	552	635	0.05%	0.006%
82	11.002	2999	3005	3010	rBV4	1031	1325	0.11%	0.012%
83	11.063	3018	3024	3025	rBV2	258	231	0.02%	0.002%
84	11.472	3144	3151	3160	rVB3	5276	7660	0.64%	0.071%
85	11.813	3244	3257	3277	rBV	505024	809596	67.13%	7.523%
86	12.028	3319	3324	3325	rBV	456	331	0.03%	0.003%
87	12.060	3327	3334	3342	rBV4	7440	12556	1.04%	0.117%
88	12.192	3363	3375	3391	rBV	505901	837180	69.42%	7.779%
89	12.671	3521	3524	3525	rBV2	468	254	0.02%	0.002%




Sum of corrected areas: 10762196

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048987.D
Acq On : 09 Jun 2022 19:39
Operator : SY/MD
Sample : N3248-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

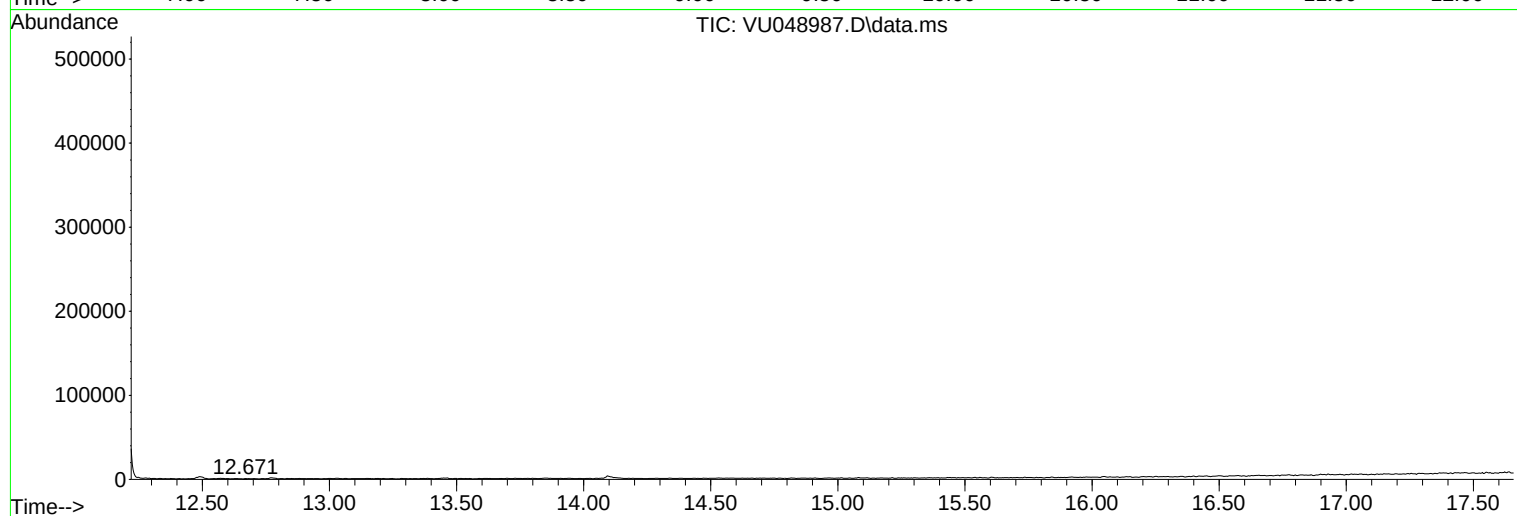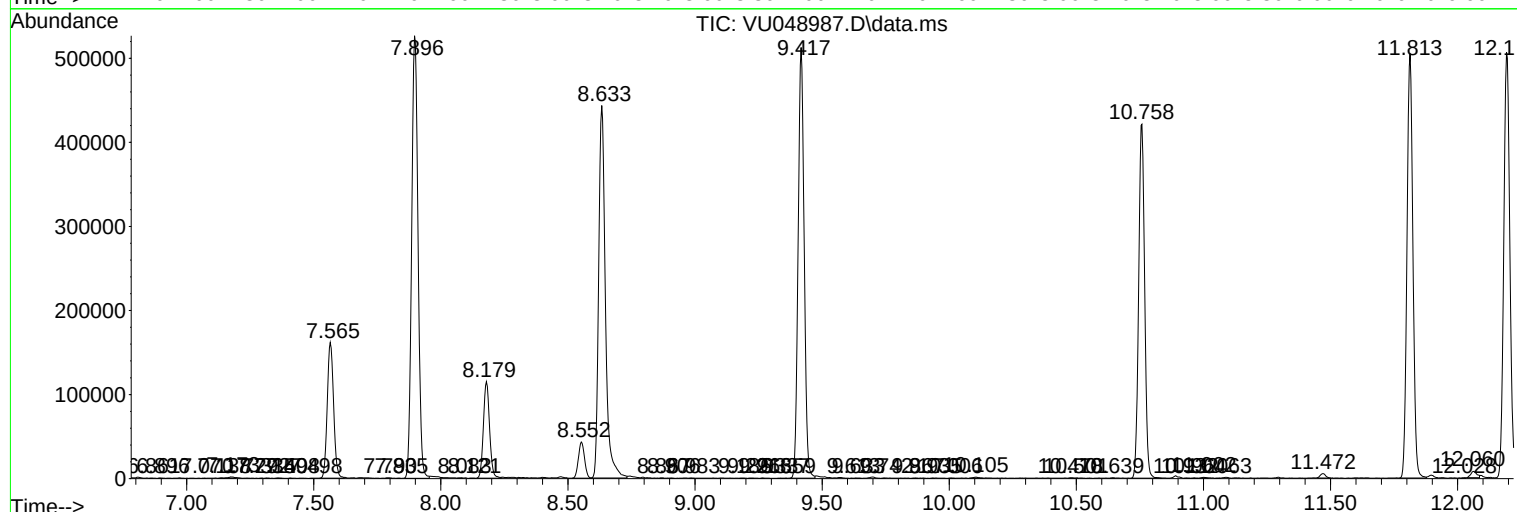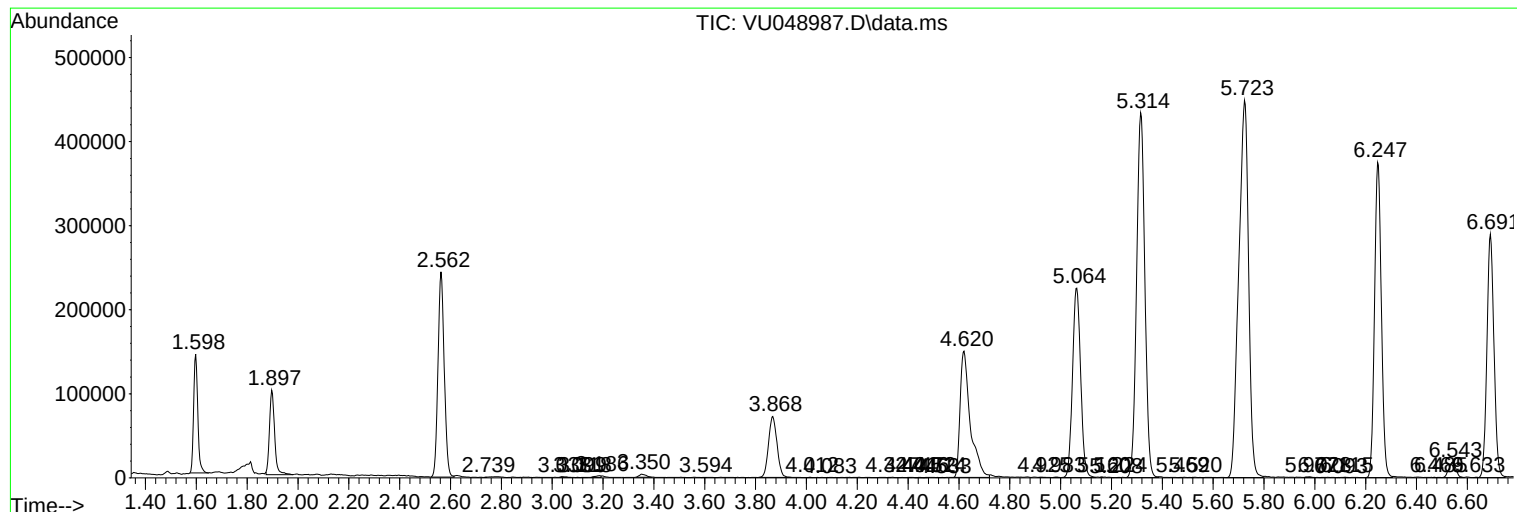

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048987.D
Acq On : 09 Jun 2022 19:39
Operator : SY/MD
Sample : N3248-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048987.D
Acq On : 09 Jun 2022 19:39
Operator : SY/MD
Sample : N3248-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------