


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048972.D
Acq On : 09 Jun 2022 08:49
Operator : SY/MD
Sample : BFB094
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB094

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Title : VOC Analysis
Last Update : Fri Jun 10 01:01:44 2022

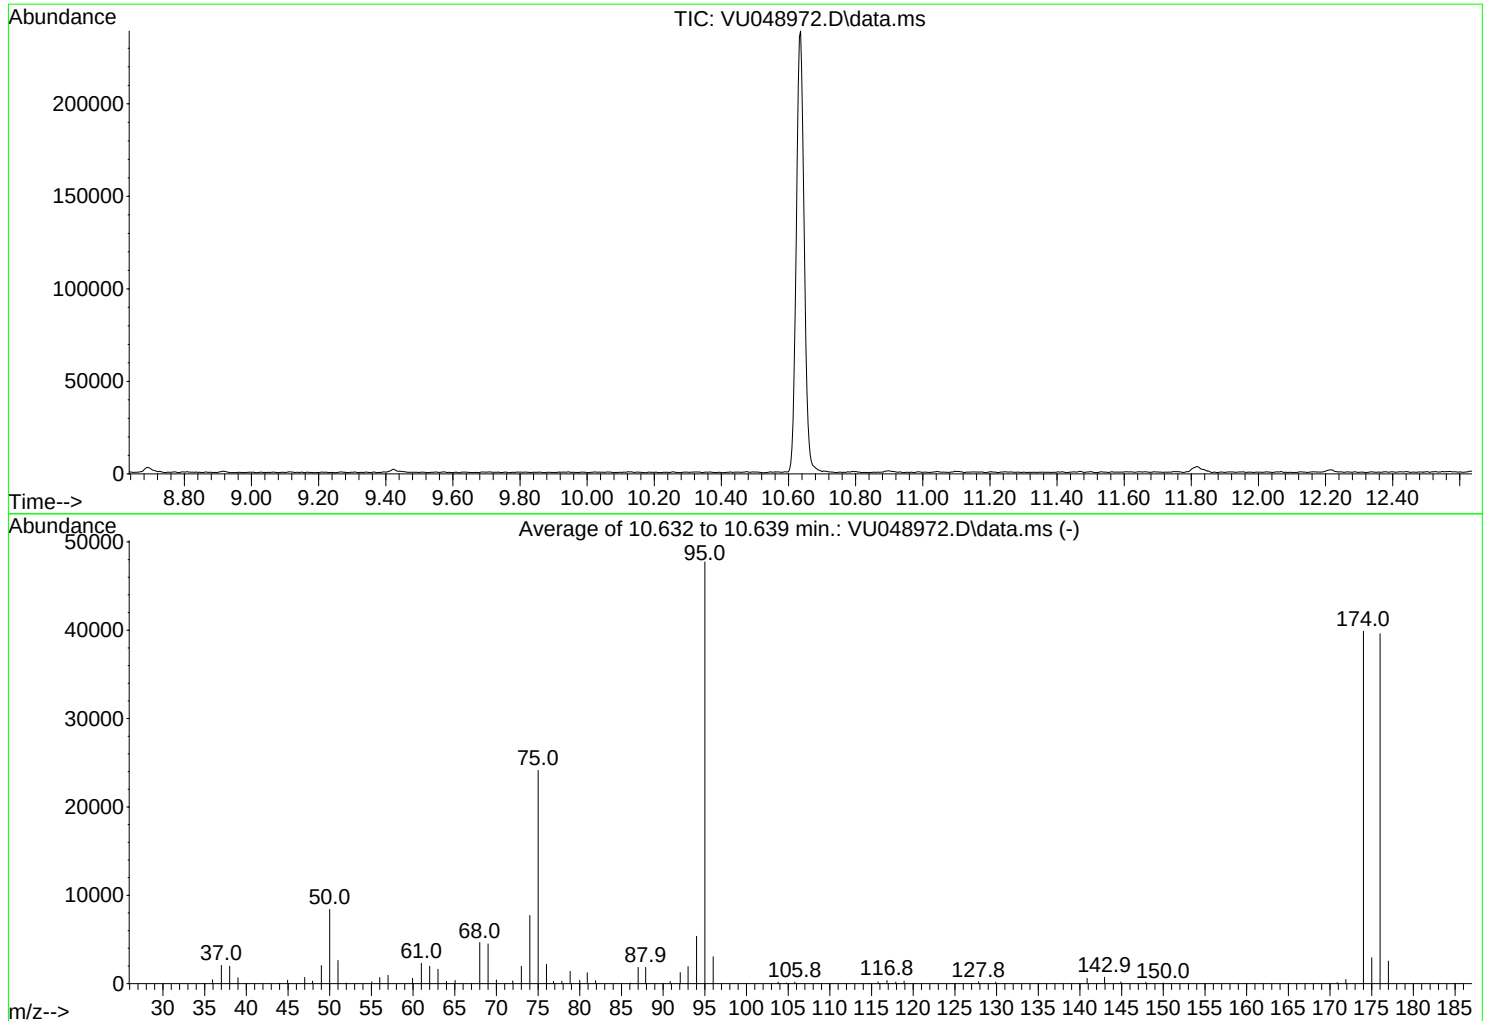

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	8404	PASS
75	95	30	80	50.6	24147	PASS
95	95	100	100	100.0	47741	PASS
96	95	5	9	6.4	3042	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.6	39896	PASS
175	174	5	9	7.3	2931	PASS
176	174	95	101	99.3	39611	PASS
177	176	5	9	6.4	2554	PASS

m/z	Abundance
39.90	593.0
44.00	505.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094

m/z	Abundance
35.90	487.0
37.00	2145.0
38.00	2142.0
39.00	742.0
39.90	448.0
43.80	546.0
45.00	417.0
46.90	756.0
47.90	323.0
49.00	2107.0
50.00	8859.0
51.00	2829.0
55.00	153.0
56.00	639.0
57.00	1042.0
59.90	668.0
61.00	2224.0
62.00	2133.0
63.00	1748.0
63.90	269.0
65.00	321.0
67.00	118.0
68.00	4521.0
69.00	4535.0
70.00	391.0
71.90	294.0
73.00	1875.0
74.00	8186.0
75.00	25000.0
76.00	2260.0
76.90	296.0
77.80	205.0
78.90	1364.0
80.00	390.0
80.90	1266.0
81.90	371.0
86.10	107.0
87.00	1904.0
87.90	1785.0
90.80	241.0
92.10	1390.0
93.00	2068.0
94.00	5733.0
95.00	48624.0
96.00	3227.0
103.70	174.0
105.80	179.0
115.80	221.0
116.90	385.0
117.90	163.0
118.90	295.0
127.80	169.0
130.00	226.0
140.80	670.0
142.90	662.0
144.90	166.0
147.90	173.0
150.00	105.0
170.90	123.0
171.90	426.0
174.00	39584.0
175.00	2887.0
176.00	39920.0
177.00	2622.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094

m/z	Abundance
36.00	433.0
37.00	2135.0
38.00	2072.0
39.00	679.0
39.90	491.0
43.80	522.0
44.90	411.0
47.00	730.0
48.00	311.0
49.00	2157.0
50.00	8729.0
51.00	2713.0
52.00	119.0
55.10	202.0
56.00	713.0
57.00	962.0
59.90	651.0
61.00	2390.0
62.00	1999.0
63.00	1659.0
64.00	243.0
65.10	386.0
68.00	4825.0
69.00	4573.0
70.00	434.0
71.90	333.0
73.00	2036.0
74.00	7914.0
75.00	24864.0
76.00	2253.0
76.90	233.0
77.80	277.0
78.80	1467.0
80.00	380.0
80.90	1244.0
81.90	368.0
86.10	114.0
87.00	1920.0
87.90	1982.0
90.80	269.0
92.00	1231.0
93.00	1978.0
94.00	5439.0
95.00	49032.0
96.00	3125.0
103.80	185.0
104.80	100.0
105.80	198.0
115.80	217.0
116.80	374.0
117.90	193.0
118.90	296.0
127.90	236.0
129.90	192.0
140.90	613.0
142.90	787.0
144.90	213.0
147.90	180.0
150.00	103.0
170.90	141.0
171.90	494.0
174.00	41104.0
175.00	2974.0
176.00	41032.0
177.00	2694.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094

m/z	Abundance
35.90	380.0
37.00	1945.0
38.00	1717.0
39.00	604.0
39.90	551.0
43.90	519.0
44.90	370.0
47.10	655.0
47.90	240.0
49.00	1890.0
50.00	7625.0
51.00	2318.0
52.00	101.0
55.00	228.0
56.00	731.0
57.00	811.0
60.00	545.0
61.00	2310.0
62.00	1790.0
63.00	1465.0
64.10	255.0
65.10	389.0
68.00	4593.0
69.00	4347.0
70.00	457.0
72.00	308.0
73.00	1978.0
74.00	7041.0
75.00	22576.0
76.00	2059.0
76.80	235.0
77.90	327.0
78.80	1374.0
80.00	378.0
80.90	1179.0
81.90	319.0
87.00	1725.0
87.90	1794.0
90.90	250.0
92.00	1122.0
93.00	1752.0
94.00	4940.0
95.00	45568.0
96.00	2774.0
103.90	196.0
104.80	115.0
105.80	197.0
114.80	104.0
115.80	158.0
116.80	351.0
117.90	178.0
118.90	299.0
127.90	262.0
129.80	141.0
140.80	507.0
143.00	749.0
144.90	247.0
147.90	153.0
170.80	106.0
171.90	522.0
174.00	39000.0
175.00	2931.0
176.00	37880.0
177.00	2347.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094