

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
 Data File : VU054463.D
 Acq On : 09 Jun 2023 15:23
 Operator : MD/SY
 Sample : 03118-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FJ8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054463.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	107	rBV	80086	95444	9.53%	1.198%
2	1.914	186	194	211	rVB	84037	118916	11.87%	1.493%
3	2.566	383	397	411	rBV	146823	243522	24.31%	3.057%
4	2.640	411	420	433	rBV	8252	17619	1.76%	0.221%
5	3.197	577	593	595	rBV4	6641	12428	1.24%	0.156%
6	4.627	1024	1038	1083	rBV	147866	458079	45.74%	5.751%
7	5.058	1156	1172	1195	rVB2	172957	393249	39.26%	4.937%
8	5.721	1355	1378	1408	rBV2	330379	888622	88.72%	11.156%
9	6.245	1527	1541	1561	rBV	358152	703992	70.29%	8.838%
10	6.685	1665	1678	1707	rBV	220746	447220	44.65%	5.614%
11	7.563	1940	1951	1966	rBV2	100067	179096	17.88%	2.248%
12	7.894	2041	2054	2071	rBV	379441	673608	67.26%	8.456%
13	7.965	2074	2076	2090	rVB4	8854	13640	1.36%	0.171%
14	8.177	2131	2142	2158	rBV2	61369	107755	10.76%	1.353%
15	8.630	2271	2283	2318	rBV3	477299	1001557	100.00%	12.573%
16	9.415	2512	2527	2555	rBV	499577	860240	85.89%	10.799%
17	10.753	2931	2943	2962	rBV	165371	279389	27.90%	3.507%
18	10.891	2975	2986	2996	rBV4	6544	10716	1.07%	0.135%
19	11.807	3259	3271	3290	rBV	502354	823252	82.20%	10.335%
20	12.190	3376	3390	3412	rBV	379411	637364	63.64%	8.001%




Sum of corrected areas: 7965708

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
Data File : VU054463.D
Acq On : 09 Jun 2023 15:23
Operator : MD/SY
Sample : 03118-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

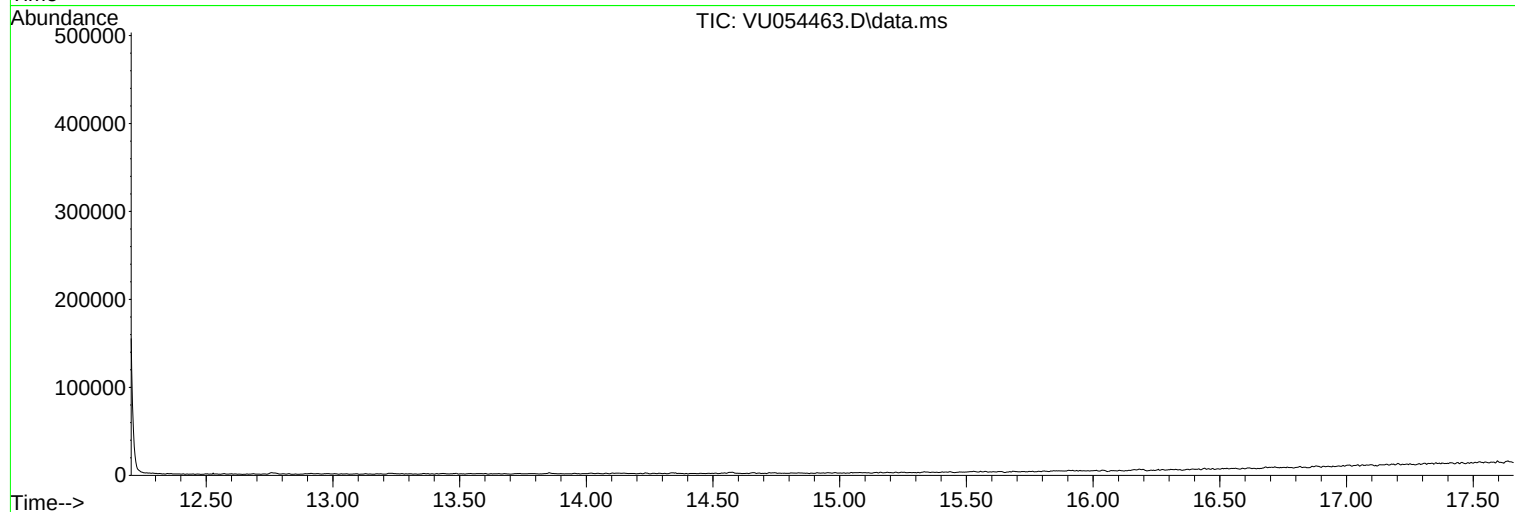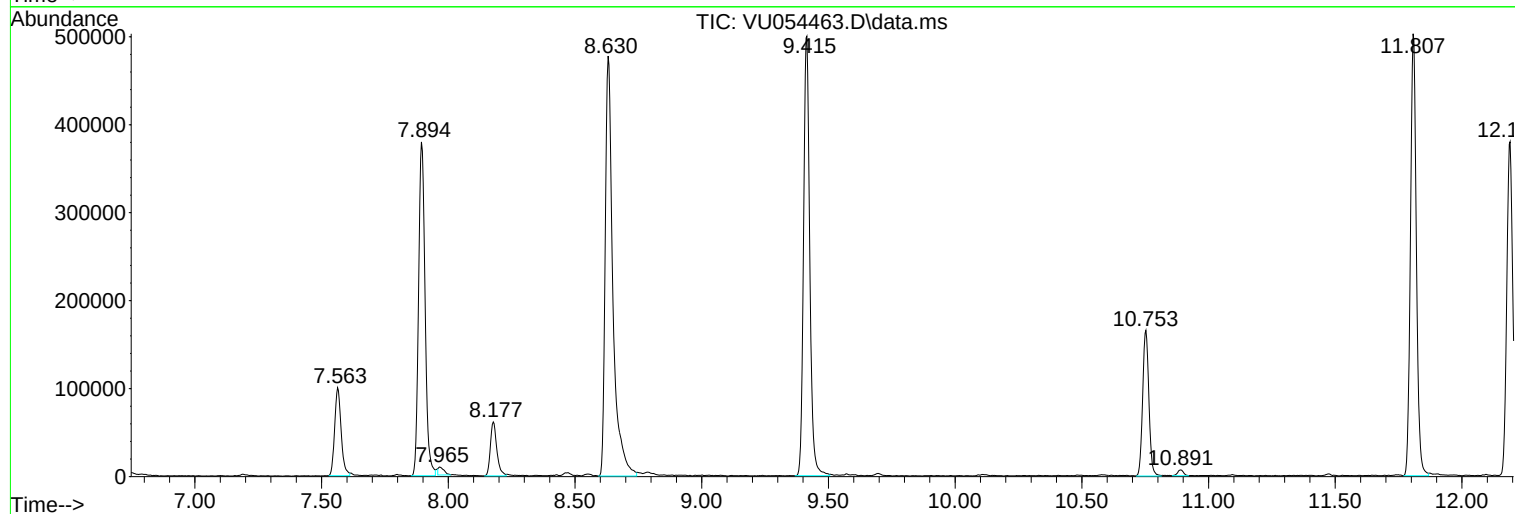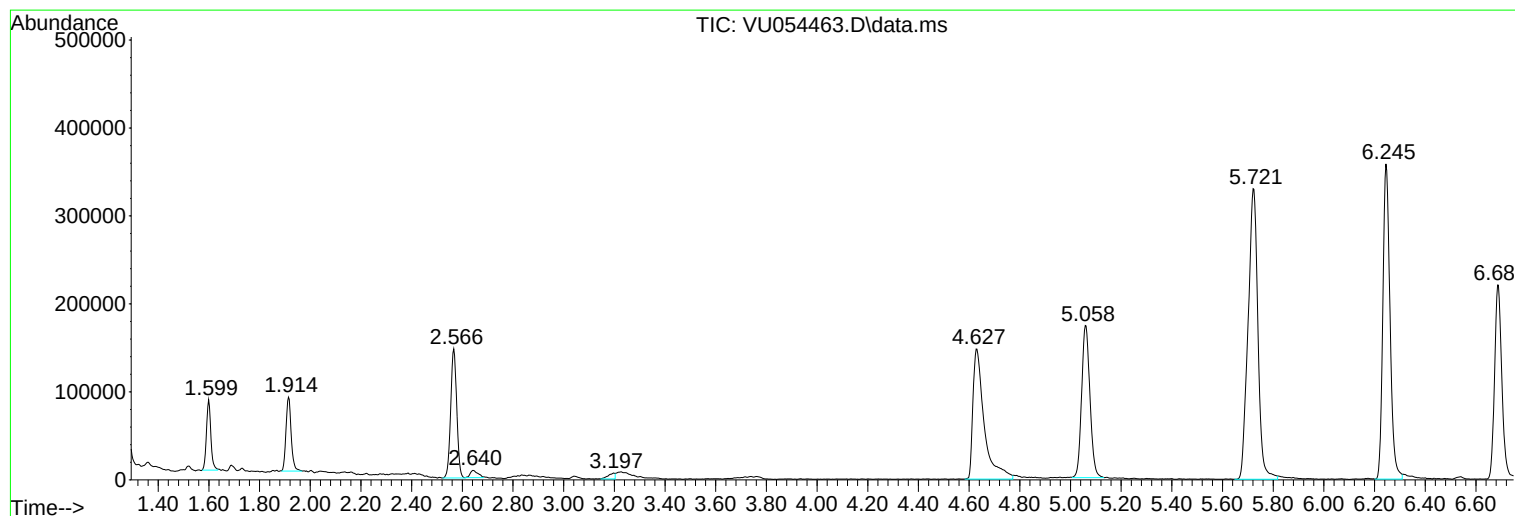

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
Data File : VU054463.D
Acq On : 09 Jun 2023 15:23
Operator : MD/SY
Sample : 03118-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
Data File : VU054463.D
Acq On : 09 Jun 2023 15:23
Operator : MD/SY
Sample : 03118-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc