

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
 Data File : VU054468.D
 Acq On : 09 Jun 2023 17:24
 Operator : MD/SY
 Sample : 03118-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FLO

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	107	rVB	86214	103573	9.49%	1.193%
2	1.914	186	194	210	rVB	95410	129994	11.91%	1.498%
3	2.563	383	396	411	rBV	160697	269292	24.68%	3.102%
4	4.631	1024	1039	1078	rBV	159688	478576	43.85%	5.513%
5	5.058	1156	1172	1196	rVB2	192377	434455	39.81%	5.005%
6	5.721	1356	1378	1403	rBV2	370840	978539	89.66%	11.273%
7	6.245	1527	1541	1570	rBV	366810	711740	65.22%	8.199%
8	6.541	1620	1633	1647	rBV6	15426	32275	2.96%	0.372%
9	6.689	1665	1679	1699	rBV2	241834	492730	45.15%	5.676%
10	7.563	1937	1951	1977	rBV	108873	203252	18.62%	2.342%
11	7.894	2040	2054	2075	rBV	426286	765460	70.14%	8.818%
12	8.177	2132	2142	2160	rBV	68066	118039	10.82%	1.360%
13	8.631	2271	2283	2319	rBV2	525489	1091337	100.00%	12.572%
14	9.412	2512	2526	2551	rBV	494191	850307	77.91%	9.796%
15	10.753	2930	2943	2963	rBV	190960	310462	28.45%	3.577%
16	11.052	3026	3036	3044	rBV5	5739	11150	1.02%	0.128%
17	11.807	3258	3271	3294	rBV	485045	794826	72.83%	9.157%
18	12.061	3339	3350	3372	rBV2	71678	182138	16.69%	2.098%
19	12.190	3378	3390	3417	rVB	432258	722222	66.18%	8.320%




Sum of corrected areas: 8680367

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
Data File : VU054468.D
Acq On : 09 Jun 2023 17:24
Operator : MD/SY
Sample : 03118-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FLO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

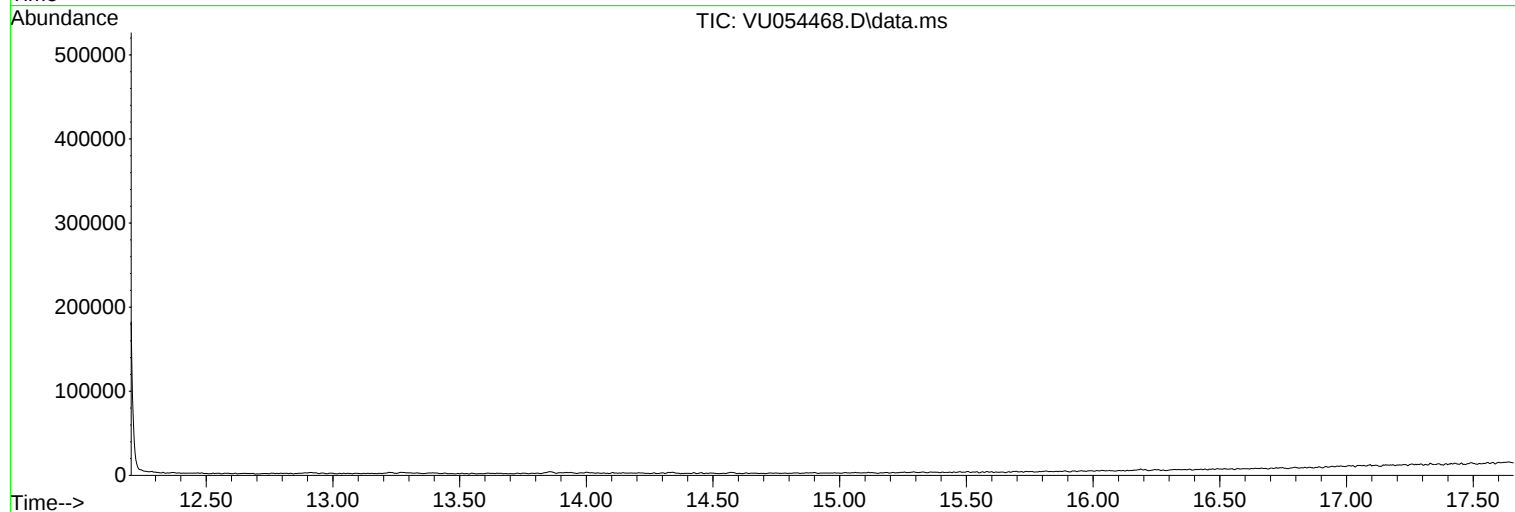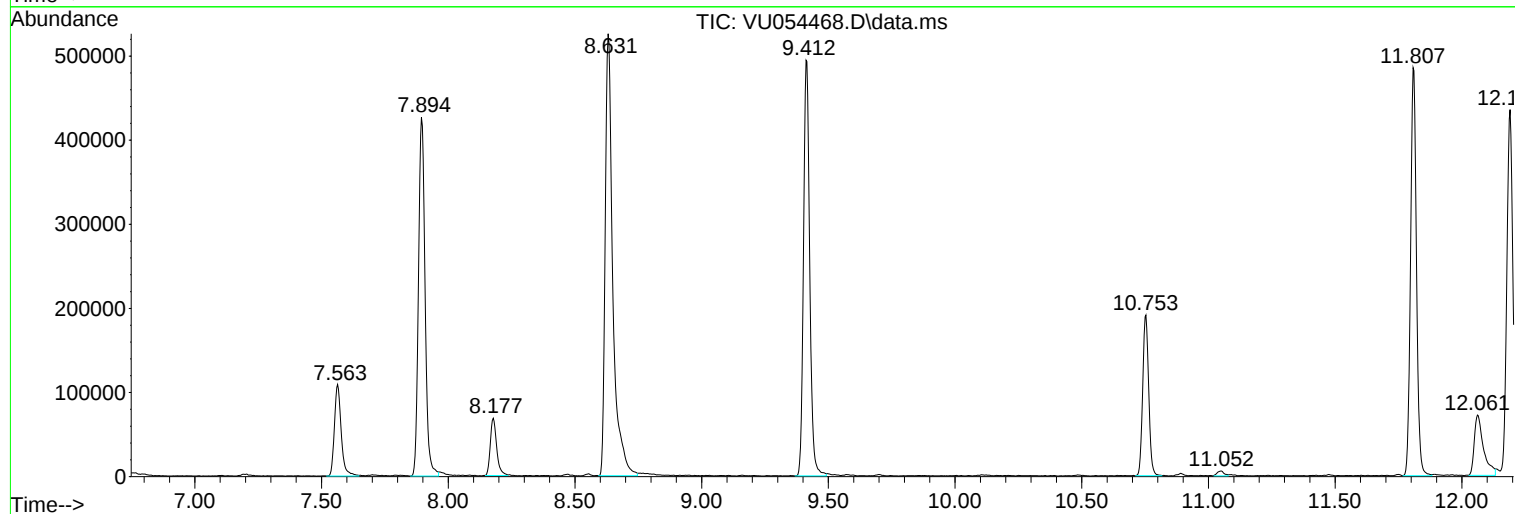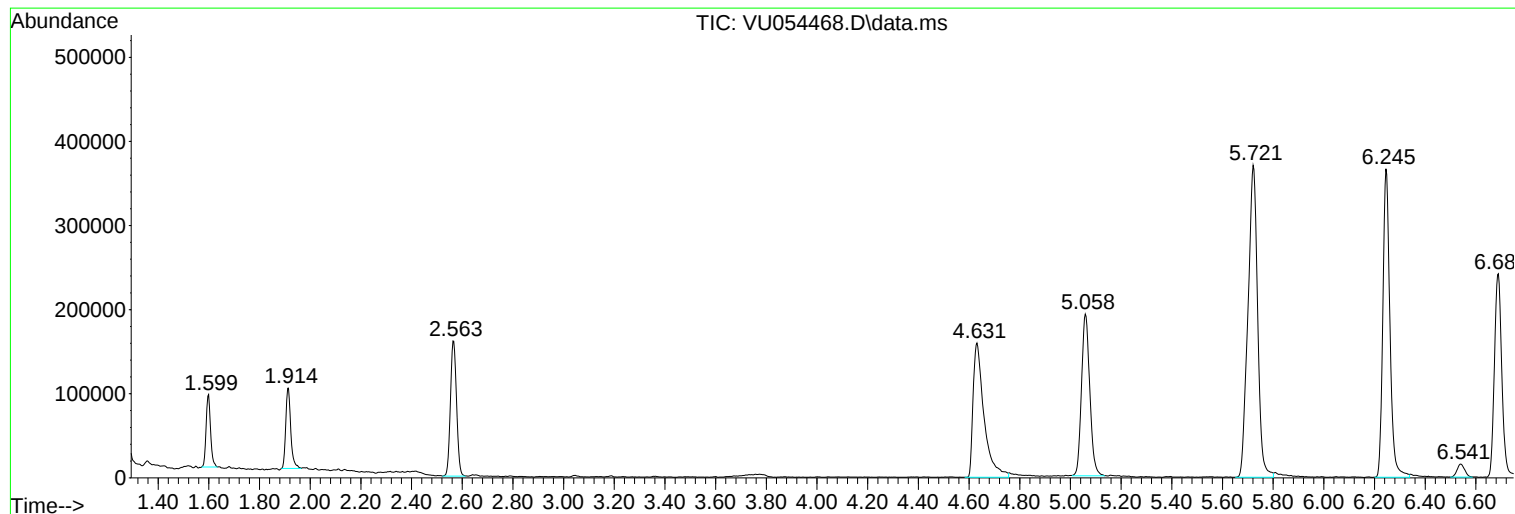

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
Data File : VU054468.D
Acq On : 09 Jun 2023 17:24
Operator : MD/SY
Sample : 03118-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COFLO










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.061	1.15 ug/L	182138	1,4-Dichlorobenzene-d4	11.811

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	83
2	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	78
3	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	78
4	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	64
5	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	64

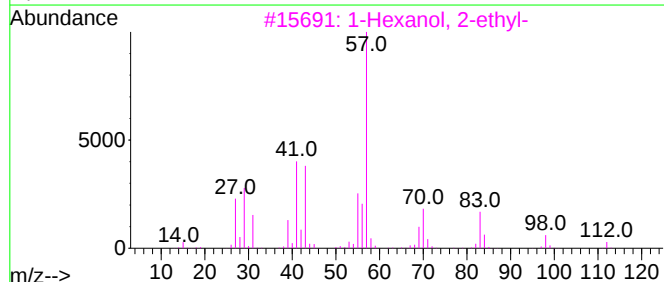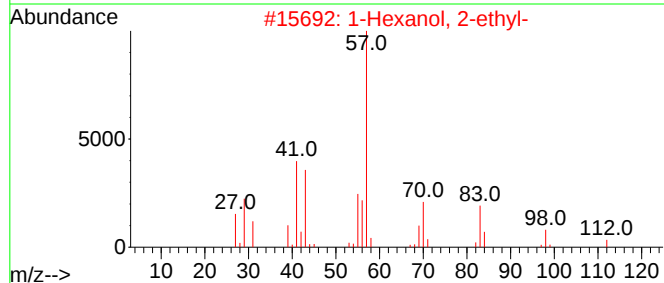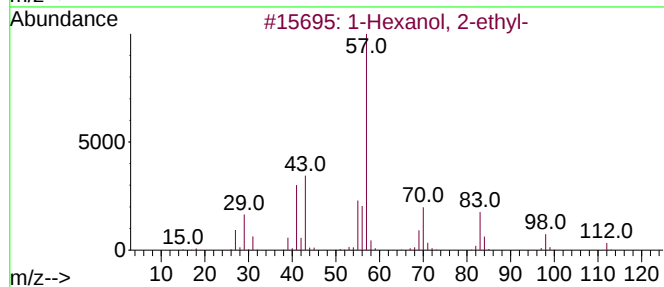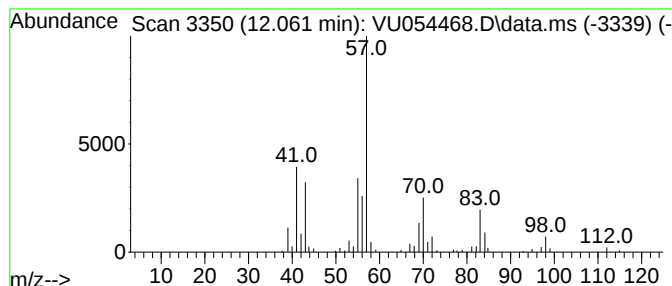

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
Data File : VU054468.D
Acq On : 09 Jun 2023 17:24
Operator : MD/SY
Sample : 03118-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FLO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	12.061	1.1	ug/L	182138	3	11.811	794826	5.0