

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
 Data File : VU054470.D
 Acq On : 09 Jun 2023 18:13
 Operator : MD/SY
 Sample : 03118-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	108	rVB	86397	105363	10.11%	1.288%
2	1.914	185	194	204	rBV	95359	130028	12.47%	1.590%
3	2.563	384	396	411	rBV	160638	263757	25.30%	3.225%
4	3.046	536	546	562	rVB4	6390	12152	1.17%	0.149%
5	4.631	1025	1039	1072	rBV	159480	467399	44.83%	5.715%
6	5.058	1156	1172	1197	rVB	185213	420741	40.35%	5.144%
7	5.721	1351	1378	1401	rBV2	354411	945200	90.66%	11.557%
8	6.245	1525	1541	1567	rBV	353271	696919	66.84%	8.521%
9	6.685	1665	1678	1697	rBV	240463	473141	45.38%	5.785%
10	7.563	1935	1951	1978	rBV	106386	199391	19.12%	2.438%
11	7.894	2040	2054	2079	rBV	416992	739158	70.89%	9.037%
12	8.177	2130	2142	2157	rBV	64625	115390	11.07%	1.411%
13	8.467	2221	2232	2244	rBV4	8555	15394	1.48%	0.188%
14	8.631	2272	2283	2324	rBV3	496181	1042612	100.00%	12.748%
15	9.412	2513	2526	2545	rBV	488790	826874	79.31%	10.110%
16	10.753	2931	2943	2960	rBV	178819	297504	28.53%	3.637%
17	10.891	2976	2986	3002	rVB2	12185	20699	1.99%	0.253%
18	11.807	3258	3271	3295	rBV	461033	753372	72.26%	9.211%
19	12.068	3343	3352	3358	rBV6	6977	13129	1.26%	0.161%
20	12.190	3378	3390	3412	rBV	384824	640677	61.45%	7.833%




Sum of corrected areas: 8178900

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
Data File : VU054470.D
Acq On : 09 Jun 2023 18:13
Operator : MD/SY
Sample : 03118-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

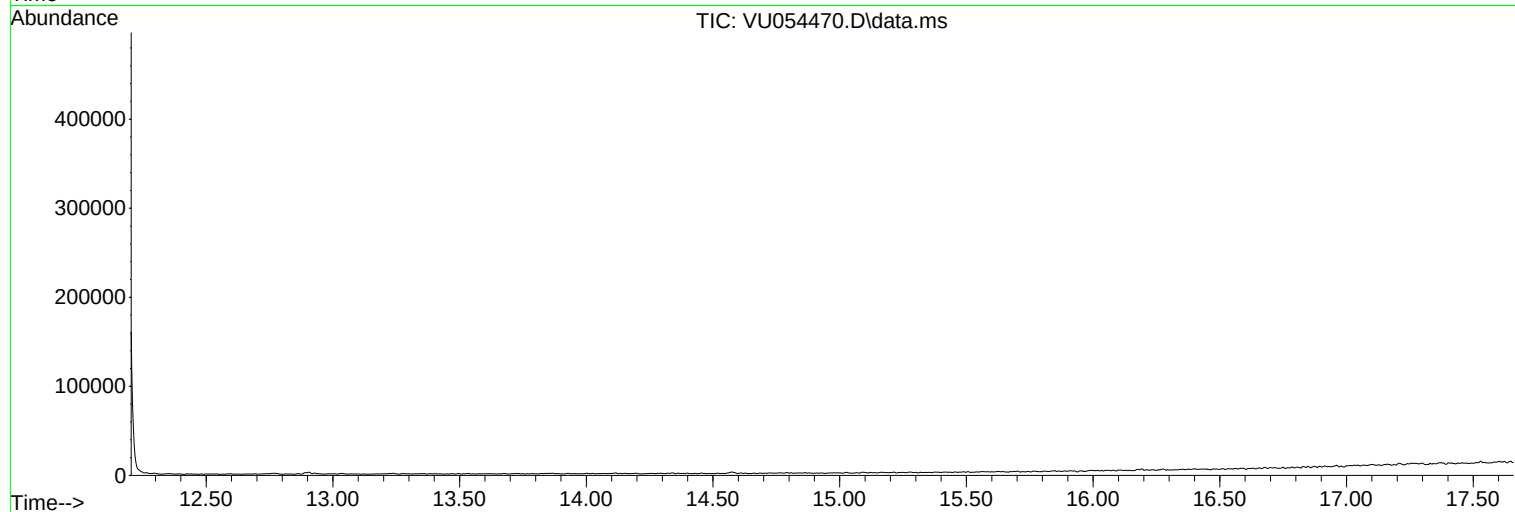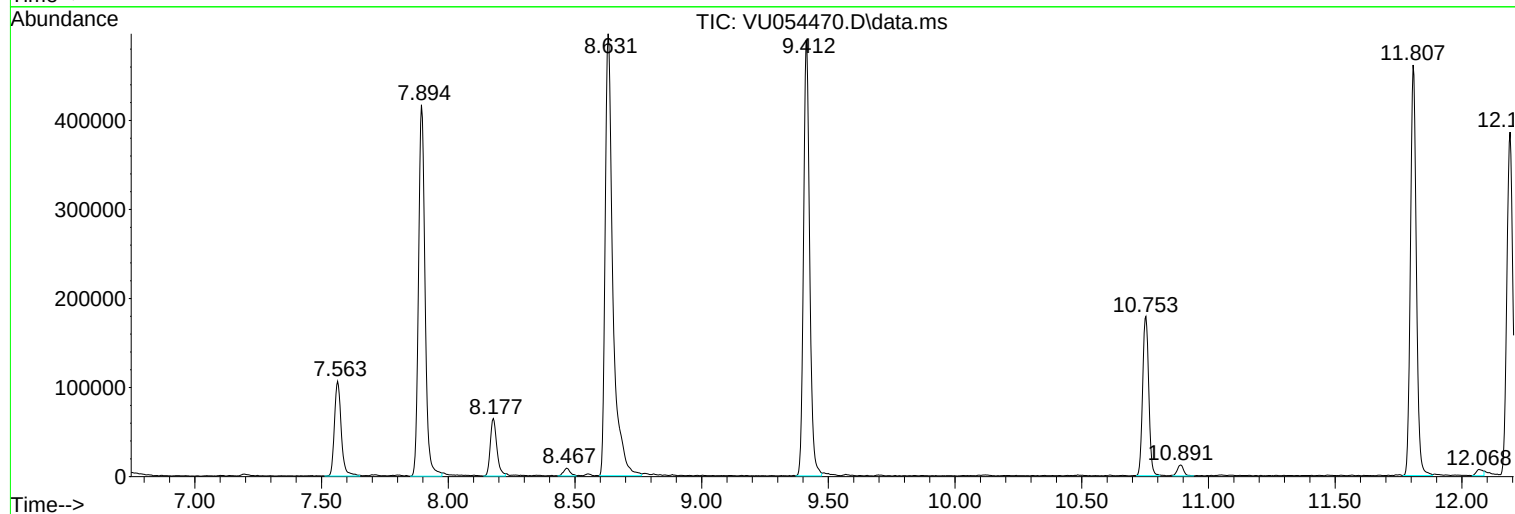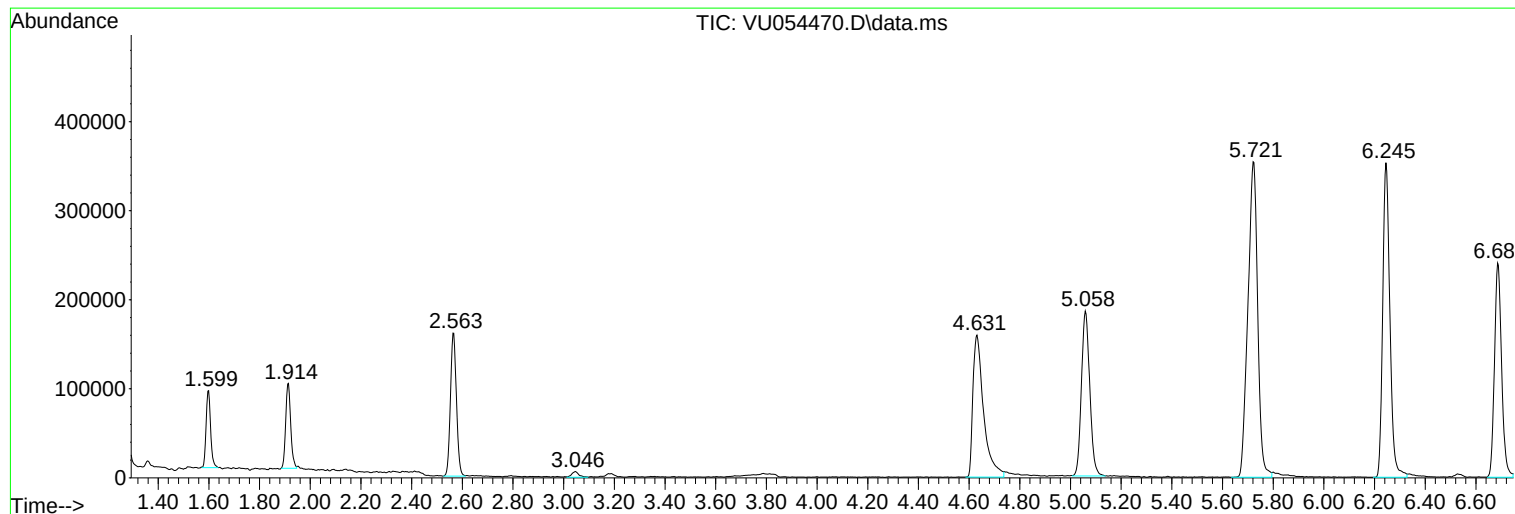

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
Data File : VU054470.D
Acq On : 09 Jun 2023 18:13
Operator : MD/SY
Sample : 03118-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
Data File : VU054470.D
Acq On : 09 Jun 2023 18:13
Operator : MD/SY
Sample : 03118-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc