


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060923\
Data File : VU054449.D
Acq On : 09 Jun 2023 09:08
Operator : MD/SY
Sample : BFB016
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB016

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Jun 12 00:58:03 2023

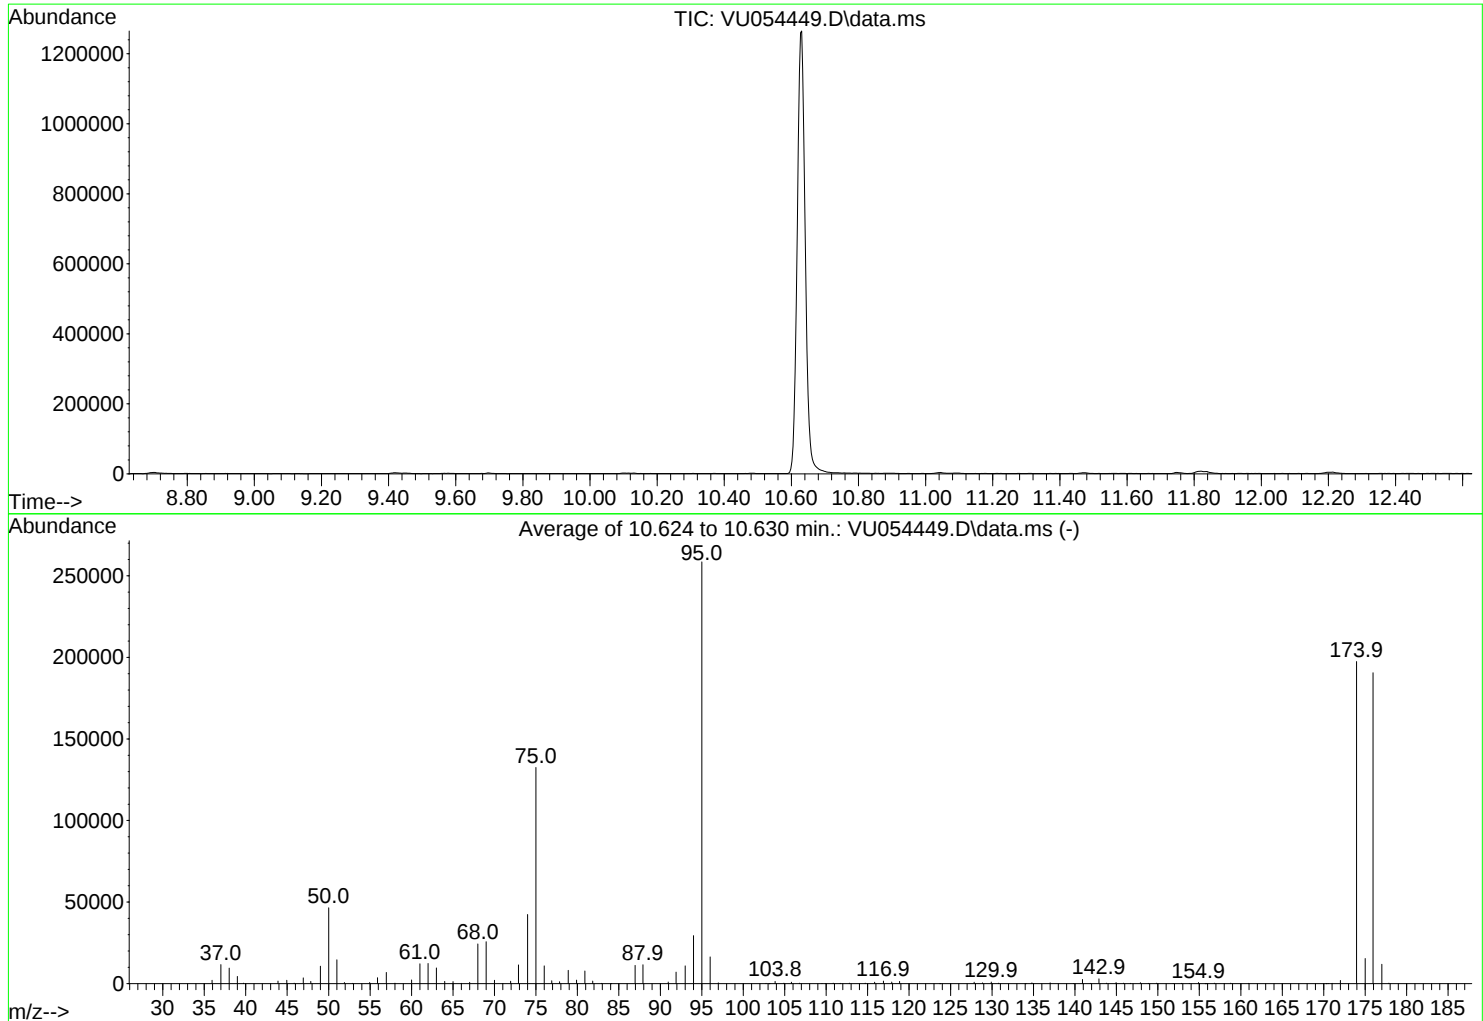

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	46520	PASS
75	95	30	80	51.3	132520	PASS
95	95	100	100	100.0	258560	PASS
96	95	5	9	6.3	16387	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.4	197419	PASS
175	174	5	9	7.8	15421	PASS
176	174	95	101	96.6	190613	PASS
177	176	5	9	6.2	11903	PASS

m/z	Abundance
39.70	225.0
43.90	574.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

m/z	Abundance
36.00	1938.0
37.00	11189.0
38.00	8995.0
39.00	4284.0
39.80	522.0
42.90	147.0
43.90	2076.0
45.00	2073.0
45.80	267.0
46.90	3489.0
47.80	1466.0
49.00	10381.0
50.00	44048.0
51.00	13863.0
51.90	770.0
52.90	124.0
55.00	632.0
55.90	3338.0
56.90	6422.0
58.00	315.0
60.00	2474.0
61.00	11458.0
62.00	11850.0
63.00	9034.0
64.00	1382.0
65.00	1165.0
66.00	216.0
67.00	777.0
68.00	22752.0
69.00	24568.0
70.00	2113.0
71.00	110.0
72.00	1314.0
72.90	10957.0
74.00	40248.0
75.00	124728.0
76.00	10921.0
76.90	1651.0
77.90	1064.0
78.90	7771.0
79.90	2073.0
80.90	7586.0
81.80	1443.0
82.80	126.0
87.00	10790.0
87.90	10913.0
90.90	863.0
91.90	6832.0
93.00	9946.0
94.00	28344.0
95.00	244608.0
96.00	15337.0
97.00	503.0
102.80	143.0
103.80	1258.0
104.90	292.0
105.80	872.0
106.80	328.0
109.50	145.0
110.80	278.0
111.60	173.0
112.80	199.0
114.70	259.0
115.90	767.0
116.90	1467.0
117.90	849.0
118.80	1321.0
127.80	876.0
128.90	419.0
129.90	1027.0
130.80	303.0
134.80	535.0
137.00	442.0
139.70	154.0
140.90	2298.0
141.90	224.0
142.90	2638.0
143.80	247.0
144.90	656.0
145.90	294.0
146.70	272.0
147.90	421.0
148.80	127.0
149.90	212.0
151.90	115.0
152.90	180.0
153.80	145.0
154.90	758.0
155.70	136.0
156.80	251.0
158.00	114.0
158.80	287.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

161.00	229.0
170.60	186.0
171.10	276.0
172.00	1835.0
173.90	180672.0
175.00	14291.0
175.90	174272.0
177.00	11064.0
177.90	310.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

m/z	Abundance
36.00	2129.0
37.00	12010.0
38.00	9852.0
39.00	4670.0
39.80	539.0
43.00	164.0
43.90	2248.0
45.00	2081.0
45.90	304.0
47.00	3680.0
47.80	1457.0
49.00	11085.0
50.00	47952.0
51.00	15094.0
51.90	723.0
52.90	183.0
54.90	780.0
55.90	3807.0
57.00	6964.0
58.00	277.0
60.00	2312.0
61.00	12506.0
62.00	12766.0
63.00	9838.0
64.00	1427.0
65.00	1266.0
66.00	150.0
67.00	817.0
68.00	24832.0
69.00	26416.0
70.00	2136.0
71.00	151.0
72.00	1448.0
72.90	11897.0
74.00	43936.0
75.00	136448.0
76.00	11096.0
76.90	1839.0
77.80	1210.0
78.90	8421.0
79.90	2193.0
80.90	7983.0
81.80	1599.0
82.90	182.0
87.00	11415.0
87.90	11953.0
90.90	972.0
91.90	7312.0
93.00	11184.0
94.00	30184.0
95.00	266688.0
96.00	16712.0
97.00	584.0
102.80	169.0
103.10	151.0
103.80	1436.0
104.90	292.0
105.80	936.0
106.80	324.0
109.50	127.0
109.90	183.0
110.80	262.0
111.70	174.0
112.80	267.0
114.70	275.0
115.80	983.0
116.90	1597.0
117.90	985.0
118.90	1446.0
127.80	852.0
128.90	485.0
129.90	1056.0
130.80	357.0
134.80	586.0
137.00	493.0
139.80	163.0
140.90	2697.0
141.80	251.0
142.90	3061.0
143.80	298.0
144.90	726.0
145.80	296.0
146.70	240.0
147.90	582.0
148.90	187.0
149.90	291.0
151.90	123.0
152.90	156.0
153.80	135.0
154.90	792.0
156.80	334.0
158.00	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

158.80	268.0
161.00	227.0
170.60	189.0
172.00	2015.0
173.90	202944.0
175.00	15824.0
176.00	196352.0
177.00	12080.0
177.80	279.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

m/z	Abundance
35.90	2219.0
37.00	11711.0
38.00	9780.0
39.00	4451.0
39.80	545.0
43.10	164.0
43.90	2260.0
44.90	2062.0
45.90	320.0
47.00	3442.0
47.90	1335.0
49.00	10607.0
50.00	47560.0
51.00	14775.0
51.90	607.0
52.90	248.0
54.90	816.0
55.90	3773.0
57.00	7250.0
58.00	245.0
60.00	2033.0
61.00	12565.0
62.00	12477.0
63.00	9988.0
64.00	1324.0
65.00	1385.0
66.00	137.0
67.00	825.0
68.00	25336.0
69.00	26064.0
70.00	1909.0
71.00	161.0
71.90	1570.0
72.90	11496.0
74.00	43104.0
75.00	136384.0
76.00	10702.0
76.90	1725.0
77.80	1284.0
78.90	8271.0
79.90	2100.0
80.90	7611.0
81.90	1614.0
83.00	212.0
84.00	107.0
86.90	11376.0
87.90	11807.0
91.00	1048.0
91.90	6974.0
93.00	11459.0
94.00	29744.0
95.00	264384.0
96.00	17112.0
97.00	499.0
102.70	235.0
103.90	1484.0
104.90	273.0
105.80	943.0
106.80	248.0
109.90	214.0
110.90	254.0
111.80	179.0
112.80	304.0
114.70	246.0
115.80	1065.0
116.90	1686.0
117.90	1106.0
118.90	1319.0
123.70	103.0
127.90	844.0
128.80	544.0
129.90	1005.0
130.80	379.0
134.00	102.0
134.80	483.0
137.00	514.0
139.90	137.0
140.90	2799.0
141.80	272.0
142.90	3180.0
143.80	251.0
145.00	729.0
145.80	327.0
146.70	146.0
147.90	661.0
148.90	205.0
149.80	366.0
151.80	132.0
152.80	156.0
154.90	682.0
155.90	104.0
156.80	384.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

158.00	119.0
158.80	245.0
160.90	229.0
170.30	139.0
170.90	205.0
172.00	2108.0
174.00	208640.0
175.00	16147.0
176.00	201216.0
177.00	12565.0
177.80	256.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016