
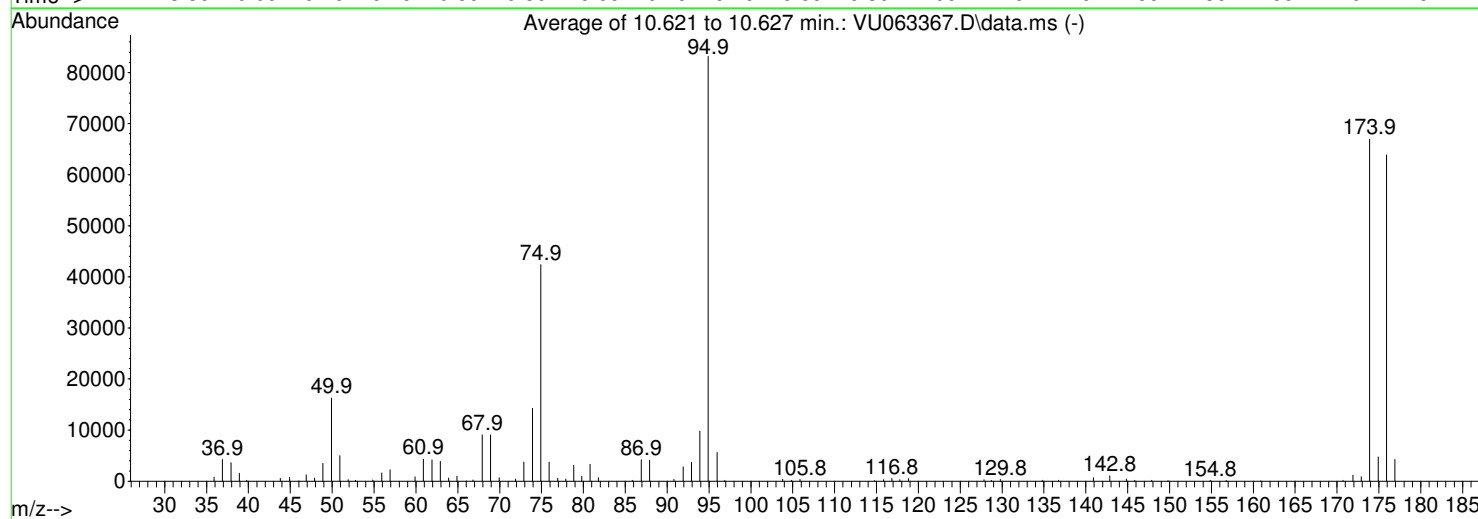


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060925\
Data File : VU063367.D
Acq On : 09 Jun 2025 09:39
Operator : MD/SY
Sample : BFB082
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB082

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jun 10 12:13:21 2025

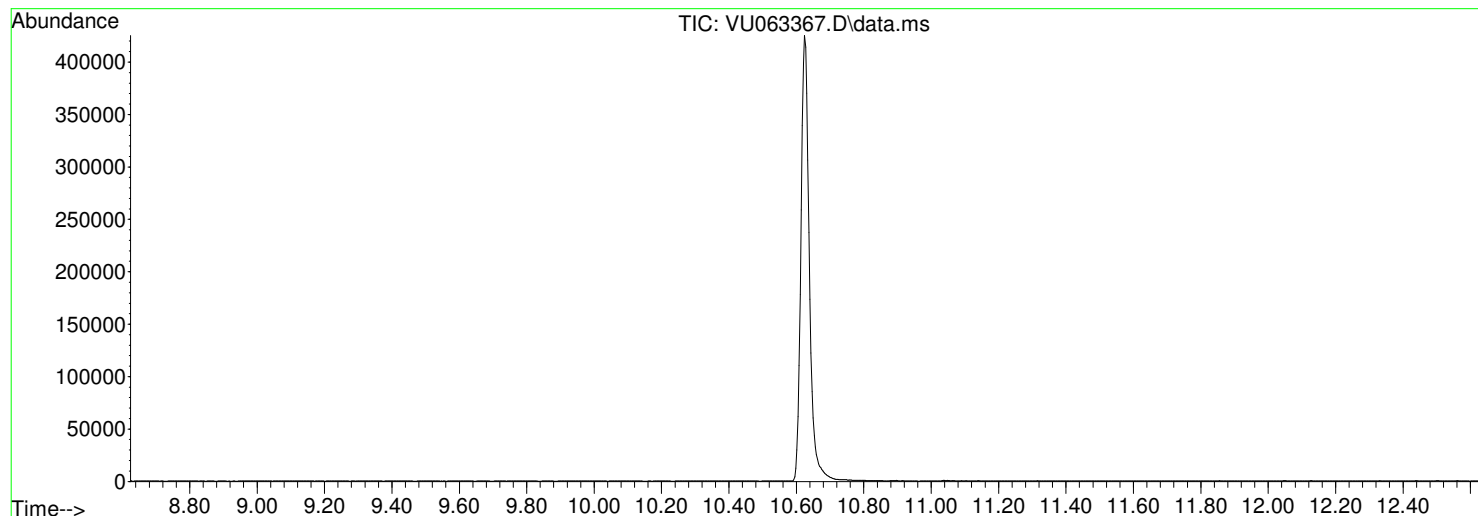

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.5	16258	PASS
75	95	30	80	50.9	42373	PASS
95	95	100	100	100.0	83181	PASS
96	95	5	9	6.7	5606	PASS
173	174	0.00	2	1.3	842	PASS
174	95	50	120	80.5	66973	PASS
175	174	5	9	7.1	4725	PASS
176	174	95	101	95.4	63907	PASS
177	176	5	9	6.6	4249	PASS

m/z	Abundance
39.70	137.0
43.80	287.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
35.90	743.0
36.90	4092.0
37.90	3412.0
38.90	1535.0
39.90	285.0
43.80	817.0
44.90	695.0
46.00	116.0
46.90	1323.0
47.90	556.0
48.90	3382.0
49.90	16225.0
50.90	5083.0
51.90	337.0
52.80	116.0
54.90	252.0
55.90	1635.0
56.90	2130.0
59.90	861.0
60.90	4226.0
61.90	4211.0
62.90	3728.0
63.90	647.0
64.90	927.0
66.80	270.0
67.90	8844.0
68.90	8643.0
70.00	653.0
71.90	430.0
72.90	3598.0
73.90	13774.0
74.90	41352.0
75.90	3710.0
77.00	538.0
77.90	471.0
78.80	3152.0
79.80	849.0
80.80	3165.0
81.80	648.0
85.80	150.0
86.90	4167.0
87.90	3861.0
90.80	358.0
91.90	2649.0
92.90	3514.0
93.90	9660.0
94.90	81016.0
96.00	5609.0
96.90	172.0
103.80	319.0
104.80	142.0
105.90	411.0
114.80	103.0
115.80	292.0
116.80	517.0
117.80	258.0
118.80	449.0
127.90	253.0
128.70	128.0
129.80	314.0
134.80	173.0
136.80	139.0
140.90	673.0
142.80	964.0
144.80	421.0
145.80	148.0
147.80	156.0
154.80	189.0
156.70	167.0
170.70	148.0
171.90	1081.0
172.90	804.0
173.90	63176.0
174.90	4591.0
175.90	60448.0
176.90	4123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
35.90	825.0
36.90	4372.0
37.90	3660.0
38.90	1601.0
39.90	317.0
43.90	791.0
44.90	747.0
46.90	1300.0
47.90	620.0
48.90	3575.0
49.90	16760.0
50.90	5115.0
51.90	321.0
52.80	131.0
54.80	240.0
55.90	1623.0
56.90	2291.0
59.90	856.0
60.90	4469.0
61.90	4263.0
62.90	3990.0
63.90	638.0
64.90	1037.0
66.00	106.0
66.80	256.0
67.90	9317.0
68.90	9404.0
69.90	683.0
71.90	427.0
72.90	3819.0
73.90	14594.0
74.90	43712.0
75.90	3884.0
77.00	572.0
77.90	452.0
78.90	3158.0
79.80	905.0
80.80	3391.0
81.80	700.0
85.80	188.0
86.90	4339.0
87.90	4200.0
90.80	377.0
91.90	2891.0
92.90	3714.0
93.90	10119.0
94.90	85728.0
96.00	5774.0
96.90	150.0
103.80	350.0
104.80	128.0
105.90	369.0
114.70	110.0
115.80	294.0
116.90	528.0
117.80	276.0
118.80	439.0
127.80	283.0
128.70	154.0
129.80	375.0
134.80	188.0
136.70	159.0
140.90	686.0
142.80	1078.0
144.90	437.0
145.90	140.0
147.90	188.0
149.80	113.0
154.80	179.0
156.80	160.0
170.70	167.0
171.90	1230.0
172.90	874.0
173.90	69032.0
174.90	4860.0
175.90	65832.0
176.90	4387.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
35.90	808.0
36.90	4161.0
37.90	3694.0
38.90	1528.0
39.80	299.0
43.90	780.0
44.90	731.0
46.90	1044.0
47.90	578.0
48.90	3509.0
49.90	15788.0
50.90	4835.0
51.90	257.0
52.80	144.0
54.90	209.0
55.90	1478.0
56.90	2344.0
59.90	801.0
60.90	4169.0
61.90	3996.0
62.90	3910.0
63.90	605.0
64.90	1000.0
66.80	198.0
67.90	9033.0
68.90	9211.0
69.90	673.0
71.90	412.0
72.90	3707.0
73.90	14382.0
74.90	42056.0
75.90	3657.0
76.90	583.0
77.90	373.0
78.90	3055.0
79.80	923.0
80.80	3377.0
81.80	693.0
85.90	171.0
86.90	4088.0
87.90	4169.0
90.80	333.0
91.90	2769.0
92.90	3679.0
93.90	9675.0
94.90	82800.0
95.90	5435.0
96.90	139.0
103.80	334.0
104.90	129.0
105.80	305.0
114.70	112.0
115.90	281.0
116.80	516.0
117.80	301.0
118.80	443.0
127.80	279.0
128.70	165.0
129.80	351.0
134.80	157.0
136.70	142.0
140.90	654.0
142.90	1143.0
144.90	376.0
145.80	110.0
147.90	206.0
149.80	118.0
154.90	189.0
156.80	144.0
160.90	126.0
170.70	166.0
171.90	1197.0
172.90	848.0
173.90	68712.0
174.90	4724.0
175.90	65440.0
176.90	4237.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082