

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061019\
Quantitation Report (QT Reviewed)


Data File : VU032585.D
Acq On : 10 Jun 2019 23:05
Operator : JC/SP
Sample : K3277-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8C6

Manual Integrations
APPROVED

MMDadoda
6/11/2019 11:55:07 AM

Quant Time: Jun 11 07:09:12 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 11 05:38:55 2019
Response via : Initial Calibration

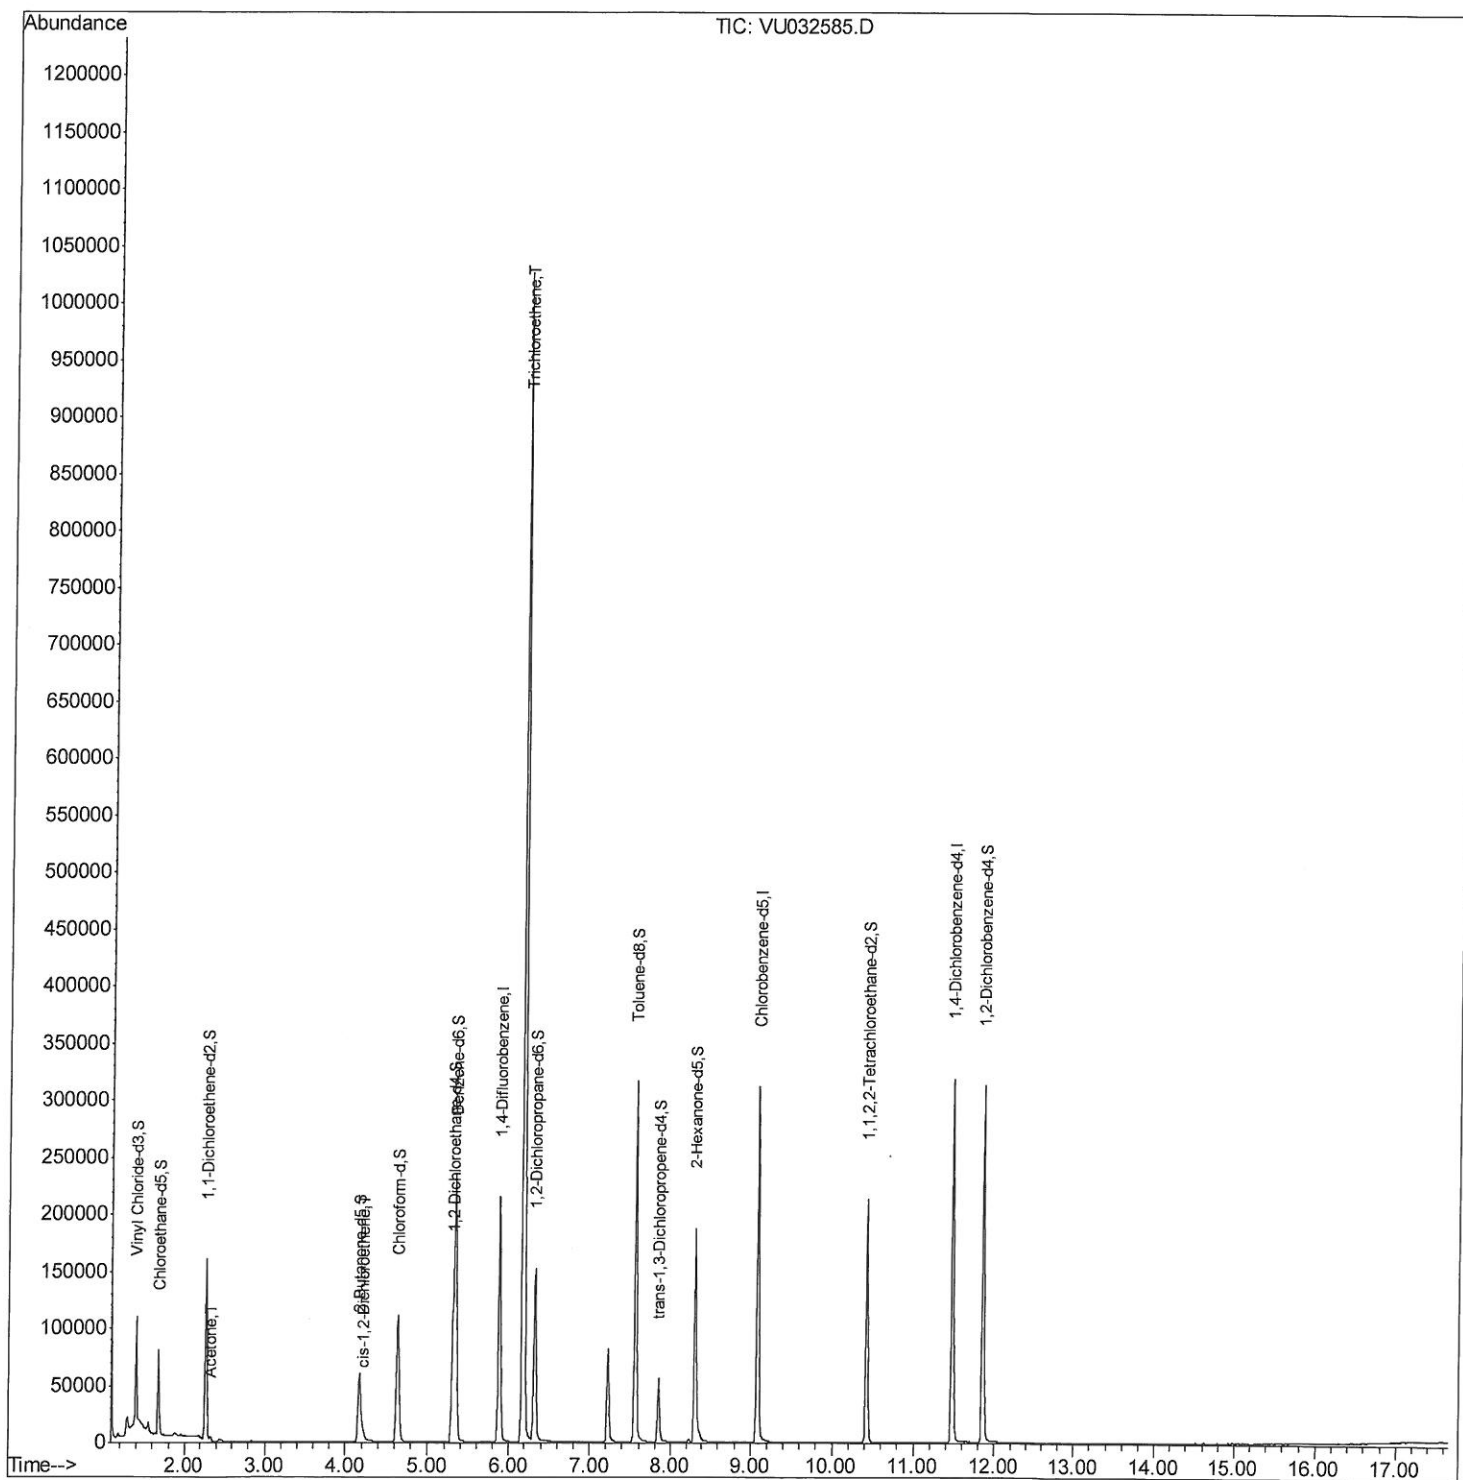

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061019\
Quantitation Report (Qedit)




Data File : VU032585.D
Acq On : 10 Jun 2019 23:05
Operator : JC/SP
Sample : K3277-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8C6

Manual Integrations
APPROVED

MMDadoda
6/11/2019 11:55:07 AM

Quant Time: Jun 11 05:44:15 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 11 05:38:55 2019
Response via : Initial Calibration

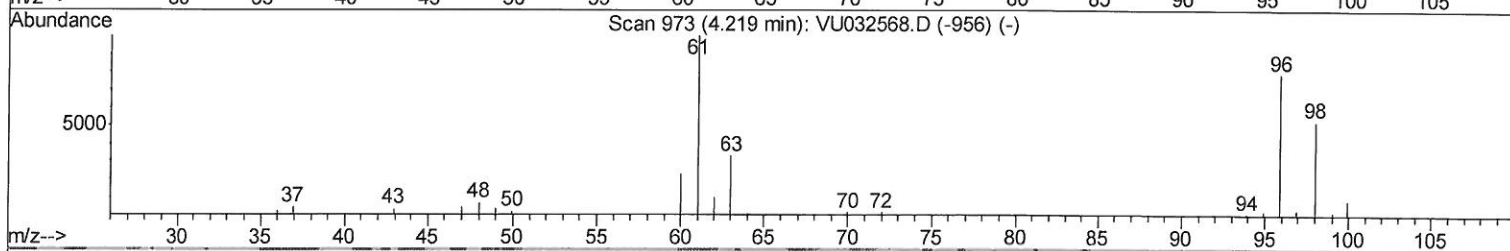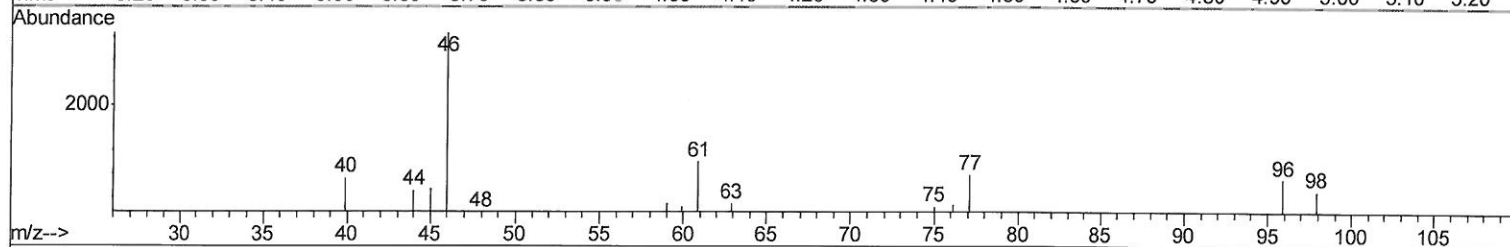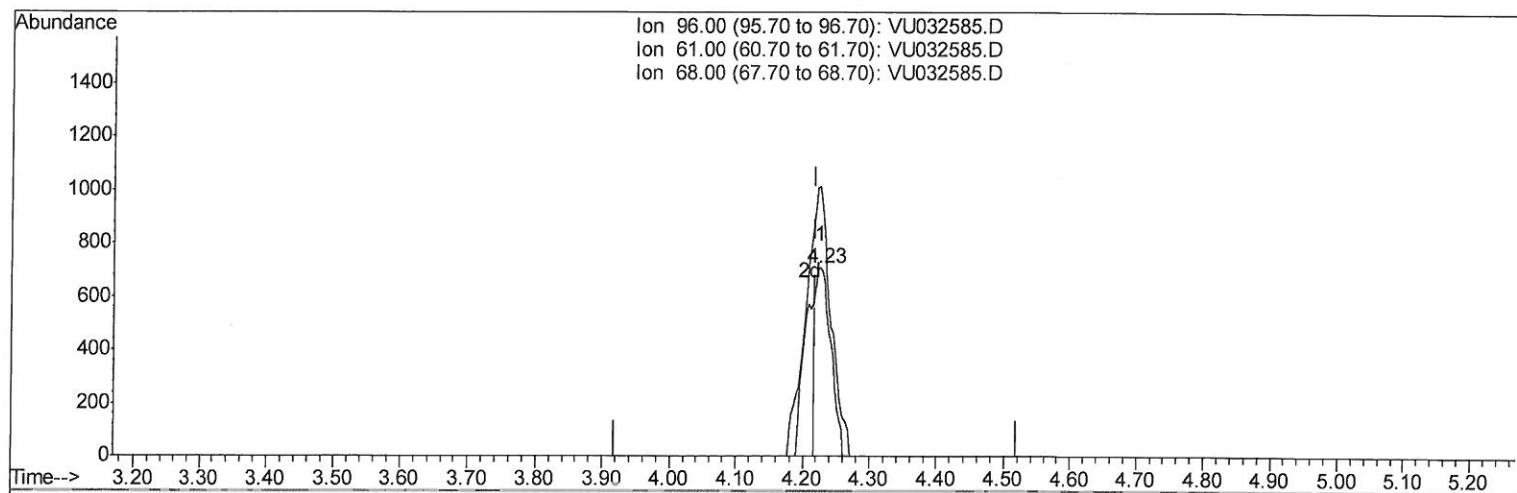

TIC: VU032585.D

(20) cis-1,2-Dichloroethene (T)

4.225min (+0.006) 0.84ug/L

response 1135

Ion	Exp%	Act%
96.00	100	100
61.00	124.60	142.94
68.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061019\
Quantitation Report (Qedit)




Data File : VU032585.D
Acq On : 10 Jun 2019 23:05
Operator : JC/SP
Sample : K3277-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8C6

Manual Integrations
APPROVED

MMDadoda
6/11/2019 11:55:07 AM

Quant Time: Jun 11 05:44:15 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 11 05:38:55 2019
Response via : Initial Calibration

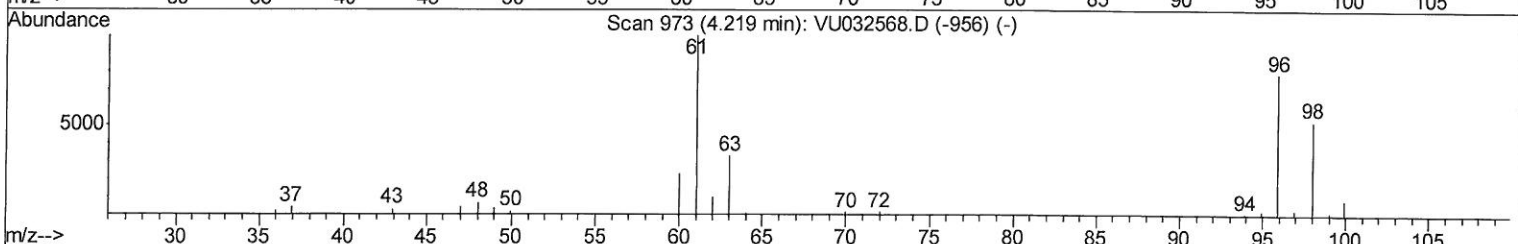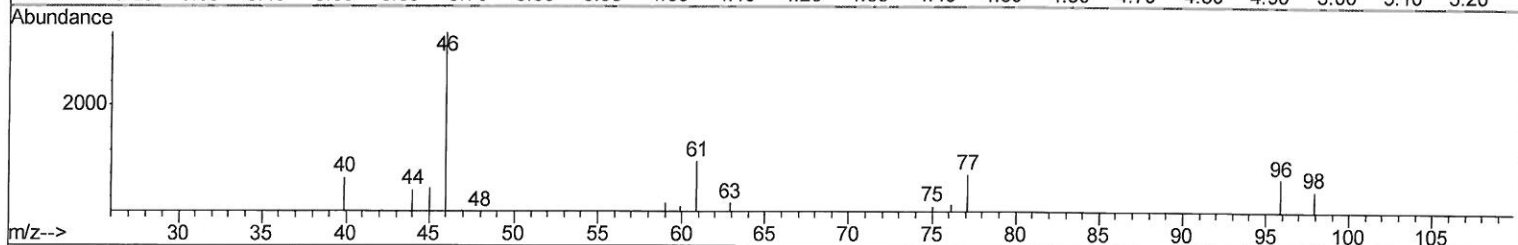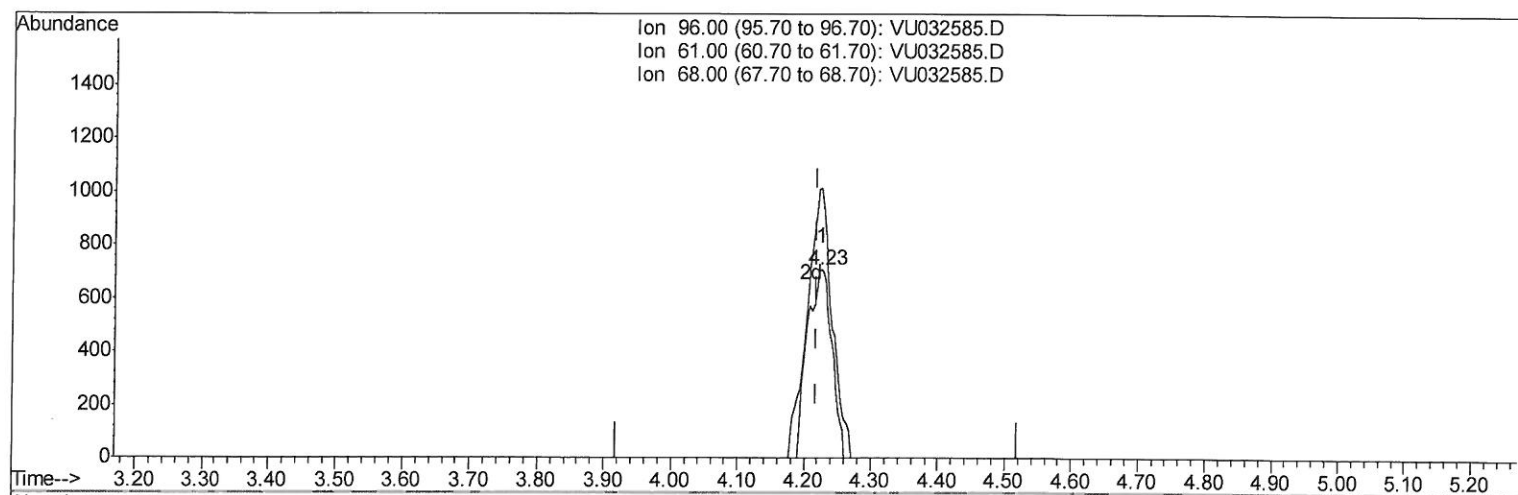

TIC: VU032585.D

(20) cis-1,2-Dichloroethene (T)

4.225min (+0.006) 1.34ug/L m

response 1813

Ion	Exp%	Act%
96.00	100	100
61.00	124.60	142.94
68.00	0.00	0.00
0.00	0.00	0.00

→ MRC
6/12/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061019\
Quantitation Report (QT Reviewed)

Data File : VU032585.D
Acq On : 10 Jun 2019 23:05
Operator : JC/SP
Sample : K3277-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8C6

Manual Integrations
APPROVED

MMDadoda
6/11/2019 11:55:07 AM

Quant Time: Jun 11 07:09:12 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 11 05:38:55 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	185555	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	171801	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	87635	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	57311	47.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	95.22%
7) Chloroethane-d5	1.68	69	47784	49.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.78%
11) 1,1-Dichloroethene-d2	2.27	63	87281	37.03	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.06%
21) 2-Butanone-d5	4.17	46	98775	98.04	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.04%
24) Chloroform-d	4.64	84	109921	48.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.92%
26) 1,2-Dichloroethane-d4	5.30	65	73373	51.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.76%
32) Benzene-d6	5.33	84	228118	51.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.30%
36) 1,2-Dichloropropane-d6	6.32	67	71786	51.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.66%
41) Toluene-d8	7.56	98	211517	50.02	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.04%
43) trans-1,3-Dichloropropene-	7.85	79	30866	46.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.24%
47) 2-Hexanone-d5	8.31	63	63809	94.06	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.06%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	101576	50.13	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.26%
64) 1,2-Dichlorobenzene-d4	11.85	152	86196	51.35	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.70%

Target Compounds					Qvalue	
13) Acetone	2.32	43	2999	2.885	ug/L	89
20) cis-1,2-Dichloroethene	4.23	96	1813m	1.343	ug/L	
34) Trichloroethene	6.18	95	339024	258.154	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed