

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061019\
Quantitation Report (QT Reviewed)


Data File : VU032589.D
Acq On : 11 Jun 2019 00:37
Operator : JC/SP
Sample : K3278-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8D0

Manual Integrations
APPROVED

MMDadoda
6/11/2019 11:55:11 AM

Quant Time: Jun 11 07:22:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 11 05:38:55 2019
Response via : Initial Calibration

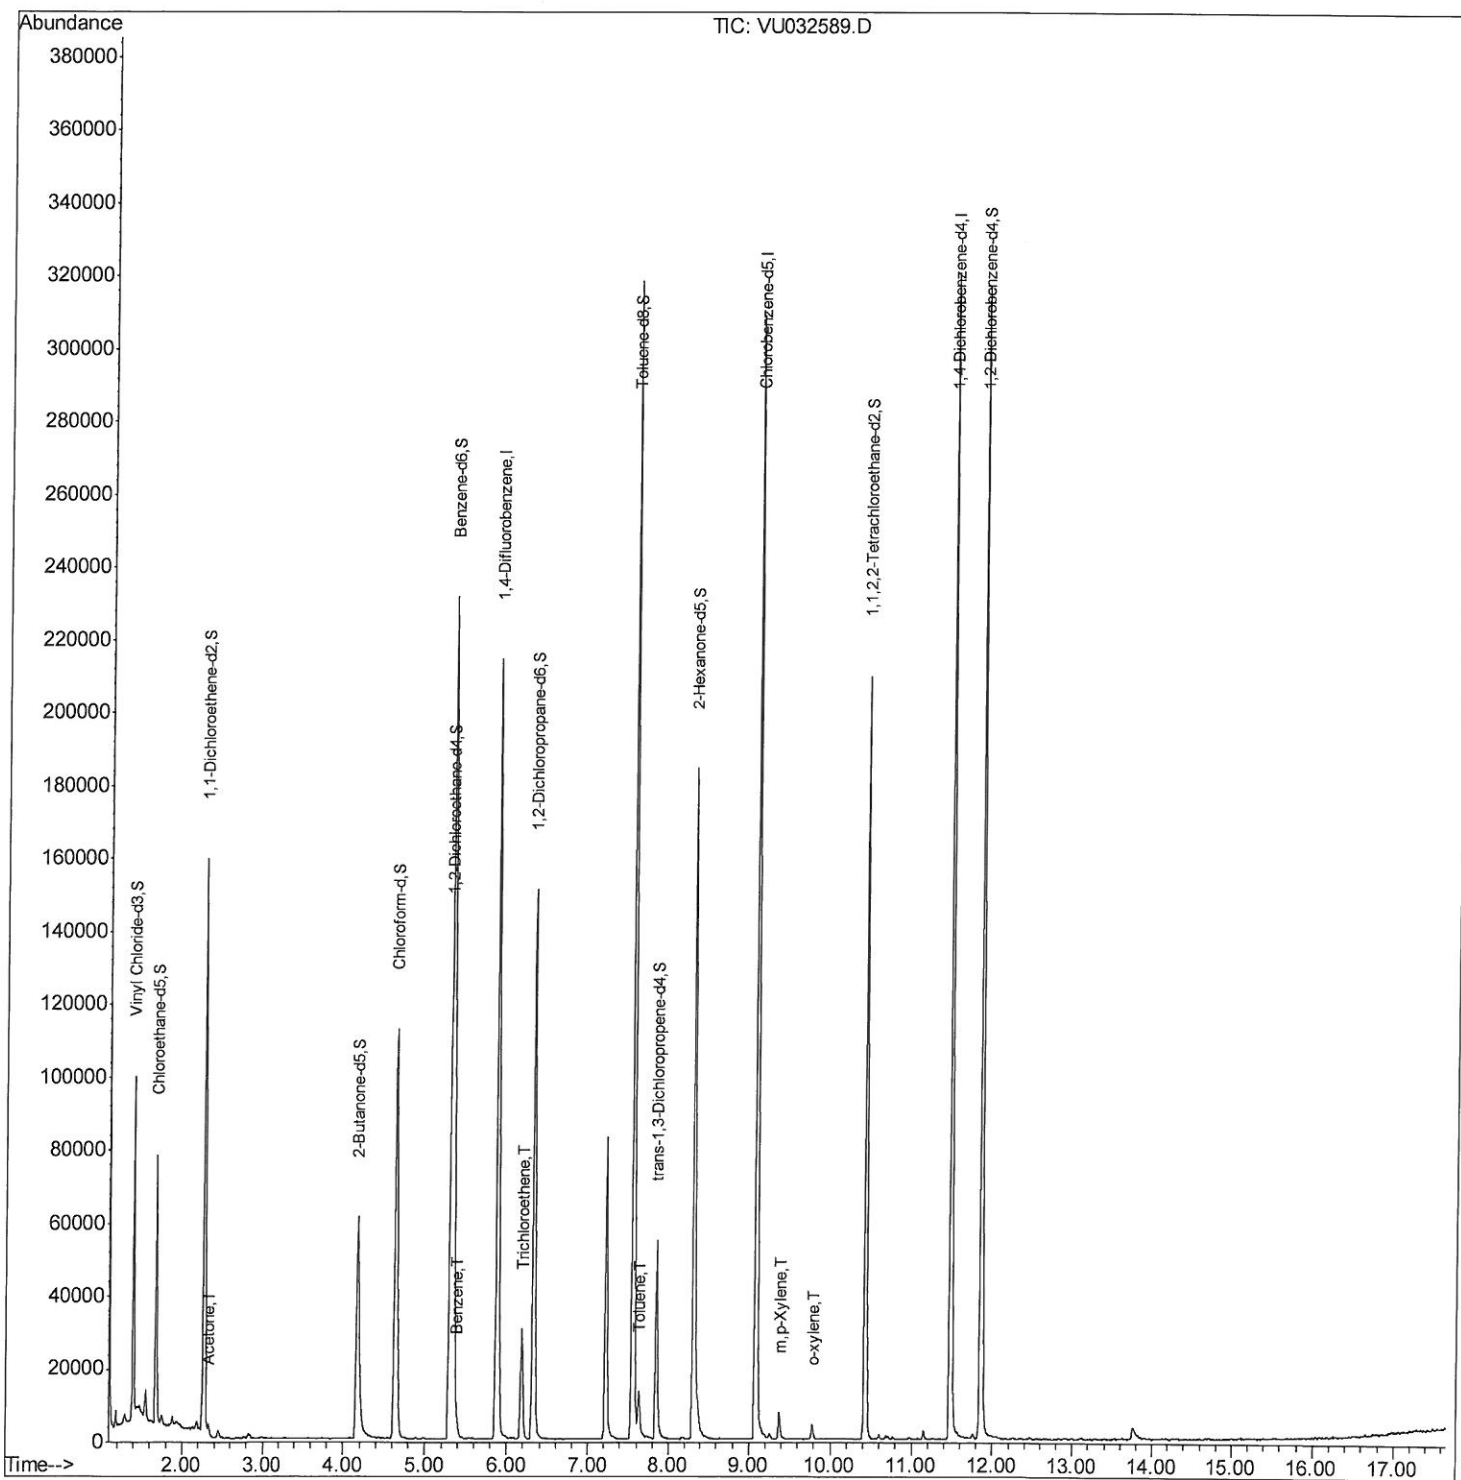

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061019\
Quantitation Report (Qedit)




Data File : VU032589.D
Acq On : 11 Jun 2019 00:37
Operator : JC/SP
Sample : K3278-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8D0

Manual Integrations
APPROVED

MMDadoda
6/11/2019 11:55:11 AM

Quant Time: Jun 11 05:44:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 11 05:38:55 2019
Response via : Initial Calibration

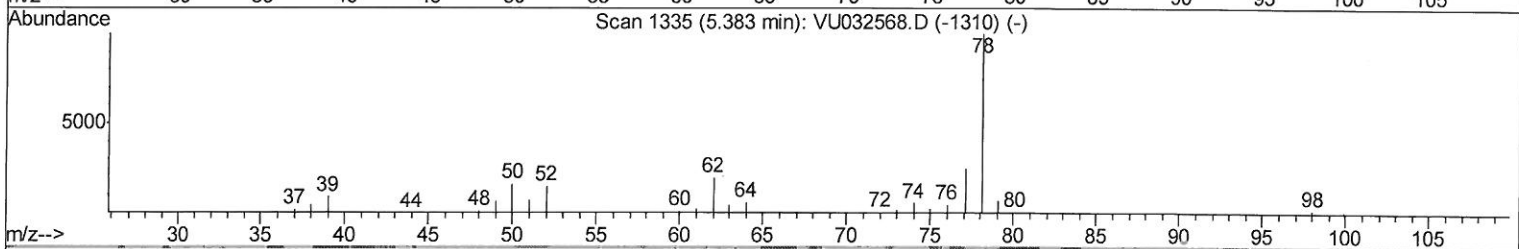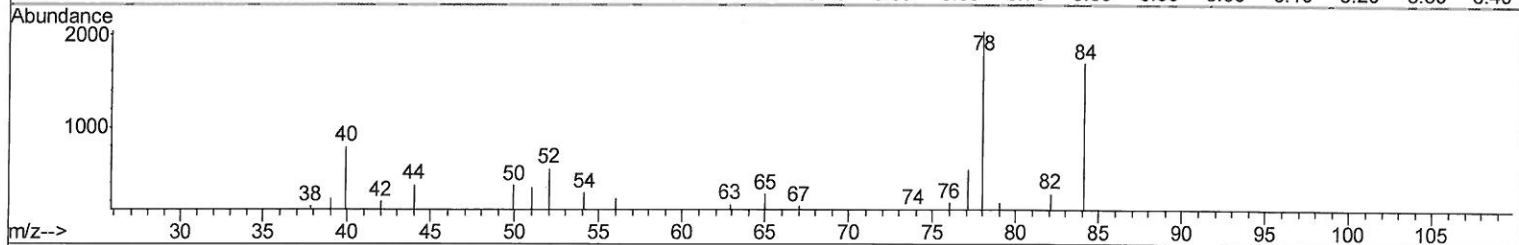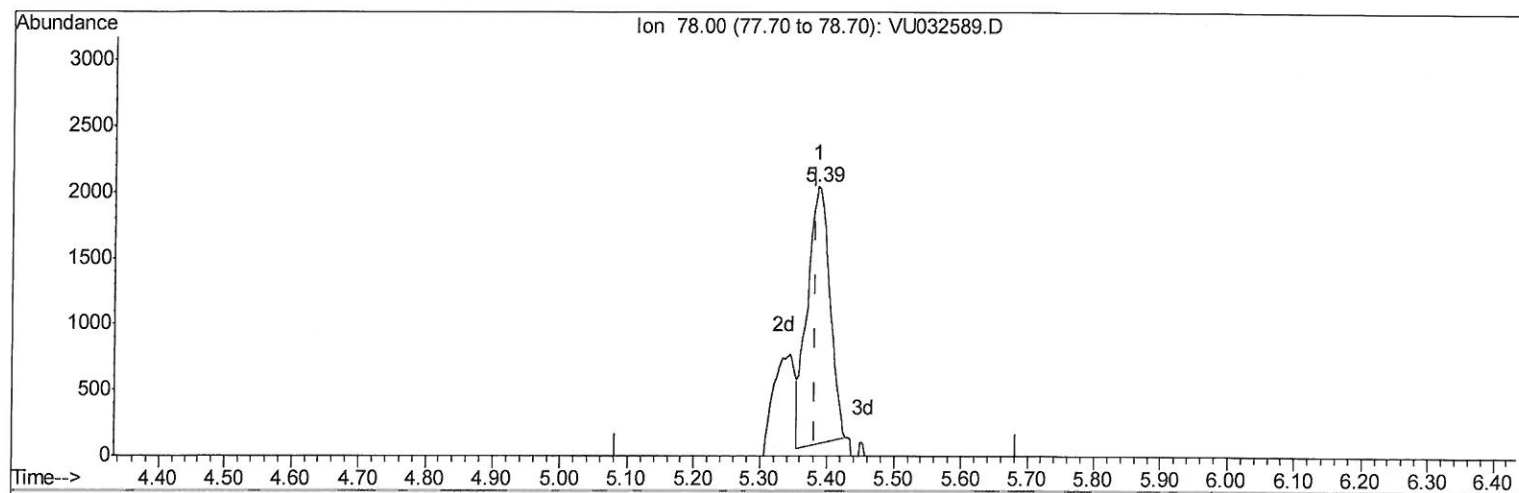

TIC: VU032589.D

(33) Benzene (T)

5.386min (+0.003) 0.95ug/L

response 4598

Ion	Exp%	Act%
78.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061019\
Quantitation Report (Qedit)




Data File : VU032589.D
Acq On : 11 Jun 2019 00:37
Operator : JC/SP
Sample : K3278-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8D0

Manual Integrations
APPROVED

MMDadoda
6/11/2019 11:55:11 AM

Quant Time: Jun 11 05:44:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 11 05:38:55 2019
Response via : Initial Calibration

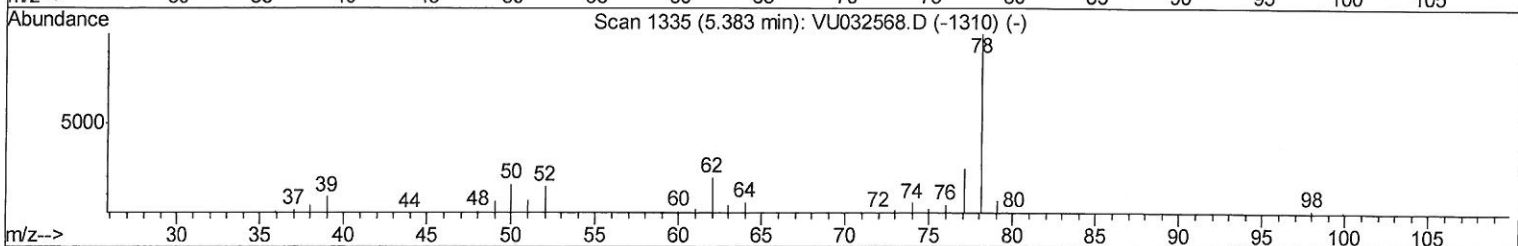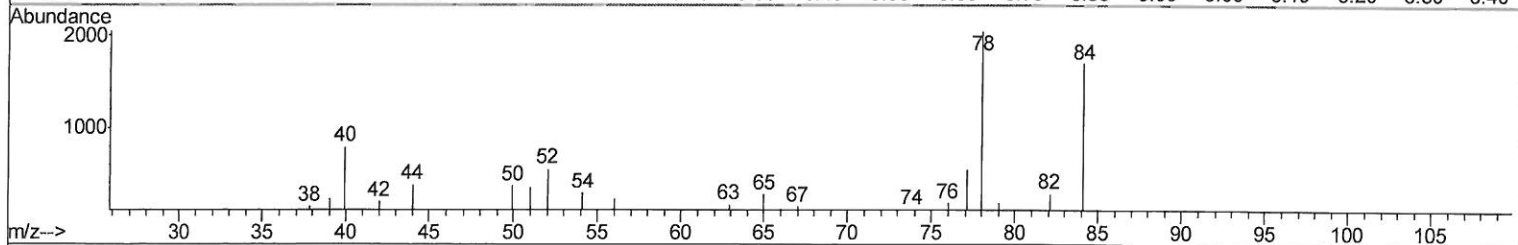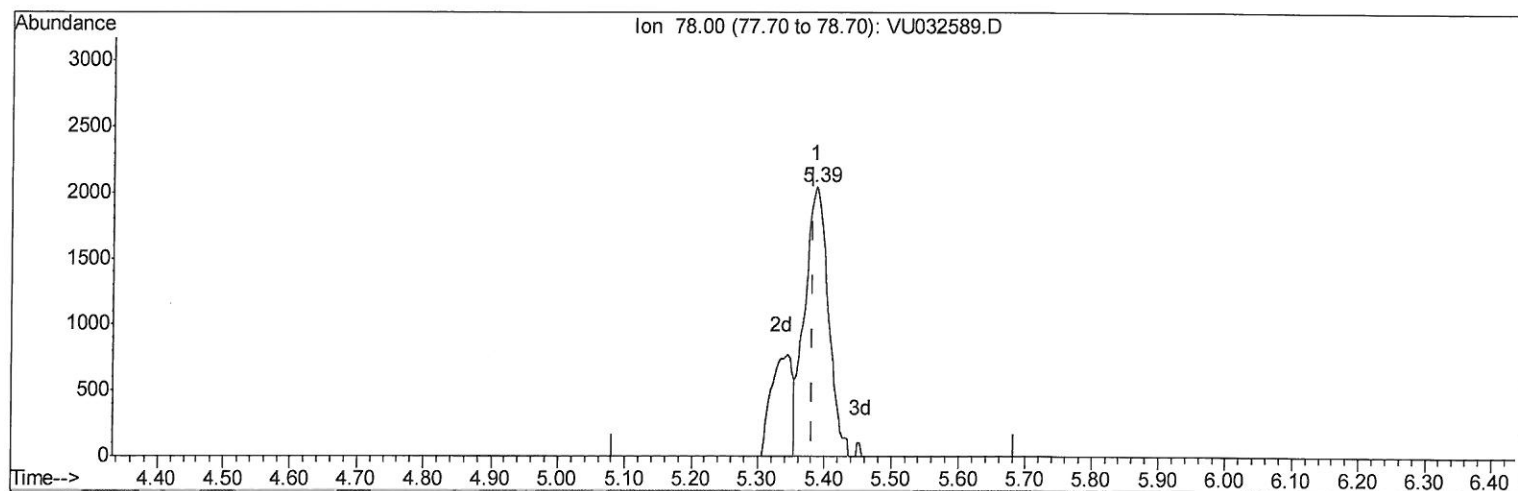

TIC: VU032589.D

(33) Benzene (T)

5.386min (+0.003) 1.05ug/L m

response 5076

Ion	Exp%	Act%
78.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

MMD
6/12/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061019\
 Quantitation Report (QT Reviewed)

Data File : VU032589.D
 Acq On : 11 Jun 2019 00:37
 Operator : JC/SP
 Sample : K3278-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleID :
 DB8D0

Manual Integrations
 APPROVED

MMDadoda
 6/11/2019 11:55:11 AM

Quant Time: Jun 11 07:22:50 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 11 05:38:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	183441	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	171438	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	85818	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	56710	47.65	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	95.30%
7) Chloroethane-d5	1.68	69	46936	49.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.16%
11) 1,1-Dichloroethene-d2	2.27	63	86728	37.22	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.44%
21) 2-Butanone-d5	4.17	46	98383	98.78	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.78%
24) Chloroform-d	4.64	84	109998	49.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.12%
26) 1,2-Dichloroethane-d4	5.30	65	72470	51.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.66%
32) Benzene-d6	5.33	84	229074	51.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.94%
36) 1,2-Dichloropropane-d6	6.32	67	71207	51.02	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.04%
41) Toluene-d8	7.56	98	210309	49.84	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.68%
43) trans-1,3-Dichloropropene-	7.85	79	32585	48.79	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.58%
47) 2-Hexanone-d5	8.31	63	61681	91.12	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.12%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	100349	49.62	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.24%
64) 1,2-Dichlorobenzene-d4	11.85	152	87463	53.21	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.42%

Target Compounds

					Qvalue
13) Acetone	2.32	43	2818	2.742 ug/L	95
33) Benzene	5.39	78	5076m	1.054 ug/L	95
34) Trichloroethene	6.18	95	10260	7.829 ug/L	95
42) Toluene	7.64	91	9990	1.894 ug/L	100
53) m,p-Xylene	9.37	106	2344	1.048 ug/L	88
54) o-xylene	9.78	106	1250	0.563 ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed