


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061019\
Data File : VU032552.D
Acq On : 10 Jun 2019 08:30
Operator : JC/SP
Sample : BFB52
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB52

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Title : VOC Analysis
Last Update : Tue Jun 11 05:38:55 2019

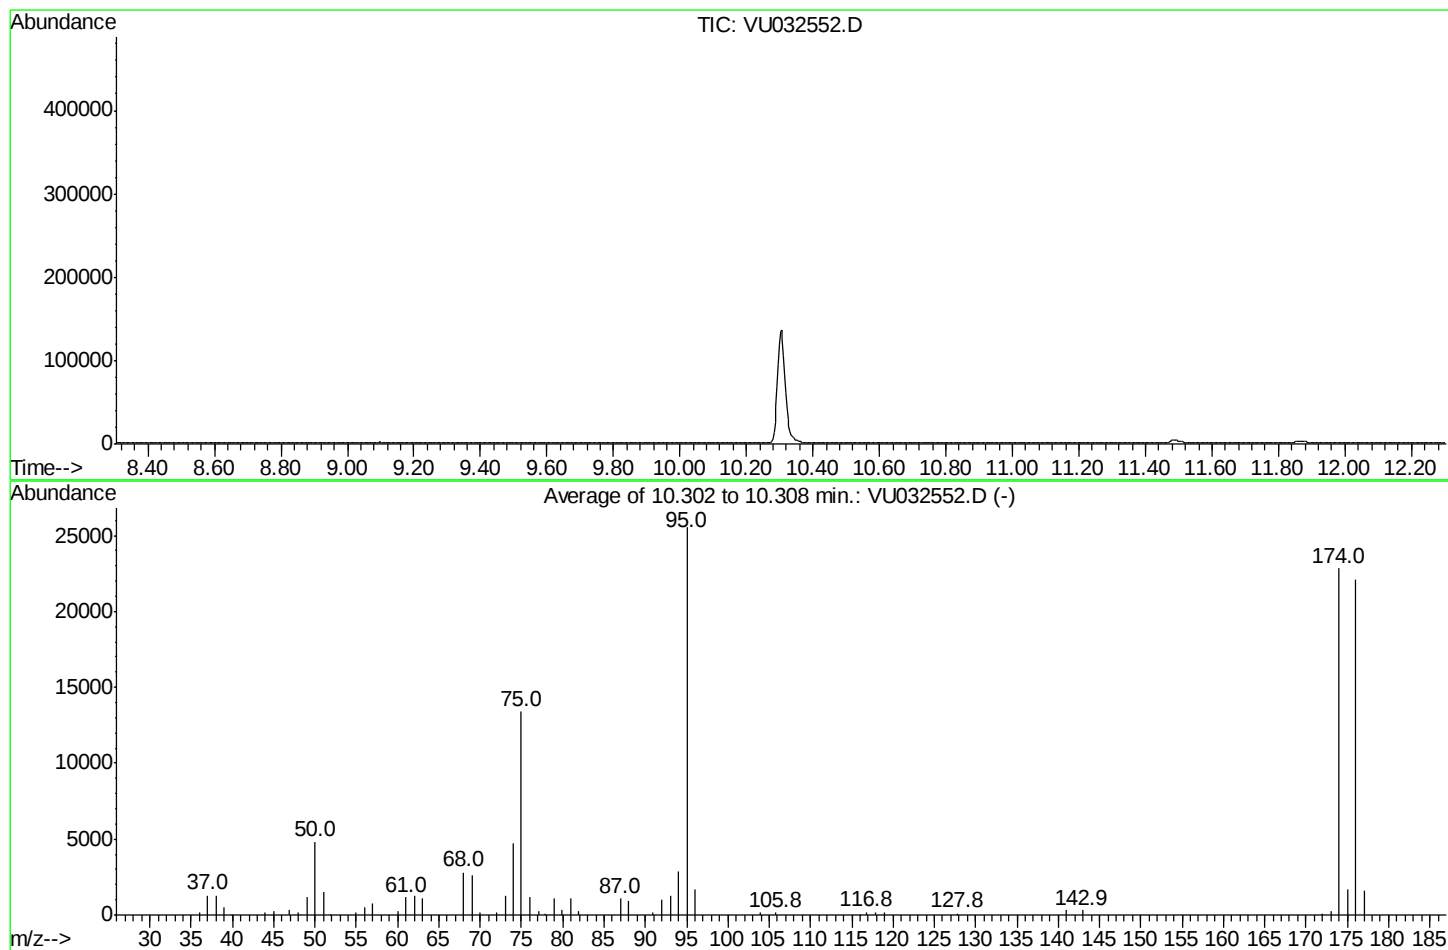

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	4825	PASS
75	95	30	80	52.5	13399	PASS
95	95	100	100	100.0	25538	PASS
96	95	5	9	6.7	1707	PASS
173	174	0.00	2	1.2	285	PASS
174	95	50	120	89.5	22850	PASS
175	174	5	9	7.4	1695	PASS
176	174	95	101	96.5	22061	PASS
177	176	5	9	7.4	1623	PASS

Scan 2854 (10.267 min): VU032552.D
BFB52

m/z	Abundance
39.90	738.0
44.00	278.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
35.90	209.0
37.00	1379.0
38.00	1295.0
39.00	561.0
40.00	744.0
44.00	505.0
45.00	298.0
46.90	305.0
47.90	184.0
49.00	1247.0
50.00	5005.0
51.00	1612.0
55.00	172.0
56.10	560.0
57.00	772.0
60.00	305.0
61.00	1229.0
62.00	1337.0
63.00	1080.0
68.00	2750.0
69.00	2716.0
69.90	222.0
71.90	189.0
73.00	1342.0
74.00	4780.0
75.00	13870.0
76.00	1220.0
77.10	219.0
77.90	100.0
78.90	1102.0
79.90	403.0
80.90	1219.0
81.90	238.0
87.00	1087.0
87.90	947.0
90.90	137.0
92.00	1042.0
93.00	1283.0
94.00	2984.0
95.00	26184.0
96.00	1737.0
103.90	131.0
105.80	179.0
116.80	204.0
117.80	134.0
119.00	145.0
127.80	105.0
141.00	326.0
143.00	266.0
171.90	113.0
173.00	299.0
174.00	22776.0
175.00	1654.0
176.00	22024.0
177.00	1610.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
35.00	199.0
37.00	1337.0
38.00	1261.0
39.00	565.0
40.00	748.0
44.00	495.0
45.00	273.0
46.00	368.0
47.00	177.0
49.00	1215.0
50.00	4976.0
51.00	1601.0
51.90	113.0
55.00	208.0
56.10	584.0
57.00	820.0
60.00	293.0
61.00	1235.0
62.00	1326.0
63.00	1106.0
68.00	2900.0
69.00	2680.0
70.00	203.0
71.00	187.0
73.00	1347.0
74.00	4830.0
75.00	13827.0
76.00	1178.0
77.10	223.0
77.80	100.0
78.90	1171.0
79.90	374.0
80.90	1142.0
81.90	269.0
86.90	1085.0
87.90	945.0
90.90	150.0
92.00	1043.0
93.00	1258.0
94.00	2915.0
95.00	26352.0
96.00	1782.0
103.80	141.0
105.80	139.0
116.80	191.0
117.80	170.0
119.00	134.0
127.80	130.0
140.90	310.0
142.90	315.0
171.90	129.0
173.00	294.0
174.00	23584.0
175.00	1729.0
176.00	22800.0
177.00	1699.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	196.0
37.00	1149.0
38.00	1132.0
39.00	505.0
40.00	742.0
44.00	471.0
45.00	246.0
46.90	393.0
47.90	149.0
49.00	1076.0
50.00	4496.0
51.10	1346.0
55.00	198.0
56.00	475.0
57.00	791.0
60.00	271.0
61.00	1077.0
62.00	1121.0
63.00	1022.0
68.00	2749.0
69.00	2435.0
70.00	179.0
72.00	169.0
73.00	1238.0
74.00	4513.0
75.00	12501.0
76.00	1072.0
77.00	240.0
77.80	107.0
78.90	1107.0
79.90	281.0
80.90	1030.0
82.00	278.0
86.90	999.0
88.00	837.0
90.90	132.0
92.00	862.0
93.00	1141.0
94.00	2695.0
95.00	24080.0
96.00	1602.0
103.80	135.0
105.90	104.0
116.00	112.0
116.90	164.0
117.80	175.0
118.80	134.0
127.80	132.0
140.90	259.0
142.90	317.0
172.00	111.0
173.00	262.0
174.00	22192.0
175.00	1702.0
176.00	21360.0
177.00	1562.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52