

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061020\
 Data File : VU038772.D
 Acq On : 10 Jun 2020 12:13
 Operator : SY/MD
 Sample : L2896-23
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Jun 11 00:53:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 11 00:28:57 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	569420	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.43	117	554439	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	256309	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	126152	39.65	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.30%
7) Chloroethane-d5	1.93	69	111456	45.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.32%
11) 1,1-Dichloroethene-d2	2.59	63	221398	31.93	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.86%
21) 2-Butanone-d5	4.66	46	296873	95.92	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.92%
24) Chloroform-d	5.10	84	305829	44.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.18%
26) 1,2-Dichloroethane-d4	5.74	65	210329	46.26	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.52%
32) Benzene-d6	5.76	84	611523	45.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.58%
36) 1,2-Dichloropropane-d6	6.72	67	189983	46.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.32%
41) Toluene-d8	7.92	98	530085	43.92	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.84%
43) trans-1,3-Dichloropropene-	8.20	79	88762	42.83	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.66%
47) 2-Hexanone-d5	8.65	63	217761	99.39	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.39%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	273372	44.53	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.06%
64) 1,2-Dichlorobenzene-d4	12.20	152	219351	49.29	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.58%


Target Compounds					Ovalue
37) 1,2-Dichloropropane	6.72	63	21686	5.055 ug/L #	87
59) 1,2,3-Trichloropropane	11.82	75	32358	5.379 ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061020\
Data File : VU038772.D
Acq On : 10 Jun 2020 12:13
Operator : SY/MD
Sample : L2896-23
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Jun 11 00:53:36 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 11 00:28:57 2020
Response via : Initial Calibration




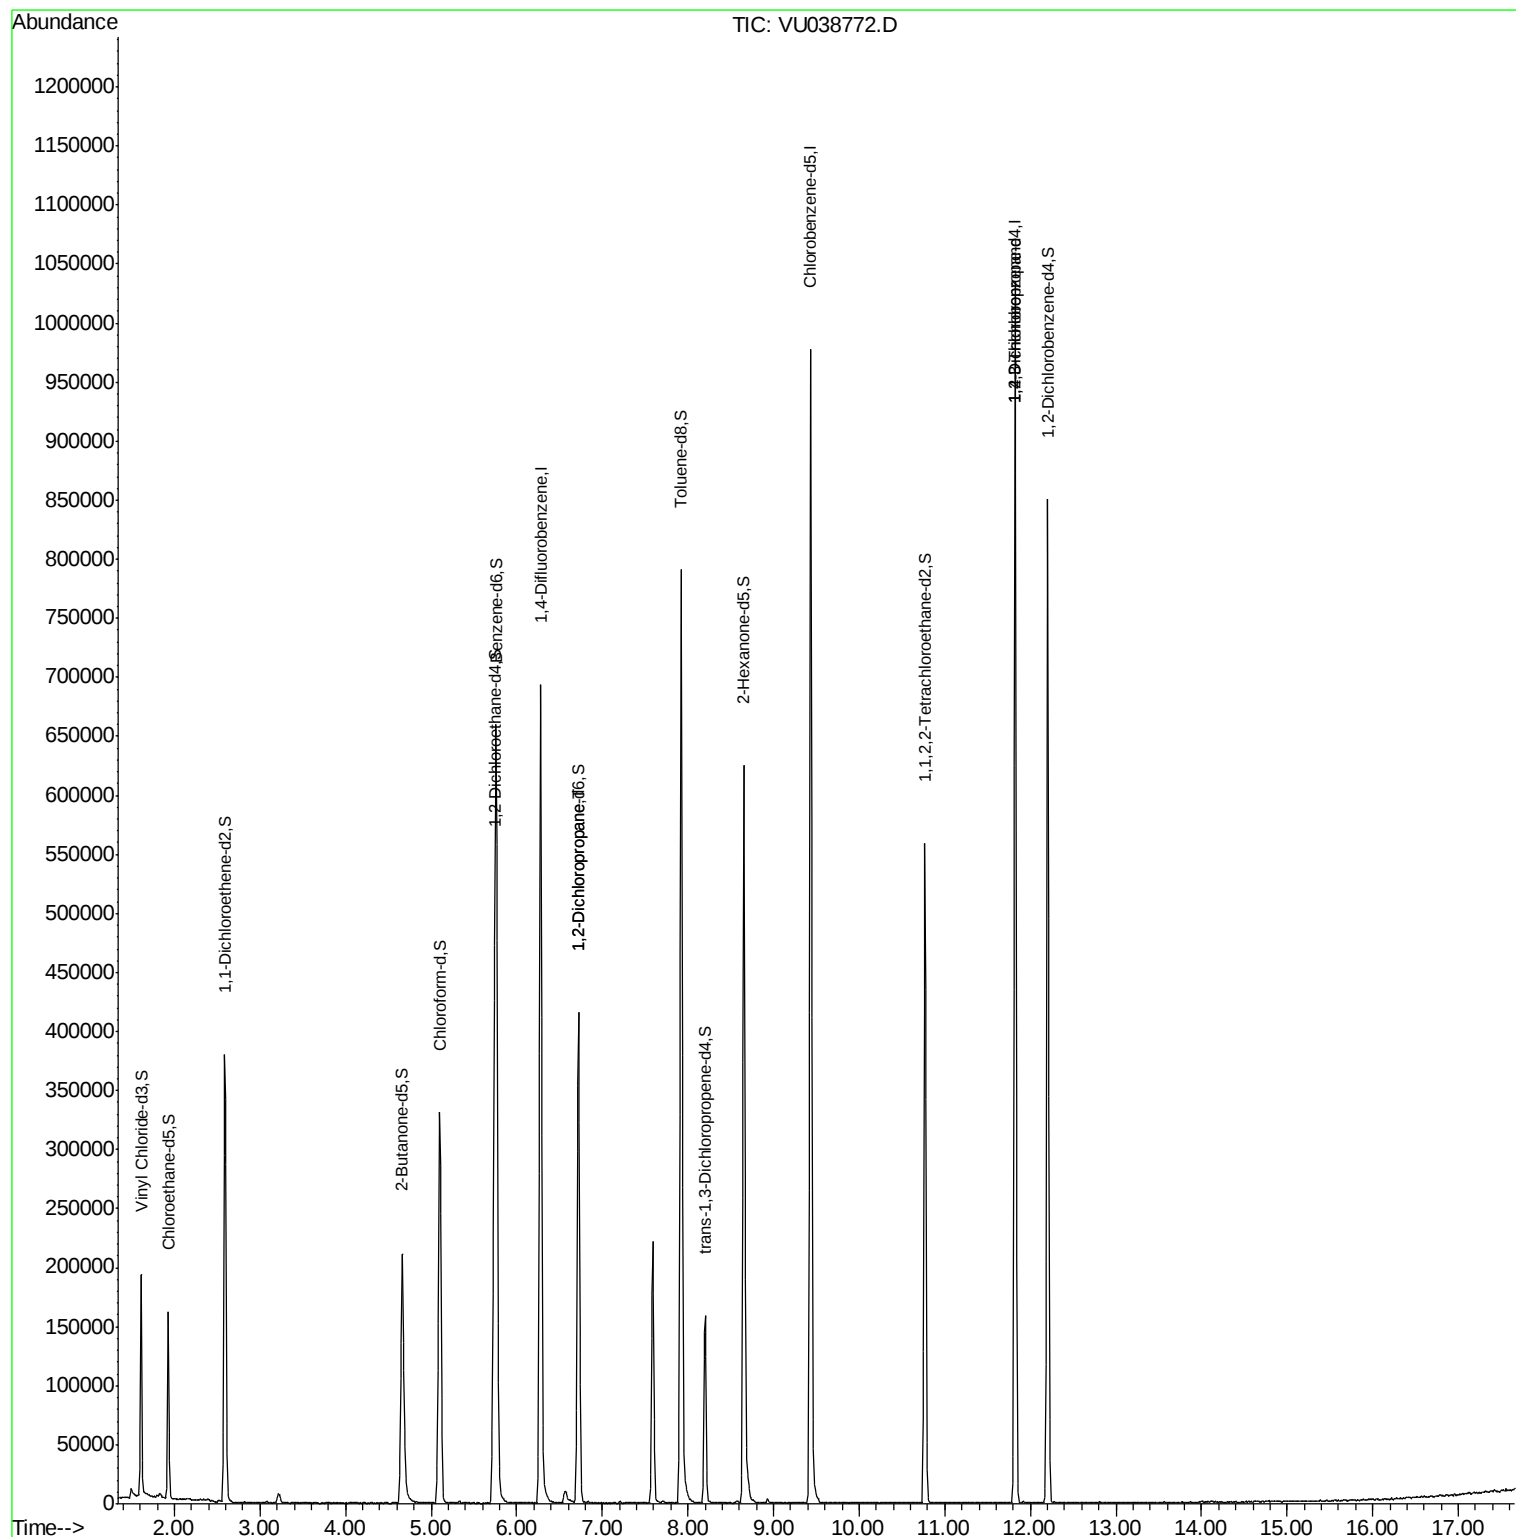


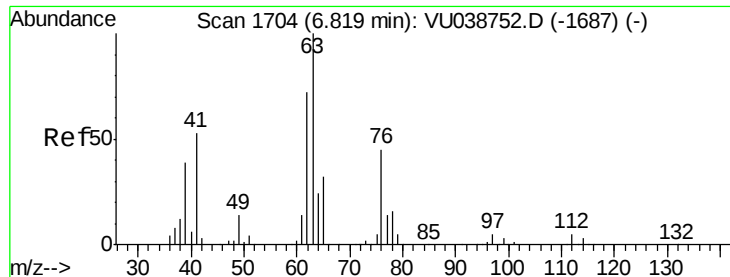

#37
 1,2-Dichloropropane
 Concen: 5.055 ug/L
 RT: 6.72 min Scan# 1673
 Delta R.T. -0.10 min
 Lab File: VU038772.D
 Acq: 10 Jun 2020 12:13

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Tot Ion: 63 Resp: 21686
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.4 5.2#

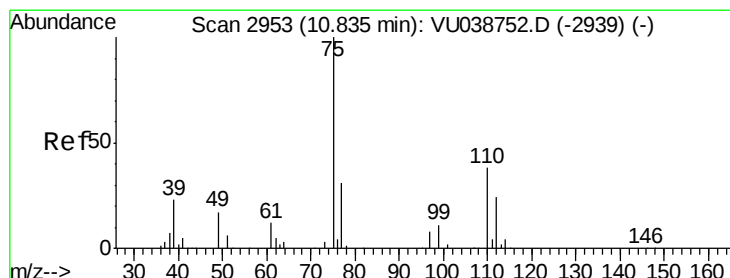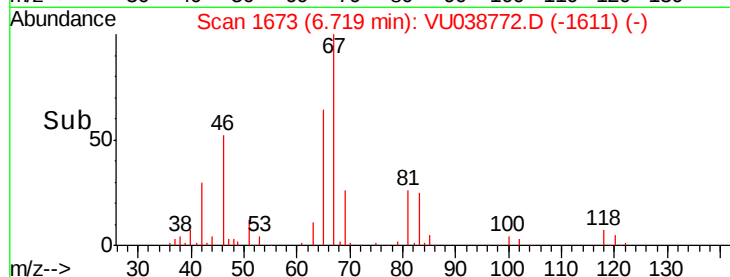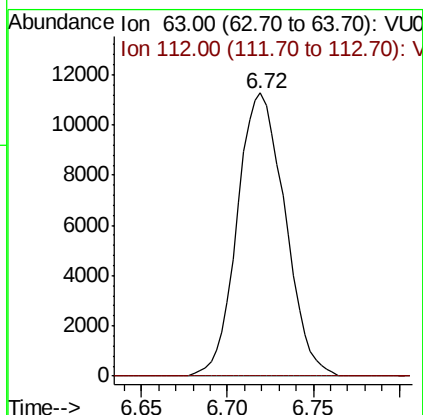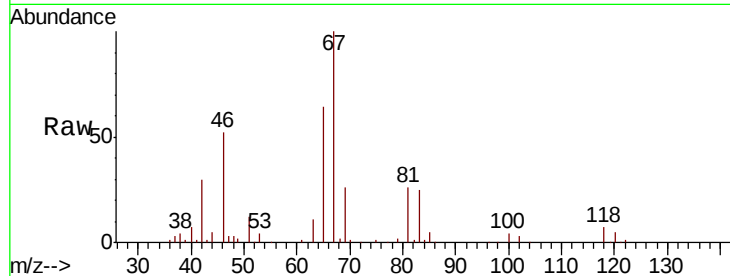

#59
 1,2,3-Trichloropropane
 Concen: 5.379 ug/L
 RT: 11.82 min Scan# 3260
 Delta R.T. 0.99 min
 Lab File: VU038772.D
 Acq: 10 Jun 2020 12:13

Tgt Ion: 75 Resp: 32358
 Ion Ratio Lower Upper
 75 100
 77 39.5 25.3 37.9#

