

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061020\
 Data File : VU038730.D
 Acq On : 09 Jun 2020 18:24
 Operator : SY/MD
 Sample : L2897-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW0K9

Quant Time: Jun 10 05:20:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 10 05:09:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	555680	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	545420	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	255517	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	142016	45.74	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.48%
7) Chloroethane-d5	1.93	69	115500	47.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.92%
11) 1,1-Dichloroethene-d2	2.59	63	223361	33.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.02%
21) 2-Butanone-d5	4.66	46	271451	89.87	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.87%
24) Chloroform-d	5.10	84	289030	43.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.36%
26) 1,2-Dichloroethane-d4	5.74	65	197477	44.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.02%
32) Benzene-d6	5.76	84	592947	45.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.26%
36) 1,2-Dichloropropane-d6	6.72	67	182421	45.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.10%
41) Toluene-d8	7.92	98	508191	42.80	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.60%
43) trans-1,3-Dichloropropene-	8.20	79	88355	43.34	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.68%
47) 2-Hexanone-d5	8.65	63	195475	90.70	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.70%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	255210	42.25	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.50%
64) 1,2-Dichlorobenzene-d4	12.21	152	201982	45.53	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.06%

Target Compounds


					Ovalue
5) Vinyl chloride	1.62	62	22251	5.005 ug/L	# 53
17) trans-1,2-Dichloroethene	3.38	96	14619	3.798 ug/L	95
20) cis-1,2-Dichloroethene	4.71	96	438952	103.170 ug/L	97
34) Trichloroethene	6.57	95	23059	5.598 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061020\
Data File : VU038730.D
Acq On : 09 Jun 2020 18:24
Operator : SY/MD
Sample : L2897-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW0K9

Quant Time: Jun 10 05:20:56 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 10 05:09:22 2020
Response via : Initial Calibration

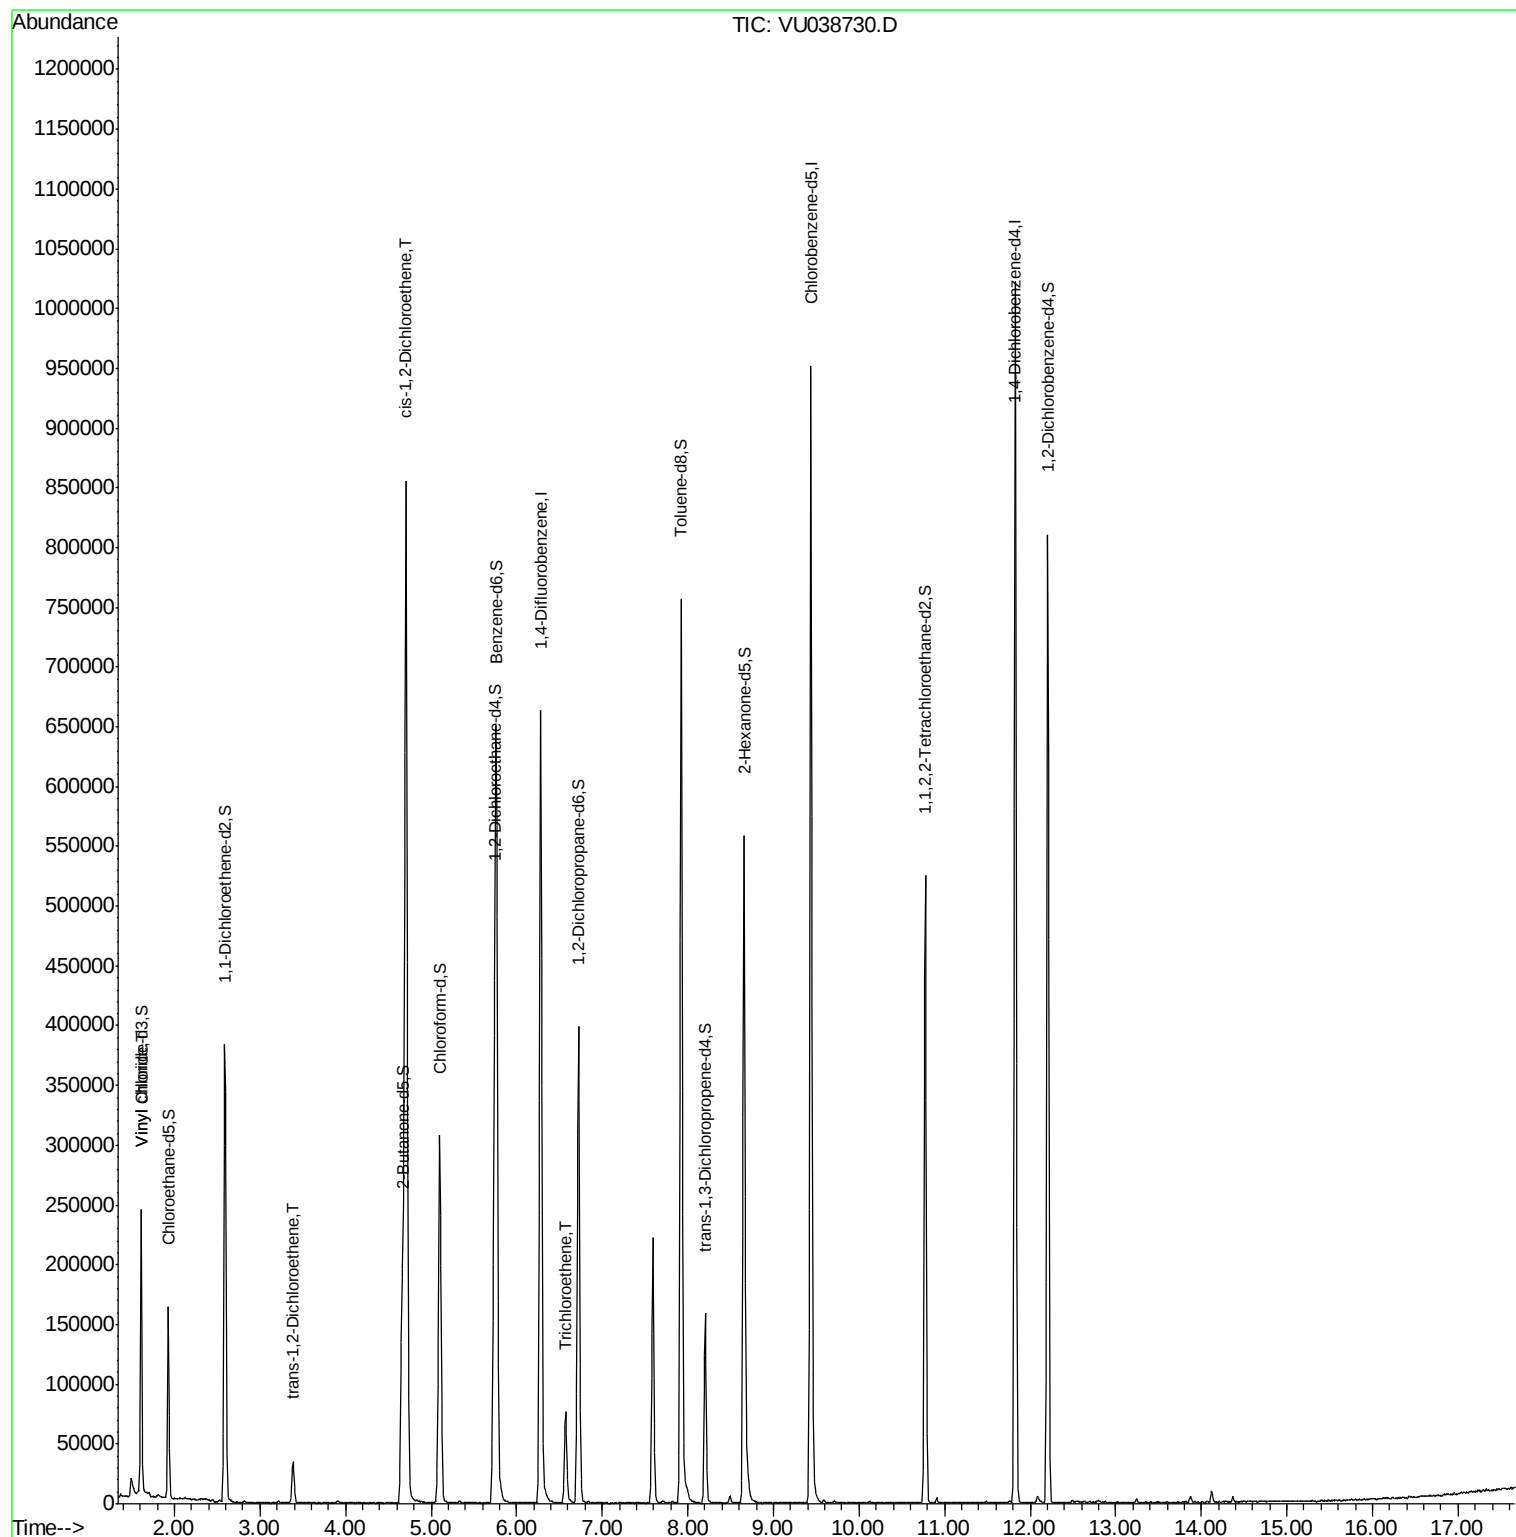

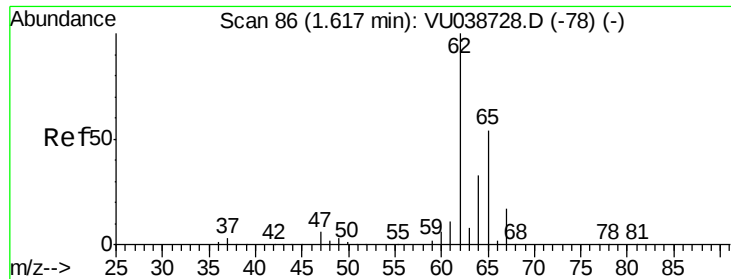

#5

Vinyl chloride

Concen: 5.005 ug/L

RT: 1.62 min Scan# 86

Delta R.T. -0.00 min

Lab File: VU038730.D

Acq: 09 Jun 2020 18:24

Instrument :

MSVOA_U

ClientSampled :


EW0K9

Tot Ion: 62 Resp: 22251

Ion Ratio Lower Upper




62 100

64 59.6 23.0 42.8#

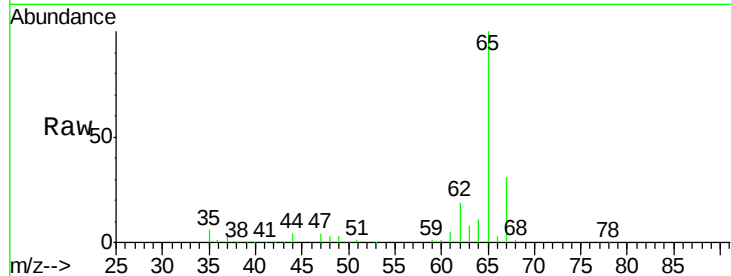

Abundance Ion 62.00 (61.70 to 62.70): VU0

Ion 64.00 (63.70 to 64.70): VU0

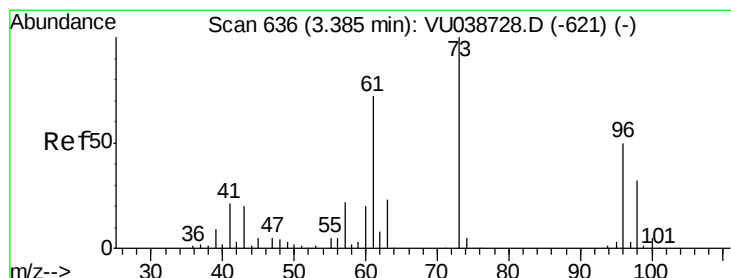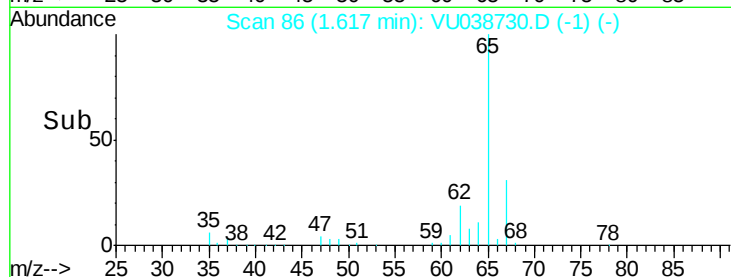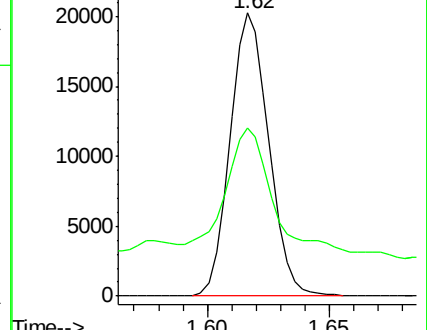

#17

trans-1,2-Dichloroethene

Concen: 3.798 ug/L

RT: 3.38 min Scan# 636

Delta R.T. -0.00 min

Lab File: VU038730.D

Acq: 09 Jun 2020 18:24


Tgt Ion: 96 Resp: 14619

Ion Ratio Lower Upper

96 100

61 135.3 98.2 182.4



98 57.0 44.3 82.3

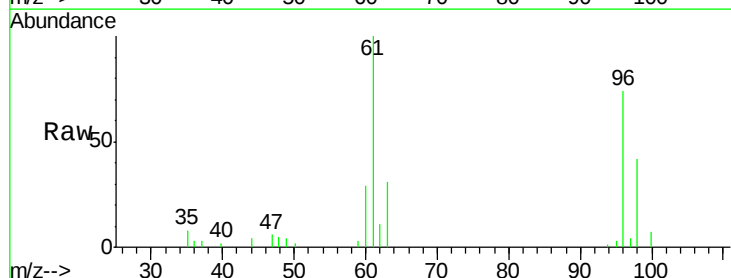


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.00 (60.70 to 61.70): VU0

Ion 98.00 (97.70 to 98.70): VU0

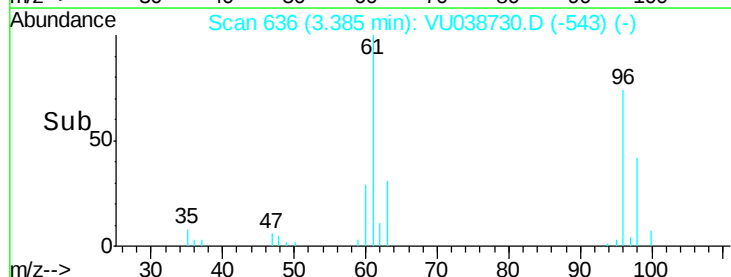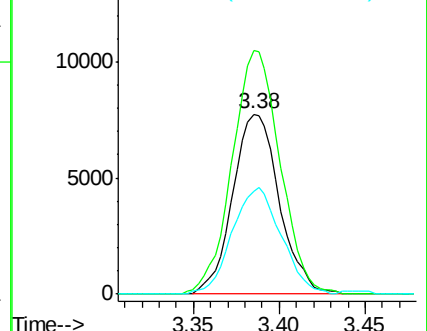

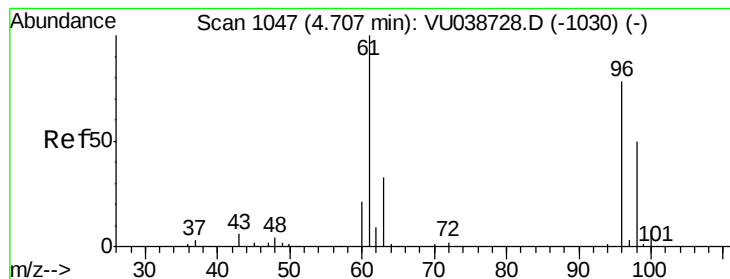

#20

cis-1,2-Dichloroethene

Concen: 103.170 ug/L

RT: 4.71 min Scan# 1047

Delta R.T. -0.00 min

Lab File: VU038730.D

Acq: 09 Jun 2020 18:24

Instrument :

MSVOA_U

ClientSampleId :

EW0K9


Tot Ion: 96 Resp: 438952

Ion Ratio Lower Upper

96 100

61 131.0 89.5 166.1




68 0.0 0.0 0.0

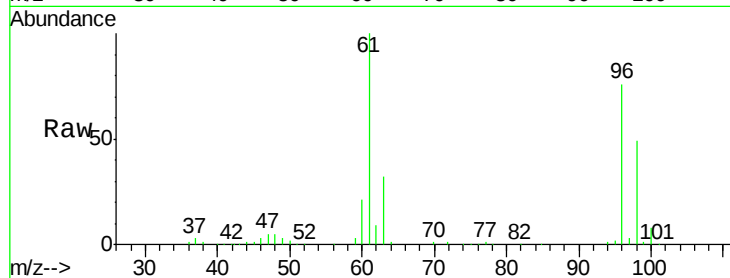

Abundance Ion 96.00 (95.70 to 96.70): VU038730.D (-1534) (-)

Ion 61.00 (60.70 to 61.70): VU038730.D (-1534) (-)

Ion 68.00 (67.70 to 68.70): VU038730.D (-1534) (-)

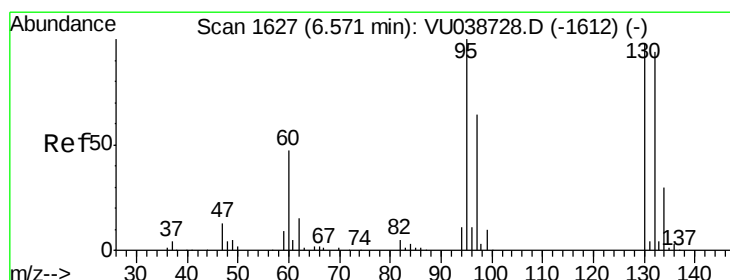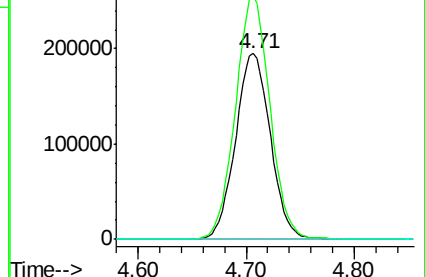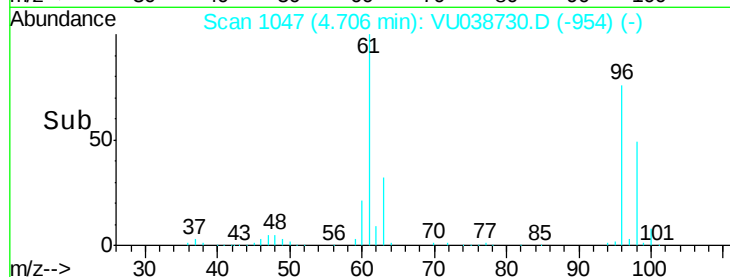

#34

Trichloroethene

Concen: 5.598 ug/L

RT: 6.57 min Scan# 1627

Delta R.T. -0.00 min

Lab File: VU038730.D

Acq: 09 Jun 2020 18:24

Tgt Ion: 95 Resp: 23059


Ion Ratio Lower Upper

95 100

97 69.0 44.4 82.4

132 102.6 64.9 120.5

130 111.4 68.6 127.4

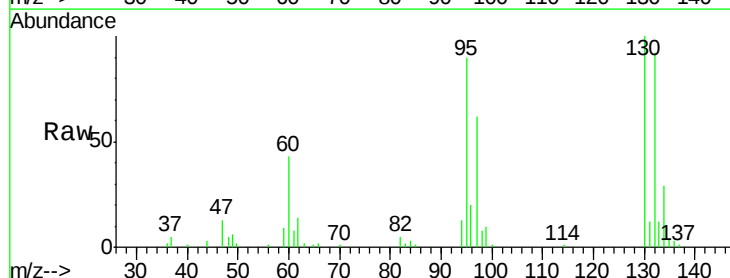

Abundance Ion 95.00 (94.70 to 95.70): VU038730.D (-1534) (-)

Ion 97.00 (96.70 to 97.70): VU038730.D (-1534) (-)

Ion 132.00 (131.70 to 132.70): VU038730.D (-1534) (-)

Ion 130.00 (129.70 to 130.70): VU038730.D (-1534) (-)

