

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061020\
 Data File : VU038729.D
 Acq On : 09 Jun 2020 17:48
 Operator : SY/MD
 Sample : VU0610WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	101	rVB	171614	190050	12.13%	1.447%
2	1.928	176	183	199	rVB	134780	176896	11.29%	1.347%
3	2.591	378	389	405	rBV	330149	539018	34.41%	4.104%
4	2.707	424	425	427	rBV2	670	275	0.02%	0.002%
5	2.944	497	499	502	rVB	471	148	0.01%	0.001%
6	2.961	502	504	507	rBV2	547	325	0.02%	0.002%
7	2.983	507	511	515	rBV2	605	504	0.03%	0.004%
8	3.080	534	541	546	rVB3	1687	2282	0.15%	0.017%
9	3.134	556	558	561	rBV2	281	198	0.01%	0.002%
10	3.150	561	563	564	rBV2	303	118	0.01%	0.001%
11	3.301	608	610	612	rBV2	298	178	0.01%	0.001%
12	3.391	629	638	642	rBV4	1254	1769	0.11%	0.013%
13	3.552	684	688	692	rBV2	378	222	0.01%	0.002%
14	3.645	715	717	718	rBV	186	78	0.00%	0.001%
15	3.671	724	725	727	rBV2	208	102	0.01%	0.001%
16	3.745	746	748	750	rBV	220	90	0.01%	0.001%
17	3.919	799	802	803	rVB	304	120	0.01%	0.001%
18	3.932	803	806	808	rBV2	235	190	0.01%	0.001%
19	4.034	835	838	843	rBV	426	367	0.02%	0.003%
20	4.060	843	846	849	rVB2	340	185	0.01%	0.001%
21	4.079	849	852	854	rBV	271	191	0.01%	0.001%
22	4.112	859	862	863	rBV	396	124	0.01%	0.001%
23	4.121	863	865	868	rBV2	203	138	0.01%	0.001%
24	4.186	883	885	887	rBV	231	105	0.01%	0.001%
25	4.266	907	910	917	rBV	253	251	0.02%	0.002%
26	4.327	926	929	932	rBV2	391	255	0.02%	0.002%
27	4.385	943	947	950	rBV3	389	303	0.02%	0.002%
28	4.398	950	951	953	rBV	169	62	0.00%	0.000%
29	4.459	968	970	972	rBV	182	108	0.01%	0.001%
30	4.510	983	986	988	rBV2	301	214	0.01%	0.002%
31	4.555	998	1000	1001	rBV	251	112	0.01%	0.001%
32	4.661	1019	1033	1064	rBV	174729	423444	27.03%	3.224%
33	4.967	1126	1128	1130	rBV2	367	136	0.01%	0.001%
34	5.018	1141	1144	1147	rBV3	353	276	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061020\
 Data File : VU038729.D
 Acq On : 09 Jun 2020 17:48
 Operator : SY/MD
 Sample : VU0610WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

35	5.102	1152	1170	1189	rBV	275016	601749	38.42%	4.582%
36	5.327	1230	1240	1248	rVB4	1874	3504	0.22%	0.027%
37	5.375	1253	1255	1257	rBV	250	139	0.01%	0.001%
38	5.411	1257	1266	1267	rBV5	1051	1366	0.09%	0.010%
39	5.472	1284	1285	1286	rBV	195	43	0.00%	0.000%
40	5.481	1286	1288	1292	rVV	153	81	0.01%	0.001%
41	5.497	1292	1293	1294	rVB	219	42	0.00%	0.000%
42	5.513	1295	1298	1303	rVV	331	281	0.02%	0.002%
43	5.533	1303	1304	1306	rVB	248	72	0.00%	0.001%
44	5.584	1317	1320	1321	rBV2	135	77	0.00%	0.001%
45	5.758	1348	1374	1402	rBV2	569574	1566385	100.00%	11.927%
46	6.031	1457	1459	1461	rBV	254	124	0.01%	0.001%
47	6.054	1464	1466	1471	rBV2	442	367	0.02%	0.003%
48	6.099	1477	1480	1482	rVB2	340	150	0.01%	0.001%
49	6.211	1512	1515	1516	rBV	329	183	0.01%	0.001%
50	6.279	1521	1536	1577	rBV	613750	1203057	76.80%	9.160%
51	6.565	1613	1625	1641	rBV7	7377	19698	1.26%	0.150%
52	6.719	1658	1673	1692	rBV	345952	669038	42.71%	5.094%
53	6.874	1719	1721	1724	rVB	590	260	0.02%	0.002%
54	6.909	1728	1732	1733	rBV2	415	300	0.02%	0.002%
55	6.954	1742	1746	1748	rBV2	255	183	0.01%	0.001%
56	7.041	1769	1773	1776	rBV2	322	292	0.02%	0.002%
57	7.128	1796	1800	1804	rBV2	285	309	0.02%	0.002%
58	7.292	1847	1851	1852	rBV	228	142	0.01%	0.001%
59	7.420	1889	1891	1893	rVB	177	65	0.00%	0.000%
60	7.472	1905	1907	1909	rBV	315	122	0.01%	0.001%
61	7.488	1909	1912	1919	rVV3	531	554	0.04%	0.004%
62	7.539	1926	1928	1930	rBV3	213	80	0.01%	0.001%
63	7.587	1930	1943	1961	rBV	195416	343913	21.96%	2.619%
64	7.812	2004	2013	2024	rBV5	2564	3746	0.24%	0.029%
65	7.922	2033	2047	2078	rBV	680812	1245017	79.48%	9.480%
66	8.201	2122	2134	2149	rBV	137015	228407	14.58%	1.739%
67	8.340	2175	2177	2178	rBV	369	137	0.01%	0.001%
68	8.439	2206	2208	2210	rBV	228	118	0.01%	0.001%
69	8.571	2247	2249	2250	rBV	375	138	0.01%	0.001%
70	8.581	2250	2252	2255	rVB2	647	364	0.02%	0.003%
71	8.652	2262	2274	2308	rBV	504747	903661	57.69%	6.881%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061020\
 Data File : VU038729.D
 Acq On : 09 Jun 2020 17:48
 Operator : SY/MD
 Sample : VU0610WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

72	8.873	2340	2343	2345	rBV2	396	203	0.01%	0.002%
73	8.899	2347	2351	2353	rBV2	381	238	0.02%	0.002%
74	8.928	2353	2360	2361	rBV3	2606	2585	0.17%	0.020%
75	9.131	2420	2423	2430	rVB	311	256	0.02%	0.002%
76	9.163	2430	2433	2435	rBV	272	174	0.01%	0.001%
77	9.436	2502	2518	2557	rBV	879057	1499348	95.72%	11.416%
78	9.587	2557	2565	2571	rBV4	4098	5822	0.37%	0.044%
79	9.709	2598	2603	2614	rVB4	1541	2569	0.16%	0.020%
80	9.822	2636	2638	2640	rBV	298	169	0.01%	0.001%
81	10.025	2696	2701	2703	rBV2	399	393	0.03%	0.003%
82	10.121	2721	2731	2741	rBV6	1915	3513	0.22%	0.027%
83	10.468	2836	2839	2842	rBV	353	172	0.01%	0.001%
84	10.500	2843	2849	2858	rVB3	1328	1624	0.10%	0.012%
85	10.771	2921	2933	2949	rBV	475885	763874	48.77%	5.816%
86	10.861	2959	2961	2962	rBV	258	105	0.01%	0.001%
87	10.906	2972	2975	2979	rBV3	576	335	0.02%	0.003%
88	11.127	3041	3044	3047	rBV2	499	311	0.02%	0.002%
89	11.163	3051	3055	3056	rBV2	334	246	0.02%	0.002%
90	11.758	3235	3240	3247	rVB6	3255	3869	0.25%	0.029%
91	11.822	3247	3260	3276	rBV	951748	1494804	95.43%	11.382%
92	12.205	3365	3379	3396	rBV	735150	1169519	74.66%	8.905%
93	12.275	3399	3401	3402	rBV	466	212	0.01%	0.002%
94	13.867	3888	3896	3903	rBV3	7896	12033	0.77%	0.092%
95	14.114	3966	3973	3984	rVB	16241	24977	1.59%	0.190%
96	14.359	4042	4049	4058	rVB4	8513	12832	0.82%	0.098%


Sum of corrected areas: 13133181

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061020\
Data File : VU038729.D
Acq On : 09 Jun 2020 17:48
Operator : SY/MD
Sample : VU0610WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK40

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

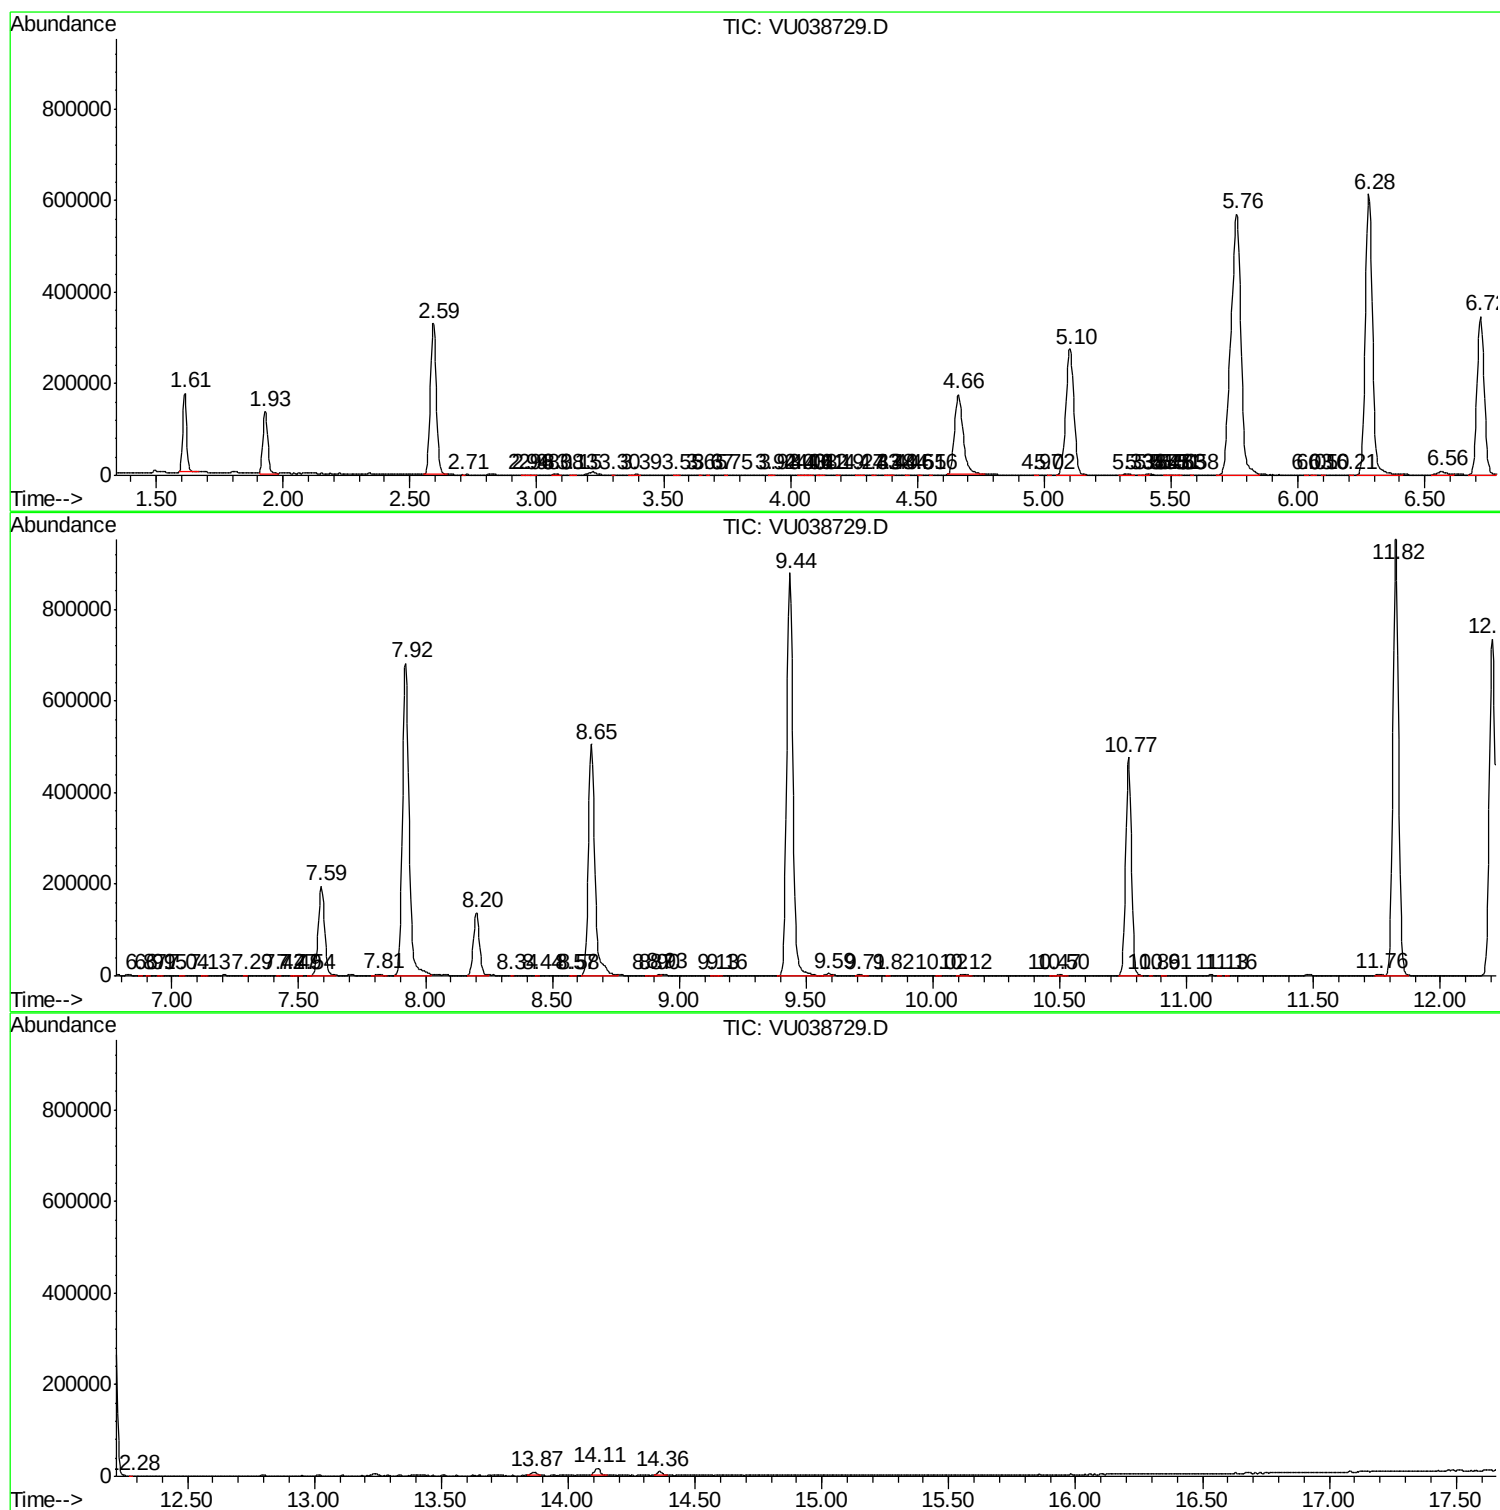

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061020\
Data File : VU038729.D
Acq On : 09 Jun 2020 17:48
Operator : SY/MD
Sample : VU0610WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061020\
Data File : VU038729.D
Acq On : 09 Jun 2020 17:48
Operator : SY/MD
Sample : VU0610WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc