

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061020\
 Data File : VU038730.D
 Acq On : 09 Jun 2020 18:24
 Operator : SY/MD
 Sample : L2897-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW0K9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	98	rVB2	236720	268417	11.54%	1.612%
2	1.928	176	183	196	rVB	160217	210831	9.07%	1.266%
3	2.591	378	389	406	rBV	381536	632606	27.20%	3.800%
4	2.896	481	484	488	rVB2	813	495	0.02%	0.003%
5	2.919	488	491	495	rVB2	351	214	0.01%	0.001%
6	2.944	495	499	500	rBV2	287	211	0.01%	0.001%
7	2.999	514	516	521	rBV3	400	256	0.01%	0.002%
8	3.157	562	565	566	rBV	401	185	0.01%	0.001%
9	3.218	575	584	586	rBV4	1157	1883	0.08%	0.011%
10	3.385	623	636	653	rBV2	35090	67948	2.92%	0.408%
11	3.674	722	726	730	rBV2	405	319	0.01%	0.002%
12	3.713	736	738	741	rBV	145	99	0.00%	0.001%
13	3.903	790	797	798	rBV3	1603	1616	0.07%	0.010%
14	3.986	821	823	828	rBV	281	240	0.01%	0.001%
15	4.224	896	897	900	rVB	228	61	0.00%	0.000%
16	4.250	903	905	907	rVB2	188	51	0.00%	0.000%
17	4.308	921	923	925	rBV2	278	115	0.00%	0.001%
18	4.359	936	939	941	rBV	243	161	0.01%	0.001%
19	4.391	947	949	953	rBV2	159	135	0.01%	0.001%
20	4.443	963	965	966	rBV	188	48	0.00%	0.000%
21	4.575	1003	1006	1009	rVB2	295	181	0.01%	0.001%
22	4.591	1009	1011	1013	rBV	323	159	0.01%	0.001%
23	4.706	1018	1047	1072	rBV2	855574	2325342	100.00%	13.967%
24	5.102	1155	1170	1189	rVB	306811	671231	28.87%	4.032%
25	5.391	1255	1260	1262	rBV2	451	425	0.02%	0.003%
26	5.411	1262	1266	1272	rVB3	713	663	0.03%	0.004%
27	5.571	1313	1316	1320	rVB2	451	312	0.01%	0.002%
28	5.591	1320	1322	1323	rBV	104	48	0.00%	0.000%
29	5.613	1327	1329	1331	rVB	172	78	0.00%	0.000%
30	5.758	1352	1374	1404	rBV2	650255	1766660	75.97%	10.611%
31	6.028	1456	1458	1462	rBV4	343	191	0.01%	0.001%
32	6.282	1520	1537	1581	rBV	663057	1305349	56.14%	7.841%
33	6.571	1614	1627	1641	rBV3	76438	151287	6.51%	0.909%
34	6.722	1659	1674	1693	rBV	397759	760533	32.71%	4.568%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061020\
 Data File : VU038730.D
 Acq On : 09 Jun 2020 18:24
 Operator : SY/MD
 Sample : L2897-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW0K9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

35	6.925	1734	1737	1740	rVB2	285	136	0.01%	0.001%
36	6.944	1740	1743	1750	rBV3	290	331	0.01%	0.002%
37	7.018	1763	1766	1768	rBV	328	193	0.01%	0.001%
38	7.079	1782	1785	1788	rBV2	158	116	0.00%	0.001%
39	7.095	1788	1790	1792	rBV	287	122	0.01%	0.001%
40	7.112	1793	1795	1799	rVB2	310	167	0.01%	0.001%
41	7.131	1799	1801	1802	rBV2	139	63	0.00%	0.000%
42	7.163	1809	1811	1813	rBV	141	67	0.00%	0.000%
43	7.211	1818	1826	1832	rVB4	1109	1752	0.08%	0.011%
44	7.240	1832	1835	1840	rVB2	380	279	0.01%	0.002%
45	7.266	1840	1843	1846	rBV	201	137	0.01%	0.001%
46	7.279	1846	1847	1849	rBV	159	75	0.00%	0.000%
47	7.346	1865	1868	1873	rBV2	259	247	0.01%	0.001%
48	7.366	1873	1874	1876	rVB	381	75	0.00%	0.000%
49	7.423	1889	1892	1897	rVB2	321	304	0.01%	0.002%
50	7.449	1897	1900	1904	rVB2	415	248	0.01%	0.001%
51	7.468	1904	1906	1910	rVB	274	132	0.01%	0.001%
52	7.513	1917	1920	1922	rBV	176	128	0.01%	0.001%
53	7.591	1928	1944	1968	rBV	221915	389249	16.74%	2.338%
54	7.710	1975	1981	1987	rVB6	1392	2129	0.09%	0.013%
55	7.819	2010	2015	2020	rVB3	1131	1141	0.05%	0.007%
56	7.922	2033	2047	2082	rBV	756491	1379961	59.34%	8.289%
57	8.202	2121	2134	2154	rBV2	158852	266283	11.45%	1.599%
58	8.407	2196	2198	2201	rBV	263	169	0.01%	0.001%
59	8.423	2201	2203	2205	rBV2	114	62	0.00%	0.000%
60	8.491	2214	2224	2236	rBV4	6022	10366	0.45%	0.062%
61	8.658	2262	2276	2306	rBV	558253	1011061	43.48%	6.073%
62	8.877	2341	2344	2345	rBV2	275	162	0.01%	0.001%
63	9.005	2380	2384	2388	rBV2	282	301	0.01%	0.002%
64	9.025	2388	2390	2393	rVB	482	258	0.01%	0.002%
65	9.073	2400	2405	2408	rBV2	248	262	0.01%	0.002%
66	9.102	2411	2414	2416	rBV2	257	178	0.01%	0.001%
67	9.150	2425	2429	2435	rBV2	324	273	0.01%	0.002%
68	9.179	2435	2438	2444	rBV2	796	698	0.03%	0.004%
69	9.375	2495	2499	2502	rBV	310	276	0.01%	0.002%
70	9.439	2505	2519	2554	rVV	951168	1631250	70.15%	9.798%
71	9.591	2559	2566	2574	rBV4	2259	3267	0.14%	0.020%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061020\
 Data File : VU038730.D
 Acq On : 09 Jun 2020 18:24
 Operator : SY/MD
 Sample : L2897-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW0K9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

72	9.709	2596	2603	2613	rVB4	1848	2462	0.11%	0.015%
73	10.028	2699	2702	2704	rBV	307	172	0.01%	0.001%
74	10.066	2712	2714	2719	rVB	277	147	0.01%	0.001%
75	10.298	2784	2786	2790	rBV2	317	218	0.01%	0.001%
76	10.420	2821	2824	2826	rBV	208	177	0.01%	0.001%
77	10.507	2844	2851	2853	rBV	710	616	0.03%	0.004%
78	10.774	2921	2934	2957	rVB	524997	840132	36.13%	5.046%
79	10.909	2967	2976	2985	rBV6	4287	6361	0.27%	0.038%
80	11.825	3249	3261	3282	rBV	1021719	1602076	68.90%	9.623%
81	12.089	3336	3343	3354	rVB7	5053	8290	0.36%	0.050%
82	12.208	3367	3380	3399	rVB	809736	1291087	55.52%	7.755%
83	12.491	3464	3468	3471	rBV	2174	1931	0.08%	0.012%
84	12.767	3552	3554	3557	rBV	878	443	0.02%	0.003%
85	13.243	3697	3702	3709	rBV4	2440	2654	0.11%	0.016%
86	14.121	3967	3975	3984	rBV3	8681	14344	0.62%	0.086%
87	14.365	4046	4051	4063	rVB6	4554	7248	0.31%	0.044%


Sum of corrected areas: 16648626

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061020\
Data File : VU038730.D
Acq On : 09 Jun 2020 18:24
Operator : SY/MD
Sample : L2897-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW0K9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

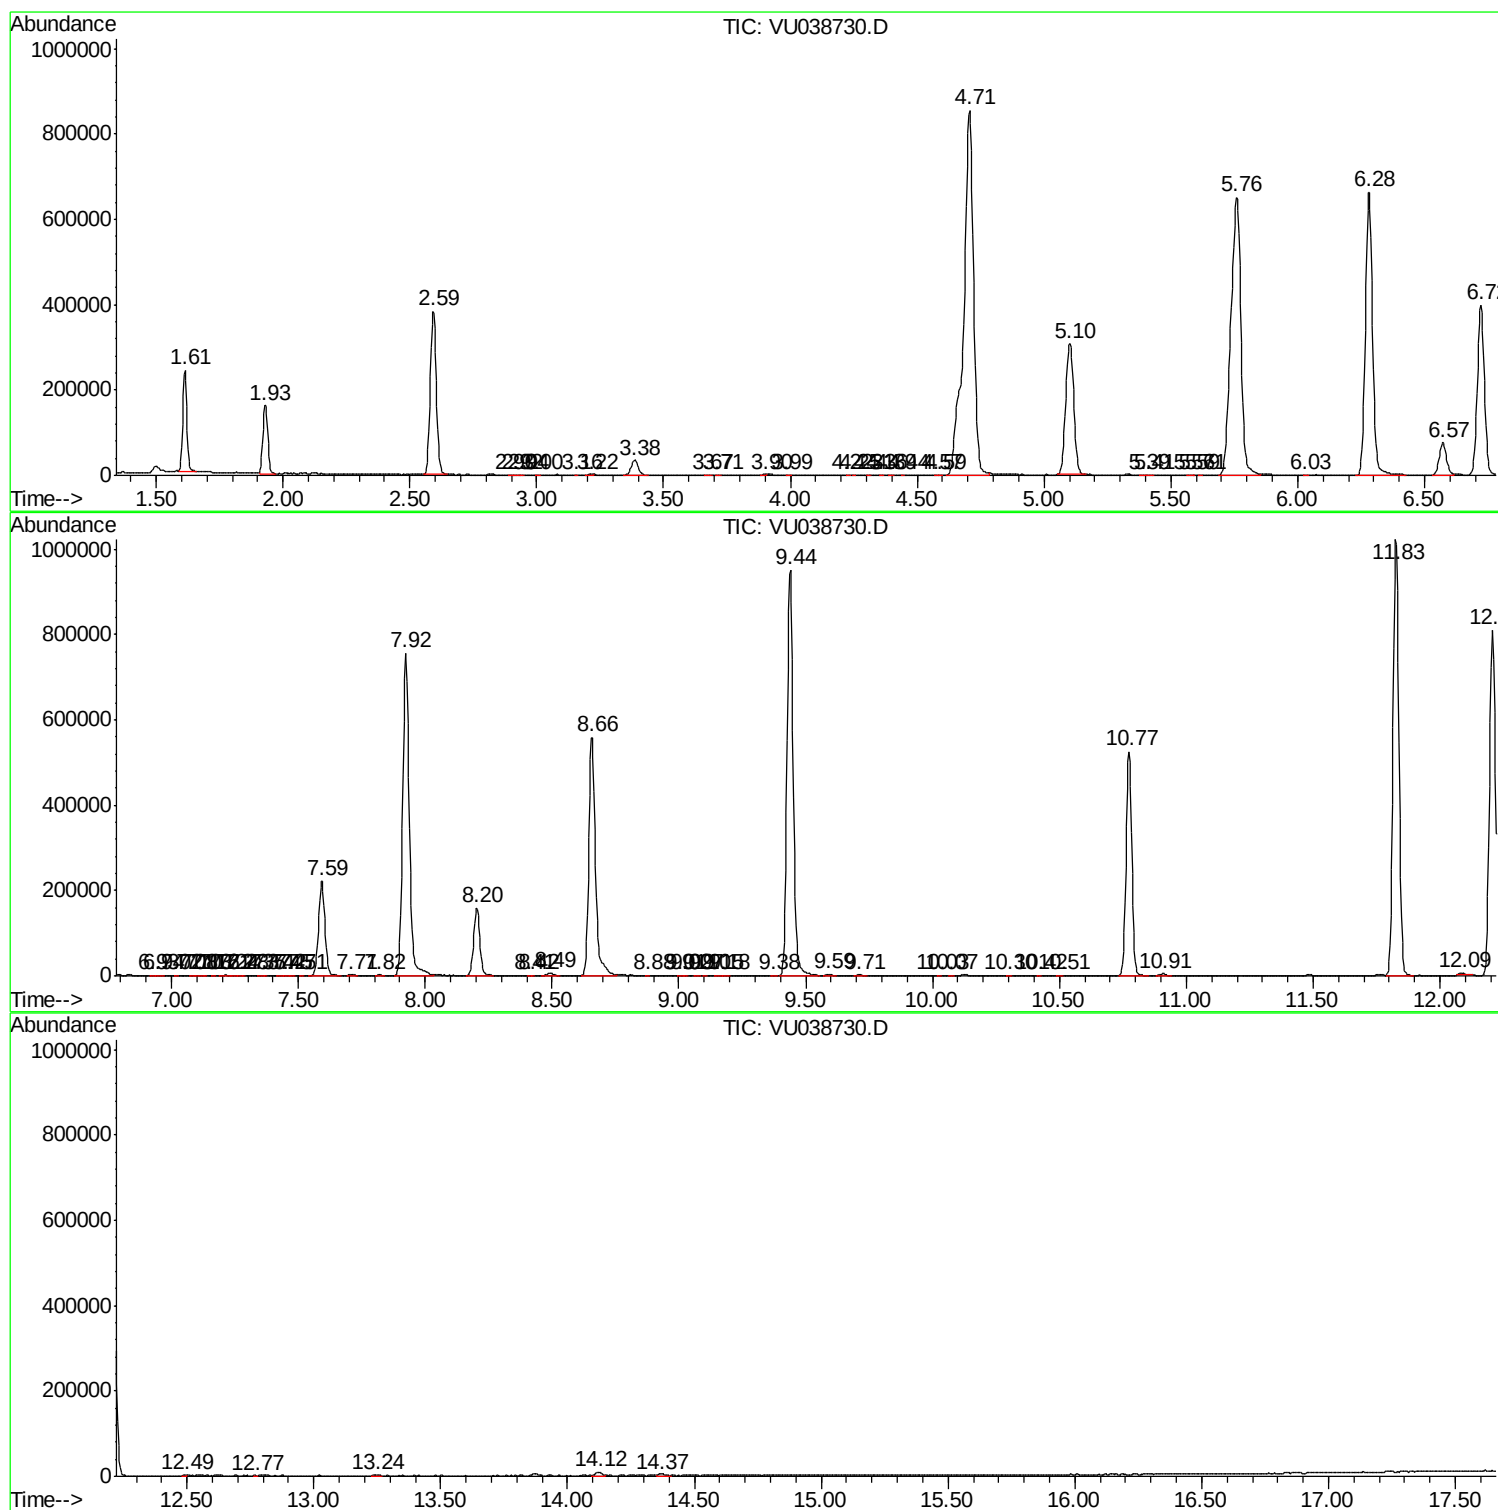

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061020\
Data File : VU038730.D
Acq On : 09 Jun 2020 18:24
Operator : SY/MD
Sample : L2897-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW0K9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061020\
Data File : VU038730.D
Acq On : 09 Jun 2020 18:24
Operator : SY/MD
Sample : L2897-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW0K9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc