

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061020\
 Data File : VU038775.D
 Acq On : 10 Jun 2020 13:18
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	77	85	97	rBV	311340	338782	14.08%	1.854%
2	1.929	175	183	198	rVB	231464	300718	12.50%	1.646%
3	2.591	378	389	416	rVB	533521	905905	37.65%	4.958%
4	2.771	443	445	449	rVB2	392	258	0.01%	0.001%
5	2.790	449	451	452	rBV	342	154	0.01%	0.001%
6	3.006	515	518	521	rBV3	388	312	0.01%	0.002%
7	3.044	527	530	531	rBV3	425	244	0.01%	0.001%
8	3.308	610	612	614	rVB2	300	118	0.00%	0.001%
9	3.334	618	620	622	rBV	278	116	0.00%	0.001%
10	3.366	626	630	631	rBV2	429	333	0.01%	0.002%
11	3.482	664	666	671	rVB2	551	296	0.01%	0.002%
12	3.549	685	687	690	rBV2	283	211	0.01%	0.001%
13	3.613	705	707	712	rVB2	289	170	0.01%	0.001%
14	3.636	712	714	715	rBV2	317	147	0.01%	0.001%
15	3.662	720	722	725	rVB	310	125	0.01%	0.001%
16	3.687	727	730	736	rBV2	358	326	0.01%	0.002%
17	3.719	736	740	742	rBV3	310	248	0.01%	0.001%
18	3.790	761	762	763	rBV3	204	54	0.00%	0.000%
19	3.880	786	790	793	rBV	243	209	0.01%	0.001%
20	4.006	826	829	832	rBV2	361	259	0.01%	0.001%
21	4.112	859	862	865	rBV2	491	266	0.01%	0.001%
22	4.150	872	874	876	rVB2	248	99	0.00%	0.001%
23	4.237	897	901	904	rBV2	287	222	0.01%	0.001%
24	4.285	913	916	918	rVB	264	144	0.01%	0.001%
25	4.298	918	920	923	rVB2	183	67	0.00%	0.000%
26	4.314	923	925	926	rBV2	339	131	0.01%	0.001%
27	4.356	935	938	940	rBV2	188	116	0.00%	0.001%
28	4.395	948	950	953	rVB2	280	142	0.01%	0.001%
29	4.453	967	968	969	rVB	235	45	0.00%	0.000%
30	4.475	969	975	976	rBV2	229	199	0.01%	0.001%
31	4.530	988	992	997	rBV3	483	414	0.02%	0.002%
32	4.572	1003	1005	1007	rBV	340	121	0.01%	0.001%
33	4.668	1020	1035	1074	rBV	251539	656751	27.30%	3.595%
34	4.871	1095	1098	1100	rBV3	674	476	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061020\
 Data File : VU038775.D
 Acq On : 10 Jun 2020 13:18
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

35	5.038	1148	1150	1152	rBV	368	183	0.01%	0.001%
36	5.102	1152	1170	1192	rBV	425343	925043	38.45%	5.063%
37	5.369	1252	1253	1254	rBV	287	59	0.00%	0.000%
38	5.408	1259	1265	1267	rBV2	786	702	0.03%	0.004%
39	5.510	1295	1297	1299	rBV2	471	233	0.01%	0.001%
40	5.546	1305	1308	1309	rBV	167	97	0.00%	0.001%
41	5.559	1309	1312	1314	rBV2	440	230	0.01%	0.001%
42	5.613	1326	1329	1332	rVB2	262	147	0.01%	0.001%
43	5.665	1341	1345	1347	rBV	364	263	0.01%	0.001%
44	5.681	1347	1350	1351	rVV	266	159	0.01%	0.001%
45	5.758	1351	1374	1415	rVV2	891839	2406113	100.00%	13.170%
46	6.002	1448	1450	1453	rVB2	746	282	0.01%	0.002%
47	6.279	1520	1536	1568	rBV	678451	1324264	55.04%	7.248%
48	6.562	1612	1624	1644	rBV4	12863	39770	1.65%	0.218%
49	6.719	1659	1673	1697	rVB	531396	1034181	42.98%	5.661%
50	6.941	1738	1742	1744	rBV2	299	172	0.01%	0.001%
51	6.970	1749	1751	1752	rBV2	190	66	0.00%	0.000%
52	7.153	1805	1808	1811	rBV	252	178	0.01%	0.001%
53	7.208	1816	1825	1832	rBV3	2338	3525	0.15%	0.019%
54	7.359	1870	1872	1873	rBV	267	101	0.00%	0.001%
55	7.411	1886	1888	1894	rBV2	178	96	0.00%	0.001%
56	7.440	1895	1897	1901	rVB	372	229	0.01%	0.001%
57	7.459	1901	1903	1905	rBV	194	71	0.00%	0.000%
58	7.485	1907	1911	1915	rBV	429	358	0.01%	0.002%
59	7.591	1930	1944	1964	rBV	295982	515040	21.41%	2.819%
60	7.838	2019	2021	2025	rVB2	428	266	0.01%	0.001%
61	7.922	2025	2047	2082	rBV	1036616	1908499	79.32%	10.446%
62	8.198	2121	2133	2159	rBV	210581	355631	14.78%	1.947%
63	8.446	2207	2210	2214	rVB	367	213	0.01%	0.001%
64	8.468	2214	2217	2218	rBV	342	169	0.01%	0.001%
65	8.520	2230	2233	2238	rBV2	338	283	0.01%	0.002%
66	8.568	2242	2248	2261	rVB4	2557	4059	0.17%	0.022%
67	8.652	2261	2274	2307	rBV	770019	1396700	58.05%	7.645%
68	8.931	2353	2361	2368	rBV5	2664	4620	0.19%	0.025%
69	8.986	2375	2378	2380	rBV	619	378	0.02%	0.002%
70	9.067	2400	2403	2407	rBV2	458	364	0.02%	0.002%
71	9.224	2449	2452	2453	rVB	350	167	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061020\
 Data File : VU038775.D
 Acq On : 10 Jun 2020 13:18
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

72	9.243	2453	2458	2464	rBV	563	771	0.03%	0.004%
73	9.433	2503	2517	2556	rVB	976981	1669907	69.40%	9.140%
74	9.575	2556	2561	2564	rBV2	604	614	0.03%	0.003%
75	9.790	2626	2628	2632	rVB	248	109	0.00%	0.001%
76	9.816	2633	2636	2638	rBV	332	179	0.01%	0.001%
77	10.012	2695	2697	2700	rBV2	301	184	0.01%	0.001%
78	10.054	2708	2710	2715	rBV2	304	205	0.01%	0.001%
79	10.230	2762	2765	2768	rBV2	479	359	0.01%	0.002%
80	10.575	2870	2872	2874	rBV	372	253	0.01%	0.001%
81	10.767	2919	2932	2951	rBV	706877	1138529	47.32%	6.232%
82	11.404	3126	3130	3134	rBV	483	510	0.02%	0.003%
83	11.423	3134	3136	3142	rVB3	618	476	0.02%	0.003%
84	11.600	3188	3191	3192	rBV	326	187	0.01%	0.001%
85	11.822	3247	3260	3281	rBV	1012082	1583727	65.82%	8.668%
86	12.201	3365	3378	3395	rBV	1089288	1742673	72.43%	9.538%
87	13.285	3713	3715	3718	rVB	565	202	0.01%	0.001%


Sum of corrected areas: 18269974

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061020\
Data File : VU038775.D
Acq On : 10 Jun 2020 13:18
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

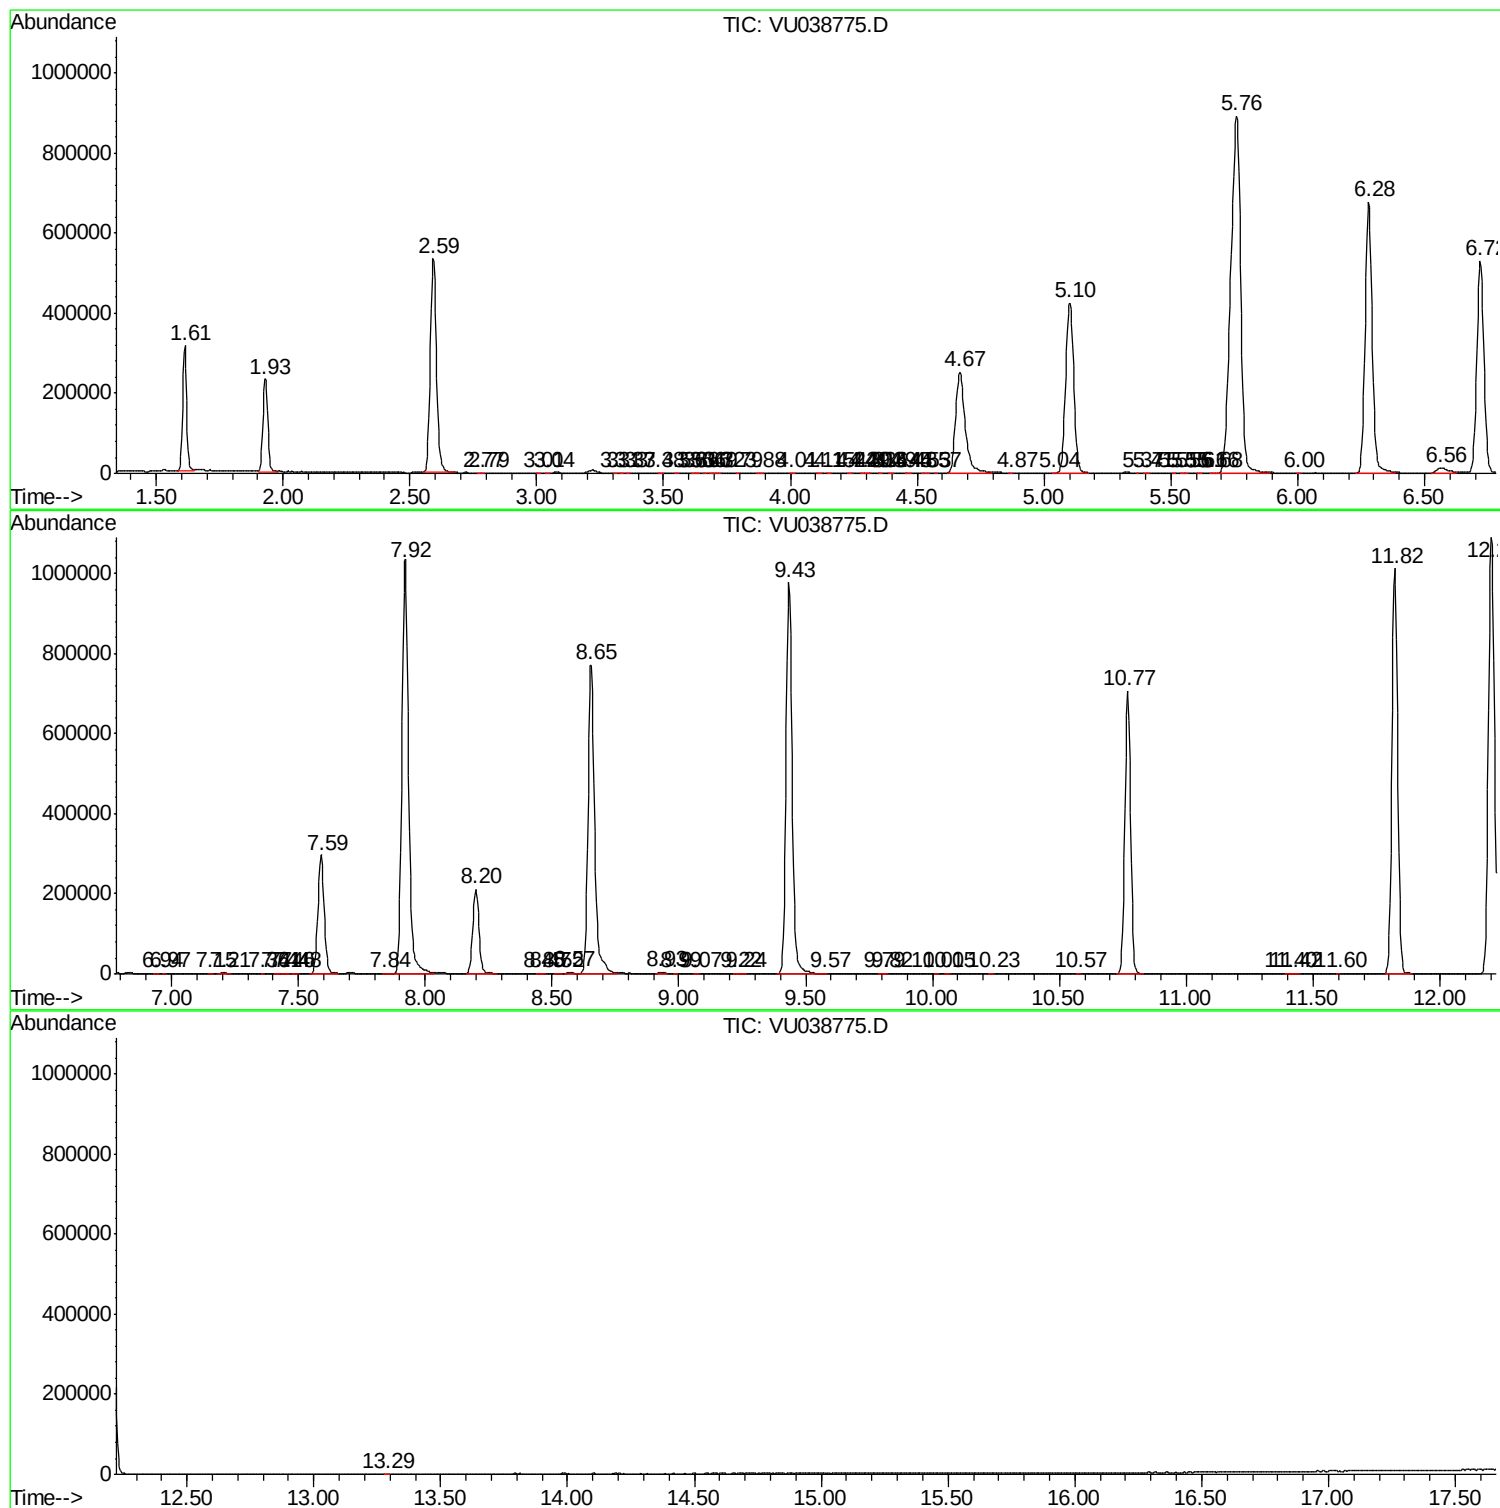

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061020\
Data File : VU038775.D
Acq On : 10 Jun 2020 13:18
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061020\
Data File : VU038775.D
Acq On : 10 Jun 2020 13:18
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc