


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061020\
 Data File : VU038727.D
 Acq On : 09 Jun 2020 16:26
 Operator : SY/MD
 Sample : BFB52
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB52

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis
 Last Update : Thu Jun 11 07:12:16 2020

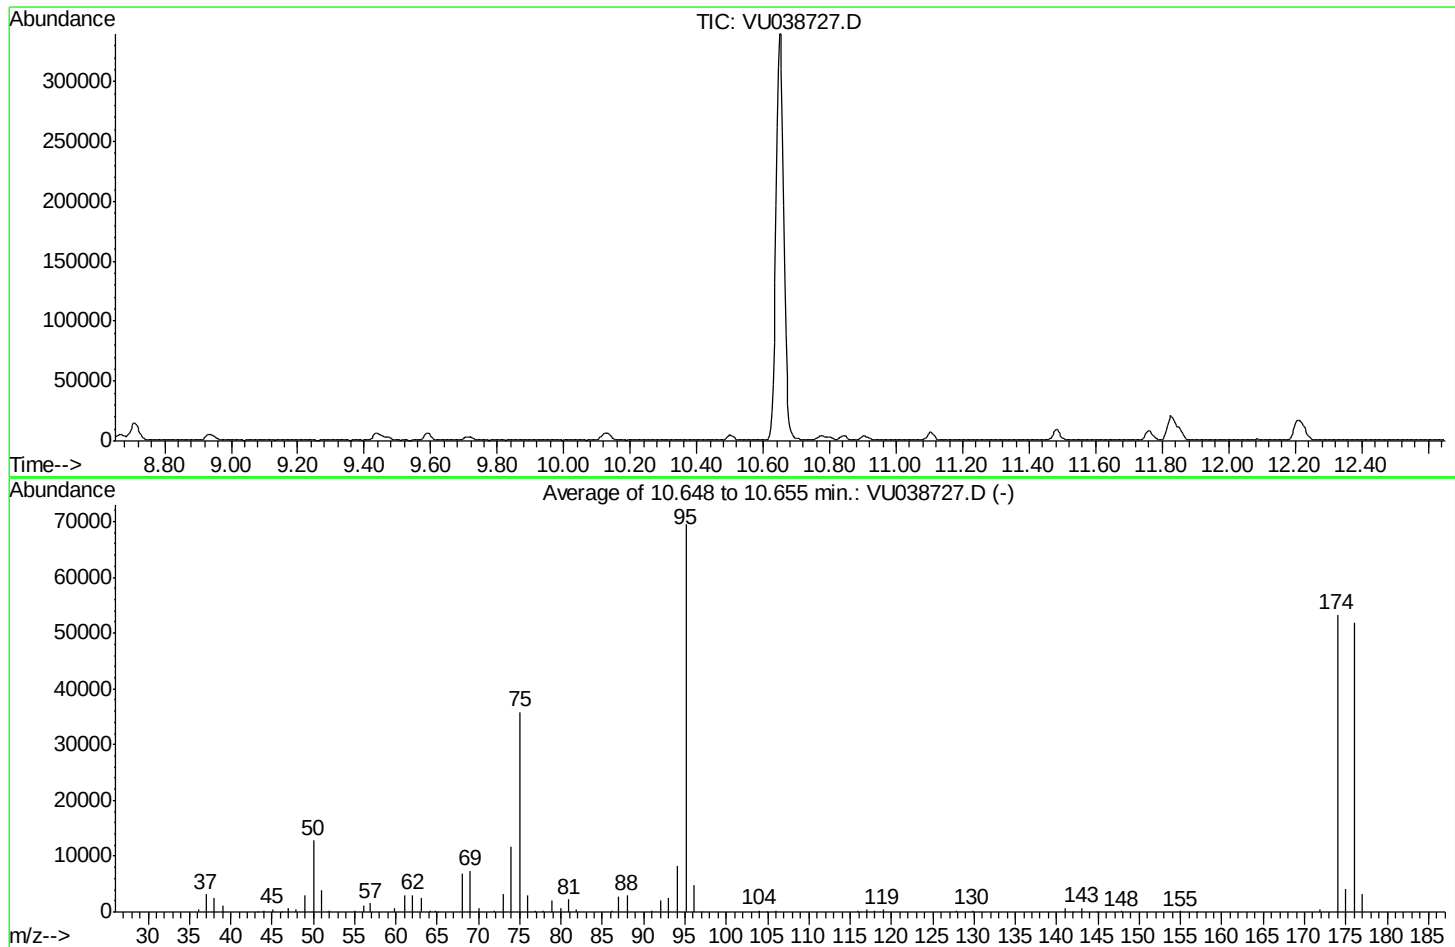

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	12829	PASS
75	95	30	80	51.6	35880	PASS
95	95	100	100	100.0	69490	PASS
96	95	5	9	7.0	4859	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.7	53301	PASS
175	174	5	9	7.7	4101	PASS
176	174	95	101	97.5	51960	PASS
177	176	5	9	6.2	3210	PASS

m/z	Abundance
36.00	579.0
37.00	3475.0
38.00	2973.0
39.10	1381.0
39.90	120.0
43.20	137.0
44.00	951.0
45.10	597.0
46.10	107.0
46.90	670.0
47.90	512.0
49.00	3189.0
50.00	13527.0
51.00	4186.0
52.00	191.0
54.90	222.0
56.10	1166.0
57.00	1743.0
59.90	889.0
61.00	3144.0
62.00	3234.0
63.10	2793.0
64.10	445.0
64.80	334.0
68.00	7080.0
69.00	7606.0
70.00	580.0
71.90	357.0
73.00	3330.0
74.00	12582.0
75.10	36968.0
76.00	3310.0
76.90	339.0
77.80	327.0
78.90	2301.0
80.00	783.0
80.90	2343.0
81.90	647.0
87.00	2548.0
88.00	2821.0
90.90	293.0
92.00	2062.0
93.00	2767.0
94.10	8886.0
95.10	70968.0
96.10	5243.0
97.00	116.0
103.90	389.0
106.00	221.0
115.90	287.0
117.00	471.0
118.00	272.0
118.90	389.0
127.80	289.0
129.80	255.0
141.00	668.0
143.10	710.0
144.90	113.0
147.90	247.0
154.90	241.0
171.80	450.0
174.00	54400.0
175.00	4134.0
176.00	51728.0
177.10	3456.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.10	578.0
37.00	3282.0
38.00	2591.0
39.10	1264.0
39.90	109.0
44.00	975.0
45.00	513.0
46.20	110.0
46.90	564.0
47.90	474.0
49.00	2985.0
50.00	13111.0
51.00	4041.0
52.00	173.0
55.00	249.0
56.00	1183.0
57.00	1591.0
59.90	830.0
61.00	3060.0
62.00	3087.0
63.00	2680.0
64.10	334.0
64.90	312.0
68.00	7052.0
69.00	7789.0
70.00	758.0
72.00	328.0
73.00	3236.0
74.00	11902.0
75.10	37192.0
76.00	3137.0
76.90	320.0
77.90	288.0
78.90	2207.0
80.00	774.0
80.90	2299.0
81.90	535.0
86.20	216.0
87.00	2758.0
88.00	3034.0
90.90	272.0
92.00	2127.0
93.00	2662.0
94.10	8565.0
95.10	71648.0
96.10	4970.0
97.00	122.0
104.00	347.0
104.80	105.0
106.00	250.0
115.90	343.0
117.00	412.0
118.00	312.0
119.00	428.0
127.90	272.0
129.80	282.0
141.00	715.0
143.10	775.0
144.80	110.0
147.90	242.0
155.00	241.0
157.00	113.0
171.90	573.0
174.00	54864.0
175.00	4244.0
176.00	53608.0
177.00	3299.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.10	555.0
37.00	2757.0
38.00	2134.0
39.10	1023.0
44.00	979.0
45.00	453.0
47.00	561.0
47.90	428.0
49.00	2478.0
50.00	11851.0
51.00	3624.0
52.00	173.0
55.10	251.0
56.00	1149.0
56.90	1480.0
59.90	631.0
61.00	2864.0
62.00	2925.0
63.00	2336.0
64.10	236.0
65.10	327.0
68.00	6257.0
69.00	6953.0
70.00	777.0
72.00	354.0
73.00	3031.0
74.00	10364.0
75.00	33480.0
76.00	2700.0
76.90	233.0
77.90	255.0
78.80	1931.0
80.00	749.0
81.00	2084.0
81.80	446.0
86.20	255.0
87.00	2830.0
88.00	2809.0
90.90	238.0
92.00	1880.0
93.00	2509.0
94.10	7586.0
95.10	65856.0
96.00	4366.0
104.10	262.0
104.90	134.0
106.00	263.0
115.90	295.0
116.90	375.0
118.00	250.0
119.00	444.0
127.90	216.0
129.80	277.0
141.00	688.0
141.90	125.0
143.10	732.0
144.80	121.0
147.90	186.0
155.10	174.0
157.00	121.0
172.00	666.0
174.00	50640.0
175.00	3926.0
176.00	50544.0
177.00	2875.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

Scan 2883 (10.610 min): VU038727.D
BFB52

m/z	Abundance
40.00	208.0
44.00	792.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52