

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061021\
 Data File : VU044146.D
 Acq On : 10 Jun 2021 11:28
 Operator : SY/MD
 Sample : M2626-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :


Quant Time: Jun 11 01:18:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060921W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 10 05:11:37 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.382	168	143143	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.256	114	286617	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.423	117	299943	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.819	152	143271	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.710	65	128285	56.356	ug/l	0.00
Spiked Amount 50.000			Recovery	=	112.720%	
35) Dibromofluoromethane	5.298	113	100199	50.256	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.520%	
50) Toluene-d8	7.906	98	394719	51.550	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.100%	
62) 4-Bromofluorobenzene	10.639	95	152696	49.761	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.520%	
Target Compounds					Qvalue	
3) Chloromethane	1.523	50	751	Below Cal		93
5) Bromomethane	1.838	94	613	0.617 ug/l		91
6) Chloroethane	1.906	64	167	Below Cal	#	42
10) Methyl Iodide	2.732	142	953	0.468 ug/l	#	82
11) Tert butyl alcohol	3.195	59	3817	6.233 ug/l	#	73
13) Acrolein	2.498	56	291	Below Cal	#	71
16) Acetone	2.633	43	11123	7.385 ug/l		99
17) Carbon Disulfide	2.797	76	1231	0.218 ug/l	#	75
18) Methyl Acetate	2.961	43	1363	0.465 ug/l	#	89
20) Methylene Chloride	3.054	84	13784	5.656 ug/l		97
25) 2-Butanone	4.716	43	2600	1.368 ug/l		98
29) Tetrahydrofuran	5.063	42	881	0.853 ug/l	#	66
31) Cyclohexane	5.382	56	3194	0.994 ug/l	#	1
36) 1,1-Dichloropropene	5.382	75	13067	4.098 ug/l	#	50
38) Carbon Tetrachloride	5.382	117	15369	5.339 ug/l	#	17
43) Isopropyl Acetate	5.922	43	18491	3.413 ug/l		98
45) 1,2-Dichloropropane	7.047	63	1645	0.641 ug/l	#	43
48) Methyl methacrylate	6.903	41	6241	2.367 ug/l	#	11
49) 1,4-Dioxane	7.047	88	193	2.799 ug/l	#	1
51) 4-Methyl-2-Pentanone	7.800	43	6503	1.658 ug/l		99
54) cis-1,3-Dichloropropene	7.745	75	30733	7.997 ug/l	#	63
57) 1,3-Dichloropropane	8.732	76	20913	5.011 ug/l	#	43
59) 2-Hexanone	8.732	43	276719	88.425 ug/l	#	49
74) N-amyl acetate	10.324	43	1645	0.382 ug/l	#	87
76) 1,2,3-Trichloropropane	10.639	75	77437	16.121 ug/l	#	47
81) trans-1,4-Dichloro-2-b...	10.639	75	77437	58.437 ug/l	#	13
89) n-Butylbenzene	12.217	91	1881	0.206 ug/l		97
93) 1,2,4-Trichlorobenzene	13.848	180	1839	0.614 ug/l		95
94) Hexachlorobutadiene	14.028	225	381	0.237 ug/l		86
95) Naphthalene	14.095	128	10465	3.816 ug/l		97
96) 1,2,3-Trichlorobenzene	14.336	180	1987	0.684 ug/l		97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jun 11 01:18:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060921W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 10 05:11:37 2021
Response via : Initial Calibration




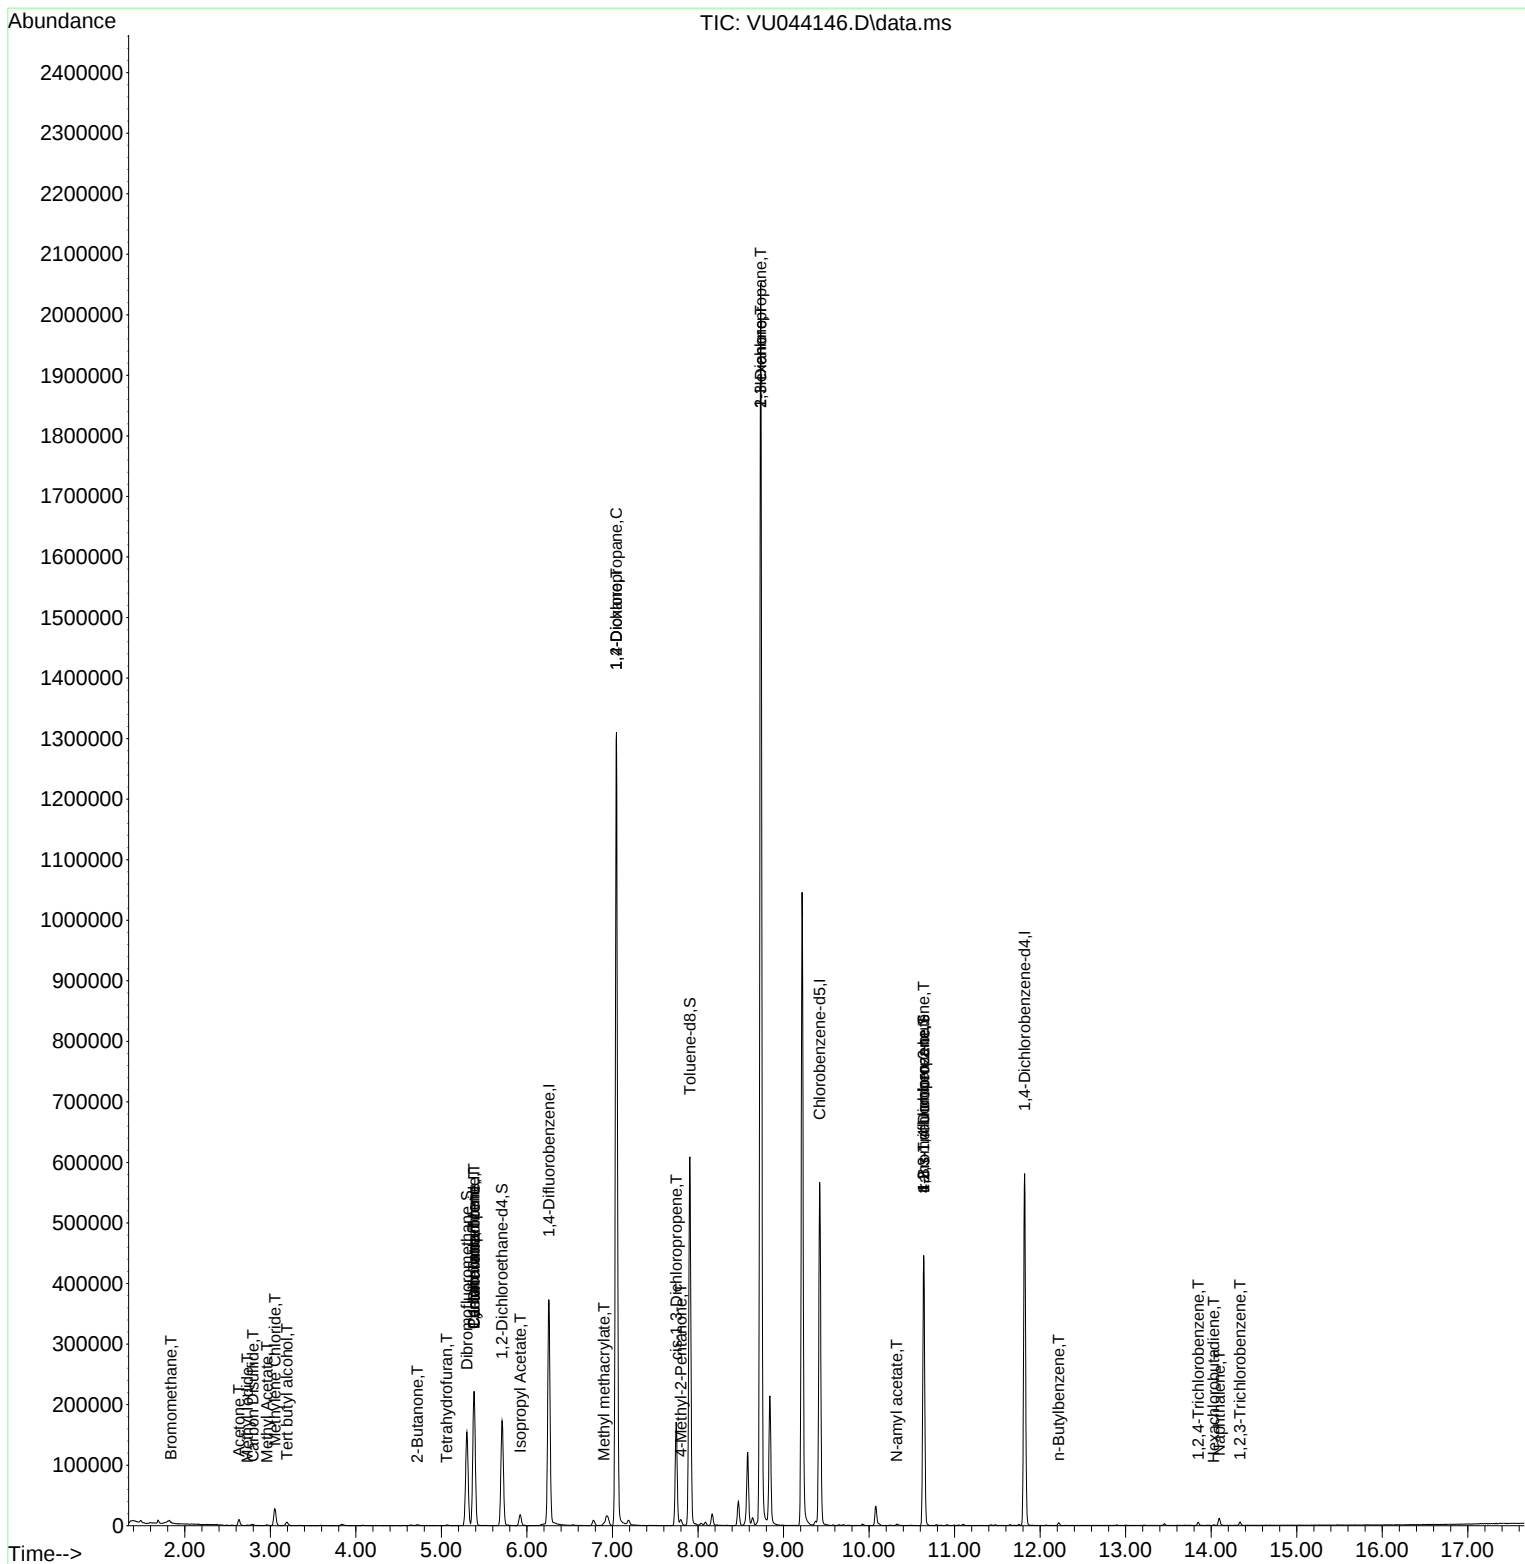


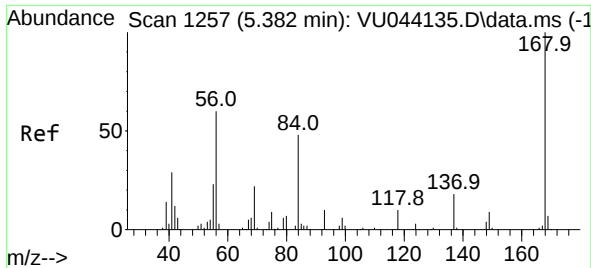

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion:168 Resp: 143143
Ion Ratio Lower Upper
168 100
99 65.2 51.3 76.9

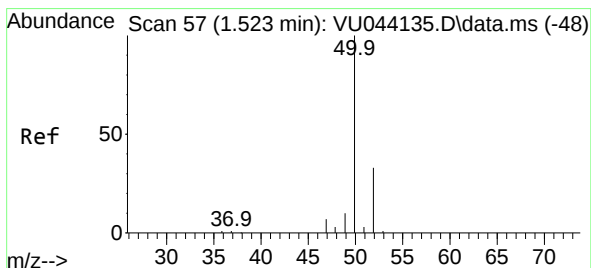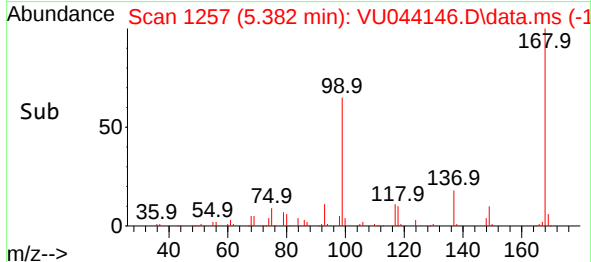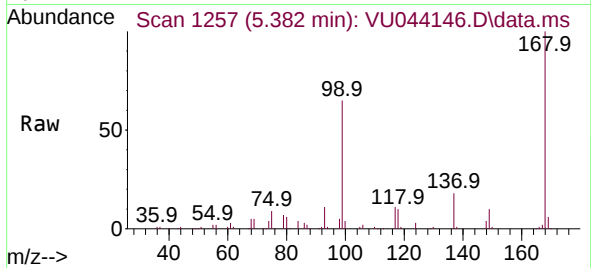

#3
Chloromethane
Concen: Below Cal
RT: 1.523 min Scan# 57
Delta R.T. 0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Tgt Ion: 50 Resp: 751
Ion Ratio Lower Upper
50 100
52 29.0 26.6 39.8


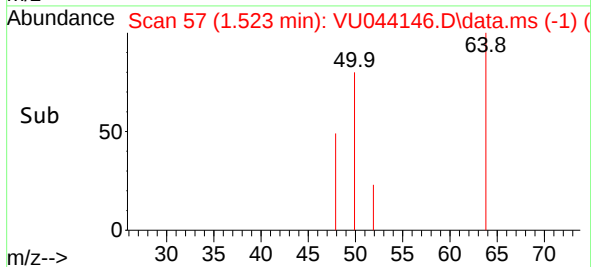

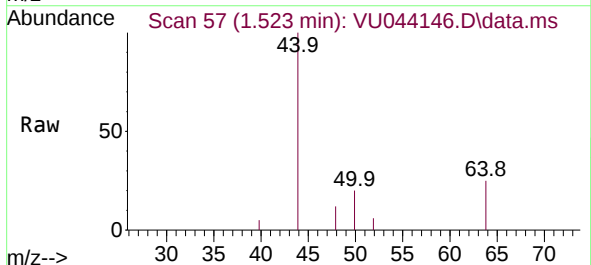




#5
Bromomethane
Concen: 0.617 ug/l
RT: 1.838 min Scan# 155
Delta R.T. -0.001 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 94 Resp: 613
Ion Ratio Lower Upper
94 100
96 83.9 74.1 111.1



#6
Chloroethane
Concen: Below Cal
RT: 1.906 min Scan# 176
Delta R.T. -0.019 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28


Tgt Ion: 64 Resp: 167
Ion Ratio Lower Upper
64 100
66 0.0 26.1 39.1#








#10
Methyl Iodide
Concen: 0.468 ug/l
RT: 2.732 min Scan# 433
Delta R.T. 0.006 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28


Instrument :
MSVOA_U
ClientSampled :





Tgt Ion:142 Resp: 953
Ion Ratio Lower Upper
142 100
127 38.0 37.0 55.6
141 0.0 11.6 17.4#

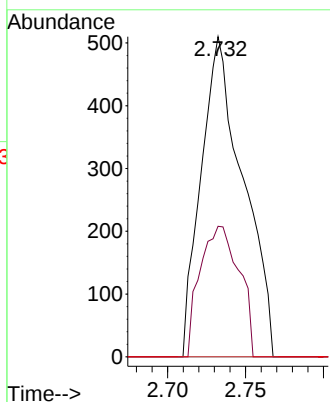


#11
Tert butyl alcohol
Concen: 6.233 ug/l
RT: 3.195 min Scan# 577
Delta R.T. -0.004 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28



Tgt Ion: 59 Resp: 3817
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#









#13
Acrolein
Concen: Below Cal
RT: 2.498 min Scan# 360
Delta R.T. 0.007 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 56 Resp: 291
Ion Ratio Lower Upper
56 100
55 45.0 55.1 82.7#

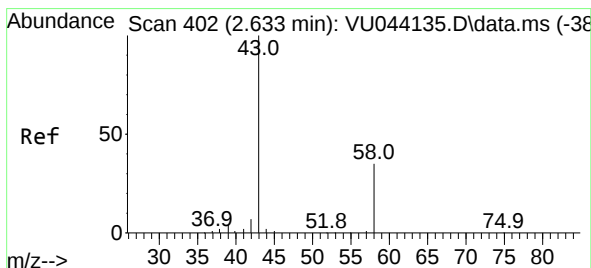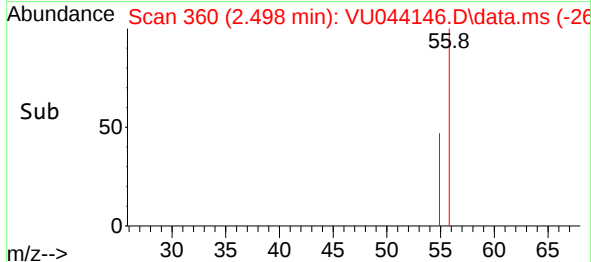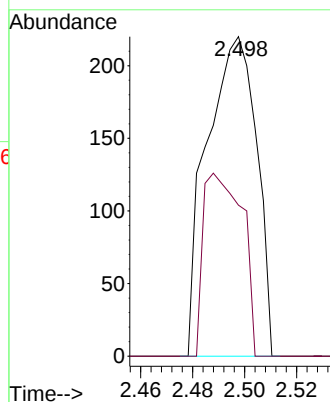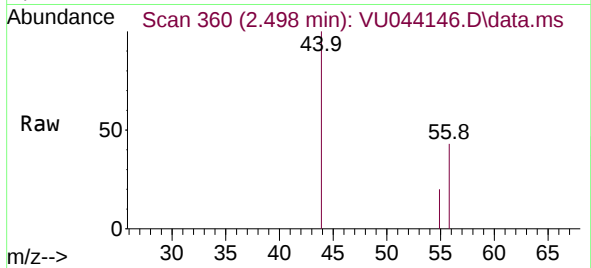

#16
Acetone
Concen: 7.385 ug/l
RT: 2.633 min Scan# 402
Delta R.T. -0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Tgt Ion: 43 Resp: 11123
Ion Ratio Lower Upper
43 100
58 35.6 28.0 42.0


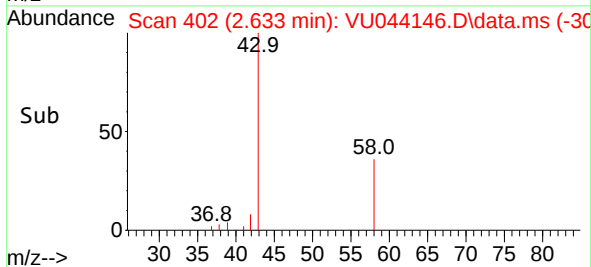

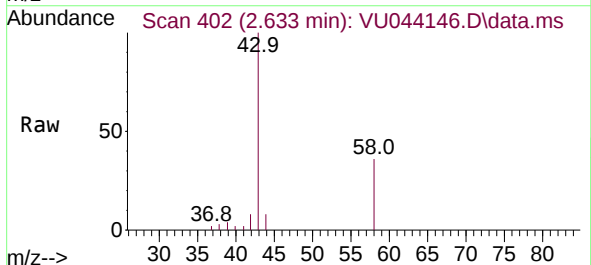




#17
Carbon Disulfide
Concen: 0.218 ug/l
RT: 2.797 min Scan# 453
Delta R.T. -0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 76 Resp: 1231
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

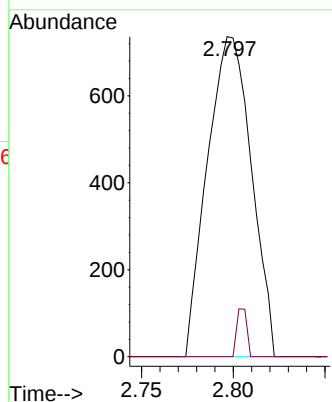

#18
Methyl Acetate
Concen: 0.465 ug/l
RT: 2.961 min Scan# 504
Delta R.T. 0.007 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Tgt Ion: 43 Resp: 1363
Ion Ratio Lower Upper
43 100
74 20.0 20.3 30.5#

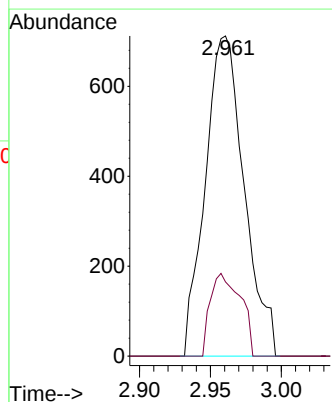



#20

Methylene Chloride

Concen: 5.656 ug/l

RT: 3.054 min Scan# 533

Delta R.T. 0.003 min

Lab File: VU044146.D

Acq: 10 Jun 2021 11:28

Instrument :
MSVOA_U
ClientSampled :

Tgt Ion: 84 Resp: 13784





Ion Ratio Lower Upper

84 100

49 126.4 96.9 145.3

51 39.9 31.0 46.6

86 64.5 51.0 76.6



#25

2-Butanone

Concen: 1.368 ug/l

RT: 4.716 min Scan# 1050

Delta R.T. 0.006 min

Lab File: VU044146.D




Acq: 10 Jun 2021 11:28


Tgt Ion: 43 Resp: 2600

Ion Ratio Lower Upper

43 100

72 26.9 22.6 33.8

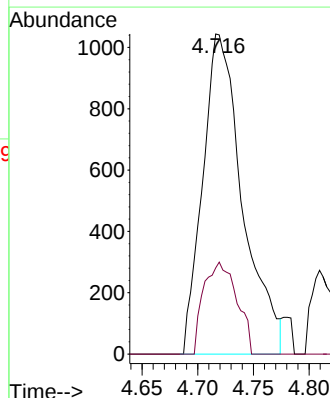



#29

Tetrahydrofuran

Concen: 0.853 ug/l

RT: 5.063 min Scan# 1158





Delta R.T. 0.006 min

Lab File: VU044146.D

Acq: 10 Jun 2021 11:28

Instrument :
MSVOA_U
ClientSampled :

Tgt Ion:	42	Resp:	881
Ion	Ratio	Lower	Upper
42	100		
72	24.9	38.6	57.8#
71	22.2	35.5	53.3#

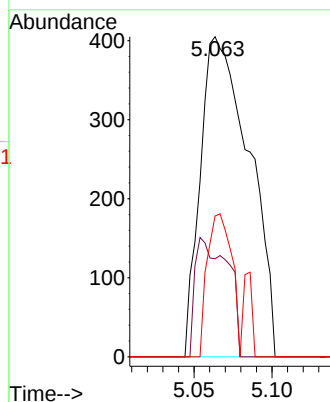

#31

Cyclohexane

Concen: 0.994 ug/l




RT: 5.382 min Scan# 1257


Delta R.T. -0.013 min

Lab File: VU044146.D

Acq: 10 Jun 2021 11:28

Tgt Ion:	56	Resp:	3194
Ion	Ratio	Lower	Upper
56	100		
69	194.5	25.5	38.3#
84	152.9	66.3	99.5#

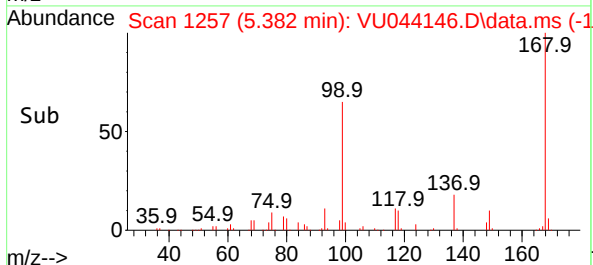







#33

1,2-Dichloroethane-d4
Concen: 56.356 ug/l
RT: 5.710 min Scan# 1359
Delta R.T. -0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Instrument :
MSVOA_U
ClientSampleId :




Tgt Ion: 65 Resp: 128285
Ion Ratio Lower Upper
65 100
67 53.6 0.0 106.6




#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.256 min Scan# 1529
Delta R.T. 0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Tgt Ion:114 Resp: 286617
Ion Ratio Lower Upper
114 100
63 22.8 0.0 45.8
88 17.0 0.0 34.0









#35
Dibromofluoromethane
Concen: 50.256 ug/l
RT: 5.298 min Scan# 1231
Delta R.T. 0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:	113	Resp:	100199
Ion	Ratio	Lower	Upper
113	100		
111	101.8	81.0	121.4
192	18.1	14.3	21.5



#36
1,1-Dichloropropene
Concen: 4.098 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.151 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28


Tgt Ion:	75	Resp:	13067
Ion	Ratio	Lower	Upper
75	100		
110	8.2	16.4	49.4#
77	0.0	24.7	37.1#








#38
Carbon Tetrachloride
Concen: 5.339 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.151 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Instrument :
MSVOA_U
ClientSampleId :







Tgt Ion:117 Resp: 15369
Ion Ratio Lower Upper
117 100
119 6.8 76.6 114.8#
121 0.0 24.6 36.8#

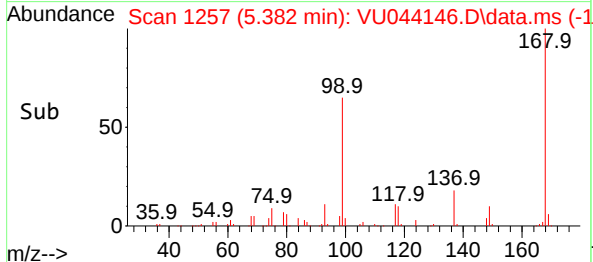

#43
Isopropyl Acetate
Concen: 3.413 ug/l
RT: 5.922 min Scan# 1425
Delta R.T. 0.003 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Tgt Ion: 43 Resp: 18491
Ion Ratio Lower Upper
43 100
61 22.5 17.8 26.8
87 12.6 11.1 16.7

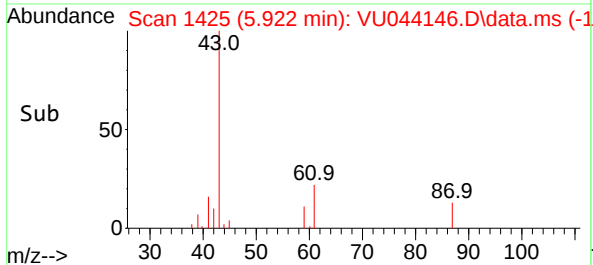







#45

1,2-Dichloropropane
Concen: 0.641 ug/l
RT: 7.047 min Scan# 1775
Delta R.T. 0.247 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Instrument :
MSVOA_U
ClientSampled :




Tgt Ion: 63 Resp: 1645
Ion Ratio Lower Upper
63 100
65 0.0 25.7 38.5#




#48

Methyl methacrylate
Concen: 2.367 ug/l
RT: 6.903 min Scan# 1730
Delta R.T. -0.064 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Tgt Ion: 41 Resp: 6241
Ion Ratio Lower Upper
41 100
69 0.0 74.0 111.0#
39 0.0 41.5 62.3#





#49

1,4-Dioxane

Concen: 2.799 ug/l

RT: 7.047 min Scan# 1775

Delta R.T. 0.077 min

Lab File: VU044146.D

Acq: 10 Jun 2021 11:28

Tgt Ion: 88 Resp: 193

Ion Ratio Lower Upper

88 100





43 606033.7 23.4 35.0#

58 3102.1 58.1 87.1#

Instrument :

MSVOA_U

ClientSampled :



#50

Toluene-d8

Concen: 51.550 ug/l

RT: 7.906 min Scan# 2042

Delta R.T. -0.000 min

Lab File: VU044146.D




Acq: 10 Jun 2021 11:28


Tgt Ion: 98 Resp: 394719

Ion Ratio Lower Upper

98 100

100 65.0 52.2 78.4









#51
4-Methyl-2-Pentanone
Concen: 1.658 ug/l
RT: 7.800 min Scan# 2009
Delta R.T. -0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 43 Resp: 6503
Ion Ratio Lower Upper
43 100
58 42.4 34.5 51.7

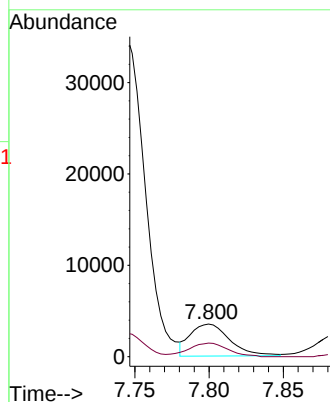

#54
cis-1,3-Dichloropropene
Concen: 7.997 ug/l
RT: 7.745 min Scan# 1992
Delta R.T. 0.132 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Tgt Ion: 75 Resp: 30733
Ion Ratio Lower Upper
75 100
77 0.7 25.9 38.9#
39 28.3 33.2 49.8#









#57

1,3-Dichloropropane
Concen: 5.011 ug/l
RT: 8.732 min Scan# 2299
Delta R.T. 0.151 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Instrument :
MSVOA_U
ClientSampled :




Tgt Ion: 76 Resp: 20913
Ion Ratio Lower Upper
76 100
78 0.3 25.9 38.9#

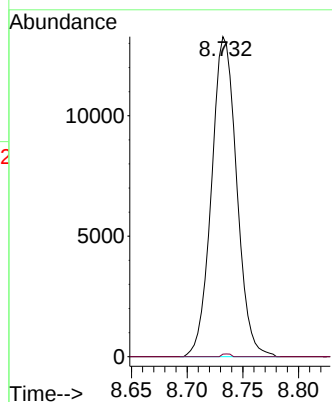


#59

2-Hexanone
Concen: 88.425 ug/l
RT: 8.732 min Scan# 2299
Delta R.T. 0.038 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Tgt Ion: 43 Resp: 276719
Ion Ratio Lower Upper
43 100
58 21.2 30.0 90.1#



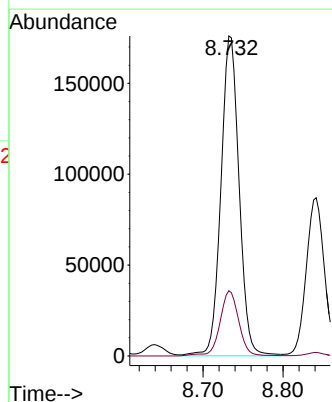





#62
4-Bromofluorobenzene
Concen: 49.761 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 95 Resp: 152696
Ion Ratio Lower Upper
95 100
174 69.9 0.0 144.4
176 67.6 0.0 138.0

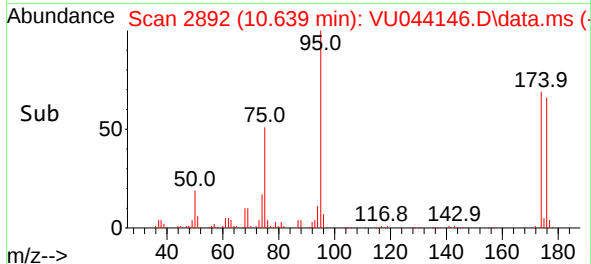

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.423 min Scan# 2514
Delta R.T. -0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Tgt Ion: 117 Resp: 299943
Ion Ratio Lower Upper
117 100
82 60.8 48.8 73.2
119 31.5 25.0 37.6


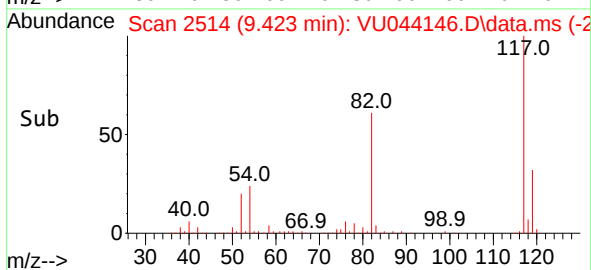

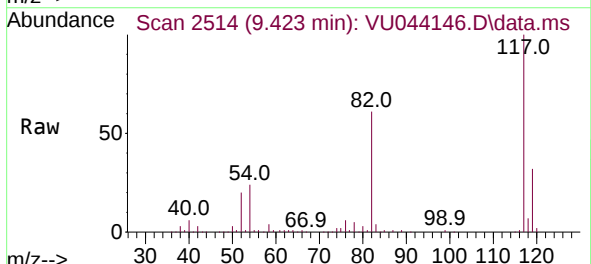


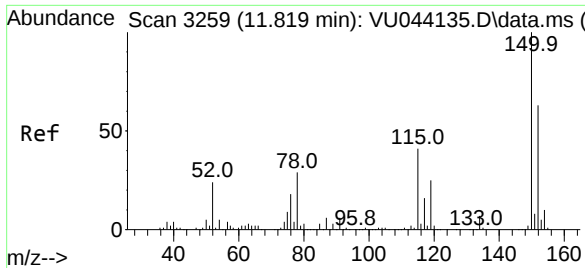

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.819 min Scan# 3259
Delta R.T. -0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion:152 Resp: 143271
Ion Ratio Lower Upper
152 100
115 63.5 43.8 131.3
150 157.0 0.0 350.6

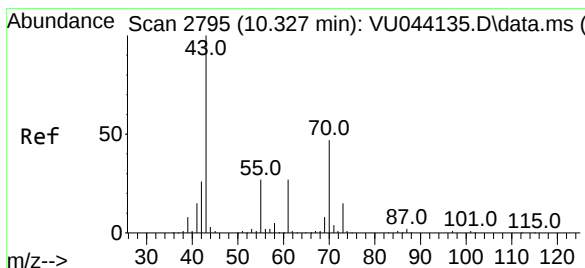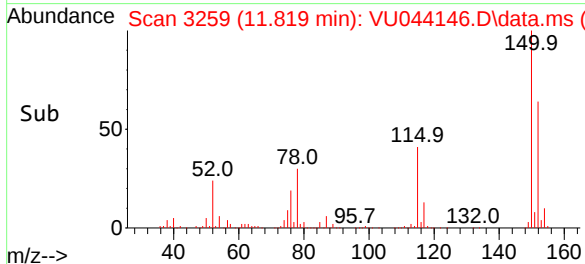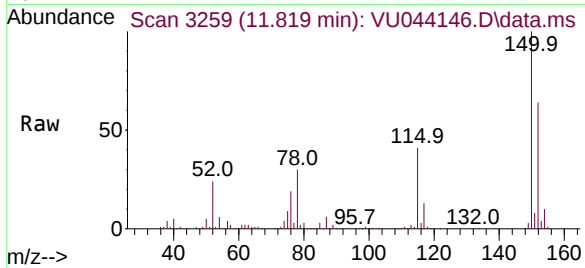

#74
N-ethyl acetate
Concen: 0.382 ug/l
RT: 10.324 min Scan# 2794
Delta R.T. -0.003 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Tgt Ion: 43 Resp: 1645
Ion Ratio Lower Upper
43 100
70 36.1 37.7 56.5#
55 25.7 22.4 33.6
61 19.3 21.5 32.3#


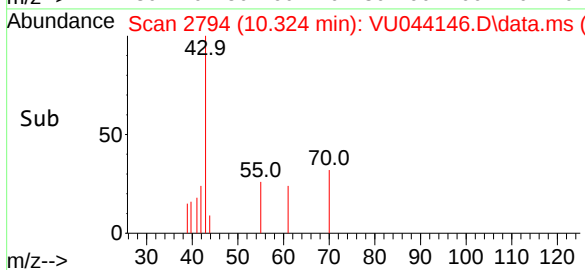

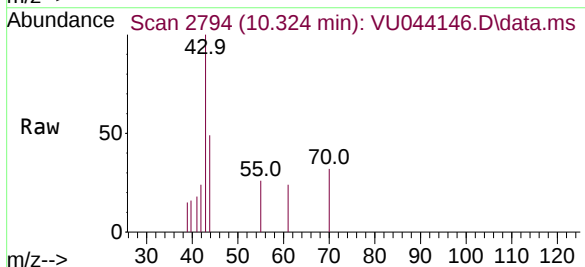




#76
1,2,3-Trichloropropane
Concen: 16.121 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.193 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 75 Resp: 77437
Ion Ratio Lower Upper
75 100
77 1.1 14.9 44.5#

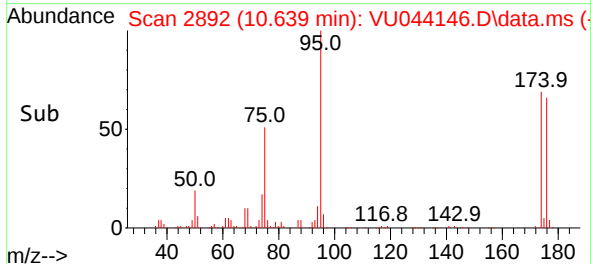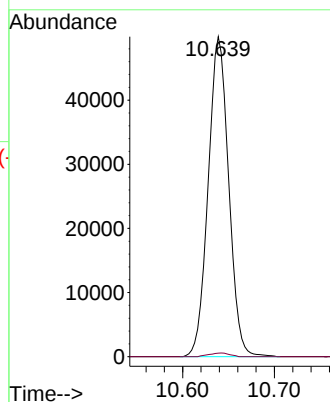

#81
trans-1,4-Dichloro-2-butene
Concen: 58.437 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.087 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

Tgt Ion: 75 Resp: 77437
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.2#
89 0.0 35.0 52.6#


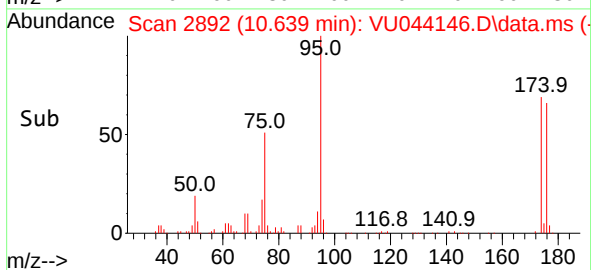

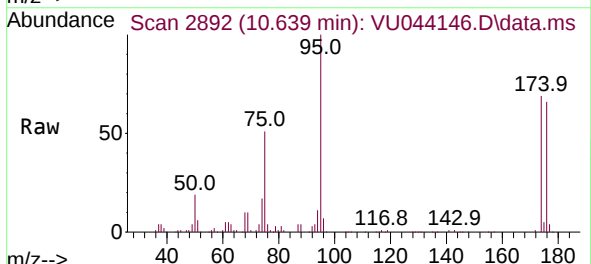




#89
n-Butylbenzene
Concen: 0.206 ug/l
RT: 12.217 min Scan# 3383
Delta R.T. 0.003 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28




Instrument :
MSVOA_U
ClientSampled :


Tgt Ion: 91	Resp: 1881
Ion Ratio	Lower Upper
91	100
92	56.5 27.1 81.2
134	22.1 11.9 35.5

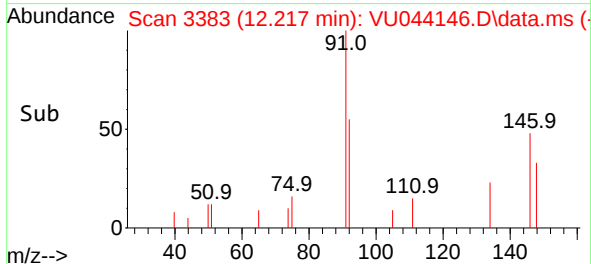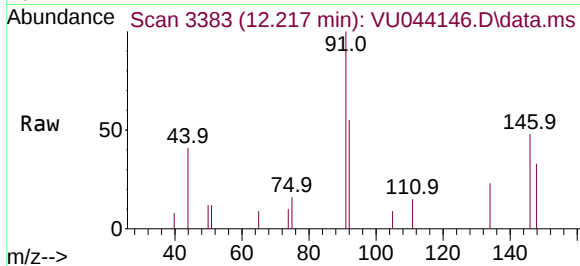

#93
1,2,4-Trichlorobenzene
Concen: 0.614 ug/l
RT: 13.848 min Scan# 3890
Delta R.T. -0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28


Tgt Ion: 180	Resp: 1839
Ion Ratio	Lower Upper
180	100
182	99.6 47.3 141.8
145	30.0 16.1 48.2

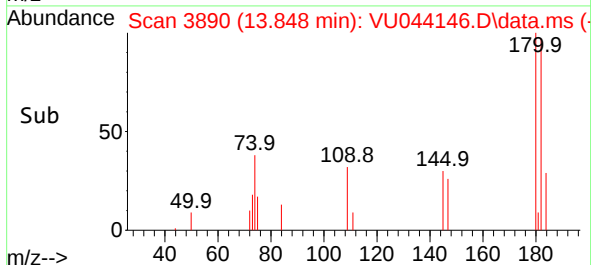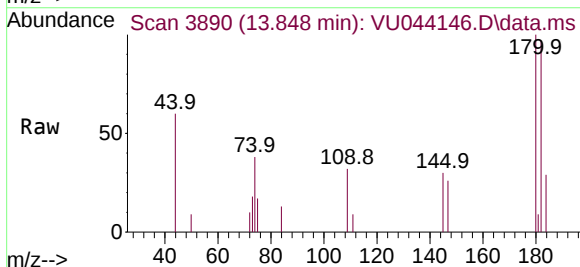






#94
Hexachlorobutadiene
Concen: 0.237 ug/l
RT: 14.028 min Scan# 3946
Delta R.T. -0.000 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28


Instrument :
MSVOA_U
ClientSampled :

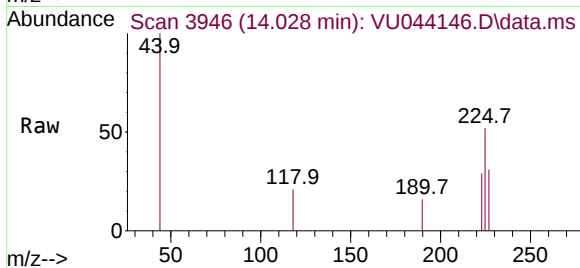



Tgt Ion:225 Resp: 381
Ion Ratio Lower Upper
225 100
223 43.8 31.2 93.6
227 60.4 32.2 96.6

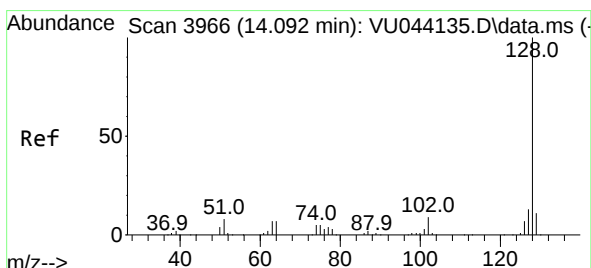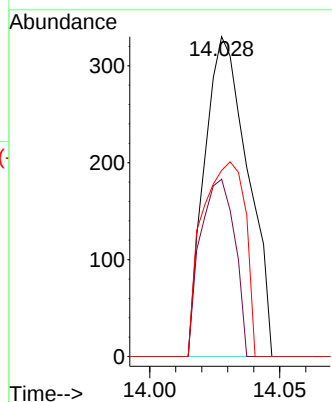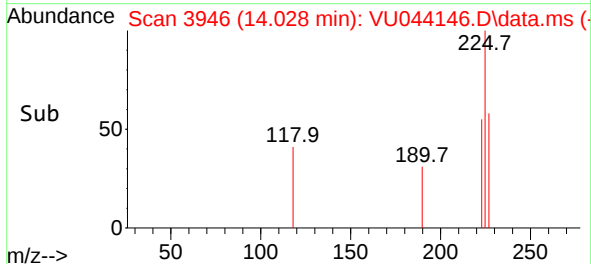


#95
Naphthalene
Concen: 3.816 ug/l
RT: 14.095 min Scan# 3967
Delta R.T. 0.003 min
Lab File: VU044146.D
Acq: 10 Jun 2021 11:28

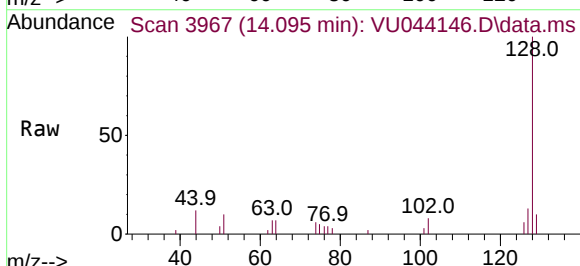

Tgt Ion:128 Resp: 10465
Ion Ratio Lower Upper
128 100
127 13.0 10.2 15.2
129 8.7 8.6 13.0

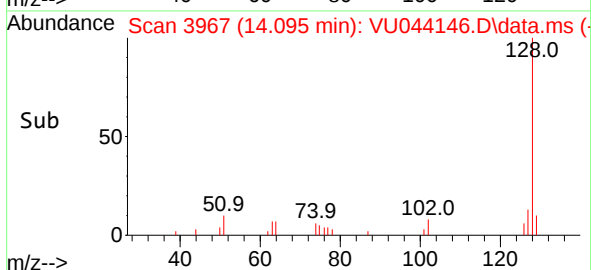

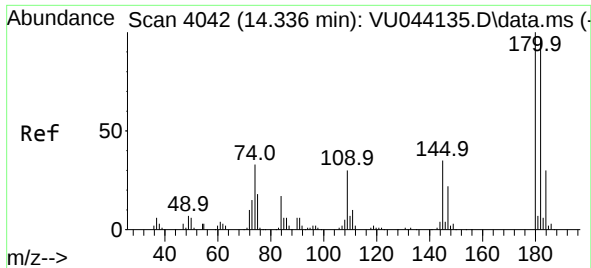

#96
 1,2,3-Trichlorobenzene
 Concen: 0.684 ug/l
 RT: 14.336 min Scan# 4042
 Delta R.T. 0.000 min
 Lab File: VU044146.D
 Acq: 10 Jun 2021 11:28

Instrument :
 MSVOA_U
 ClientSampleId :

Tgt Ion:180 Resp: 1987
 Ion Ratio Lower Upper
 180 100
 182 92.2 47.9 143.7
 145 34.7 17.2 51.6

