

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061021\
 Data File : VU044166.D
 Acq On : 10 Jun 2021 19:18
 Operator : SY/MD
 Sample : M2658-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 G-FLOOR-1

Quant Time: Jun 11 01:22:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060921W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 10 05:11:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.382	168	142260	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.256	114	280229	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.423	117	292771	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.819	152	151613	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.710	65	121611	53.756	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.520%	
35) Dibromofluoromethane	5.298	113	88958	45.635	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.260%	
50) Toluene-d8	7.906	98	371803	49.664	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.320%	
62) 4-Bromofluorobenzene	10.639	95	148818	49.603	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.200%	
Target Compounds						
						Qvalue
16) Acetone	2.633	43	47670	39.003	ug/l	96
20) Methylene Chloride	3.051	84	13274	5.443	ug/l	98
51) 4-Methyl-2-Pentanone	7.800	43	4893	1.276	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061021\
Data File : VU044166.D
Acq On : 10 Jun 2021 19:18
Operator : SY/MD
Sample : M2658-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
G-FLOOR-1

Quant Time: Jun 11 01:22:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060921W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 10 05:11:37 2021
Response via : Initial Calibration



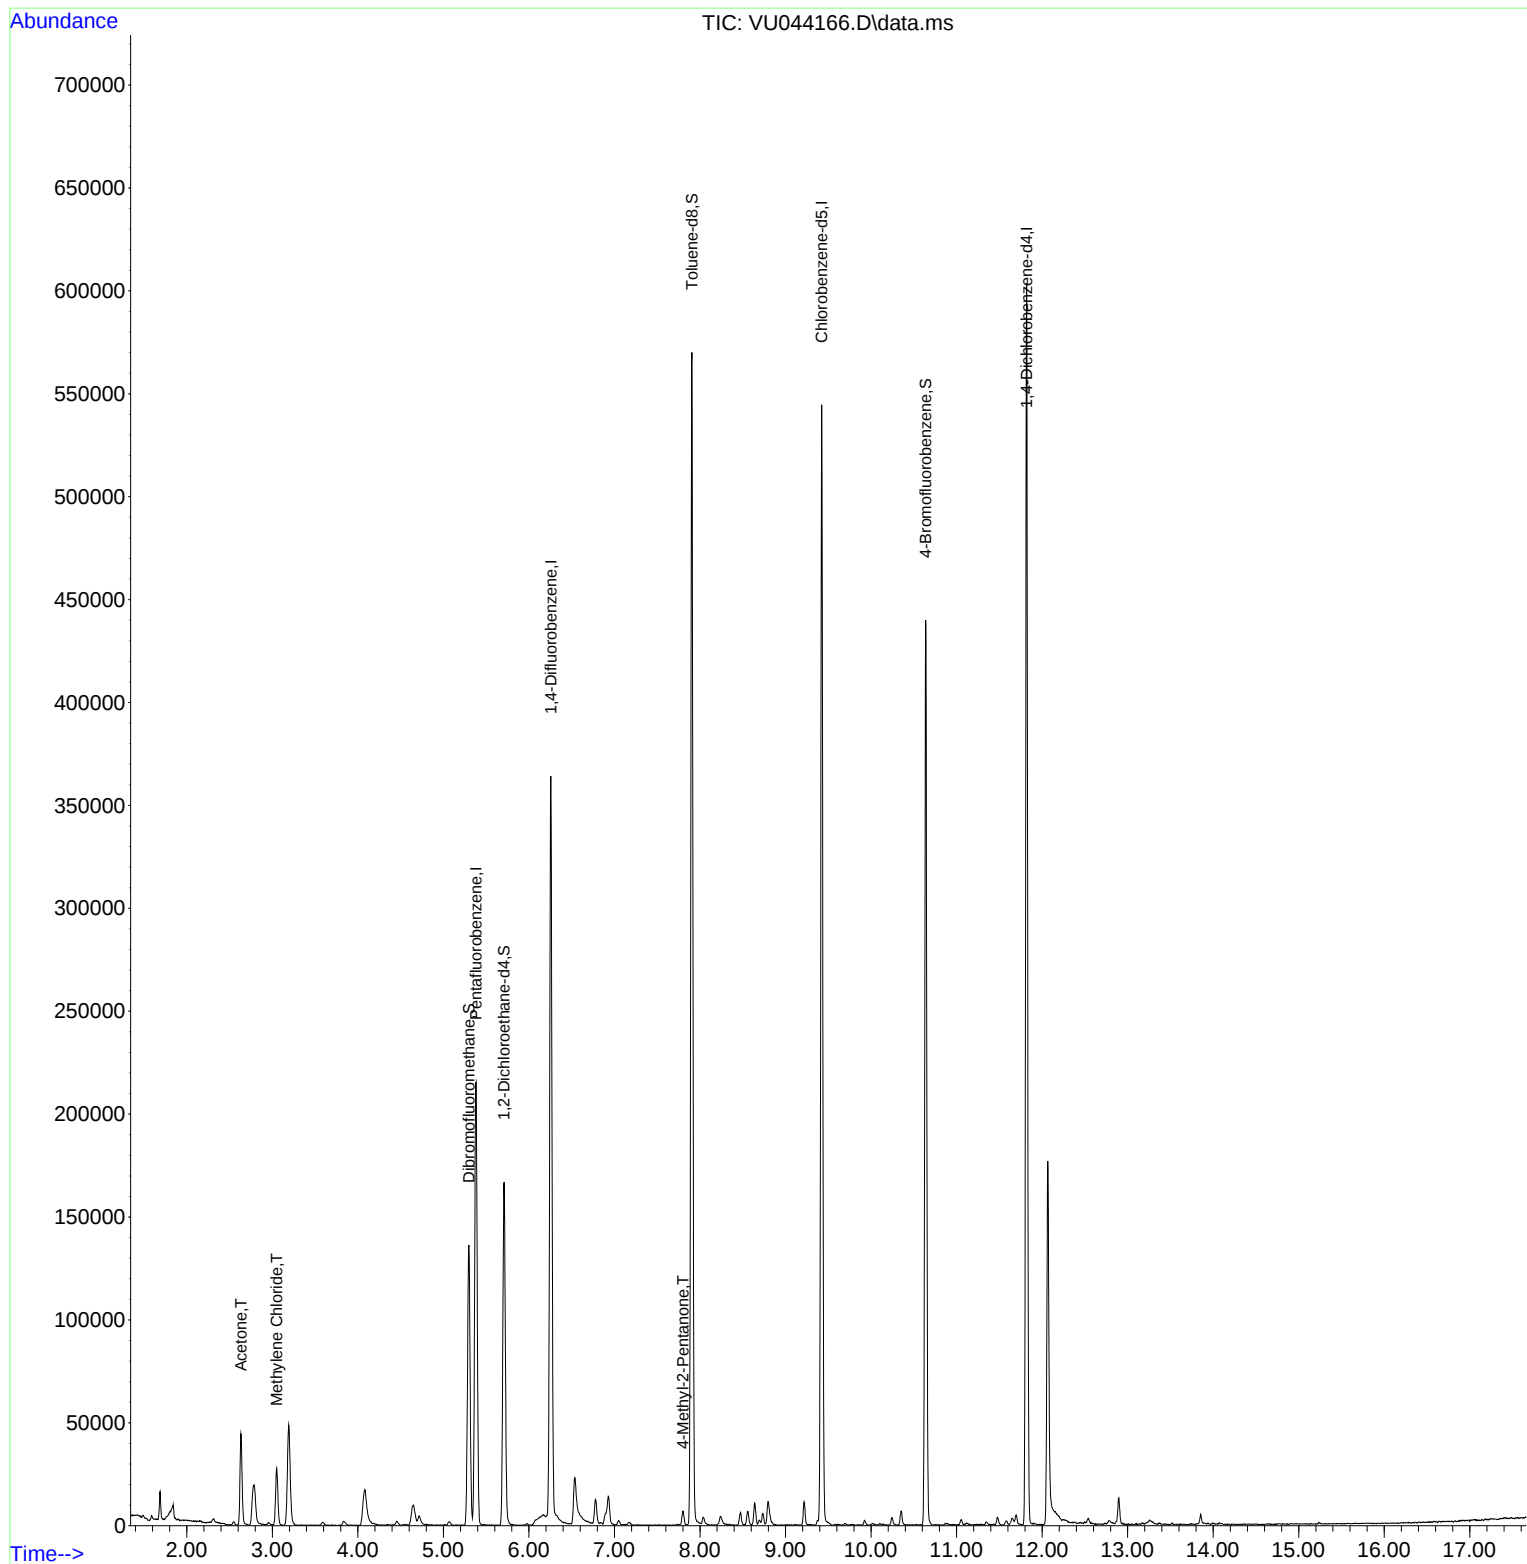


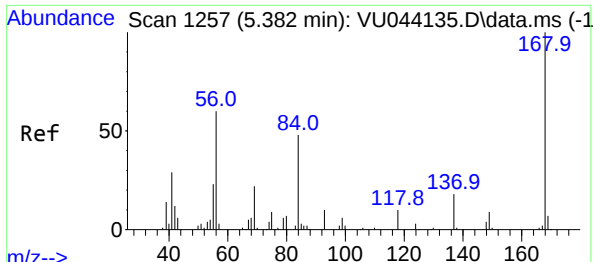

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.000 min
Lab File: VU044166.D
Acq: 10 Jun 2021 19:18




Instrument :
MSVOA_U
ClientSampled :
G-FLOOR-1


Tgt Ion:168 Resp: 142260
Ion Ratio Lower Upper
168 100
99 62.9 51.3 76.9

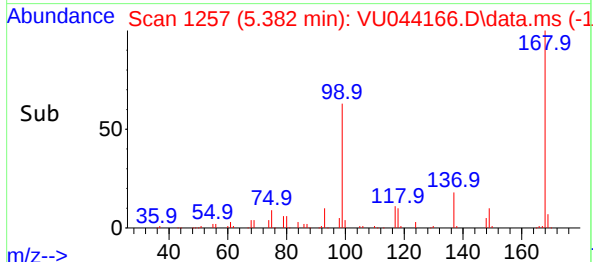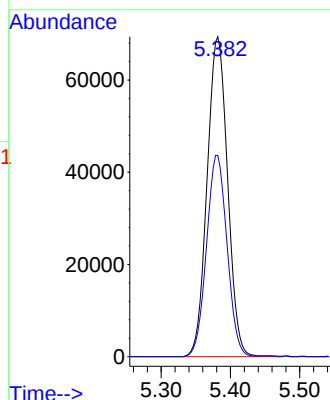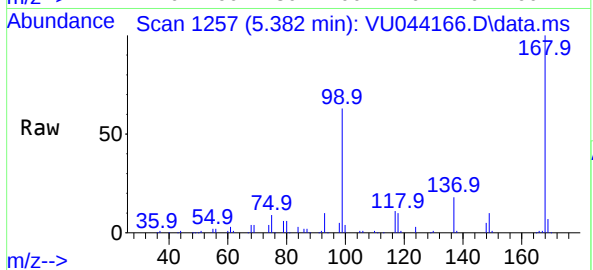

#16
Acetone
Concen: 39.003 ug/l
RT: 2.633 min Scan# 402
Delta R.T. -0.000 min
Lab File: VU044166.D
Acq: 10 Jun 2021 19:18

Tgt Ion: 43 Resp: 47670
Ion Ratio Lower Upper
43 100
58 37.0 28.0 42.0

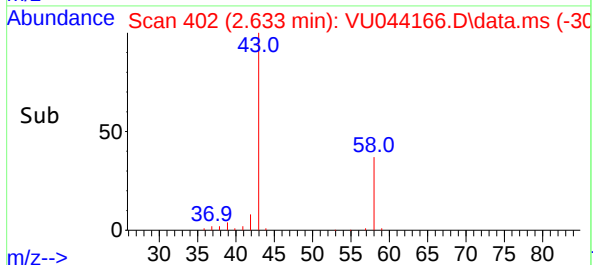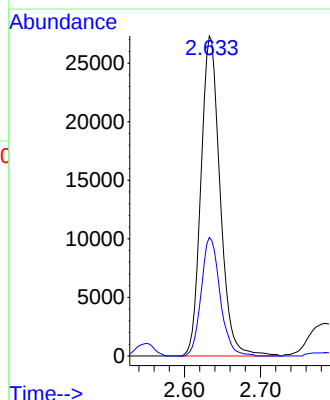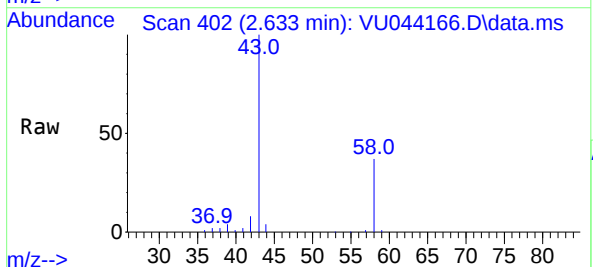




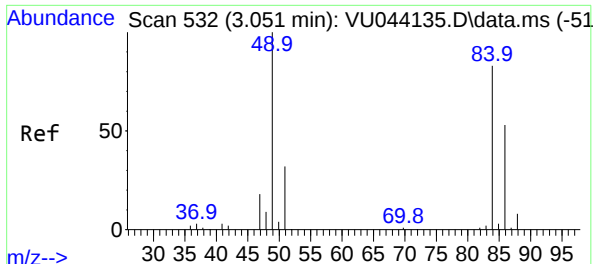


#20
Methylene Chloride
Concen: 5.443 ug/l
RT: 3.051 min Scan# 532
Delta R.T. -0.000 min
Lab File: VU044166.D
Acq: 10 Jun 2021 19:18

Instrument :
MSVOA_U
ClientSampled :
G-FLOOR-1

Tgt Ion: 84 Resp: 13274




Ion	Ratio	Lower	Upper
84	100		
49	117.8	96.9	145.3
51	37.6	31.0	46.6
86	63.8	51.0	76.6

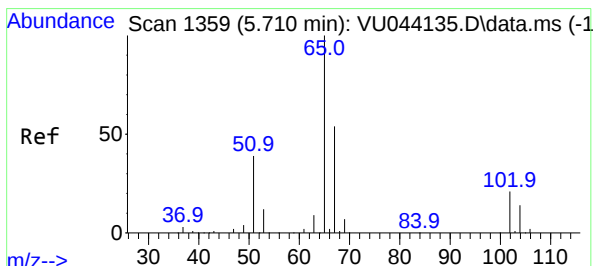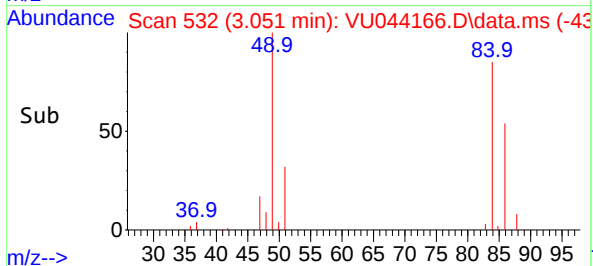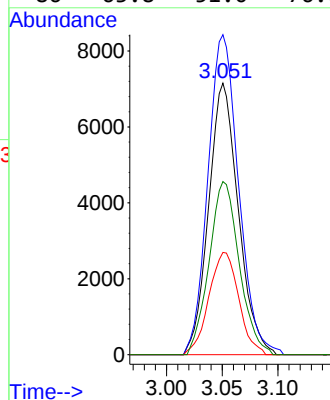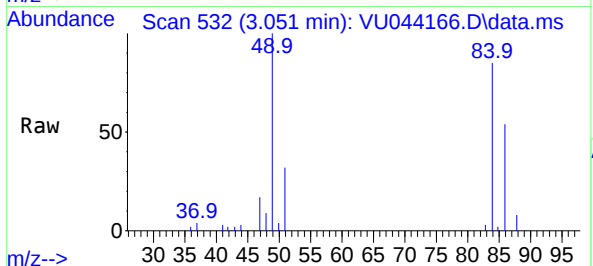


#33
1,2-Dichloroethane-d4
Concen: 53.756 ug/l
RT: 5.710 min Scan# 1359
Delta R.T. -0.000 min
Lab File: VU044166.D
Acq: 10 Jun 2021 19:18

Tgt Ion: 65 Resp: 121611

Ion	Ratio	Lower	Upper
65	100		
67	54.2	0.0	106.6


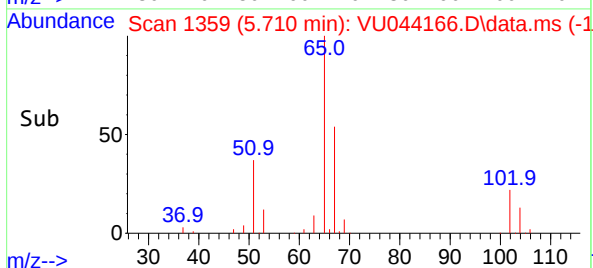
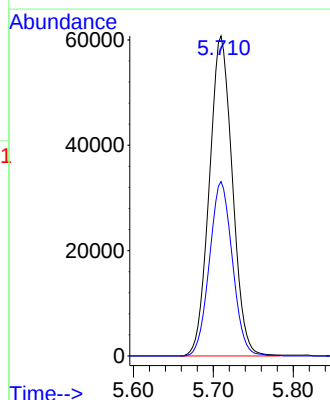
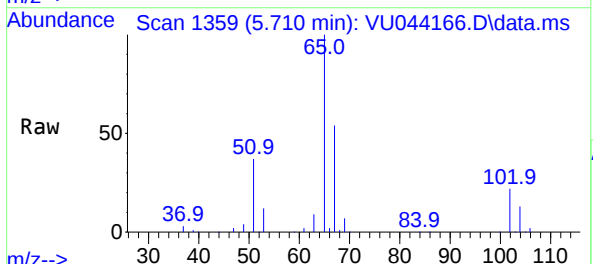


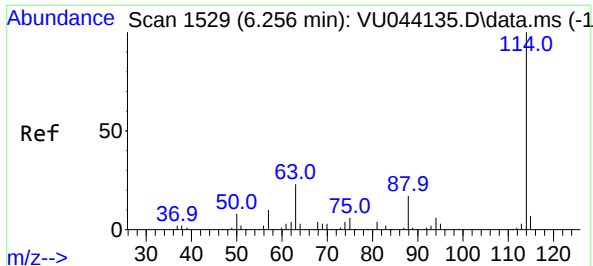

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.256 min Scan# 1529
Delta R.T. 0.000 min
Lab File: VU044166.D
Acq: 10 Jun 2021 19:18




Instrument :
MSVOA_U
ClientSampled :
G-FLOOR-1


Tgt Ion:114 Resp: 280229
Ion Ratio Lower Upper
114 100
63 22.4 0.0 45.8
88 17.4 0.0 34.0

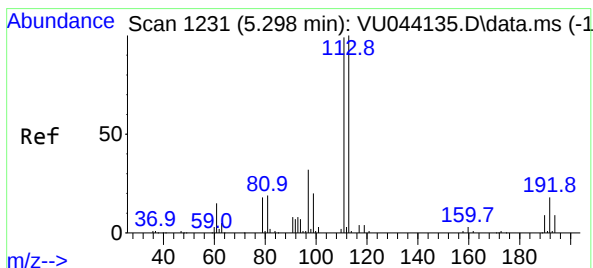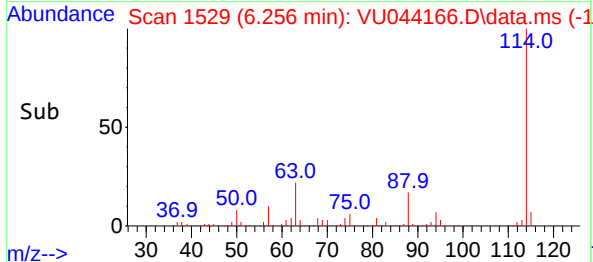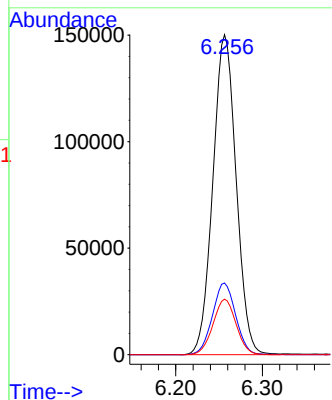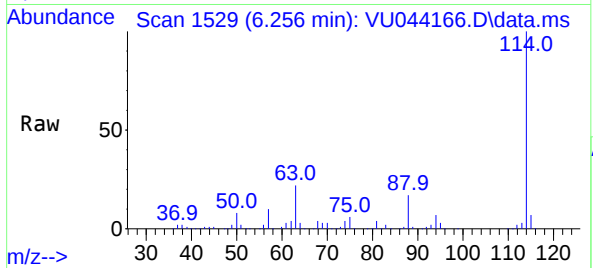

#35
Dibromofluoromethane
Concen: 45.635 ug/l
RT: 5.298 min Scan# 1231
Delta R.T. 0.000 min
Lab File: VU044166.D
Acq: 10 Jun 2021 19:18

Tgt Ion:113 Resp: 88958
Ion Ratio Lower Upper
113 100
111 102.2 81.0 121.4
192 18.3 14.3 21.5


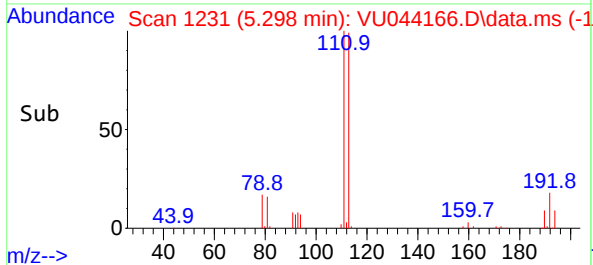
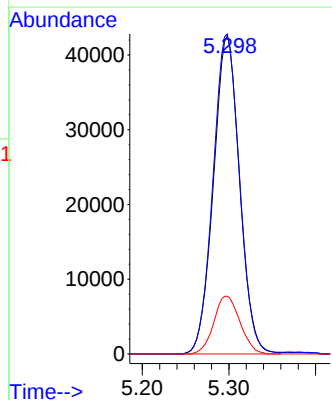
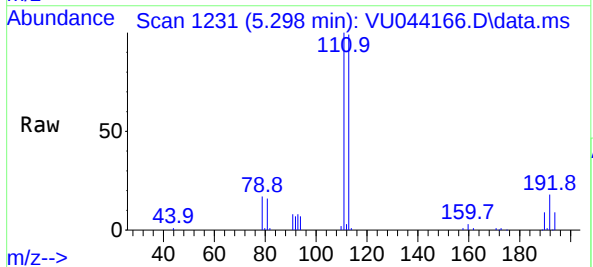


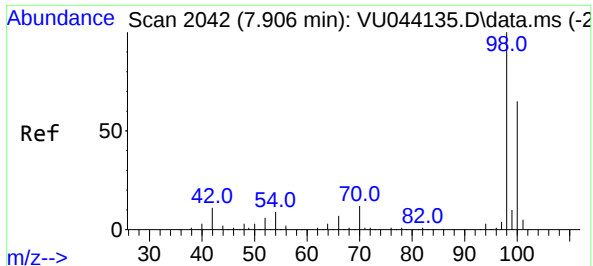

#50
Toluene-d8
Concen: 49.664 ug/l
RT: 7.906 min Scan# 2042
Delta R.T. -0.000 min
Lab File: VU044166.D
Acq: 10 Jun 2021 19:18




Instrument :
MSVOA_U
ClientSampled :
G-FLOOR-1


Tgt Ion: 98 Resp: 371803
Ion Ratio Lower Upper
98 100
100 64.6 52.2 78.4

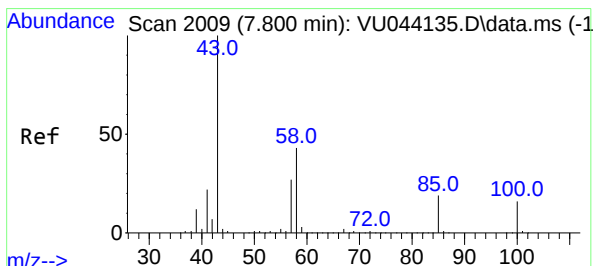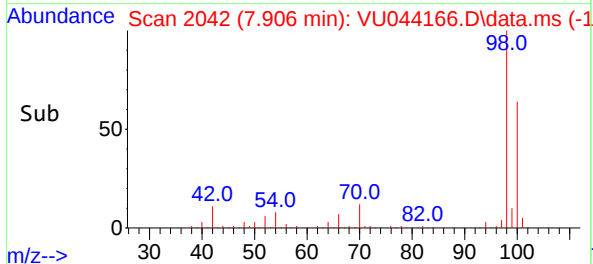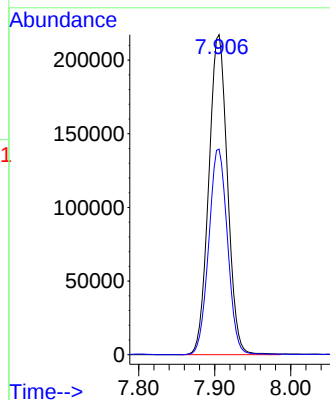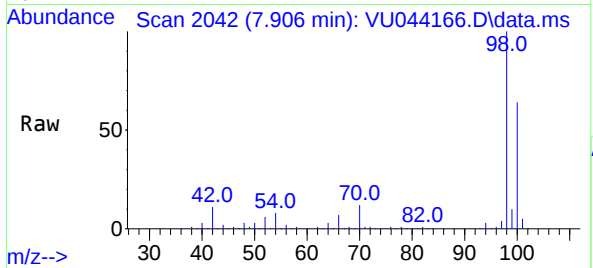

#51
4-Methyl-2-Pentanone
Concen: 1.276 ug/l
RT: 7.800 min Scan# 2009
Delta R.T. -0.000 min
Lab File: VU044166.D
Acq: 10 Jun 2021 19:18

Tgt Ion: 43 Resp: 4893
Ion Ratio Lower Upper
43 100
58 38.7 34.5 51.7


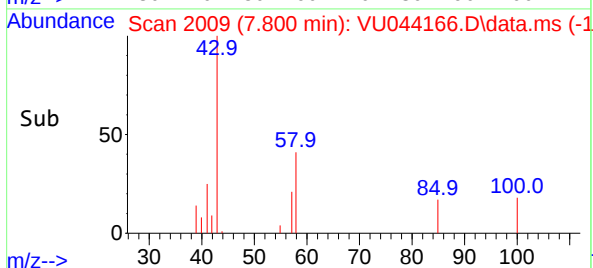
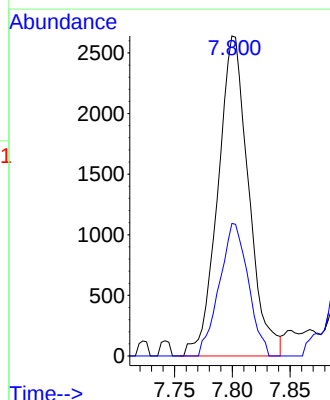
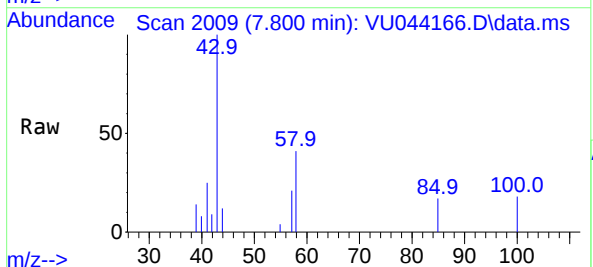


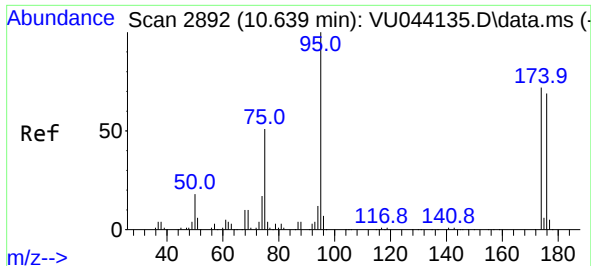

#62
4-Bromofluorobenzene
Concen: 49.603 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU044166.D
Acq: 10 Jun 2021 19:18




Instrument :
MSVOA_U
ClientSampleId :
G-FLOOR-1


Tgt Ion: 95 Resp: 148818
Ion Ratio Lower Upper
95 100
174 74.3 0.0 144.4
176 70.7 0.0 138.0

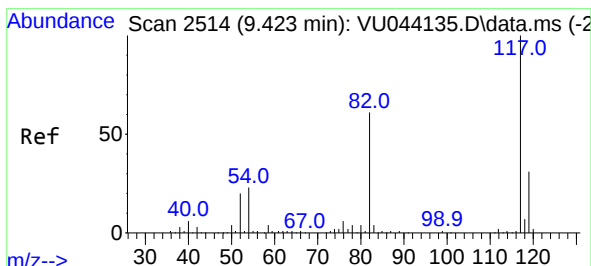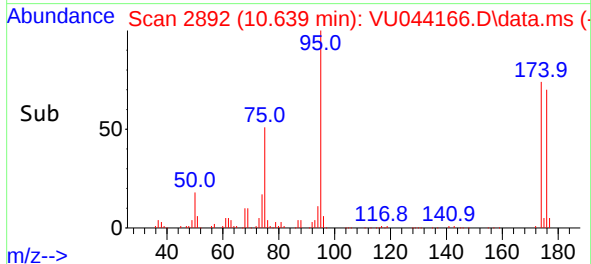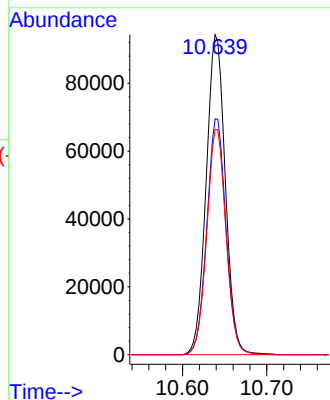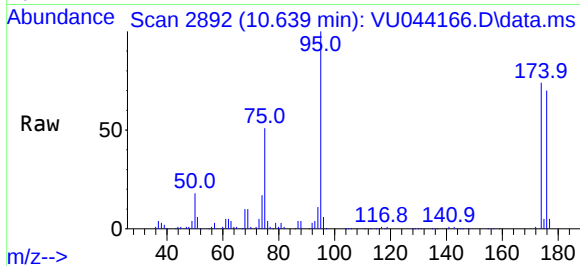

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.423 min Scan# 2514
Delta R.T. -0.000 min
Lab File: VU044166.D
Acq: 10 Jun 2021 19:18

Tgt Ion: 117 Resp: 292771
Ion Ratio Lower Upper
117 100
82 60.6 48.8 73.2
119 31.6 25.0 37.6

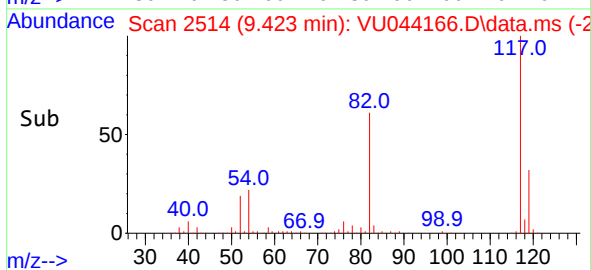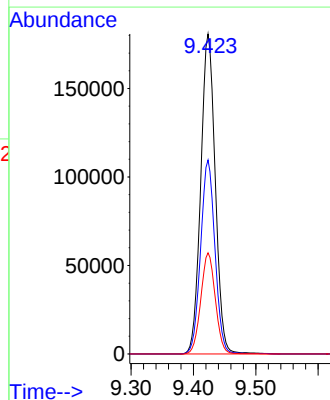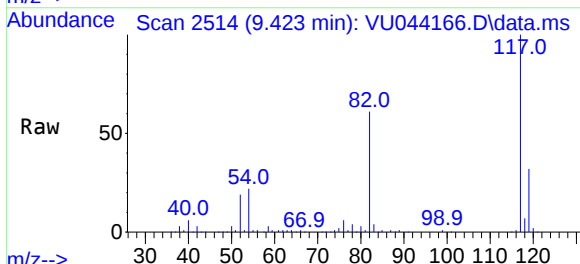

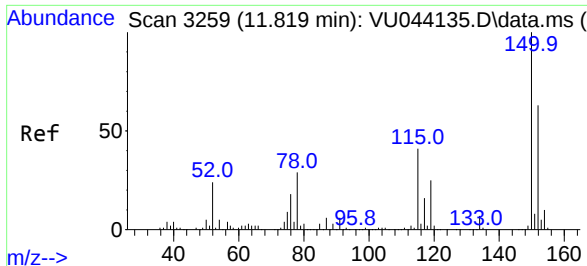

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 11.819 min Scan# 3259
 Delta R.T. -0.000 min
 Lab File: VU044166.D
 Acq: 10 Jun 2021 19:18

Instrument :
 MSVOA_U
 ClientSampleId :
 G-FLOOR-1

Tgt Ion:152 Resp: 151613
 Ion Ratio Lower Upper
 152 100
 115 61.8 43.8 131.3
 150 155.9 0.0 350.6

