
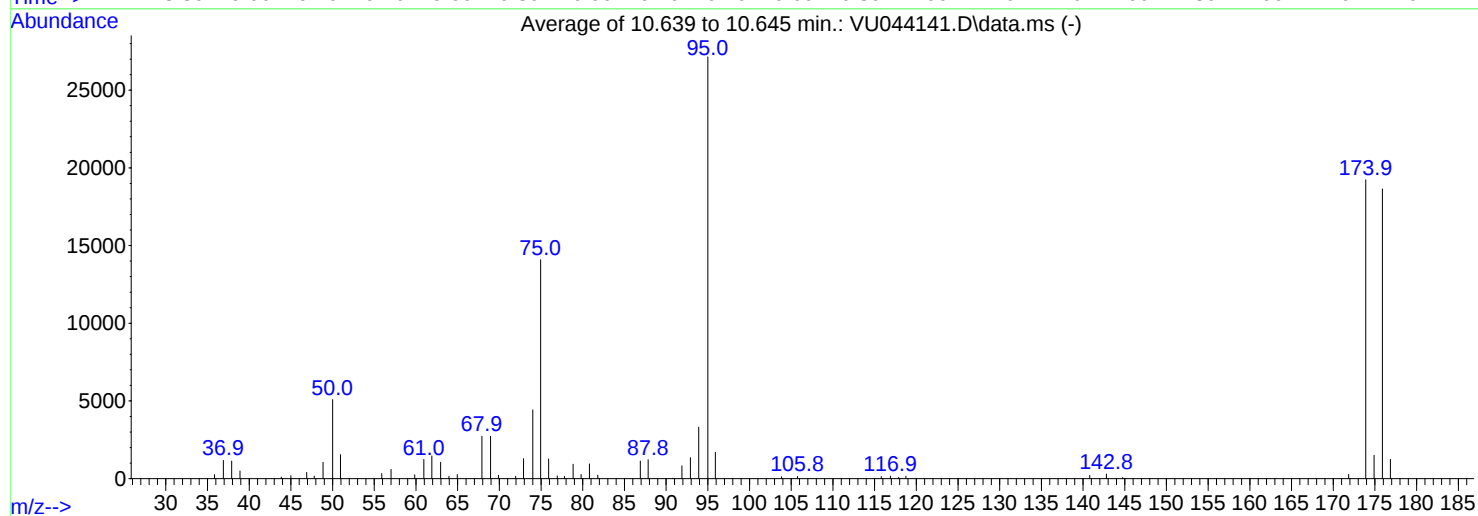


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061021\
 Data File : VU044141.D
 Acq On : 10 Jun 2021 09:04
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060921W.M
 Title : SW846 8260
 Last Update : Thu Jun 10 05:11:37 2021

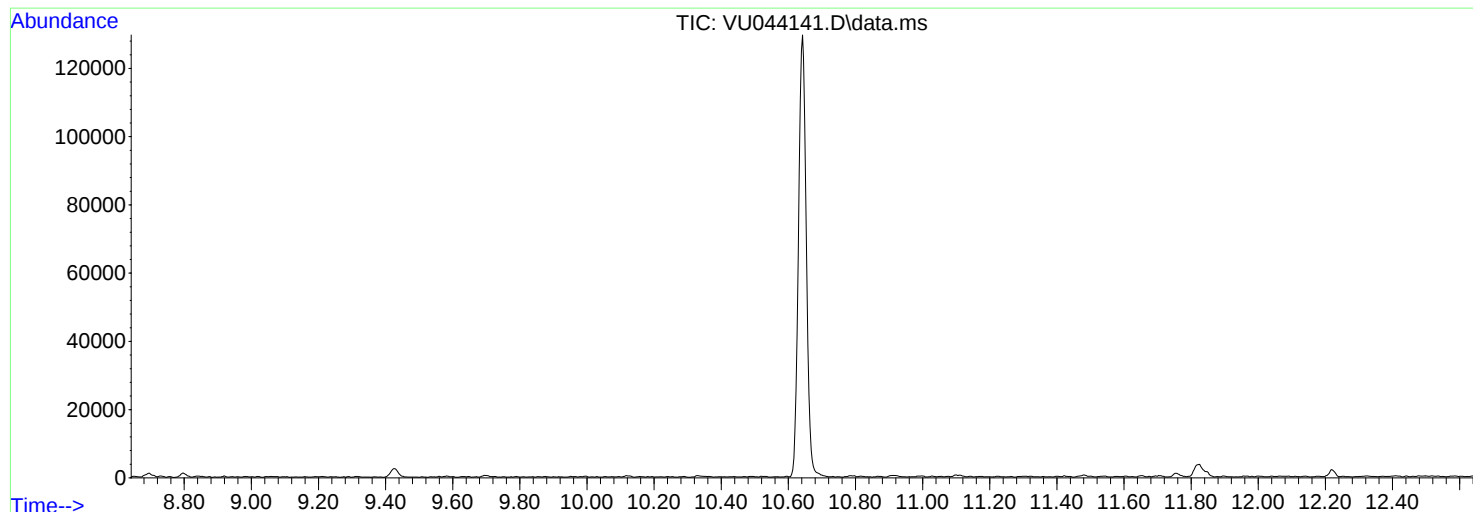

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	5084	PASS
75	95	30	60	51.9	14086	PASS
95	95	100	100	100.0	27144	PASS
96	95	5	9	6.2	1696	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.9	19235	PASS
175	174	5	9	7.8	1508	PASS
176	174	95	101	97.0	18651	PASS
177	176	5	9	6.7	1247	PASS