

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049010.D
 Acq On : 10 Jun 2022 20:35
 Operator : SY/MD
 Sample : N3254-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG5

Quant Time: Jun 11 02:45:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 10 22:44:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	284208	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	267233	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	99960	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	81172	46.361	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	92.720%	
7) Chloroethane-d5	1.900	69	61037	47.479	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	94.960%	
11) 1,1-Dichloroethene-d2	2.562	63	113511	34.358	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	68.720%	
21) 2-Butanone-d5	4.620	46	194674	101.413	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	101.410%	
24) Chloroform-d	5.060	84	182117	48.759	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.520%	
26) 1,2-Dichloroethane-d4	5.700	65	123030	50.843	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.680%	
32) Benzene-d6	5.726	84	335459	50.624	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.240%	
36) 1,2-Dichloropropane-d6	6.690	67	117606	52.794	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	105.580%	
41) Toluene-d8	7.899	98	281261	48.128	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	96.260%	
43) trans-1,3-Dichloroprop...	8.179	79	50904	48.572	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	97.140%	
47) 2-Hexanone-d5	8.632	63	112904	96.839	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	96.840%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	184717	49.646	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	99.300%	
66) 1,2-Dichlorobenzene-d4	12.195	152	95580	54.955	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	109.900%	
Target Compounds						
13) Acetone	2.626	43	7025	4.651	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049010.D
Acq On : 10 Jun 2022 20:35
Operator : SY/MD
Sample : N3254-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG5


Quant Time: Jun 11 02:45:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 10 22:44:31 2022
Response via : Initial Calibration

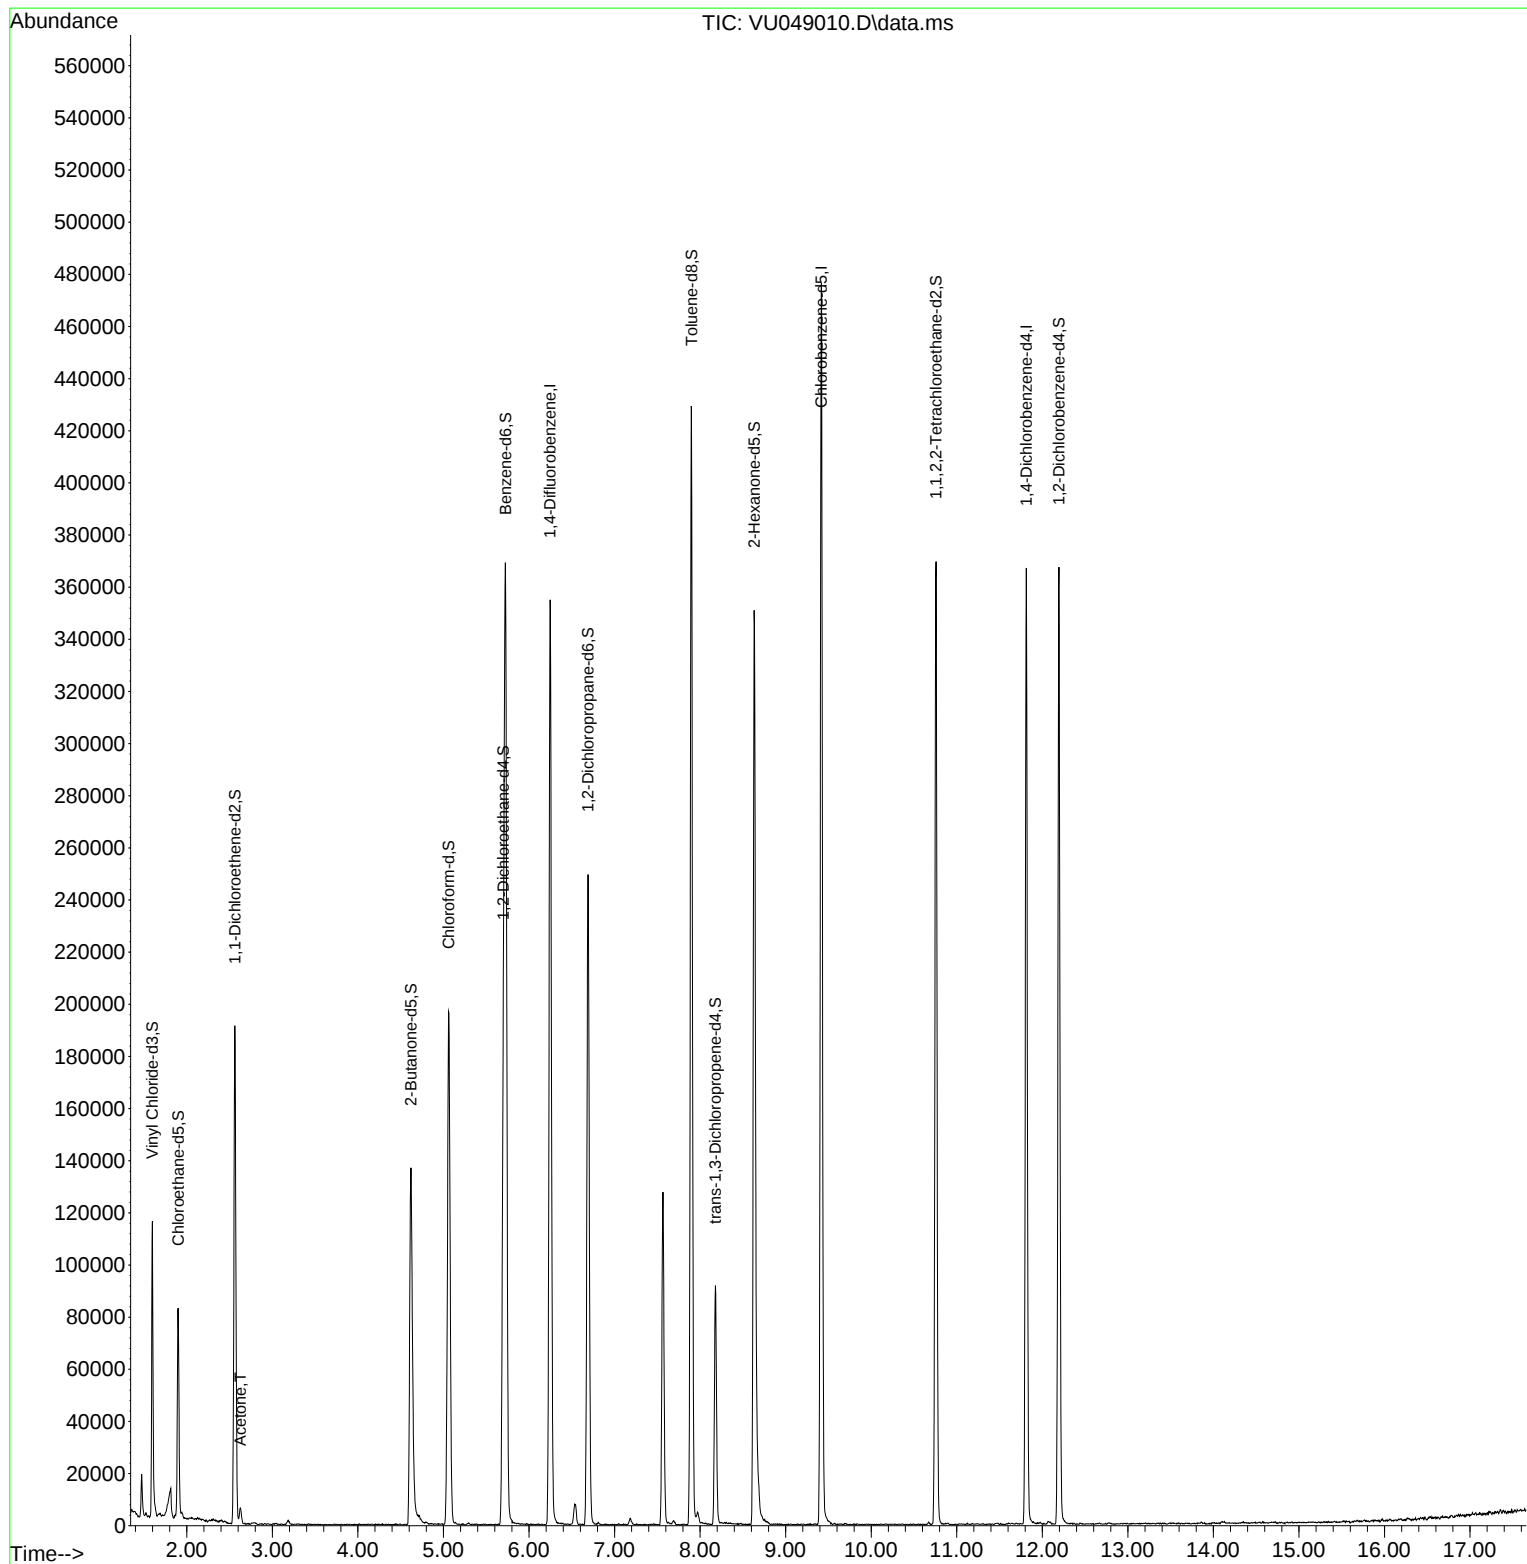

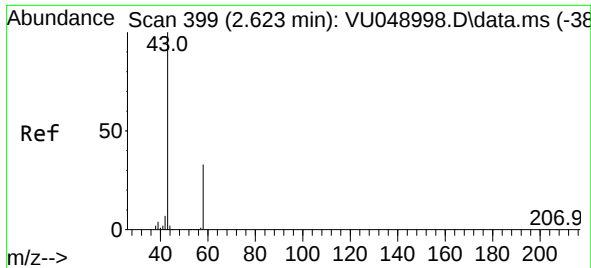

#13
 Acetone
 Concen: 4.651 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU049010.D
 Acq: 10 Jun 2022 20:35

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG5

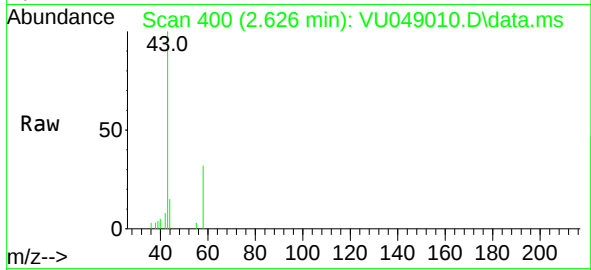

Tgt Ion: 43 Resp: 7025
 Ion Ratio Lower Upper
 43 100
 58 30.5 0.0 66.4

