

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049016.D
 Acq On : 10 Jun 2022 22:56
 Operator : SY/MD
 Sample : N3254-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DH4

Quant Time: Jun 11 02:46:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 10 22:44:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	279616	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	265735	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	115027	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	74663	43.344	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.680%
7) Chloroethane-d5	1.896	69	57723	45.639	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.280%
11) 1,1-Dichloroethene-d2	2.562	63	108245	33.302	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.600%
21) 2-Butanone-d5	4.620	46	176048	93.216	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.220%
24) Chloroform-d	5.063	84	170996	46.534	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.060%
26) 1,2-Dichloroethane-d4	5.700	65	119023	49.995	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.980%
32) Benzene-d6	5.726	84	320369	48.619	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.240%
36) 1,2-Dichloropropane-d6	6.690	67	108896	49.159	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.320%
41) Toluene-d8	7.896	98	264035	45.435	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.880%
43) trans-1,3-Dichloroprop...	8.179	79	46811	44.918	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.840%
47) 2-Hexanone-d5	8.632	63	103455	89.235	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.230%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	175298	47.380	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.760%
66) 1,2-Dichlorobenzene-d4	12.195	152	106642	53.284	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.560%
Target Compounds						
13) Acetone	2.623	43	3371	2.268	ug/L	Qvalue 79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049016.D
Acq On : 10 Jun 2022 22:56
Operator : SY/MD
Sample : N3254-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DH4


Quant Time: Jun 11 02:46:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 10 22:44:31 2022
Response via : Initial Calibration

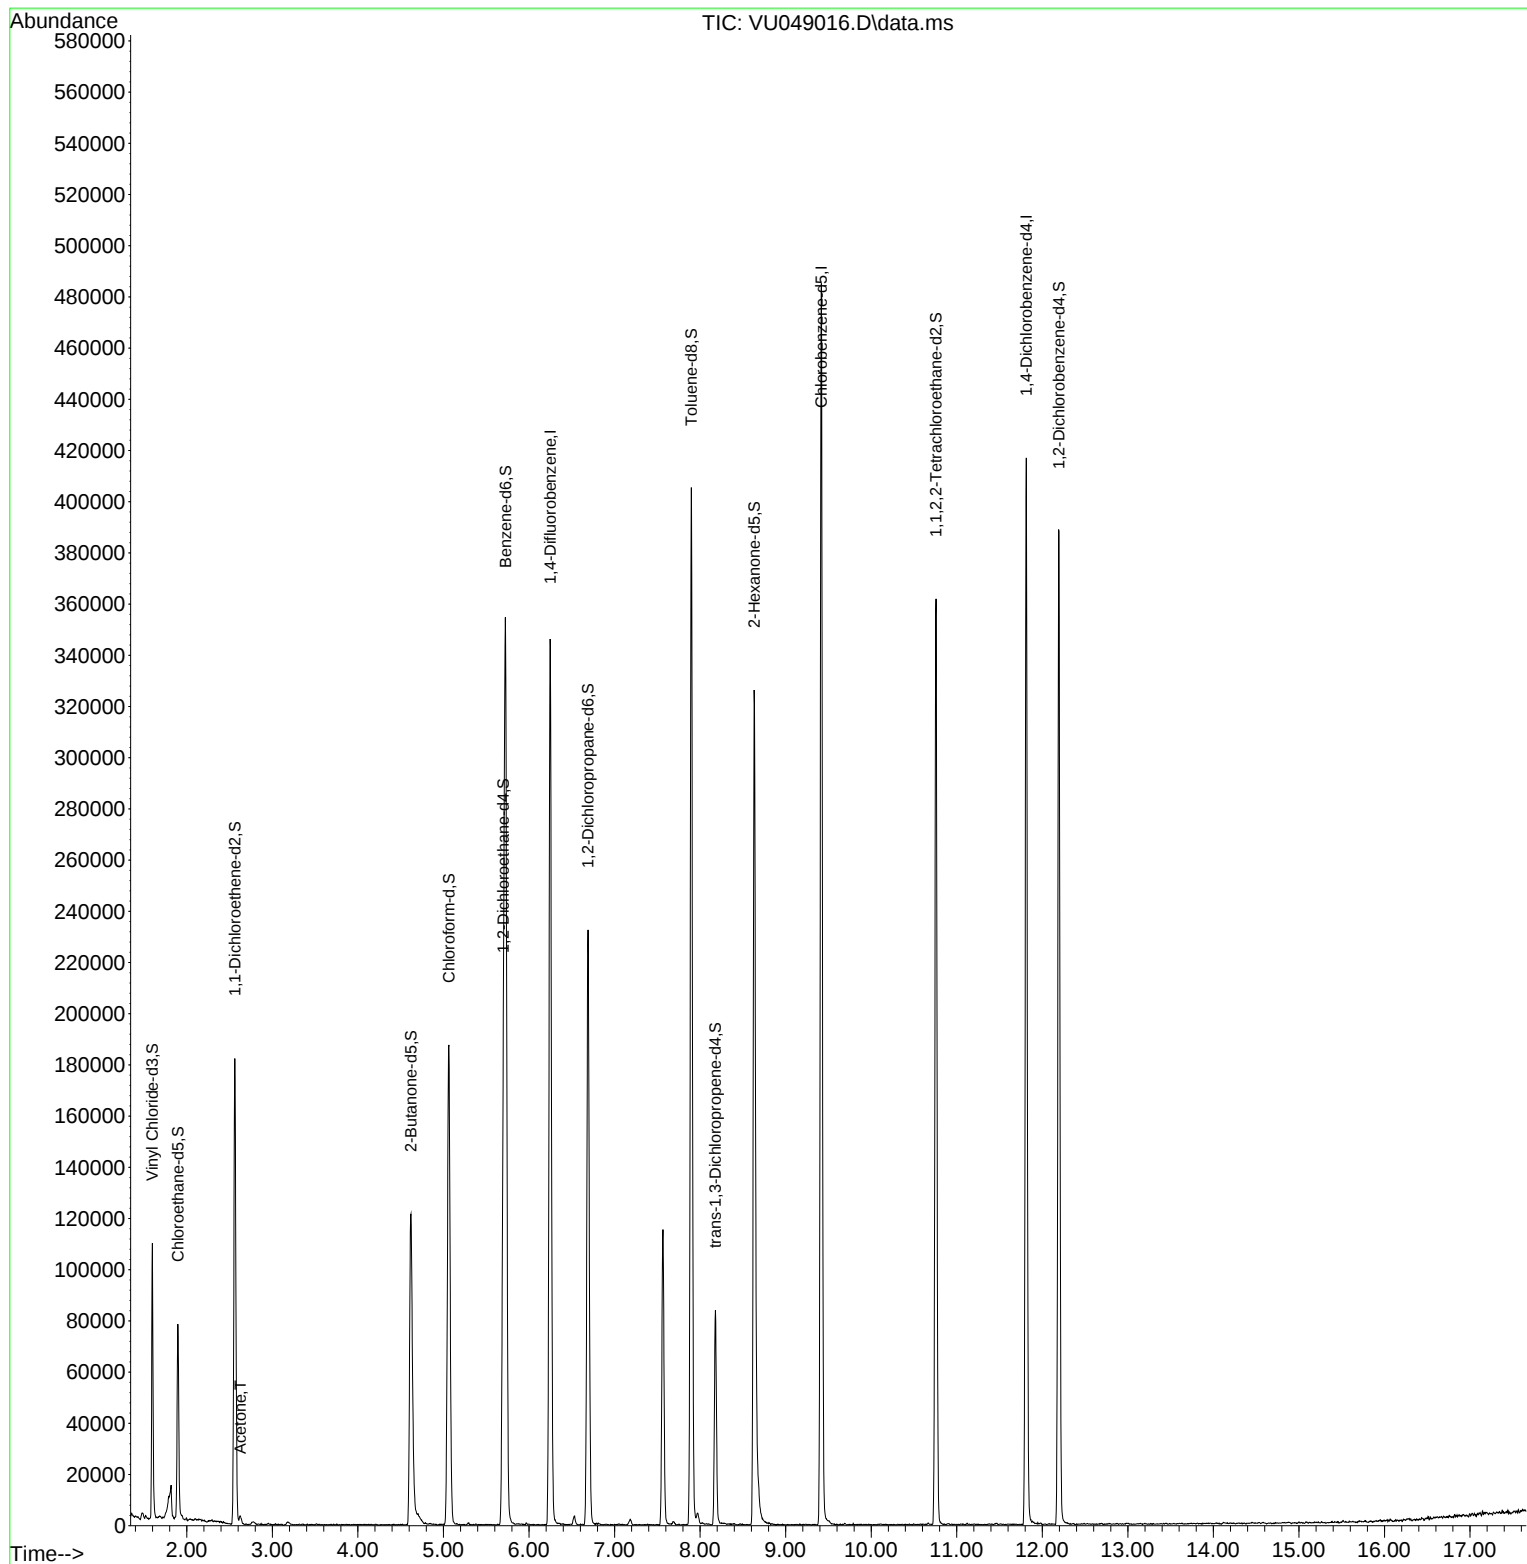

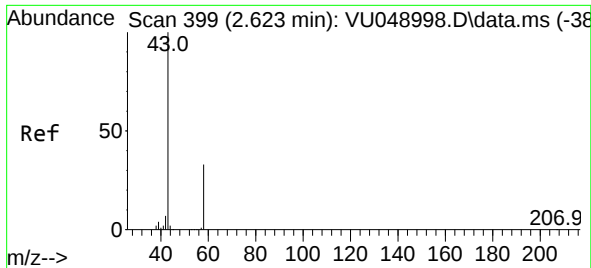

#13
 Acetone
 Concen: 2.268 ug/L
 RT: 2.623 min Scan# 399
 Delta R.T. -0.000 min
 Lab File: VU049016.D
 Acq: 10 Jun 2022 22:56

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DH4

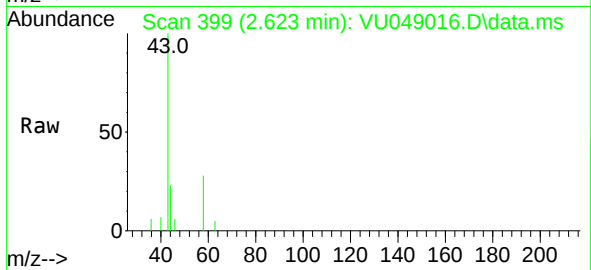

Tgt Ion: 43 Resp: 3371
 Ion Ratio Lower Upper
 43 100
 58 21.3 0.0 66.4

