

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049022.D
 Acq On : 11 Jun 2022 01:18
 Operator : SY/MD
 Sample : N3291-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DT7

Quant Time: Jun 11 02:47:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 10 22:44:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	261252	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	265191	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	111392	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	68554	42.595	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.200%
7) Chloroethane-d5	1.890	69	53037	44.882	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.760%
11) 1,1-Dichloroethene-d2	2.559	63	92844	30.572	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.140%
21) 2-Butanone-d5	4.620	46	184909	104.790	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.790%
24) Chloroform-d	5.060	84	165391	48.172	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.340%
26) 1,2-Dichloroethane-d4	5.700	65	117995	53.047	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.100%
32) Benzene-d6	5.726	84	315085	47.915	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.840%
36) 1,2-Dichloropropane-d6	6.690	67	108111	48.905	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.800%
41) Toluene-d8	7.896	98	257900	44.470	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.940%
43) trans-1,3-Dichloroprop...	8.179	79	45007	43.276	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.560%
47) 2-Hexanone-d5	8.632	63	106658	92.186	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.190%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	185584	50.263	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.520%
66) 1,2-Dichlorobenzene-d4	12.195	152	105981	54.681	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.360%
Target Compounds						
13) Acetone	2.626	43	5524	3.978	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049022.D
Acq On : 11 Jun 2022 01:18
Operator : SY/MD
Sample : N3291-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DT7

Quant Time: Jun 11 02:47:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 10 22:44:31 2022
Response via : Initial Calibration

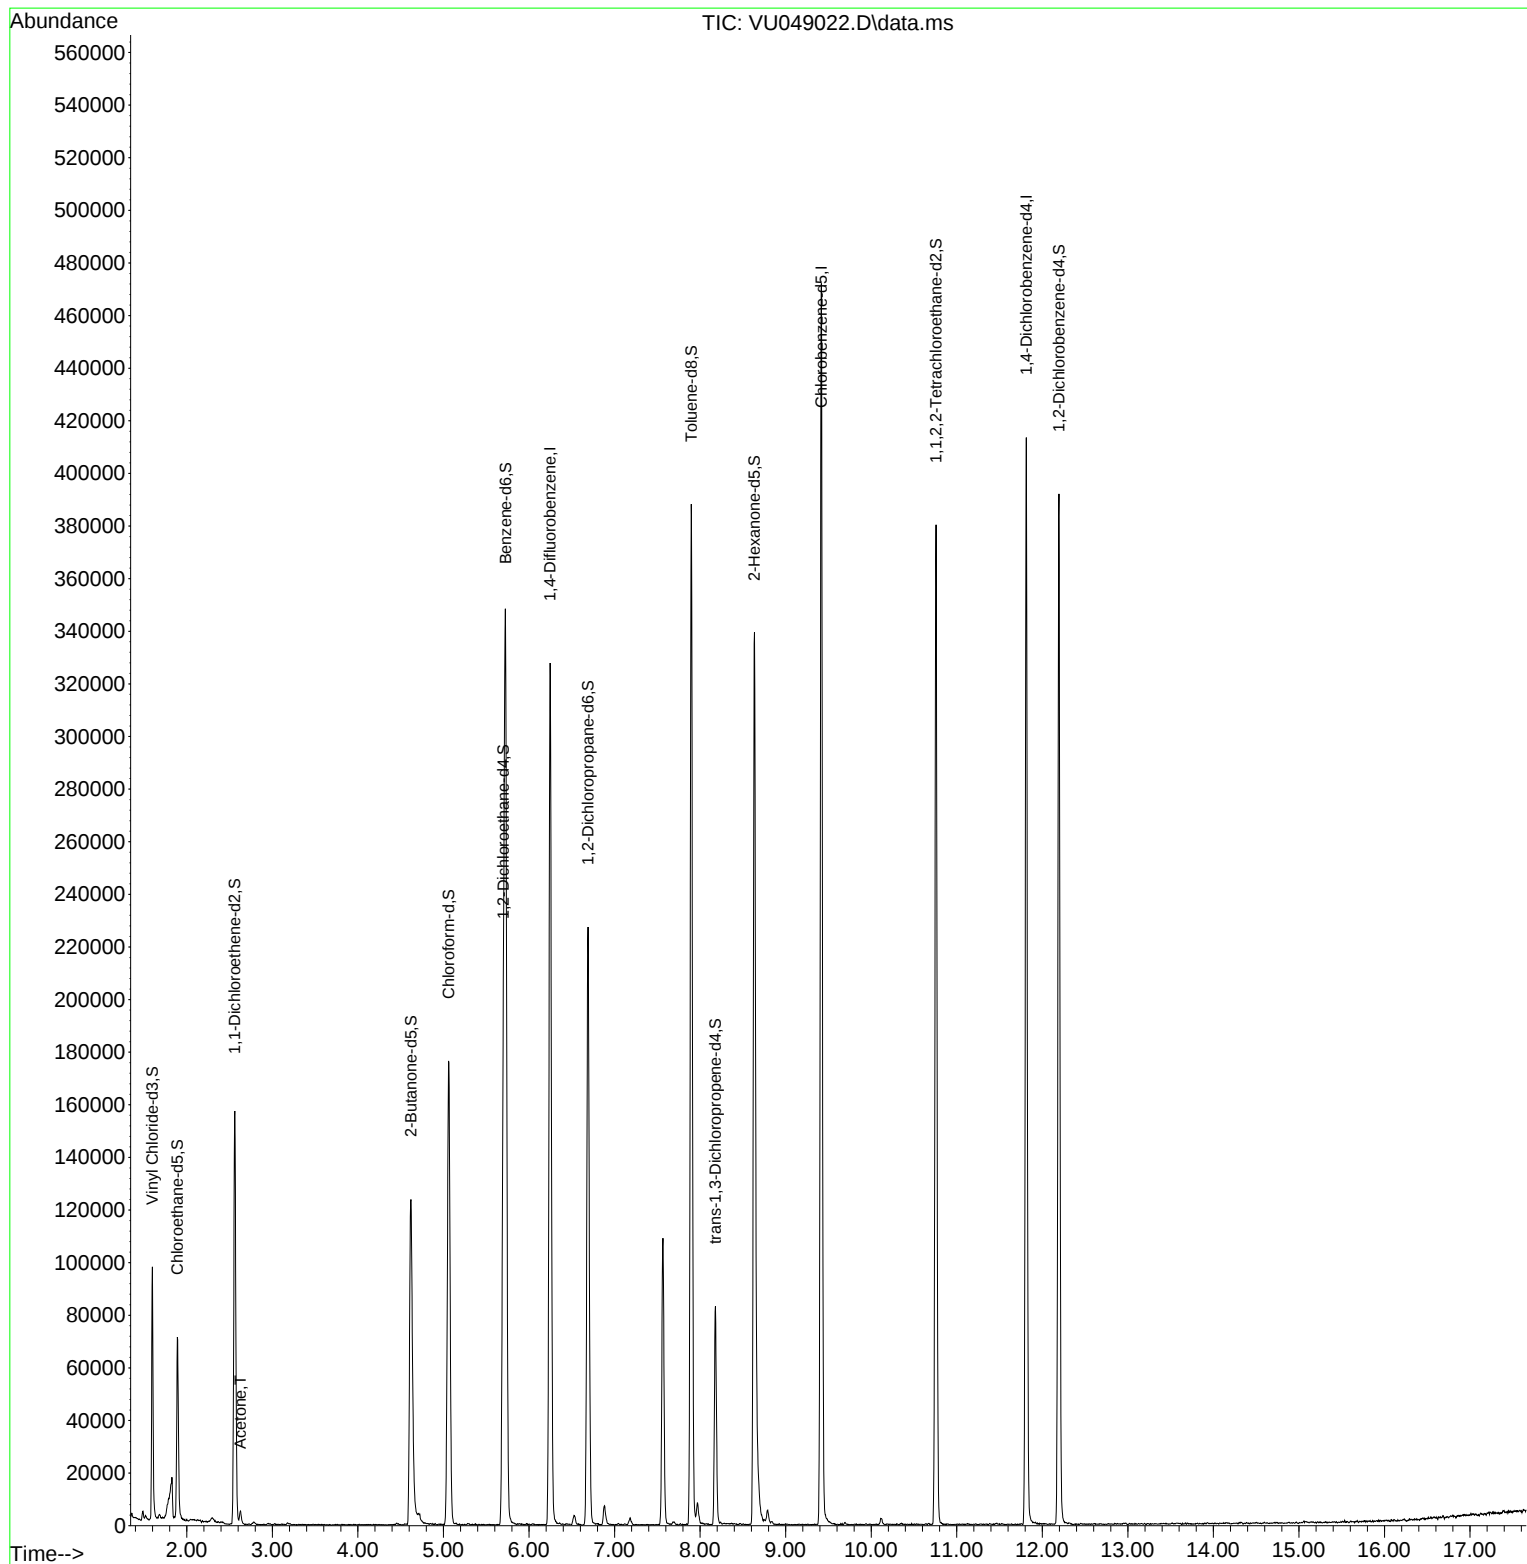

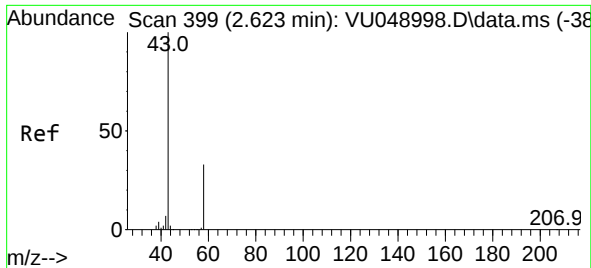

#13

Acetone

Concen: 3.978 ug/L

RT: 2.626 min Scan# 40

Delta R.T. 0.003 min

Lab File: VU049022.D


Acq: 11 Jun 2022 01:18

Instrument :

MSVOA_U

ClientSampleId :

C0DT7

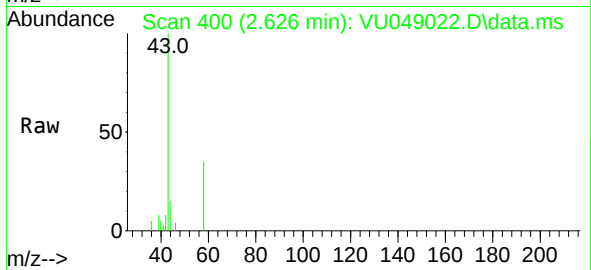

Tgt Ion: 43 Resp: 5524

Ion Ratio Lower Upper

43 100

58 32.3 0.0 66.4

