

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU048999.D
 Acq On : 10 Jun 2022 16:16
 Operator : SY/MD
 Sample : VU0610WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK140

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

Signal : TIC: VU048999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rBV	137088	153593	13.59%	1.723%
2	1.899	167	174	187	rVB	95216	122991	10.89%	1.380%
3	2.562	369	380	400	rBV	220855	361765	32.02%	4.059%
4	2.790	442	451	460	rVB3	1598	2628	0.23%	0.029%
5	3.005	516	518	521	rBV	179	136	0.01%	0.002%
6	3.121	551	554	556	rBV2	256	187	0.02%	0.002%
7	3.186	563	574	583	rBV3	1213	2602	0.23%	0.029%
8	3.301	608	610	615	rVB	290	248	0.02%	0.003%
9	3.340	615	622	625	rBV3	707	799	0.07%	0.009%
10	3.462	657	660	663	rBV2	271	213	0.02%	0.002%
11	3.475	663	664	665	rVV	232	63	0.01%	0.001%
12	3.485	665	667	670	rVV2	282	182	0.02%	0.002%
13	3.501	670	672	675	rVB	294	153	0.01%	0.002%
14	3.539	682	684	686	rBV	182	47	0.00%	0.001%
15	3.555	686	689	691	rBV2	290	195	0.02%	0.002%
16	3.668	723	724	725	rBV	174	55	0.00%	0.001%
17	3.909	796	799	805	rBV	344	305	0.03%	0.003%
18	4.620	1006	1020	1044	rBV	147756	351365	31.10%	3.943%
19	5.063	1142	1158	1180	rBV	210655	456461	40.40%	5.122%
20	5.221	1201	1207	1212	rBV4	402	447	0.04%	0.005%
21	5.272	1218	1223	1225	rBV2	589	496	0.04%	0.006%
22	5.330	1239	1241	1242	rBV2	213	74	0.01%	0.001%
23	5.369	1251	1253	1254	rBV	332	76	0.01%	0.001%
24	5.722	1341	1363	1388	rBV2	410005	1129784	100.00%	12.677%
25	5.964	1436	1438	1440	rBV	310	152	0.01%	0.002%
26	6.034	1457	1460	1465	rBV	369	373	0.03%	0.004%
27	6.089	1475	1477	1479	rBV2	99	59	0.01%	0.001%
28	6.108	1480	1483	1485	rBV	314	240	0.02%	0.003%
29	6.185	1505	1507	1512	rBV	209	132	0.01%	0.001%
30	6.250	1512	1527	1554	rBV	392631	742566	65.73%	8.332%
31	6.468	1593	1595	1598	rBV2	236	134	0.01%	0.002%
32	6.533	1606	1615	1626	rVB8	3799	8239	0.73%	0.092%
33	6.610	1637	1639	1640	rBV	170	67	0.01%	0.001%
34	6.619	1640	1642	1644	rBV	224	118	0.01%	0.001%
35	6.690	1649	1664	1686	rBV	275067	528062	46.74%	5.925%
36	6.809	1697	1701	1708	rVB3	872	888	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU048999.D
 Acq On : 10 Jun 2022 16:16
 Operator : SY/MD
 Sample : VU0610WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK140

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.864	1715	1718	1722	rBV2	283	162	0.01%	0.002%
38	6.954	1744	1746	1748	rVB	188	79	0.01%	0.001%
39	6.999	1752	1760	1763	rBV2	392	560	0.05%	0.006%
40	7.182	1810	1817	1826	rBV5	2683	4375	0.39%	0.049%
41	7.263	1840	1842	1846	rVB2	374	181	0.02%	0.002%
42	7.372	1874	1876	1881	rVB	332	182	0.02%	0.002%
43	7.565	1923	1936	1955	rBV	143831	248575	22.00%	2.789%
44	7.748	1990	1993	1997	rBV	335	238	0.02%	0.003%
45	7.899	2026	2040	2054	rBV	484980	832085	73.65%	9.337%
46	8.108	2103	2105	2107	rVB	245	132	0.01%	0.001%
47	8.179	2114	2127	2141	rBV	101111	170712	15.11%	1.916%
48	8.336	2172	2176	2183	rVB4	521	537	0.05%	0.006%
49	8.510	2227	2230	2232	rBV	283	179	0.02%	0.002%
50	8.632	2256	2268	2296	rBV2	392649	730069	64.62%	8.192%
51	8.925	2355	2359	2361	rBV	441	317	0.03%	0.004%
52	8.963	2368	2371	2378	rBV2	252	216	0.02%	0.002%
53	9.140	2422	2426	2428	rBV2	329	258	0.02%	0.003%
54	9.211	2444	2448	2449	rBV	343	186	0.02%	0.002%
55	9.417	2499	2512	2539	rBV	528003	880092	77.90%	9.875%
56	9.703	2592	2601	2606	rBV4	1302	2256	0.20%	0.025%
57	9.777	2623	2624	2629	rVB2	305	230	0.02%	0.003%
58	9.809	2629	2634	2637	rBV2	523	488	0.04%	0.005%
59	10.471	2837	2840	2841	rBV	669	287	0.03%	0.003%
60	10.603	2879	2881	2883	rVB	238	77	0.01%	0.001%
61	10.632	2883	2890	2899	rBV4	4712	7516	0.67%	0.084%
62	10.758	2916	2929	2945	rBV	402960	646233	57.20%	7.251%
63	10.954	2989	2990	2991	rBV	308	76	0.01%	0.001%
64	11.256	3081	3084	3086	rBV2	349	202	0.02%	0.002%
65	11.439	3139	3141	3143	rBV2	364	213	0.02%	0.002%
66	11.471	3144	3151	3159	rVB6	2342	3631	0.32%	0.041%
67	11.504	3159	3161	3166	rBV2	440	480	0.04%	0.005%
68	11.745	3230	3236	3245	rVB4	2377	3519	0.31%	0.039%
69	11.812	3245	3257	3276	rBV	467265	745131	65.95%	8.361%
70	12.195	3362	3376	3400	rBV	433014	725313	64.20%	8.139%
71	12.700	3532	3533	3534	rBV	460	106	0.01%	0.001%
72	12.790	3557	3561	3563	rBV2	386	275	0.02%	0.003%
73	14.092	3957	3966	3983	rBV	15268	28698	2.54%	0.322%
74	14.336	4034	4042	4054	rVB4	6770	12327	1.09%	0.138%

Sum of corrected areas: 8912088




Instrument :
MSVOA_U
ClientSampleId :
VBLK140

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU048999.D
Acq On : 10 Jun 2022 16:16
Operator : SY/MD
Sample : VU0610WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK140

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

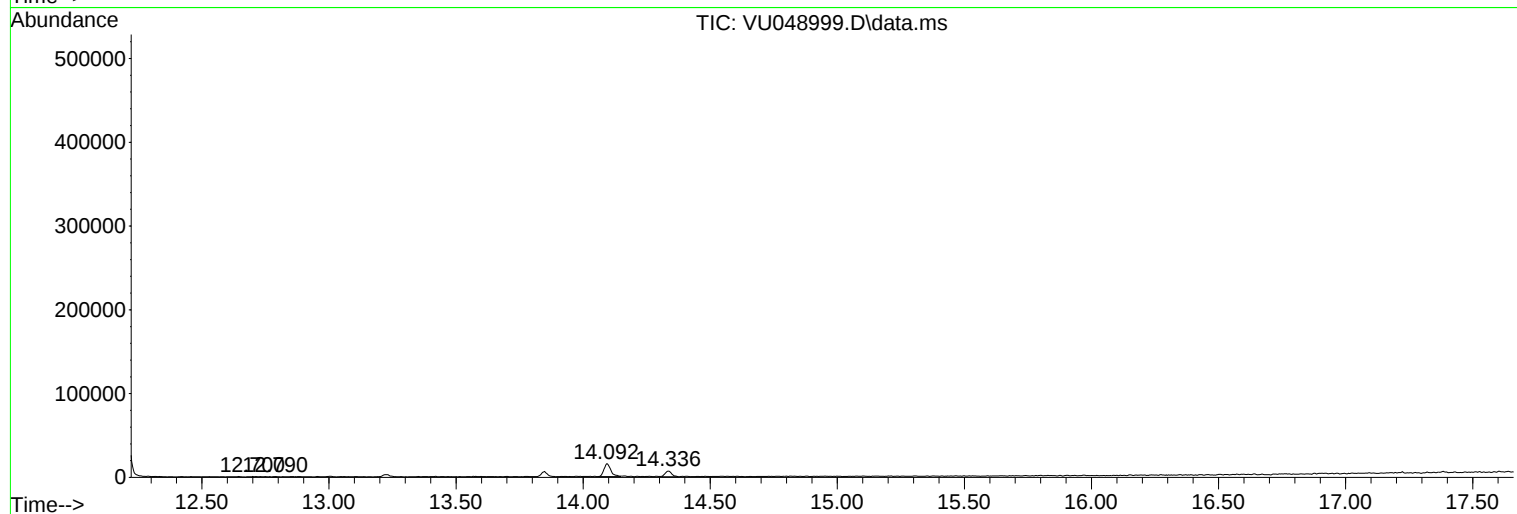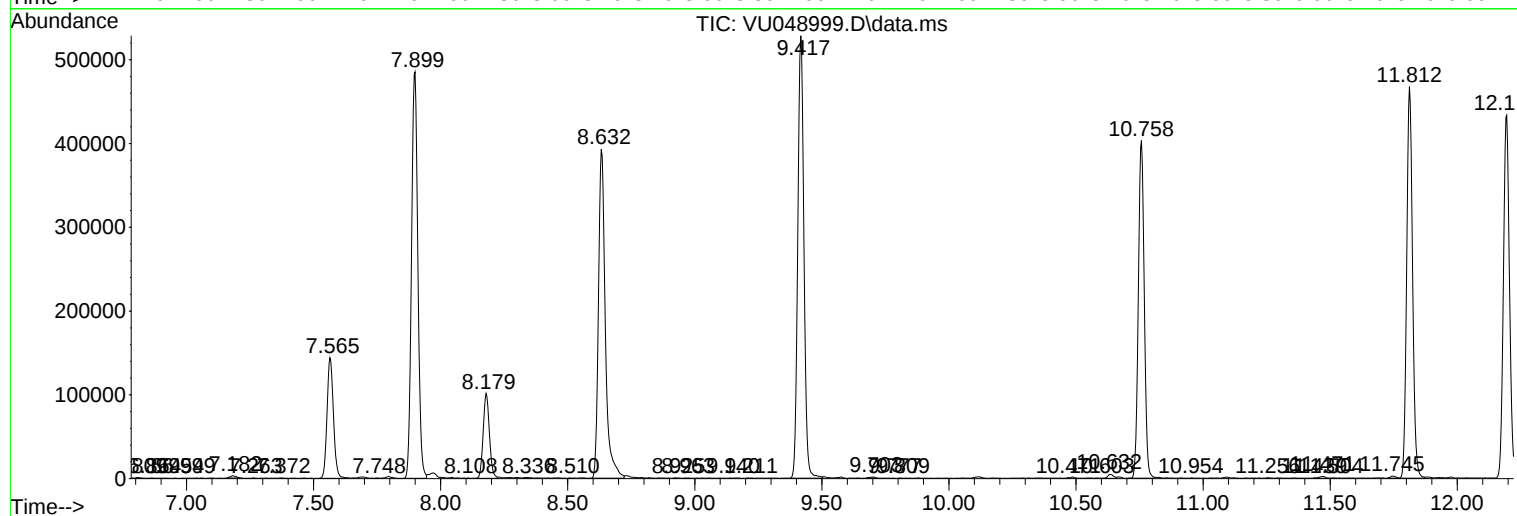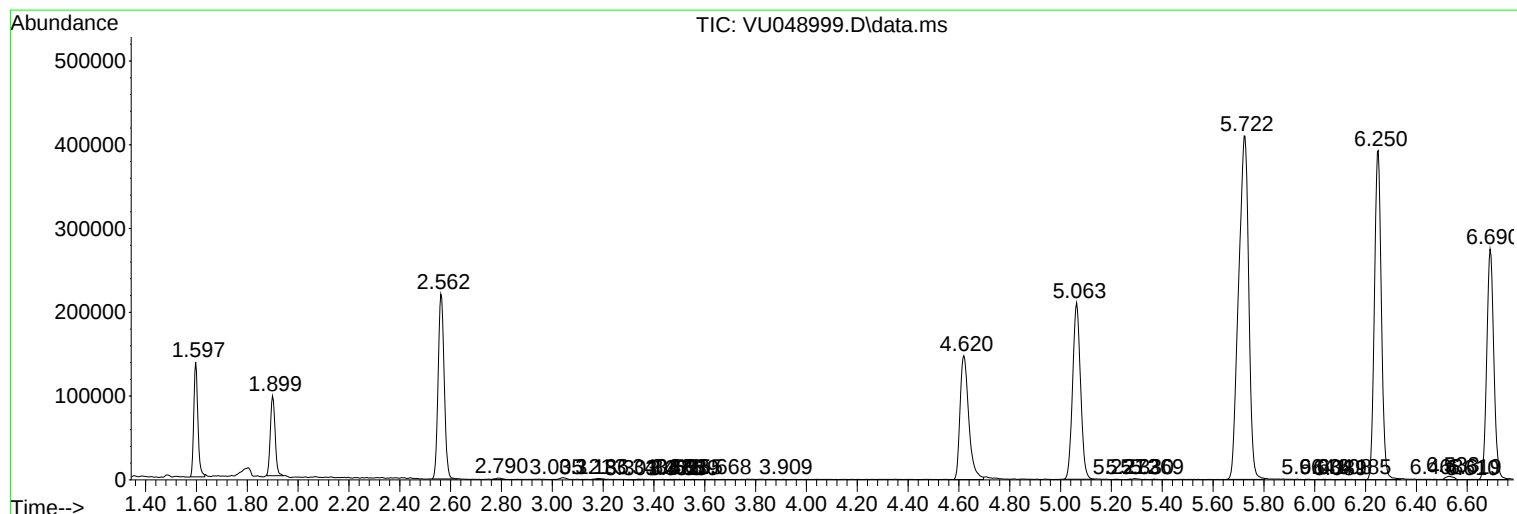

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU048999.D
Acq On : 10 Jun 2022 16:16
Operator : SY/MD
Sample : VU0610WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK140

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU048999.D
Acq On : 10 Jun 2022 16:16
Operator : SY/MD
Sample : VU0610WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK140

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------