

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049001.D
 Acq On : 10 Jun 2022 17:03
 Operator : SY/MD
 Sample : N3254-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rBV	109729	123389	12.51%	1.588%
2	1.896	166	173	187	rVB	78143	101664	10.31%	1.309%
3	2.562	368	380	395	rBV	178842	290876	29.49%	3.744%
4	2.880	473	479	481	rBV2	403	389	0.04%	0.005%
5	3.186	562	574	584	rBV2	4180	8241	0.84%	0.106%
6	3.334	617	620	625	rBV4	405	442	0.04%	0.006%
7	3.427	646	649	650	rBV	198	116	0.01%	0.001%
8	3.684	726	729	734	rBV2	203	237	0.02%	0.003%
9	3.732	742	744	750	rBV2	269	236	0.02%	0.003%
10	3.793	760	763	766	rBV2	217	144	0.01%	0.002%
11	3.864	782	785	790	rBV3	517	468	0.05%	0.006%
12	3.993	822	825	826	rBV	131	76	0.01%	0.001%
13	4.054	840	844	848	rBV2	211	171	0.02%	0.002%
14	4.073	848	850	854	rVB	220	133	0.01%	0.002%
15	4.102	857	859	860	rBV	293	120	0.01%	0.002%
16	4.160	873	877	882	rBV	284	320	0.03%	0.004%
17	4.244	902	903	906	rBV2	203	121	0.01%	0.002%
18	4.414	955	956	957	rBV	192	52	0.01%	0.001%
19	4.433	958	962	966	rVV2	226	251	0.03%	0.003%
20	4.536	989	994	996	rBV2	259	230	0.02%	0.003%
21	4.559	999	1001	1006	rVB2	220	155	0.02%	0.002%
22	4.620	1007	1020	1043	rBV	126546	311287	31.55%	4.007%
23	5.064	1142	1158	1179	rBV	191968	426841	43.27%	5.494%
24	5.224	1203	1208	1210	rBV2	225	166	0.02%	0.002%
25	5.273	1220	1223	1225	rBV2	445	277	0.03%	0.004%
26	5.459	1277	1281	1282	rBV	167	107	0.01%	0.001%
27	5.507	1293	1296	1299	rBV2	285	223	0.02%	0.003%
28	5.588	1318	1321	1324	rBV	246	174	0.02%	0.002%
29	5.723	1339	1363	1392	rBV3	359753	986504	100.00%	12.698%
30	5.922	1418	1425	1427	rBV2	264	267	0.03%	0.003%
31	5.961	1434	1437	1440	rBV3	601	374	0.04%	0.005%
32	5.977	1440	1442	1444	rVB2	292	97	0.01%	0.001%
33	5.990	1444	1446	1453	rVB3	459	366	0.04%	0.005%
34	6.022	1454	1456	1461	rVB	261	158	0.02%	0.002%
35	6.057	1461	1467	1468	rBV	265	203	0.02%	0.003%
36	6.089	1475	1477	1480	rVB	132	52	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049001.D
 Acq On : 10 Jun 2022 17:03
 Operator : SY/MD
 Sample : N3254-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.112	1481	1484	1486	rBV2	208	152	0.02%	0.002%
38	6.247	1513	1526	1552	rBV	316320	608426	61.67%	7.831%
39	6.456	1588	1591	1594	rBV	321	211	0.02%	0.003%
40	6.475	1596	1597	1599	rVB	231	57	0.01%	0.001%
41	6.488	1599	1601	1605	rBV	284	218	0.02%	0.003%
42	6.543	1605	1618	1633	rBV4	56696	108929	11.04%	1.402%
43	6.690	1646	1664	1682	rBV2	243382	476925	48.34%	6.139%
44	6.848	1710	1713	1714	rBV	91	50	0.01%	0.001%
45	6.944	1741	1743	1745	rBV	164	75	0.01%	0.001%
46	7.022	1764	1767	1770	rBV2	130	94	0.01%	0.001%
47	7.060	1772	1779	1781	rBV4	1258	1484	0.15%	0.019%
48	7.128	1798	1800	1804	rBV3	319	190	0.02%	0.002%
49	7.147	1804	1806	1807	rBV	181	58	0.01%	0.001%
50	7.160	1807	1810	1811	rBV2	582	293	0.03%	0.004%
51	7.317	1855	1859	1865	rBV2	261	332	0.03%	0.004%
52	7.346	1865	1868	1870	rBV	229	150	0.02%	0.002%
53	7.411	1886	1888	1891	rVB	241	103	0.01%	0.001%
54	7.565	1923	1936	1953	rBV2	112044	196816	19.95%	2.533%
55	7.681	1969	1972	1973	rBV2	533	306	0.03%	0.004%
56	7.793	2000	2007	2020	rVB6	2290	4256	0.43%	0.055%
57	7.848	2020	2024	2026	rBV	237	199	0.02%	0.003%
58	7.896	2026	2039	2061	rBV	434111	738150	74.82%	9.501%
59	8.179	2115	2127	2140	rBV	82694	137832	13.97%	1.774%
60	8.633	2257	2268	2301	rBV2	362462	666848	67.60%	8.583%
61	8.874	2339	2343	2346	rBV2	354	254	0.03%	0.003%
62	8.912	2354	2355	2356	rBV	111	22	0.00%	0.000%
63	9.034	2391	2393	2394	rBV	276	114	0.01%	0.001%
64	9.102	2412	2414	2417	rBV2	225	153	0.02%	0.002%
65	9.147	2422	2428	2431	rBV2	270	319	0.03%	0.004%
66	9.176	2435	2437	2440	rBV2	210	67	0.01%	0.001%
67	9.195	2440	2443	2447	rVB3	354	279	0.03%	0.004%
68	9.224	2447	2452	2456	rBV2	291	358	0.04%	0.005%
69	9.417	2499	2512	2532	rBV	431314	721416	73.13%	9.286%
70	9.642	2580	2582	2584	rVB	336	80	0.01%	0.001%
71	9.694	2592	2598	2599	rBV3	923	734	0.07%	0.009%
72	9.793	2627	2629	2632	rBV	235	146	0.01%	0.002%
73	10.263	2774	2775	2776	rBV	435	99	0.01%	0.001%
74	10.485	2838	2844	2850	rBV3	440	583	0.06%	0.008%
75	10.636	2886	2891	2892	rBV2	652	516	0.05%	0.007%
76	10.755	2916	2928	2944	rBV	360065	588555	59.66%	7.575%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049001.D
 Acq On : 10 Jun 2022 17:03
 Operator : SY/MD
 Sample : N3254-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

77	11.205	3065	3068	3073	rBV	342	278	0.03%	0.004%
78	11.317	3101	3103	3106	rBV	307	206	0.02%	0.003%
79	11.446	3139	3143	3145	rBV	241	175	0.02%	0.002%
80	11.468	3145	3150	3157	rVV4	975	1328	0.13%	0.017%
81	11.693	3217	3220	3226	rVB6	1210	1247	0.13%	0.016%
82	11.812	3245	3257	3278	rBV	379123	608690	61.70%	7.835%
83	12.128	3353	3355	3357	rBV	251	115	0.01%	0.001%
84	12.192	3363	3375	3398	rBV	386200	638960	64.77%	8.224%
85	14.099	3962	3968	3984	rVB4	4504	7497	0.76%	0.096%




Sum of corrected areas: 7769272

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049001.D
Acq On : 10 Jun 2022 17:03
Operator : SY/MD
Sample : N3254-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

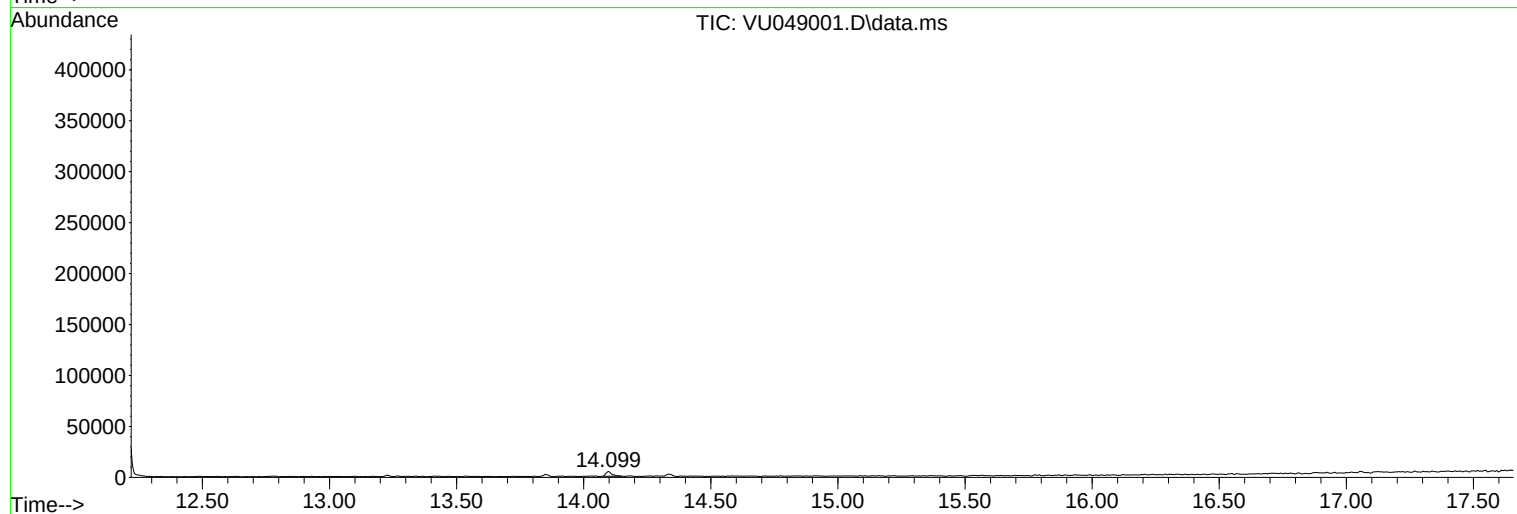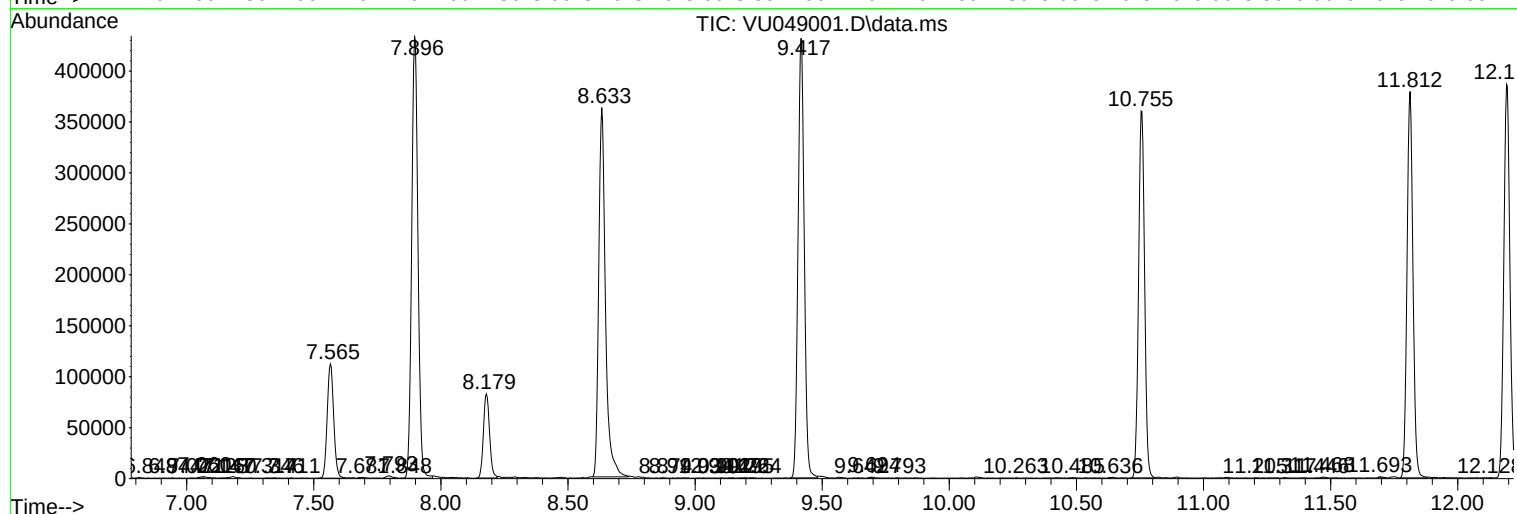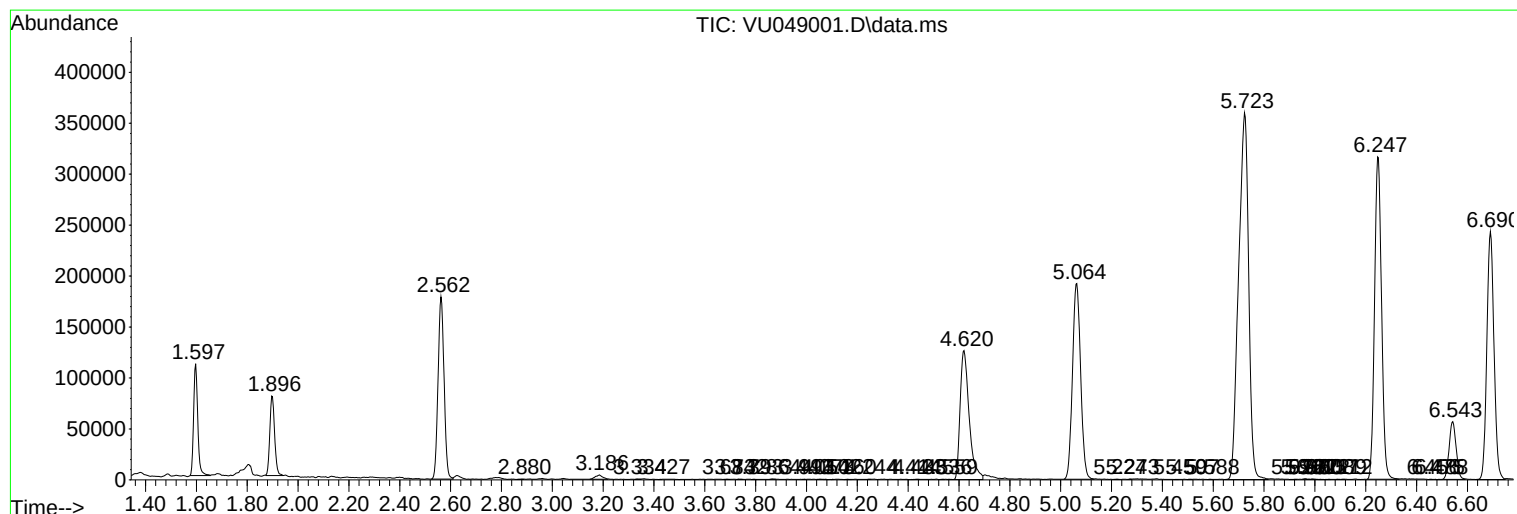

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049001.D
Acq On : 10 Jun 2022 17:03
Operator : SY/MD
Sample : N3254-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049001.D
Acq On : 10 Jun 2022 17:03
Operator : SY/MD
Sample : N3254-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------