

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049002.D
 Acq On : 10 Jun 2022 17:26
 Operator : SY/MD
 Sample : N3254-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rBV	111972	129010	13.07%	1.679%
2	1.896	166	173	184	rVB	75402	98612	9.99%	1.283%
3	2.562	367	380	393	rBV	174739	286133	28.99%	3.723%
4	2.716	424	428	432	rBV2	457	430	0.04%	0.006%
5	2.880	477	479	481	rBV2	232	127	0.01%	0.002%
6	3.035	521	527	528	rBV2	1025	803	0.08%	0.010%
7	3.115	550	552	556	rVB2	108	73	0.01%	0.001%
8	3.179	557	572	586	rBV	6357	14588	1.48%	0.190%
9	3.350	621	625	626	rBV	262	148	0.01%	0.002%
10	3.398	637	640	643	rBV2	260	216	0.02%	0.003%
11	3.543	682	685	688	rBV2	206	146	0.01%	0.002%
12	3.623	707	710	713	rBV2	237	154	0.02%	0.002%
13	3.703	730	735	737	rBV	261	196	0.02%	0.003%
14	3.755	749	751	754	rBV	263	123	0.01%	0.002%
15	3.784	756	760	766	rVB2	448	503	0.05%	0.007%
16	3.909	797	799	801	rVB	400	111	0.01%	0.001%
17	3.954	810	813	814	rBV2	144	69	0.01%	0.001%
18	4.031	833	837	838	rBV	175	116	0.01%	0.002%
19	4.089	852	855	861	rBV2	318	363	0.04%	0.005%
20	4.144	868	872	876	rBV2	226	226	0.02%	0.003%
21	4.314	919	925	931	rBV2	223	321	0.03%	0.004%
22	4.433	958	962	969	rBV2	198	247	0.03%	0.003%
23	4.488	977	979	981	rBV	42	16	0.00%	0.000%
24	4.507	981	985	988	rBV2	135	124	0.01%	0.002%
25	4.620	1007	1020	1039	rBV	127120	301051	30.50%	3.917%
26	4.903	1106	1108	1111	rVB	244	73	0.01%	0.001%
27	4.932	1113	1117	1121	rBV3	360	395	0.04%	0.005%
28	4.951	1121	1123	1124	rBV	376	110	0.01%	0.001%
29	5.060	1141	1157	1183	rBV	203583	449886	45.57%	5.853%
30	5.263	1216	1220	1221	rBV2	266	196	0.02%	0.003%
31	5.485	1284	1289	1291	rBV2	465	346	0.04%	0.005%
32	5.559	1308	1312	1315	rBV	122	129	0.01%	0.002%
33	5.723	1341	1363	1392	rBV2	361934	987152	100.00%	12.844%
34	5.925	1423	1426	1429	rBV2	263	168	0.02%	0.002%
35	5.970	1435	1440	1442	rBV3	604	629	0.06%	0.008%
36	6.012	1451	1453	1456	rBV	193	99	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049002.D
 Acq On : 10 Jun 2022 17:26
 Operator : SY/MD
 Sample : N3254-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.057	1465	1467	1468	rBV	150	51	0.01%	0.001%
38	6.118	1481	1486	1492	rBV3	339	510	0.05%	0.007%
39	6.144	1492	1494	1496	rVB	266	92	0.01%	0.001%
40	6.157	1496	1498	1501	rBV	135	73	0.01%	0.001%
41	6.173	1501	1503	1504	rBV	193	72	0.01%	0.001%
42	6.247	1513	1526	1547	rBV	315934	603010	61.09%	7.846%
43	6.369	1561	1564	1567	rBV2	273	144	0.01%	0.002%
44	6.385	1567	1569	1578	rVB3	507	562	0.06%	0.007%
45	6.427	1578	1582	1585	rBV2	257	265	0.03%	0.003%
46	6.462	1590	1593	1599	rVB2	389	345	0.03%	0.004%
47	6.494	1601	1603	1605	rVB	298	113	0.01%	0.001%
48	6.530	1606	1614	1624	rBV8	2719	5153	0.52%	0.067%
49	6.584	1627	1631	1635	rBV3	410	438	0.04%	0.006%
50	6.623	1640	1643	1650	rBV2	180	225	0.02%	0.003%
51	6.690	1650	1664	1684	rBV	238628	464173	47.02%	6.039%
52	6.787	1692	1694	1696	rVB3	438	201	0.02%	0.003%
53	6.903	1727	1730	1735	rVB2	246	155	0.02%	0.002%
54	6.925	1735	1737	1738	rBV	104	43	0.00%	0.001%
55	7.073	1780	1783	1786	rBV2	289	205	0.02%	0.003%
56	7.131	1799	1801	1802	rBV2	110	28	0.00%	0.000%
57	7.282	1844	1848	1851	rVB2	240	194	0.02%	0.003%
58	7.369	1872	1875	1878	rBV2	145	80	0.01%	0.001%
59	7.401	1883	1885	1889	rVB	276	184	0.02%	0.002%
60	7.417	1889	1890	1892	rBV	210	73	0.01%	0.001%
61	7.436	1893	1896	1897	rBV	208	119	0.01%	0.002%
62	7.468	1904	1906	1910	rBV2	250	143	0.01%	0.002%
63	7.523	1918	1923	1924	rBV2	241	182	0.02%	0.002%
64	7.565	1924	1936	1956	rVV	110723	194531	19.71%	2.531%
65	7.739	1987	1990	1995	rVB2	374	272	0.03%	0.004%
66	7.758	1995	1996	1999	rVB	117	47	0.00%	0.001%
67	7.793	1999	2007	2012	rBV4	1276	1269	0.13%	0.017%
68	7.896	2025	2039	2060	rBV	416883	723077	73.25%	9.408%
69	8.179	2116	2127	2143	rBV	82027	136427	13.82%	1.775%
70	8.475	2211	2219	2228	rVB3	4327	7313	0.74%	0.095%
71	8.558	2243	2245	2247	rBV	471	228	0.02%	0.003%
72	8.632	2256	2268	2303	rBV2	368067	684520	69.34%	8.906%
73	8.877	2342	2344	2347	rBV	237	150	0.02%	0.002%
74	8.944	2362	2365	2367	rBV	211	141	0.01%	0.002%
75	8.999	2380	2382	2384	rBV	128	67	0.01%	0.001%
76	9.086	2405	2409	2411	rBV2	188	147	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049002.D
 Acq On : 10 Jun 2022 17:26
 Operator : SY/MD
 Sample : N3254-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.417	2499	2512	2540	rBV	436389	711626	72.09%	9.259%
78	9.565	2553	2558	2567	rBV5	747	1065	0.11%	0.014%
79	9.648	2580	2584	2586	rBV	333	268	0.03%	0.003%
80	9.681	2592	2594	2595	rBV	406	150	0.02%	0.002%
81	9.918	2666	2668	2670	rVB	222	56	0.01%	0.001%
82	10.224	2759	2763	2765	rBV2	225	173	0.02%	0.002%
83	10.263	2771	2775	2778	rBV2	478	393	0.04%	0.005%
84	10.632	2887	2890	2891	rBV	403	230	0.02%	0.003%
85	10.758	2917	2929	2947	rBV	367567	584287	59.19%	7.602%
86	10.890	2963	2970	2984	rVB2	5984	9295	0.94%	0.121%
87	11.134	3042	3046	3050	rBV2	398	395	0.04%	0.005%
88	11.320	3101	3104	3106	rBV	253	157	0.02%	0.002%
89	11.410	3128	3132	3135	rBV2	360	329	0.03%	0.004%
90	11.812	3245	3257	3282	rBV	390155	621982	63.01%	8.093%
91	12.195	3363	3376	3400	rBV	401400	652718	66.12%	8.493%
92	12.774	3549	3556	3565	rVB3	2661	4556	0.46%	0.059%




Sum of corrected areas: 7685791

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049002.D
Acq On : 10 Jun 2022 17:26
Operator : SY/MD
Sample : N3254-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

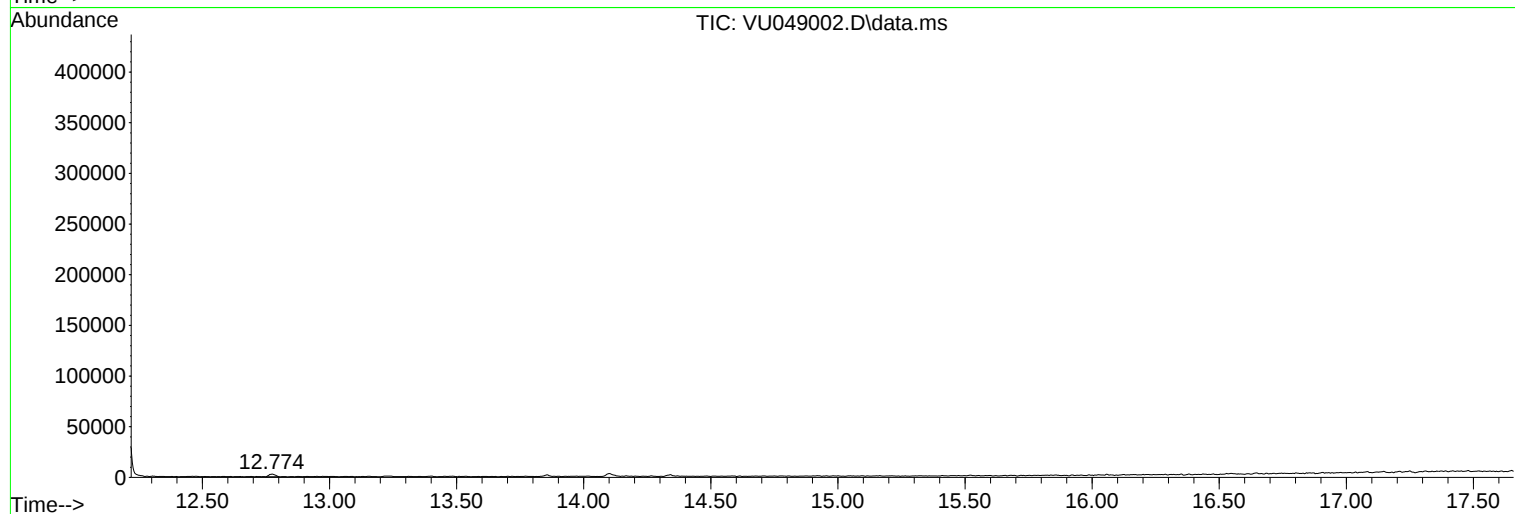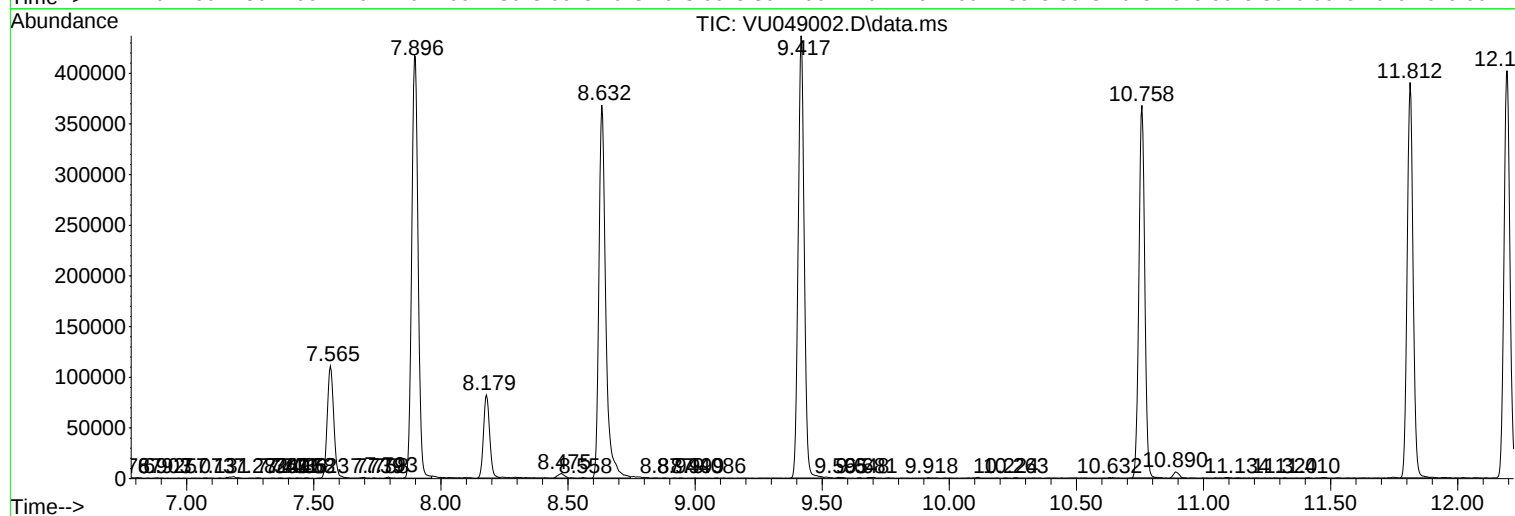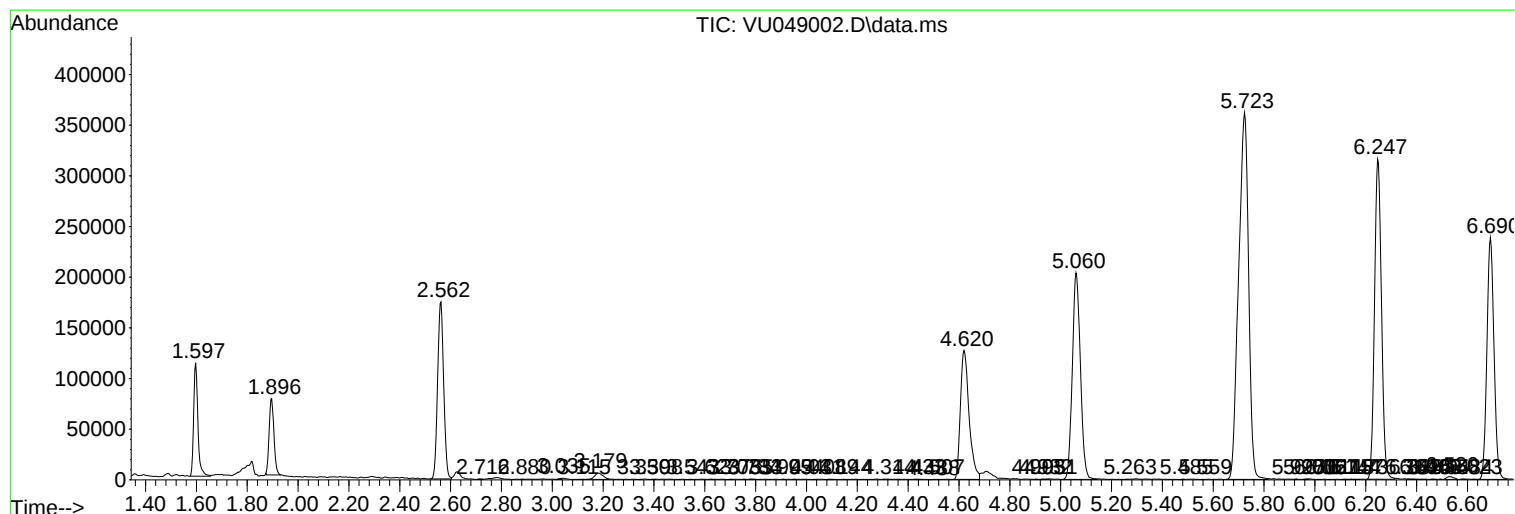

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049002.D
Acq On : 10 Jun 2022 17:26
Operator : SY/MD
Sample : N3254-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049002.D
Acq On : 10 Jun 2022 17:26
Operator : SY/MD
Sample : N3254-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------