

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049003.D
 Acq On : 10 Jun 2022 17:50
 Operator : SY/MD
 Sample : N3254-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	109246	124098	2.56%	0.952%
2	1.896	165	173	185	rVB	76022	100342	2.07%	0.770%
3	2.279	288	292	296	rBV4	1329	1332	0.03%	0.010%
4	2.433	338	340	348	rVB3	962	960	0.02%	0.007%
5	2.565	366	381	397	rBV3	268292	531940	10.97%	4.082%
6	2.765	434	443	444	rBV2	1333	1359	0.03%	0.010%
7	2.890	475	482	485	rBV	284	251	0.01%	0.002%
8	2.906	485	487	493	rVB2	398	429	0.01%	0.003%
9	2.941	493	498	501	rBV2	560	592	0.01%	0.005%
10	3.035	521	527	529	rBV3	627	572	0.01%	0.004%
11	3.144	558	561	563	rVV	402	326	0.01%	0.003%
12	3.183	563	573	587	rVV2	2903	6332	0.13%	0.049%
13	3.353	619	626	638	rVB3	2379	3588	0.07%	0.028%
14	3.867	776	786	799	rVB2	3885	7739	0.16%	0.059%
15	4.321	923	927	932	rVB2	355	315	0.01%	0.002%
16	4.620	1007	1020	1026	rBV	130728	274785	5.67%	2.109%
17	4.980	1129	1132	1137	rVB2	420	368	0.01%	0.003%
18	5.063	1141	1158	1183	rVV	189714	425229	8.77%	3.263%
19	5.224	1206	1208	1215	rVB	385	248	0.01%	0.002%
20	5.314	1215	1236	1260	rBV	113716	256267	5.28%	1.966%
21	5.523	1298	1301	1305	rVB2	454	277	0.01%	0.002%
22	5.723	1340	1363	1381	rBV2	359935	986939	20.35%	7.573%
23	5.842	1396	1400	1405	rVB3	468	402	0.01%	0.003%
24	5.941	1424	1431	1434	rVB2	370	392	0.01%	0.003%
25	5.973	1434	1441	1451	rBV3	580	863	0.02%	0.007%
26	6.025	1454	1457	1460	rBV2	413	264	0.01%	0.002%
27	6.112	1481	1484	1490	rVB3	713	690	0.01%	0.005%
28	6.247	1512	1526	1549	rBV	304065	580490	11.97%	4.454%
29	6.414	1576	1578	1582	rVB2	482	266	0.01%	0.002%
30	6.459	1588	1592	1596	rBV2	263	244	0.01%	0.002%
31	6.543	1600	1618	1645	rBV	2579303	4849661	100.00%	37.213%
32	6.690	1651	1664	1685	rVB2	245143	476479	9.82%	3.656%
33	6.954	1742	1746	1750	rBV2	366	241	0.00%	0.002%
34	6.999	1756	1760	1763	rBV2	349	357	0.01%	0.003%
35	7.166	1805	1812	1814	rBV3	1108	1080	0.02%	0.008%
36	7.263	1836	1842	1845	rBV3	408	413	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049003.D
 Acq On : 10 Jun 2022 17:50
 Operator : SY/MD
 Sample : N3254-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	7.346	1865	1868	1874	rVB2	372	331	0.01%	0.003%
38	7.424	1888	1892	1895	rBV	282	244	0.01%	0.002%
39	7.565	1923	1936	1953	rBV	117322	203069	4.19%	1.558%
40	7.700	1975	1978	1982	rVV4	753	609	0.01%	0.005%
41	7.793	2004	2007	2014	rBV4	523	551	0.01%	0.004%
42	7.896	2025	2039	2059	rBV	435464	749398	15.45%	5.750%
43	8.047	2082	2086	2088	rBV	456	365	0.01%	0.003%
44	8.073	2092	2094	2098	rVB2	469	281	0.01%	0.002%
45	8.092	2098	2100	2103	rVB3	400	254	0.01%	0.002%
46	8.118	2103	2108	2112	rVB2	383	326	0.01%	0.003%
47	8.179	2112	2127	2139	rBV	83312	138726	2.86%	1.065%
48	8.401	2188	2196	2205	rVB6	3184	4821	0.10%	0.037%
49	8.443	2205	2209	2211	rBV2	314	261	0.01%	0.002%
50	8.523	2231	2234	2238	rBV3	345	258	0.01%	0.002%
51	8.549	2238	2242	2246	rBV4	864	867	0.02%	0.007%
52	8.632	2255	2268	2299	rBV2	369138	695616	14.34%	5.338%
53	8.858	2336	2338	2344	rVB2	270	253	0.01%	0.002%
54	8.922	2355	2358	2363	rVB3	309	266	0.01%	0.002%
55	8.973	2371	2374	2376	rBV	382	244	0.01%	0.002%
56	9.173	2432	2436	2440	rBV2	468	366	0.01%	0.003%
57	9.359	2488	2494	2498	rBV2	284	303	0.01%	0.002%
58	9.417	2498	2512	2534	rBV	429546	709811	14.64%	5.447%
59	9.533	2544	2548	2558	rVB6	1554	2247	0.05%	0.017%
60	9.690	2592	2597	2601	rVV	484	539	0.01%	0.004%
61	9.713	2601	2604	2612	rVV2	550	482	0.01%	0.004%
62	9.948	2671	2677	2680	rVB	248	252	0.01%	0.002%
63	10.021	2697	2700	2706	rVB	406	384	0.01%	0.003%
64	10.173	2740	2747	2748	rBV2	333	379	0.01%	0.003%
65	10.230	2763	2765	2772	rVB2	335	323	0.01%	0.002%
66	10.314	2785	2791	2794	rBV	535	595	0.01%	0.005%
67	10.488	2838	2845	2848	rBV	791	936	0.02%	0.007%
68	10.636	2886	2891	2893	rBV2	530	370	0.01%	0.003%
69	10.690	2905	2908	2913	rVV2	224	247	0.01%	0.002%
70	10.758	2915	2929	2955	rVB	370245	599474	12.36%	4.600%
71	10.890	2967	2970	2974	rBV	449	409	0.01%	0.003%
72	11.227	3070	3075	3080	rBV2	365	453	0.01%	0.003%
73	11.462	3144	3148	3150	rBV2	412	308	0.01%	0.002%
74	11.571	3179	3182	3189	rVB2	242	266	0.01%	0.002%
75	11.697	3217	3221	3226	rVB2	312	314	0.01%	0.002%
76	11.735	3230	3233	3235	rBV2	555	385	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049003.D
 Acq On : 10 Jun 2022 17:50
 Operator : SY/MD
 Sample : N3254-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.751	3235	3238	3244	rVB3	872	697	0.01%	0.005%
78	11.812	3244	3257	3281	rBV	384486	611833	12.62%	4.695%
79	11.973	3301	3307	3310	rBV2	678	735	0.02%	0.006%
80	12.092	3337	3344	3346	rBV2	401	397	0.01%	0.003%
81	12.195	3363	3376	3393	rBV	395937	654907	13.50%	5.025%
82	12.327	3412	3417	3421	rBV2	642	637	0.01%	0.005%
83	12.420	3442	3446	3450	rBV2	500	387	0.01%	0.003%
84	12.787	3558	3560	3567	rVB3	381	251	0.01%	0.002%
85	13.015	3626	3631	3634	rBV3	525	568	0.01%	0.004%
86	13.134	3662	3668	3670	rBV2	422	367	0.01%	0.003%
87	13.227	3690	3697	3702	rBV4	1097	1301	0.03%	0.010%
88	13.452	3765	3767	3770	rVB2	516	268	0.01%	0.002%
89	13.488	3774	3778	3780	rBV2	328	288	0.01%	0.002%
90	13.555	3795	3799	3805	rVB3	394	443	0.01%	0.003%
91	13.616	3814	3818	3821	rBV	463	360	0.01%	0.003%
92	13.658	3828	3831	3837	rVB	349	326	0.01%	0.003%
93	13.690	3837	3841	3848	rBV2	612	654	0.01%	0.005%
94	13.854	3889	3892	3898	rVB3	1238	944	0.02%	0.007%
95	13.986	3929	3933	3935	rBV2	406	357	0.01%	0.003%
96	14.098	3962	3968	3979	rBV6	1980	3231	0.07%	0.025%
97	14.844	4198	4200	4204	rVB2	656	330	0.01%	0.003%
98	15.459	4389	4391	4394	rBV3	532	389	0.01%	0.003%
99	15.735	4475	4477	4479	rBV2	558	252	0.01%	0.002%
100	15.809	4498	4500	4504	rVV2	803	386	0.01%	0.003%




Sum of corrected areas: 13032021

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049003.D
Acq On : 10 Jun 2022 17:50
Operator : SY/MD
Sample : N3254-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

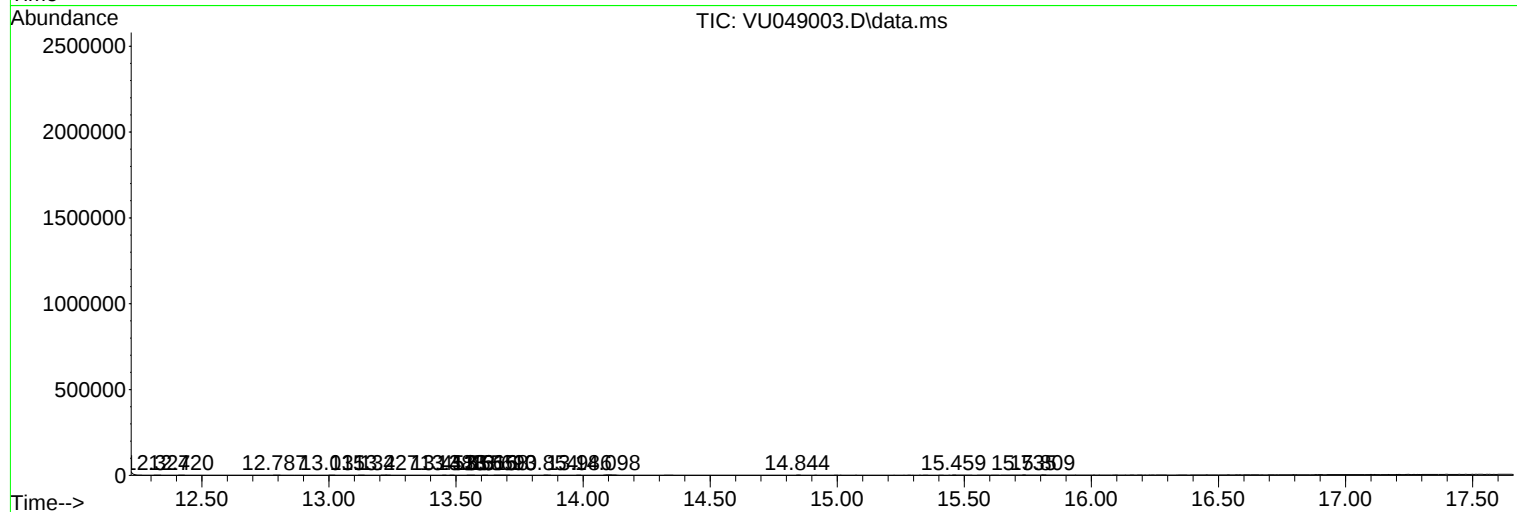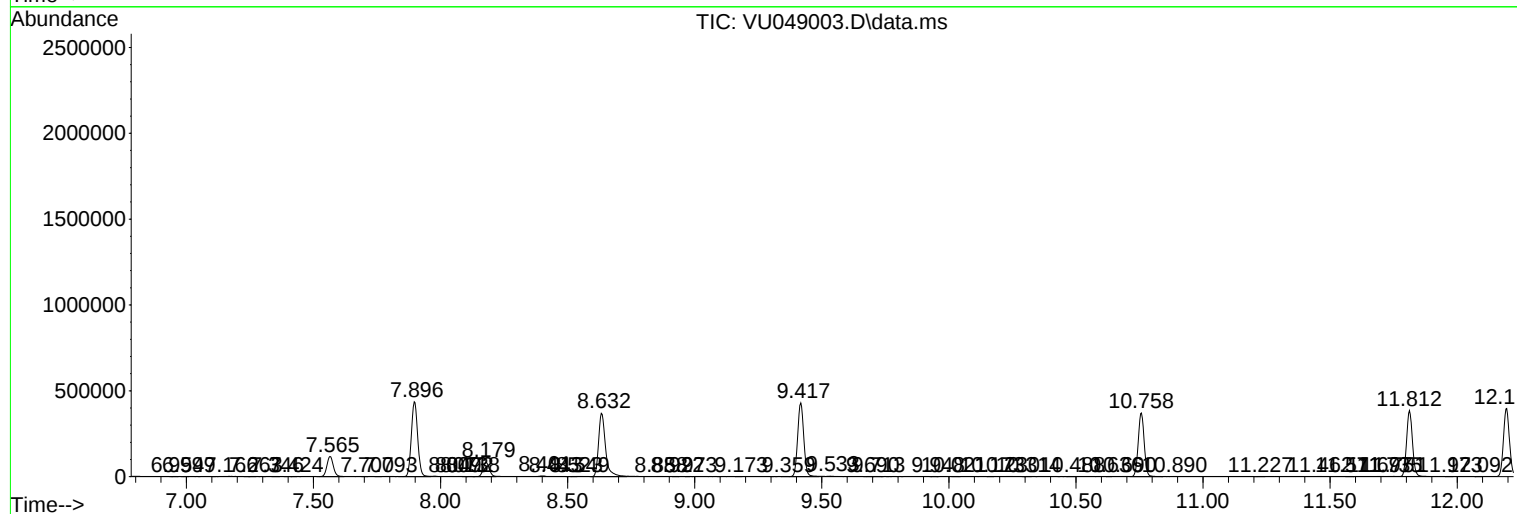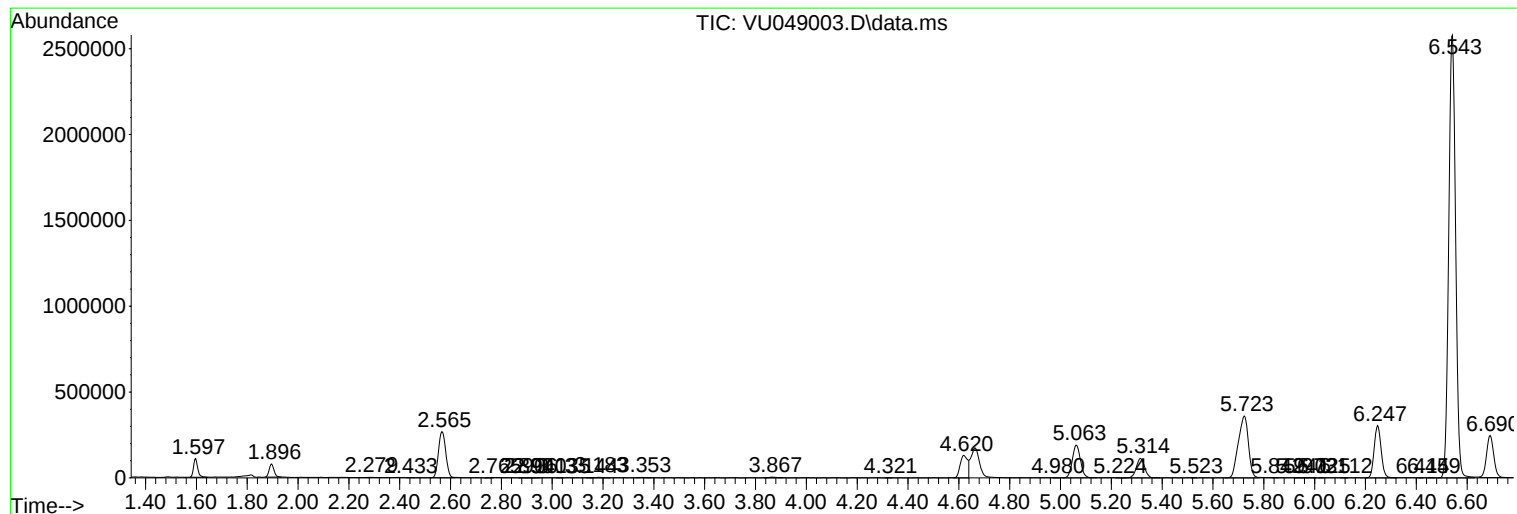

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049003.D
Acq On : 10 Jun 2022 17:50
Operator : SY/MD
Sample : N3254-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049003.D
Acq On : 10 Jun 2022 17:50
Operator : SY/MD
Sample : N3254-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------