

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049005.D
 Acq On : 10 Jun 2022 18:37
 Operator : SY/MD
 Sample : N3254-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	99	rVB	103198	117254	12.70%	1.612%
2	1.893	165	172	186	rVB	73298	96843	10.49%	1.331%
3	2.559	367	379	393	rBV	176799	282153	30.56%	3.878%
4	2.958	500	503	508	rVB	593	380	0.04%	0.005%
5	3.038	523	528	529	rBV3	613	577	0.06%	0.008%
6	3.176	560	571	573	rBV5	4746	5634	0.61%	0.077%
7	3.292	605	607	611	rBV	164	173	0.02%	0.002%
8	3.353	624	626	633	rVB	406	228	0.02%	0.003%
9	3.691	728	731	735	rBV	223	161	0.02%	0.002%
10	3.813	766	769	771	rBV	124	66	0.01%	0.001%
11	3.826	771	773	775	rBV	245	134	0.01%	0.002%
12	4.031	834	837	838	rBV	189	98	0.01%	0.001%
13	4.109	859	861	862	rBV	243	83	0.01%	0.001%
14	4.144	870	872	873	rVB	193	42	0.00%	0.001%
15	4.167	875	879	881	rBV2	255	209	0.02%	0.003%
16	4.279	912	914	915	rBV	185	58	0.01%	0.001%
17	4.314	921	925	929	rVB2	284	227	0.02%	0.003%
18	4.417	955	957	959	rBV2	153	89	0.01%	0.001%
19	4.462	968	971	976	rBV2	148	154	0.02%	0.002%
20	4.620	1007	1020	1042	rBV	119899	291341	31.56%	4.004%
21	4.986	1130	1134	1135	rBV	337	224	0.02%	0.003%
22	5.060	1138	1157	1184	rVV	184543	411757	44.60%	5.659%
23	5.215	1204	1205	1206	rBV	135	33	0.00%	0.000%
24	5.237	1210	1212	1215	rBV	249	168	0.02%	0.002%
25	5.279	1220	1225	1236	rBV4	845	1418	0.15%	0.019%
26	5.324	1236	1239	1241	rBV	237	190	0.02%	0.003%
27	5.446	1273	1277	1281	rBV2	225	274	0.03%	0.004%
28	5.568	1313	1315	1317	rBV	125	72	0.01%	0.001%
29	5.617	1325	1330	1333	rBV2	152	153	0.02%	0.002%
30	5.633	1333	1335	1337	rBV	179	110	0.01%	0.002%
31	5.723	1342	1363	1388	rBV3	339735	923222	100.00%	12.689%
32	5.829	1394	1396	1399	rBV3	399	251	0.03%	0.003%
33	5.967	1434	1439	1441	rBV5	502	528	0.06%	0.007%
34	6.022	1454	1456	1461	rVV2	154	85	0.01%	0.001%
35	6.044	1461	1463	1467	rVB	265	142	0.02%	0.002%
36	6.102	1478	1481	1485	rBV2	194	149	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049005.D
 Acq On : 10 Jun 2022 18:37
 Operator : SY/MD
 Sample : N3254-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.125	1485	1488	1493	rVV3	306	283	0.03%	0.004%
38	6.160	1496	1499	1503	rVB2	222	117	0.01%	0.002%
39	6.247	1510	1526	1556	rBV	292191	553713	59.98%	7.611%
40	6.420	1577	1580	1582	rBV2	364	258	0.03%	0.004%
41	6.465	1589	1594	1599	rBV3	335	448	0.05%	0.006%
42	6.491	1599	1602	1604	rVV3	269	175	0.02%	0.002%
43	6.543	1605	1618	1635	rVB3	48741	95640	10.36%	1.315%
44	6.607	1635	1638	1641	rBV2	232	149	0.02%	0.002%
45	6.691	1649	1664	1686	rBV	228559	443256	48.01%	6.092%
46	6.900	1726	1729	1736	rVB	282	192	0.02%	0.003%
47	6.932	1736	1739	1742	rVB	200	109	0.01%	0.001%
48	7.019	1764	1766	1767	rBV	190	78	0.01%	0.001%
49	7.057	1776	1778	1780	rVB	239	59	0.01%	0.001%
50	7.112	1794	1795	1797	rBV	162	57	0.01%	0.001%
51	7.157	1807	1809	1810	rBV	378	127	0.01%	0.002%
52	7.276	1840	1846	1849	rBV2	199	237	0.03%	0.003%
53	7.318	1856	1859	1861	rBV	162	106	0.01%	0.001%
54	7.356	1868	1871	1873	rVB	197	109	0.01%	0.001%
55	7.411	1885	1888	1893	rBV2	245	249	0.03%	0.003%
56	7.449	1897	1900	1901	rBV	94	59	0.01%	0.001%
57	7.565	1923	1936	1953	rBV	105219	182766	19.80%	2.512%
58	7.671	1966	1969	1972	rBV	297	171	0.02%	0.002%
59	7.684	1972	1973	1974	rBV	293	98	0.01%	0.001%
60	7.755	1993	1995	1997	rBV2	220	115	0.01%	0.002%
61	7.784	2001	2004	2006	rBV2	228	154	0.02%	0.002%
62	7.896	2026	2039	2057	rBV	392769	677786	73.42%	9.316%
63	8.080	2094	2096	2101	rVB3	575	425	0.05%	0.006%
64	8.179	2115	2127	2144	rBV2	76194	126902	13.75%	1.744%
65	8.430	2203	2205	2208	rBV2	274	183	0.02%	0.003%
66	8.559	2242	2245	2250	rBV3	376	300	0.03%	0.004%
67	8.633	2255	2268	2299	rBV2	338444	643768	69.73%	8.848%
68	9.144	2424	2427	2430	rBV	340	202	0.02%	0.003%
69	9.195	2440	2443	2447	rBV2	242	191	0.02%	0.003%
70	9.324	2477	2483	2487	rBV2	297	403	0.04%	0.006%
71	9.362	2493	2495	2496	rBV	160	40	0.00%	0.001%
72	9.417	2499	2512	2531	rBV	402458	662606	71.77%	9.107%
73	9.613	2570	2573	2578	rBV2	227	290	0.03%	0.004%
74	9.636	2578	2580	2582	rVB2	191	72	0.01%	0.001%
75	9.806	2630	2633	2635	rBV	261	160	0.02%	0.002%
76	10.015	2696	2698	2700	rBV	195	119	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049005.D
 Acq On : 10 Jun 2022 18:37
 Operator : SY/MD
 Sample : N3254-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	10.279	2777	2780	2781	rBV	164	108	0.01%	0.001%
78	10.639	2889	2892	2897	rVB2	398	260	0.03%	0.004%
79	10.758	2916	2929	2952	rBV	347104	565932	61.30%	7.779%
80	10.890	2961	2970	2977	rBV5	849	1378	0.15%	0.019%
81	10.964	2991	2993	2996	rVB	313	129	0.01%	0.002%
82	11.610	3190	3194	3199	rBV2	513	553	0.06%	0.008%
83	11.813	3245	3257	3275	rBV	355387	565938	61.30%	7.779%
84	12.195	3362	3376	3399	rBV	372721	612957	66.39%	8.425%
85	12.677	3523	3526	3529	rBV3	526	415	0.04%	0.006%
86	13.221	3693	3695	3698	rBV2	707	569	0.06%	0.008%
87	13.362	3736	3739	3744	rBV2	479	415	0.04%	0.006%




Sum of corrected areas: 7275506

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049005.D
Acq On : 10 Jun 2022 18:37
Operator : SY/MD
Sample : N3254-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

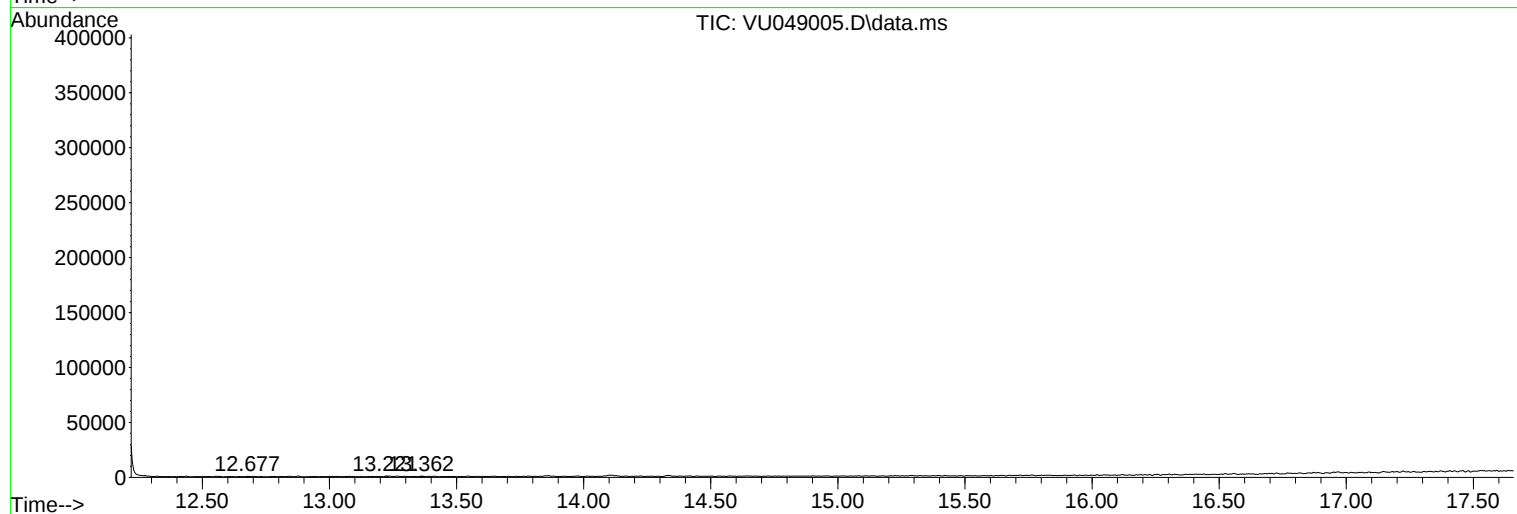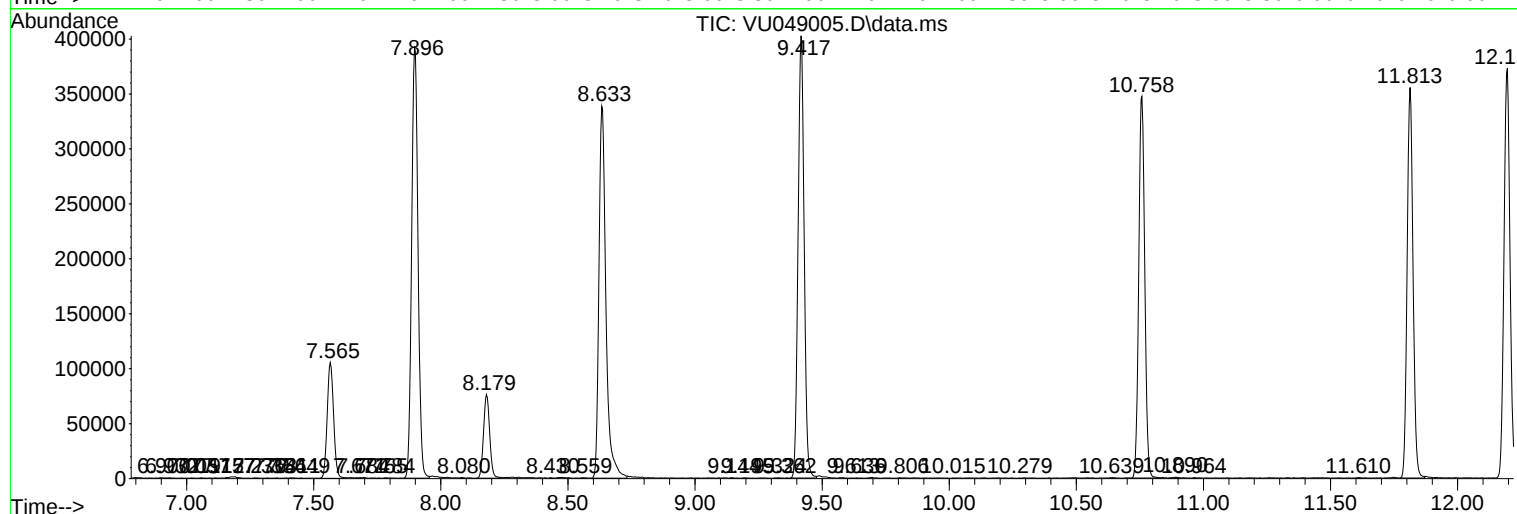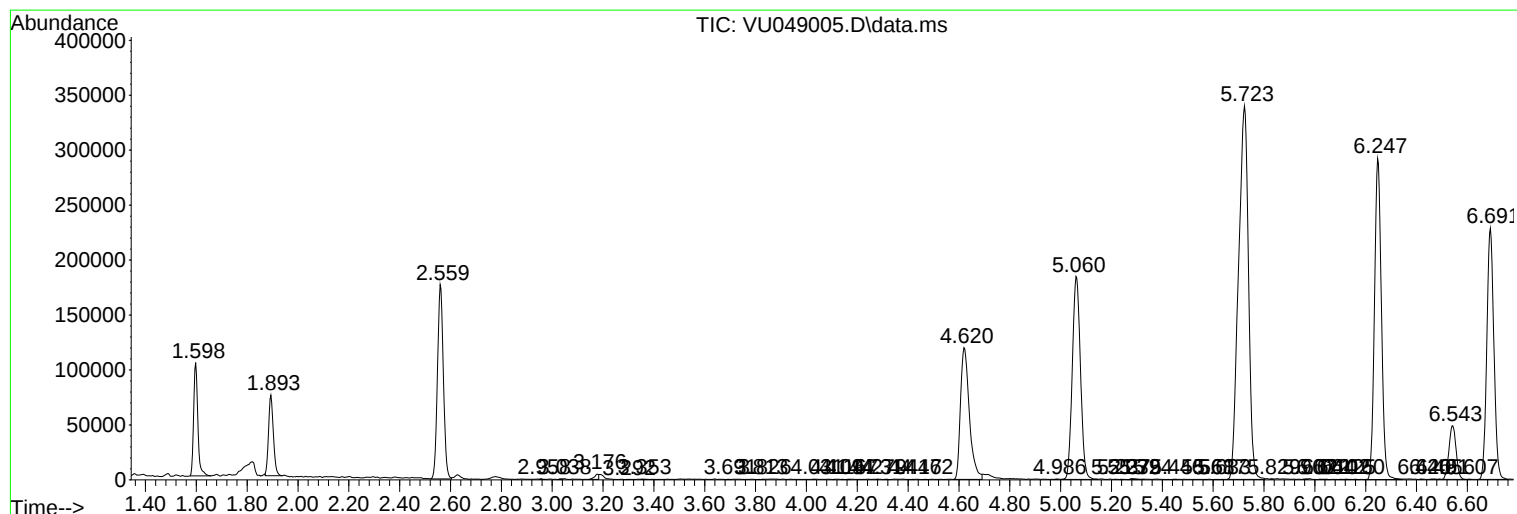

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049005.D
Acq On : 10 Jun 2022 18:37
Operator : SY/MD
Sample : N3254-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049005.D
Acq On : 10 Jun 2022 18:37
Operator : SY/MD
Sample : N3254-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc