

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049006.D
 Acq On : 10 Jun 2022 19:01
 Operator : SY/MD
 Sample : N3254-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	120207	134295	13.20%	1.624%
2	1.887	163	170	185	rVB	82963	112932	11.10%	1.366%
3	2.559	367	379	394	rBV	197770	323613	31.81%	3.914%
4	2.735	431	434	436	rBV	250	167	0.02%	0.002%
5	2.835	463	465	468	rVB2	412	209	0.02%	0.003%
6	2.854	468	471	473	rBV	126	91	0.01%	0.001%
7	2.996	512	515	517	rBV	235	157	0.02%	0.002%
8	3.038	524	528	529	rBV	473	342	0.03%	0.004%
9	3.067	534	537	540	rBV	231	151	0.01%	0.002%
10	3.176	563	571	572	rBV2	1378	1432	0.14%	0.017%
11	3.317	611	615	619	rBV2	467	392	0.04%	0.005%
12	3.398	635	640	643	rBV2	397	392	0.04%	0.005%
13	3.539	680	684	688	rBV2	239	273	0.03%	0.003%
14	3.703	732	735	741	rBV	237	193	0.02%	0.002%
15	3.903	794	797	799	rBV2	103	62	0.01%	0.001%
16	3.928	802	805	806	rBV	125	65	0.01%	0.001%
17	3.980	815	821	823	rBV2	171	198	0.02%	0.002%
18	4.057	842	845	850	rBV	183	119	0.01%	0.001%
19	4.083	850	853	854	rBV	103	59	0.01%	0.001%
20	4.462	964	971	974	rBV2	431	419	0.04%	0.005%
21	4.501	981	983	986	rBV	211	142	0.01%	0.002%
22	4.568	1001	1004	1006	rBV2	173	111	0.01%	0.001%
23	4.620	1007	1020	1043	rBV	131017	317191	31.18%	3.836%
24	5.060	1141	1157	1177	rBV	196433	435498	42.81%	5.267%
25	5.173	1189	1192	1194	rBV2	256	156	0.02%	0.002%
26	5.214	1203	1205	1207	rBV	215	119	0.01%	0.001%
27	5.285	1223	1227	1229	rBV3	380	359	0.04%	0.004%
28	5.362	1248	1251	1254	rBV2	302	198	0.02%	0.002%
29	5.378	1254	1256	1263	rVB2	252	279	0.03%	0.003%
30	5.430	1269	1272	1273	rBV	225	127	0.01%	0.002%
31	5.449	1277	1278	1280	rVB	241	96	0.01%	0.001%
32	5.494	1286	1292	1294	rBV2	216	258	0.03%	0.003%
33	5.562	1310	1313	1315	rBV	249	162	0.02%	0.002%
34	5.594	1320	1323	1326	rVB	159	86	0.01%	0.001%
35	5.610	1326	1328	1329	rBV	103	48	0.00%	0.001%
36	5.723	1342	1363	1390	rBV2	375284	1017395	100.00%	12.304%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049006.D
 Acq On : 10 Jun 2022 19:01
 Operator : SY/MD
 Sample : N3254-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.938	1426	1430	1431	rBV2	234	176	0.02%	0.002%
38	5.964	1436	1438	1441	rVV2	534	367	0.04%	0.004%
39	6.079	1471	1474	1477	rBV2	223	149	0.01%	0.002%
40	6.247	1512	1526	1547	rBV	354461	664869	65.35%	8.041%
41	6.468	1592	1595	1597	rVB2	251	149	0.01%	0.002%
42	6.485	1597	1600	1604	rBV2	294	195	0.02%	0.002%
43	6.533	1604	1615	1629	rVV9	4669	8612	0.85%	0.104%
44	6.587	1629	1632	1635	rVB	412	254	0.02%	0.003%
45	6.690	1650	1664	1687	rBV	246570	474075	46.60%	5.733%
46	6.813	1697	1702	1704	rBV3	906	691	0.07%	0.008%
47	6.841	1709	1711	1715	rVB2	279	179	0.02%	0.002%
48	6.861	1715	1717	1718	rBV	265	92	0.01%	0.001%
49	7.044	1770	1774	1775	rBV2	225	147	0.01%	0.002%
50	7.121	1795	1798	1800	rBV2	202	141	0.01%	0.002%
51	7.179	1805	1816	1828	rVV7	2862	5901	0.58%	0.071%
52	7.288	1847	1850	1852	rBV	123	77	0.01%	0.001%
53	7.439	1894	1897	1901	rBV2	219	152	0.01%	0.002%
54	7.565	1921	1936	1954	rBV2	128270	226415	22.25%	2.738%
55	7.690	1966	1975	1978	rBV5	1371	2085	0.20%	0.025%
56	7.780	2000	2003	2006	rVB	316	209	0.02%	0.003%
57	7.806	2007	2011	2016	rVV2	429	333	0.03%	0.004%
58	7.896	2026	2039	2057	rBV	435539	749978	73.72%	9.070%
59	8.179	2115	2127	2140	rBV2	92454	153006	15.04%	1.850%
60	8.388	2191	2192	2193	rBV	269	85	0.01%	0.001%
61	8.636	2255	2269	2298	rBV2	372051	702728	69.07%	8.499%
62	8.825	2324	2328	2329	rBV2	371	236	0.02%	0.003%
63	8.896	2348	2350	2353	rVB2	408	174	0.02%	0.002%
64	8.915	2353	2356	2357	rBV	148	90	0.01%	0.001%
65	8.944	2363	2365	2366	rBV	131	38	0.00%	0.000%
66	8.957	2366	2369	2373	rVB2	374	267	0.03%	0.003%
67	8.976	2373	2375	2376	rBV	234	82	0.01%	0.001%
68	9.050	2394	2398	2401	rBV	234	197	0.02%	0.002%
69	9.082	2407	2408	2410	rBV	305	91	0.01%	0.001%
70	9.102	2411	2414	2419	rBV2	245	316	0.03%	0.004%
71	9.140	2424	2426	2429	rBV	228	146	0.01%	0.002%
72	9.198	2441	2444	2446	rBV	222	126	0.01%	0.002%
73	9.417	2498	2512	2529	rBV	505986	823539	80.95%	9.960%
74	9.806	2629	2633	2638	rBV	360	321	0.03%	0.004%
75	10.131	2732	2734	2736	rBV3	273	93	0.01%	0.001%
76	10.198	2750	2755	2757	rBV2	301	310	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049006.D
 Acq On : 10 Jun 2022 19:01
 Operator : SY/MD
 Sample : N3254-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	10.253	2769	2772	2774	rBV2	219	166	0.02%	0.002%
78	10.291	2779	2784	2786	rBV2	357	327	0.03%	0.004%
79	10.394	2813	2816	2818	rBV	213	129	0.01%	0.002%
80	10.494	2843	2847	2853	rBV2	375	359	0.04%	0.004%
81	10.671	2897	2902	2914	rVB6	1249	1722	0.17%	0.021%
82	10.758	2915	2929	2950	rBV	401252	643482	63.25%	7.782%
83	10.986	2999	3000	3001	rVB	322	62	0.01%	0.001%
84	11.111	3037	3039	3045	rBV2	425	278	0.03%	0.003%
85	11.574	3181	3183	3186	rBV2	246	194	0.02%	0.002%
86	11.693	3218	3220	3222	rBV	255	124	0.01%	0.001%
87	11.725	3227	3230	3232	rVB2	244	115	0.01%	0.001%
88	11.745	3232	3236	3239	rBV3	431	493	0.05%	0.006%
89	11.812	3245	3257	3282	rBV	461877	734836	72.23%	8.887%
90	12.195	3363	3376	3395	rBV	440769	720599	70.83%	8.715%
91	12.340	3418	3421	3428	rBV2	339	291	0.03%	0.004%
92	12.420	3443	3446	3448	rBV	268	194	0.02%	0.002%
93	12.767	3552	3554	3556	rVB	314	77	0.01%	0.001%
94	12.854	3578	3581	3584	rBV2	284	240	0.02%	0.003%




Sum of corrected areas: 8268565

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049006.D
Acq On : 10 Jun 2022 19:01
Operator : SY/MD
Sample : N3254-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

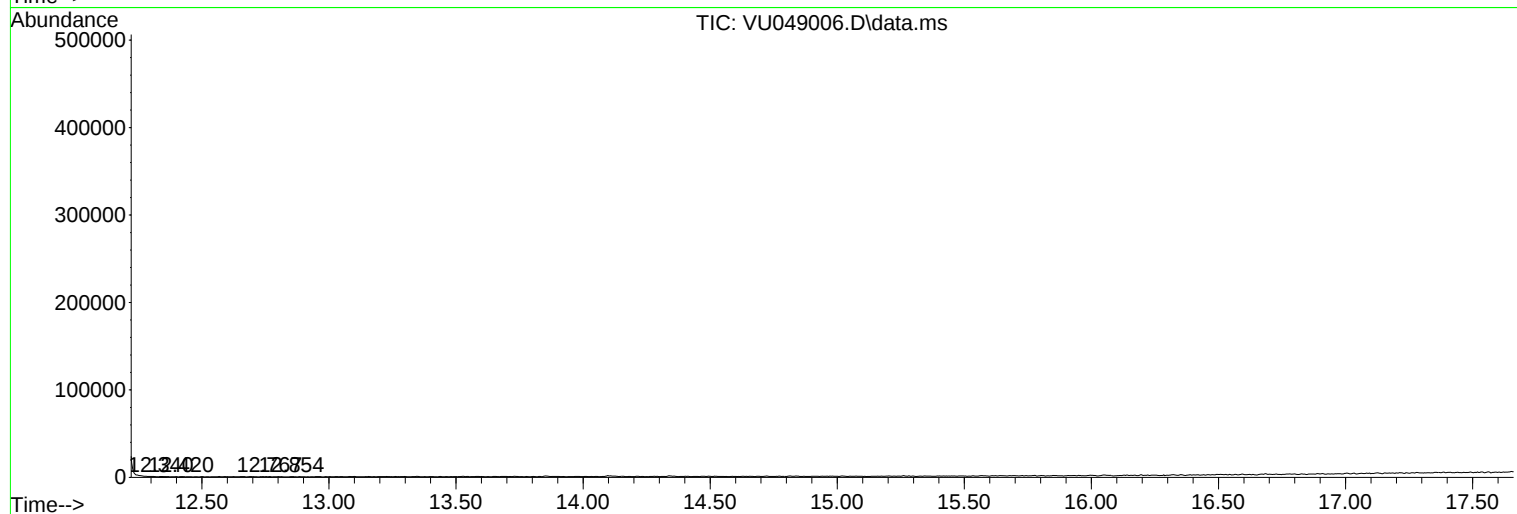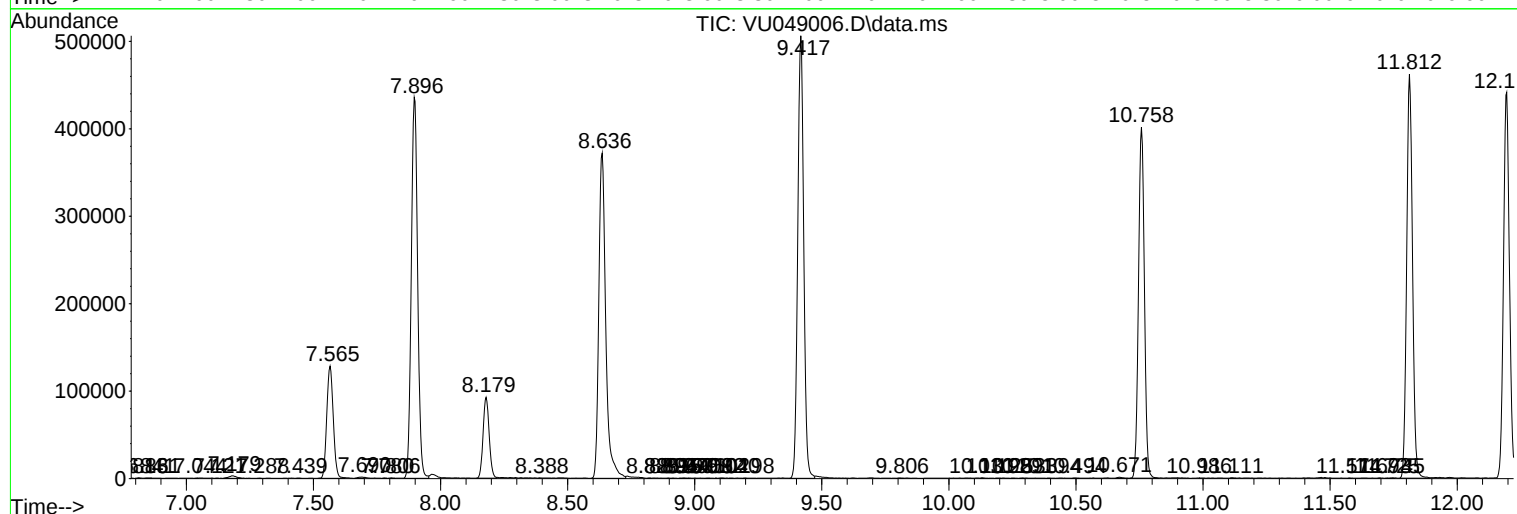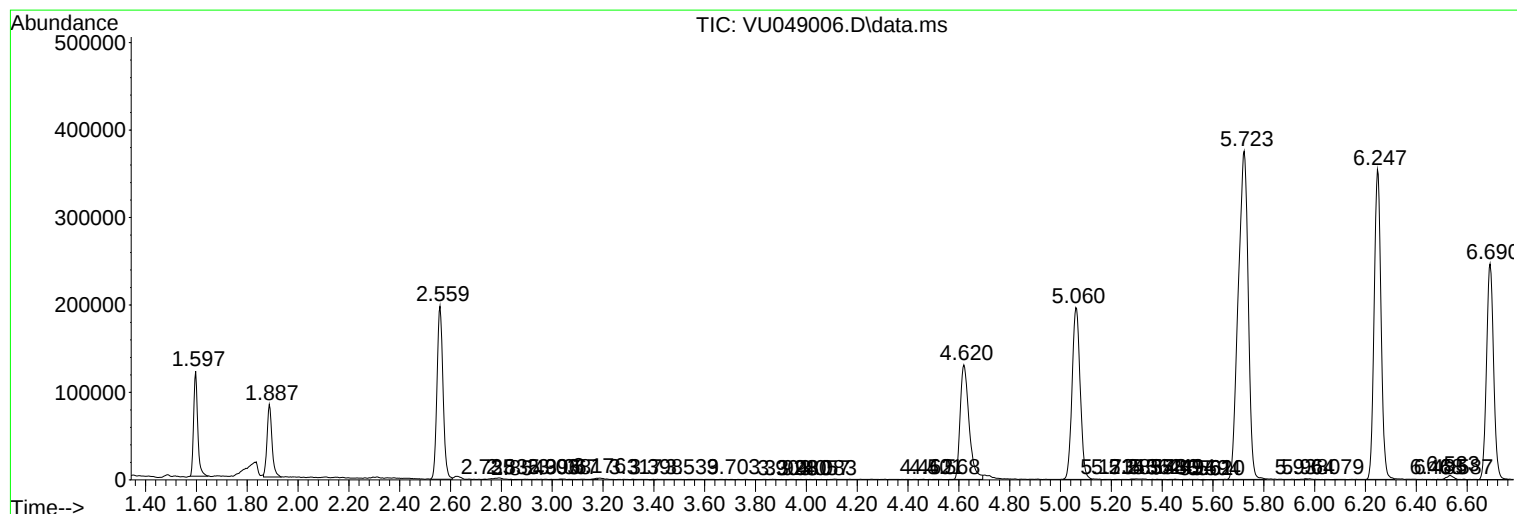

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049006.D
Acq On : 10 Jun 2022 19:01
Operator : SY/MD
Sample : N3254-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049006.D
Acq On : 10 Jun 2022 19:01
Operator : SY/MD
Sample : N3254-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc