

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049008.D
 Acq On : 10 Jun 2022 19:48
 Operator : SY/MD
 Sample : N3254-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	40	44	52	rVB3	5864	7273	0.71%	0.088%
2	1.597	73	80	96	rBV	117047	132936	12.92%	1.605%
3	1.896	165	173	191	rVB	84929	114415	11.12%	1.381%
4	2.498	356	360	362	rBV2	499	322	0.03%	0.004%
5	2.562	368	380	395	rBV	200216	326447	31.73%	3.941%
6	2.681	415	417	420	rVB	415	196	0.02%	0.002%
7	2.755	437	440	442	rBV	479	299	0.03%	0.004%
8	2.816	457	459	468	rVB2	220	233	0.02%	0.003%
9	2.925	488	493	495	rBV2	214	205	0.02%	0.002%
10	2.958	500	503	508	rVB2	536	525	0.05%	0.006%
11	3.041	524	529	538	rVB3	1155	1493	0.15%	0.018%
12	3.170	566	569	571	rBV	645	506	0.05%	0.006%
13	3.237	586	590	595	rVV2	313	265	0.03%	0.003%
14	3.388	635	637	641	rBV	385	339	0.03%	0.004%
15	3.832	767	775	778	rBV2	398	510	0.05%	0.006%
16	4.244	901	903	908	rVB2	301	201	0.02%	0.002%
17	4.318	924	926	929	rVB	530	212	0.02%	0.003%
18	4.340	929	933	938	rBV2	308	368	0.04%	0.004%
19	4.372	938	943	949	rVV2	211	267	0.03%	0.003%
20	4.549	994	998	1001	rBV2	201	187	0.02%	0.002%
21	4.620	1007	1020	1045	rBV2	133221	322393	31.33%	3.892%
22	5.064	1140	1158	1181	rBV	196126	431790	41.96%	5.212%
23	5.192	1195	1198	1201	rBV2	355	212	0.02%	0.003%
24	5.228	1206	1209	1213	rVB	268	200	0.02%	0.002%
25	5.285	1223	1227	1229	rBV2	588	462	0.04%	0.006%
26	5.334	1239	1242	1244	rBV2	397	290	0.03%	0.004%
27	5.530	1297	1303	1306	rBV	258	296	0.03%	0.004%
28	5.723	1342	1363	1388	rBV2	379296	1028982	100.00%	12.421%
29	5.829	1394	1396	1405	rVB3	329	439	0.04%	0.005%
30	5.967	1437	1439	1444	rVV	493	451	0.04%	0.005%
31	6.121	1485	1487	1492	rVB3	325	298	0.03%	0.004%
32	6.247	1512	1526	1546	rVV	370859	705811	68.59%	8.520%
33	6.388	1567	1570	1573	rVB2	312	213	0.02%	0.003%
34	6.420	1577	1580	1585	rBV2	228	272	0.03%	0.003%
35	6.539	1604	1617	1630	rVV8	21608	41864	4.07%	0.505%
36	6.591	1630	1633	1636	rVB2	629	414	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049008.D
 Acq On : 10 Jun 2022 19:48
 Operator : SY/MD
 Sample : N3254-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.690	1650	1664	1688	rBV	255396	485376	47.17%	5.859%
38	6.945	1737	1743	1746	rBV2	382	459	0.04%	0.006%
39	7.054	1773	1777	1782	rBV	447	358	0.03%	0.004%
40	7.179	1809	1816	1828	rVB5	2405	4635	0.45%	0.056%
41	7.417	1886	1890	1896	rVB2	264	239	0.02%	0.003%
42	7.565	1923	1936	1952	rBV	128026	222631	21.64%	2.687%
43	7.690	1968	1975	1983	rVB5	1389	2022	0.20%	0.024%
44	7.896	2025	2039	2056	rBV	431797	749925	72.88%	9.052%
45	8.044	2082	2085	2087	rVB2	437	277	0.03%	0.003%
46	8.179	2114	2127	2141	rBV2	91206	151658	14.74%	1.831%
47	8.324	2170	2172	2176	rVB2	415	201	0.02%	0.002%
48	8.633	2252	2268	2299	rBV2	357596	677800	65.87%	8.182%
49	8.787	2314	2316	2320	rVB4	787	540	0.05%	0.007%
50	8.880	2340	2345	2350	rBV2	307	291	0.03%	0.004%
51	9.070	2401	2404	2409	rBV2	264	216	0.02%	0.003%
52	9.166	2429	2434	2440	rVV3	410	459	0.04%	0.006%
53	9.314	2477	2480	2483	rVB2	349	217	0.02%	0.003%
54	9.333	2483	2486	2487	rBV	303	189	0.02%	0.002%
55	9.417	2499	2512	2529	rBV	514705	857735	83.36%	10.354%
56	9.636	2576	2580	2583	rBV2	281	266	0.03%	0.003%
57	9.694	2592	2598	2602	rBV2	525	529	0.05%	0.006%
58	9.758	2613	2618	2622	rBV2	168	198	0.02%	0.002%
59	9.944	2673	2676	2681	rBV2	278	210	0.02%	0.003%
60	10.179	2745	2749	2760	rVB2	274	466	0.05%	0.006%
61	10.301	2783	2787	2794	rVB2	265	304	0.03%	0.004%
62	10.359	2801	2805	2806	rBV	292	187	0.02%	0.002%
63	10.517	2849	2854	2856	rBV	211	205	0.02%	0.002%
64	10.591	2874	2877	2880	rBV2	321	198	0.02%	0.002%
65	10.607	2880	2882	2888	rBV	300	196	0.02%	0.002%
66	10.636	2888	2891	2893	rVB2	527	259	0.03%	0.003%
67	10.671	2893	2902	2910	rBV4	996	1640	0.16%	0.020%
68	10.758	2916	2929	2948	rVV	379197	605778	58.87%	7.312%
69	11.079	3026	3029	3033	rBV2	247	198	0.02%	0.002%
70	11.121	3040	3042	3045	rVB2	522	238	0.02%	0.003%
71	11.343	3109	3111	3117	rVB2	246	244	0.02%	0.003%
72	11.404	3127	3130	3133	rVB	398	227	0.02%	0.003%
73	11.443	3139	3142	3145	rBV2	280	186	0.02%	0.002%
74	11.462	3146	3148	3150	rBV	431	206	0.02%	0.002%
75	11.690	3215	3219	3221	rBV2	254	199	0.02%	0.002%
76	11.719	3225	3228	3231	rBV	503	414	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049008.D
 Acq On : 10 Jun 2022 19:48
 Operator : SY/MD
 Sample : N3254-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.812	3242	3257	3273	rBV	445241	714215	69.41%	8.621%
78	11.935	3293	3295	3302	rVB4	561	576	0.06%	0.007%
79	11.973	3302	3307	3308	rBV2	841	760	0.07%	0.009%
80	12.028	3321	3324	3330	rVB2	386	388	0.04%	0.005%
81	12.192	3363	3375	3398	rBV	405257	672701	65.38%	8.120%
82	12.337	3418	3420	3425	rBV3	500	352	0.03%	0.004%
83	12.401	3436	3440	3443	rBV2	334	219	0.02%	0.003%
84	12.423	3445	3447	3453	rVB2	340	227	0.02%	0.003%
85	12.497	3467	3470	3474	rBV2	263	238	0.02%	0.003%
86	12.636	3509	3513	3518	rBV2	332	396	0.04%	0.005%
87	12.812	3564	3568	3572	rBV2	724	459	0.04%	0.006%
88	12.890	3588	3592	3596	rBV2	555	700	0.07%	0.008%
89	12.941	3605	3608	3610	rBV2	337	244	0.02%	0.003%
90	13.404	3748	3752	3754	rBV2	409	321	0.03%	0.004%
91	13.597	3810	3812	3818	rVB2	463	350	0.03%	0.004%
92	13.626	3818	3821	3822	rBV	381	209	0.02%	0.003%
93	13.697	3839	3843	3845	rBV	478	396	0.04%	0.005%
94	13.857	3888	3893	3894	rBV2	774	590	0.06%	0.007%
95	14.028	3941	3946	3950	rBV2	385	366	0.04%	0.004%
96	14.208	3999	4002	4005	rBV	437	371	0.04%	0.004%
97	14.449	4075	4077	4081	rVB2	407	251	0.02%	0.003%
98	14.819	4190	4192	4195	rBV	449	235	0.02%	0.003%
99	14.941	4228	4230	4233	rBV2	516	291	0.03%	0.004%
100	15.944	4540	4542	4544	rBV2	573	285	0.03%	0.003%




Sum of corrected areas: 8284302

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049008.D
Acq On : 10 Jun 2022 19:48
Operator : SY/MD
Sample : N3254-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

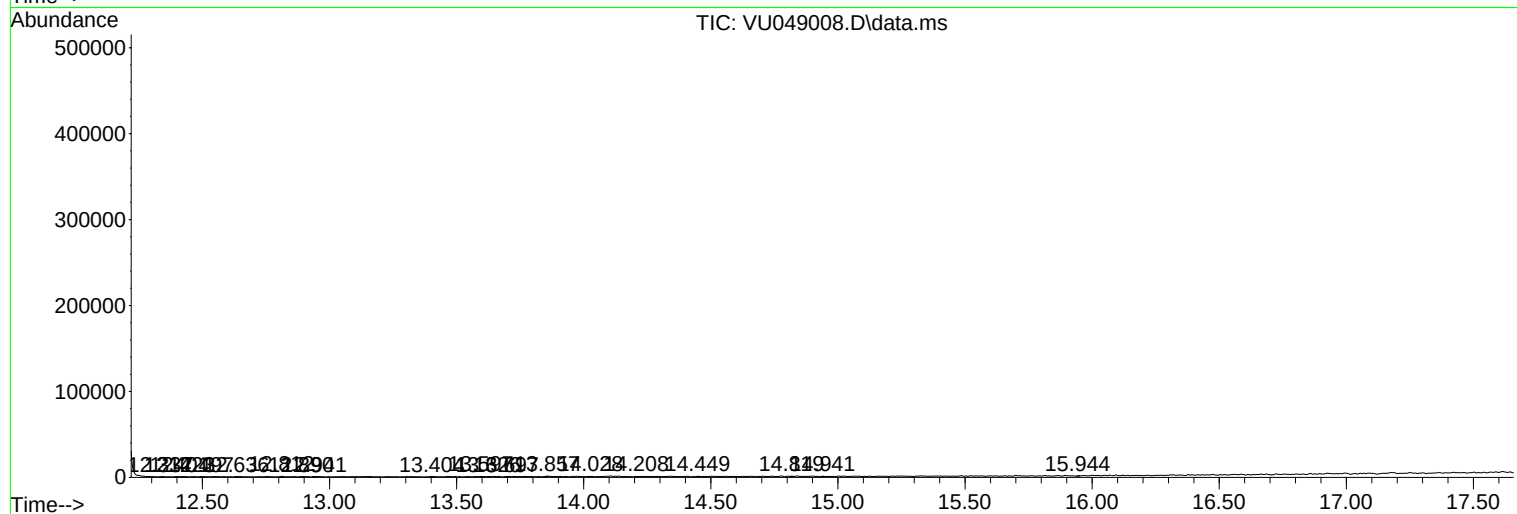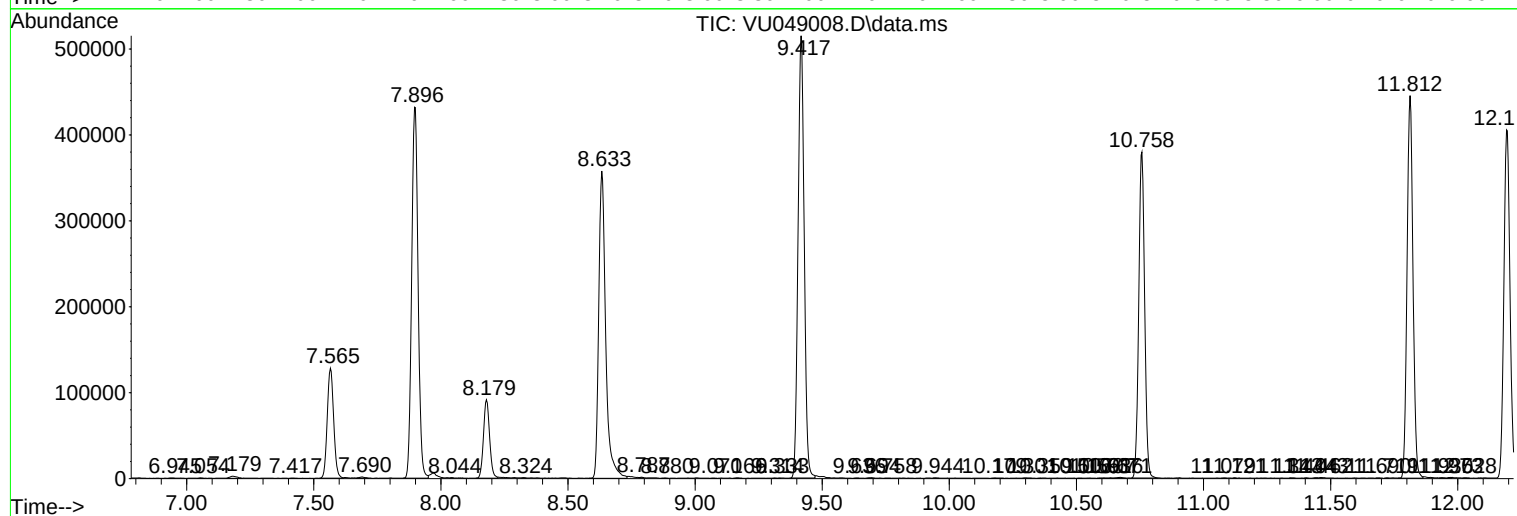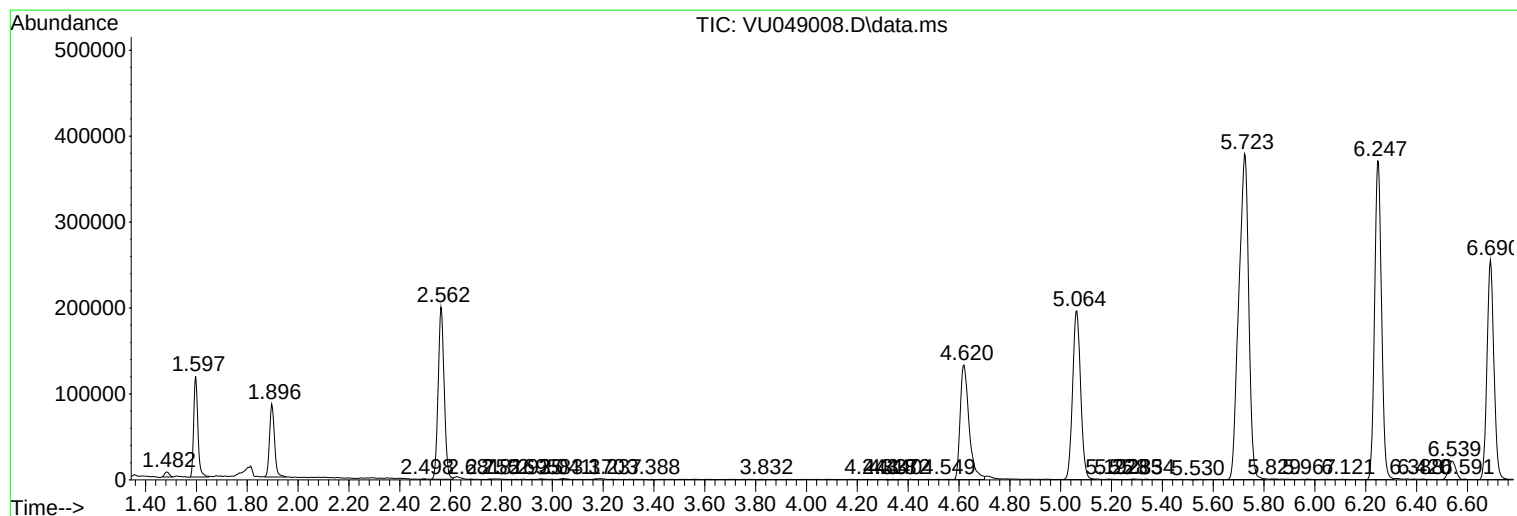

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049008.D
Acq On : 10 Jun 2022 19:48
Operator : SY/MD
Sample : N3254-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049008.D
Acq On : 10 Jun 2022 19:48
Operator : SY/MD
Sample : N3254-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------