

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049009.D
 Acq On : 10 Jun 2022 20:12
 Operator : SY/MD
 Sample : N3254-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	40	44	50	rVB3	3263	3436	0.33%	0.041%
2	1.594	72	79	94	rBV	110574	132564	12.80%	1.579%
3	1.896	164	173	186	rBV	81349	109613	10.59%	1.306%
4	2.388	324	326	330	rBV3	703	581	0.06%	0.007%
5	2.408	330	332	345	rVB5	1243	1567	0.15%	0.019%
6	2.462	346	349	353	rVB2	621	388	0.04%	0.005%
7	2.562	367	380	394	rBV	199708	329917	31.86%	3.931%
8	2.623	395	399	411	rVB2	5267	8067	0.78%	0.096%
9	2.758	437	441	443	rBV	951	720	0.07%	0.009%
10	3.031	524	526	528	rVV	496	335	0.03%	0.004%
11	3.044	528	530	539	rVB3	718	679	0.07%	0.008%
12	3.189	565	575	580	rBV4	776	1444	0.14%	0.017%
13	3.250	591	594	596	rBV2	254	183	0.02%	0.002%
14	3.392	634	638	641	rBV2	351	277	0.03%	0.003%
15	3.578	692	696	699	rBV	261	188	0.02%	0.002%
16	3.755	747	751	754	rVB	293	257	0.02%	0.003%
17	3.781	755	759	761	rBV	397	271	0.03%	0.003%
18	4.002	822	828	829	rBV	213	212	0.02%	0.003%
19	4.330	927	930	936	rVB	217	183	0.02%	0.002%
20	4.366	936	941	945	rBV	246	254	0.02%	0.003%
21	4.446	962	966	972	rBV	281	299	0.03%	0.004%
22	4.517	985	988	991	rVV	294	201	0.02%	0.002%
23	4.543	991	996	1001	rVB	463	468	0.05%	0.006%
24	4.620	1006	1020	1043	rBV	138859	328302	31.70%	3.912%
25	4.929	1113	1116	1118	rBV2	284	214	0.02%	0.003%
26	5.060	1142	1157	1179	rBV	204778	452259	43.67%	5.389%
27	5.179	1191	1194	1198	rVB2	399	294	0.03%	0.004%
28	5.289	1224	1228	1229	rBV2	514	363	0.04%	0.004%
29	5.327	1236	1240	1242	rVB	548	455	0.04%	0.005%
30	5.350	1242	1247	1248	rBV3	483	452	0.04%	0.005%
31	5.427	1264	1271	1274	rBV2	330	455	0.04%	0.005%
32	5.523	1291	1301	1304	rBV2	329	536	0.05%	0.006%
33	5.723	1339	1363	1381	rBV2	377154	1035529	100.00%	12.338%
34	5.864	1405	1407	1409	rBV2	382	192	0.02%	0.002%
35	5.948	1429	1433	1435	rBV	453	215	0.02%	0.003%
36	5.964	1435	1438	1441	rBV2	576	430	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049009.D
 Acq On : 10 Jun 2022 20:12
 Operator : SY/MD
 Sample : N3254-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.035	1458	1460	1464	rVB2	350	214	0.02%	0.003%
38	6.247	1510	1526	1547	rBV	369693	700454	67.64%	8.346%
39	6.539	1602	1617	1630	rBV7	25025	49831	4.81%	0.594%
40	6.690	1649	1664	1686	rVV	255722	491967	47.51%	5.862%
41	6.768	1686	1688	1690	rVV2	504	285	0.03%	0.003%
42	6.809	1694	1701	1704	rVV2	862	757	0.07%	0.009%
43	6.883	1717	1724	1727	rBV2	299	358	0.03%	0.004%
44	6.980	1749	1754	1757	rBV2	225	253	0.02%	0.003%
45	7.182	1808	1817	1826	rBV5	2329	3719	0.36%	0.044%
46	7.327	1857	1862	1865	rVB2	297	211	0.02%	0.003%
47	7.565	1923	1936	1954	rBV	129349	226522	21.88%	2.699%
48	7.690	1969	1975	1985	rVB6	1672	2573	0.25%	0.031%
49	7.813	2010	2013	2020	rVB2	347	411	0.04%	0.005%
50	7.851	2020	2025	2026	rBV	379	328	0.03%	0.004%
51	7.896	2026	2039	2056	rBV	446533	768509	74.21%	9.157%
52	8.047	2083	2086	2088	rBV2	357	233	0.02%	0.003%
53	8.092	2096	2100	2103	rVB4	348	221	0.02%	0.003%
54	8.108	2103	2105	2111	rVB2	692	485	0.05%	0.006%
55	8.179	2111	2127	2142	rBV	93661	153574	14.83%	1.830%
56	8.334	2172	2175	2178	rBV	360	239	0.02%	0.003%
57	8.404	2195	2197	2202	rBV3	396	282	0.03%	0.003%
58	8.452	2209	2212	2213	rBV	365	214	0.02%	0.003%
59	8.571	2245	2249	2253	rVB2	245	206	0.02%	0.002%
60	8.633	2255	2268	2303	rBV2	370234	693308	66.95%	8.261%
61	8.903	2348	2352	2354	rVV2	366	236	0.02%	0.003%
62	8.983	2375	2377	2379	rVB2	414	199	0.02%	0.002%
63	9.147	2423	2428	2431	rBV2	440	404	0.04%	0.005%
64	9.221	2447	2451	2453	rBV2	261	217	0.02%	0.003%
65	9.301	2474	2476	2481	rVB2	311	268	0.03%	0.003%
66	9.417	2498	2512	2531	rBV	517696	846624	81.76%	10.087%
67	9.575	2557	2561	2565	rBV3	369	308	0.03%	0.004%
68	9.703	2595	2601	2605	rVB2	714	820	0.08%	0.010%
69	10.279	2777	2780	2782	rBV	260	188	0.02%	0.002%
70	10.417	2820	2823	2825	rBV	263	185	0.02%	0.002%
71	10.542	2857	2862	2865	rBV	396	416	0.04%	0.005%
72	10.668	2895	2901	2905	rBV4	1089	1263	0.12%	0.015%
73	10.758	2915	2929	2944	rBV	389372	622490	60.11%	7.417%
74	10.893	2969	2971	2978	rVB	653	525	0.05%	0.006%
75	10.948	2983	2988	2991	rVB2	484	363	0.04%	0.004%
76	11.147	3047	3050	3057	rVB2	467	420	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049009.D
 Acq On : 10 Jun 2022 20:12
 Operator : SY/MD
 Sample : N3254-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.189	3060	3063	3067	rBV	485	320	0.03%	0.004%
78	11.385	3121	3124	3126	rBV	272	224	0.02%	0.003%
79	11.462	3146	3148	3151	rBV2	353	193	0.02%	0.002%
80	11.658	3205	3209	3212	rBV2	358	331	0.03%	0.004%
81	11.812	3245	3257	3280	rBV	440724	714579	69.01%	8.514%
82	11.938	3293	3296	3299	rBV2	648	422	0.04%	0.005%
83	12.195	3361	3376	3396	rBV	422135	689155	66.55%	8.211%
84	12.494	3467	3469	3474	rVB2	410	189	0.02%	0.002%
85	12.735	3541	3544	3546	rBV	384	221	0.02%	0.003%
86	12.771	3553	3555	3564	rBV3	332	315	0.03%	0.004%
87	12.861	3580	3583	3589	rBV2	458	423	0.04%	0.005%
88	12.951	3608	3611	3614	rBV2	347	298	0.03%	0.004%
89	13.041	3637	3639	3643	rVB3	591	433	0.04%	0.005%
90	13.115	3660	3662	3666	rVB	461	321	0.03%	0.004%
91	13.144	3666	3671	3676	rBV2	331	458	0.04%	0.005%
92	13.253	3703	3705	3710	rVB2	385	303	0.03%	0.004%
93	13.626	3819	3821	3826	rBV2	285	209	0.02%	0.002%
94	13.677	3835	3837	3841	rVB2	384	212	0.02%	0.003%
95	13.854	3889	3892	3896	rBV3	625	513	0.05%	0.006%
96	13.890	3900	3903	3907	rBV2	389	289	0.03%	0.003%
97	14.079	3959	3962	3963	rBV	526	302	0.03%	0.004%
98	14.227	4002	4008	4009	rBV3	595	543	0.05%	0.006%
99	14.295	4026	4029	4030	rBV	341	196	0.02%	0.002%
100	15.844	4509	4511	4519	rVB4	737	675	0.07%	0.008%




Sum of corrected areas: 8393004

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049009.D
Acq On : 10 Jun 2022 20:12
Operator : SY/MD
Sample : N3254-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

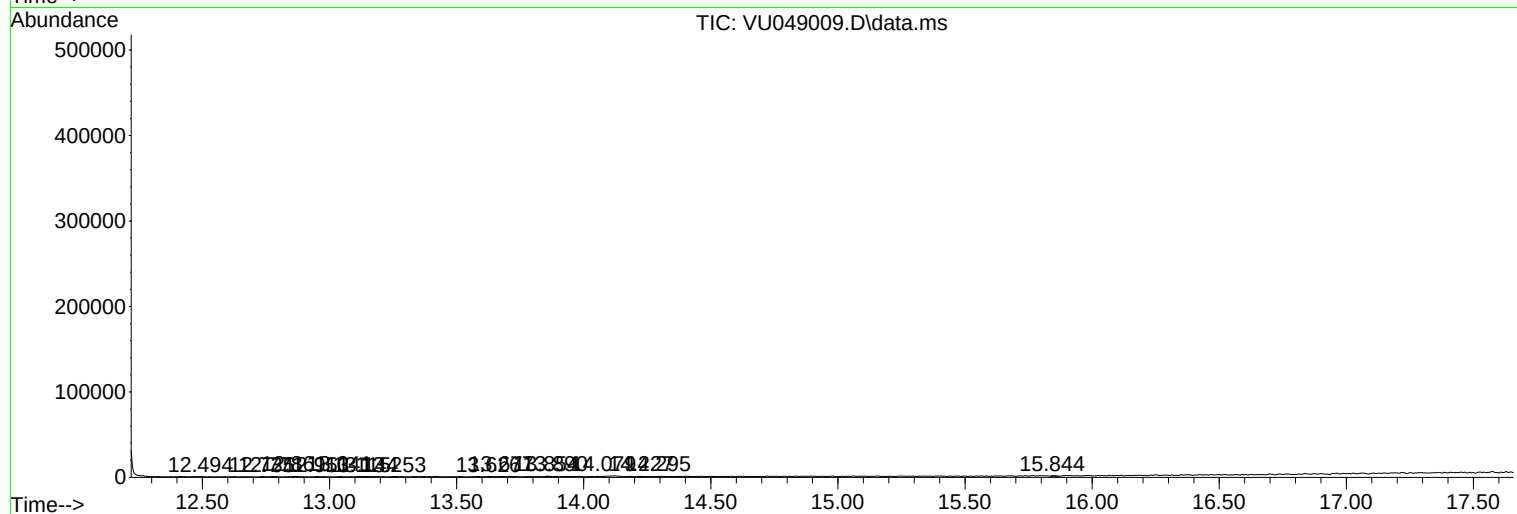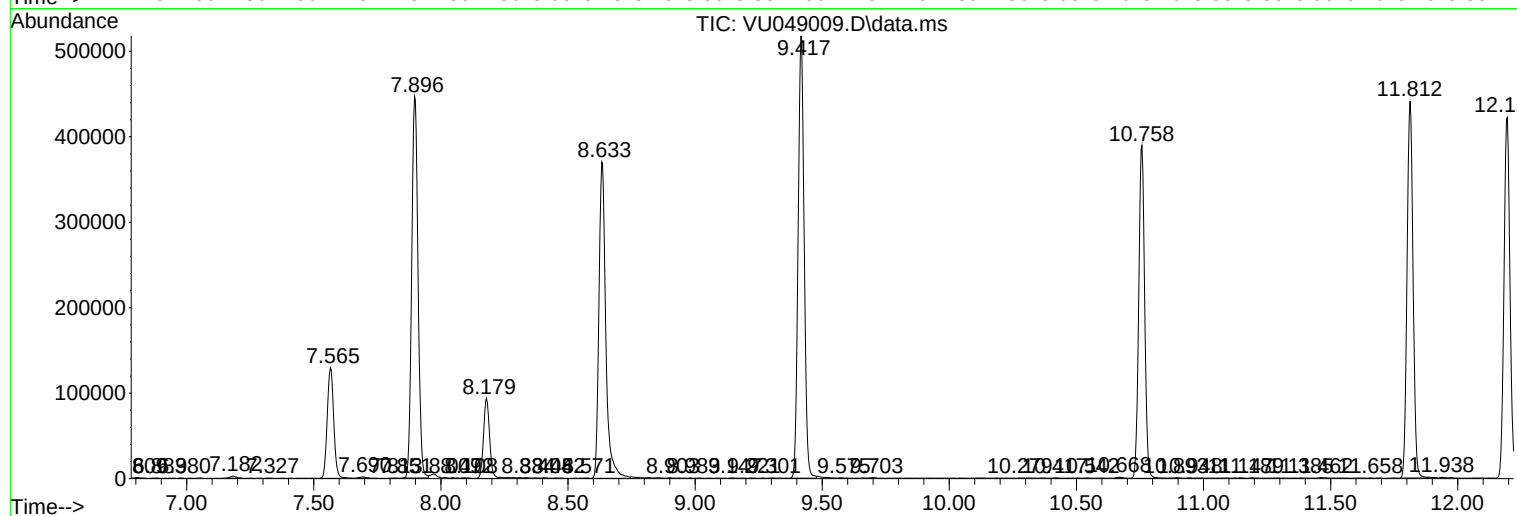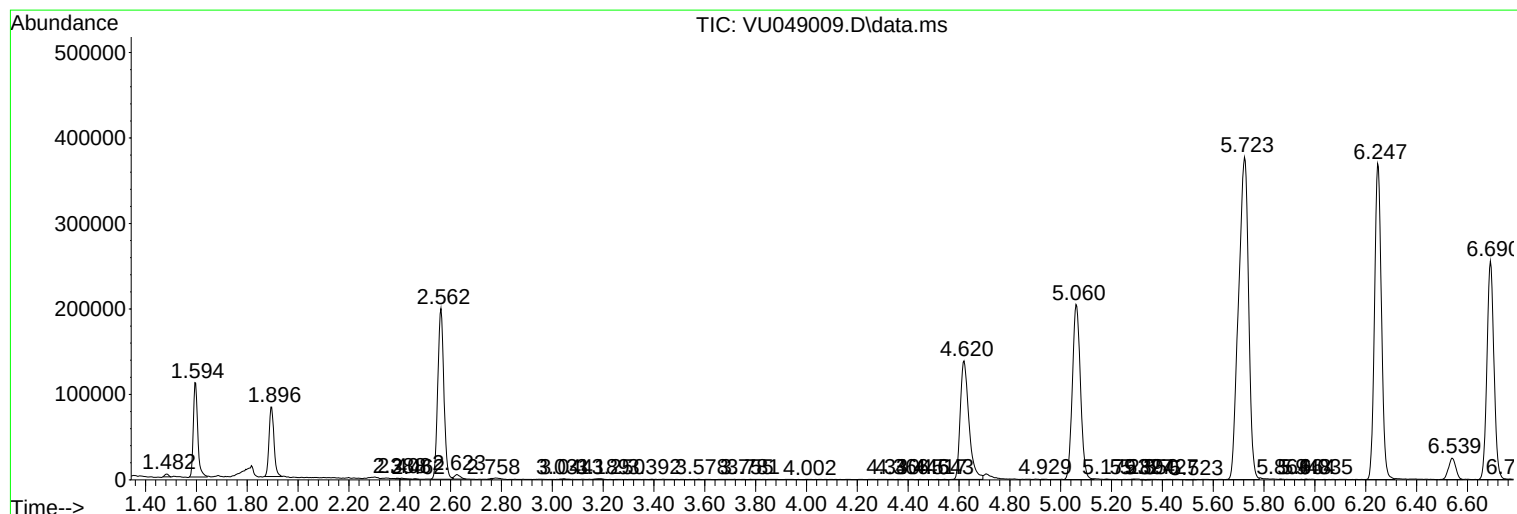

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049009.D
Acq On : 10 Jun 2022 20:12
Operator : SY/MD
Sample : N3254-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049009.D
Acq On : 10 Jun 2022 20:12
Operator : SY/MD
Sample : N3254-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------