

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049010.D
 Acq On : 10 Jun 2022 20:35
 Operator : SY/MD
 Sample : N3254-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049010.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.472	37	41	52	rVB	15856	16437	1.63%	0.209%
2	1.597	73	80	97	rVB	113156	127674	12.69%	1.621%
3	1.900	166	174	184	rBV	78781	102140	10.16%	1.297%
4	2.562	368	380	393	rBV	190999	311441	30.97%	3.954%
5	3.006	514	518	520	rBV2	350	264	0.03%	0.003%
6	3.099	545	547	549	rBV2	196	95	0.01%	0.001%
7	3.186	565	574	576	rBV3	1676	2174	0.22%	0.028%
8	3.260	592	597	600	rBV2	239	266	0.03%	0.003%
9	3.427	645	649	653	rBV2	313	270	0.03%	0.003%
10	3.584	694	698	702	rBV2	122	127	0.01%	0.002%
11	3.867	783	786	787	rBV2	148	92	0.01%	0.001%
12	3.964	812	816	819	rBV	363	242	0.02%	0.003%
13	3.993	819	825	829	rVV2	182	245	0.02%	0.003%
14	4.018	829	833	837	rVV	347	306	0.03%	0.004%
15	4.060	840	846	849	rBV2	210	231	0.02%	0.003%
16	4.108	854	861	863	rBV2	242	291	0.03%	0.004%
17	4.160	871	877	879	rBV2	249	281	0.03%	0.004%
18	4.195	884	888	889	rBV2	210	126	0.01%	0.002%
19	4.208	889	892	894	rBV	264	153	0.02%	0.002%
20	4.398	948	951	953	rBV	222	157	0.02%	0.002%
21	4.430	958	961	963	rVV2	307	205	0.02%	0.003%
22	4.440	963	964	966	rVV	347	152	0.02%	0.002%
23	4.456	966	969	972	rVB	305	188	0.02%	0.002%
24	4.494	975	981	988	rVB2	398	498	0.05%	0.006%
25	4.533	988	993	994	rBV	239	174	0.02%	0.002%
26	4.568	1001	1004	1007	rBV	232	218	0.02%	0.003%
27	4.620	1007	1020	1044	rBV	136830	322529	32.07%	4.095%
28	5.060	1142	1157	1179	rBV	196565	426516	42.41%	5.415%
29	5.263	1217	1220	1221	rBV	178	113	0.01%	0.001%
30	5.279	1221	1225	1227	rBV3	354	323	0.03%	0.004%
31	5.469	1277	1284	1287	rBV2	270	301	0.03%	0.004%
32	5.584	1316	1320	1324	rBV2	172	184	0.02%	0.002%
33	5.639	1335	1337	1342	rBV2	211	90	0.01%	0.001%
34	5.723	1342	1363	1391	rBV2	368970	1005709	100.00%	12.769%
35	5.970	1437	1440	1444	rBV3	404	333	0.03%	0.004%
36	6.022	1453	1456	1459	rVB2	386	247	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049010.D
 Acq On : 10 Jun 2022 20:35
 Operator : SY/MD
 Sample : N3254-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.054	1463	1466	1470	rBV2	173	116	0.01%	0.001%
38	6.153	1490	1497	1501	rBV2	304	368	0.04%	0.005%
39	6.247	1511	1526	1551	rBV	354602	674699	67.09%	8.566%
40	6.478	1595	1598	1600	rBV	199	155	0.02%	0.002%
41	6.491	1600	1602	1604	rVV	342	242	0.02%	0.003%
42	6.536	1606	1616	1632	rVV8	7871	16943	1.68%	0.215%
43	6.597	1632	1635	1640	rVV3	224	209	0.02%	0.003%
44	6.690	1650	1664	1689	rBV	249374	480289	47.76%	6.098%
45	6.793	1693	1696	1698	rVV2	309	194	0.02%	0.002%
46	6.809	1698	1701	1709	rVB4	795	772	0.08%	0.010%
47	6.880	1720	1723	1724	rBV	189	109	0.01%	0.001%
48	6.899	1726	1729	1736	rVB2	392	406	0.04%	0.005%
49	6.928	1736	1738	1742	rBV	201	116	0.01%	0.001%
50	6.951	1742	1745	1749	rBV2	162	155	0.02%	0.002%
51	6.973	1749	1752	1755	rVB2	227	148	0.01%	0.002%
52	7.105	1790	1793	1796	rVB	304	166	0.02%	0.002%
53	7.124	1796	1799	1800	rBV2	233	117	0.01%	0.001%
54	7.182	1809	1817	1829	rBV6	2312	3946	0.39%	0.050%
55	7.349	1866	1869	1872	rVB	295	194	0.02%	0.002%
56	7.366	1872	1874	1877	rBV2	238	110	0.01%	0.001%
57	7.404	1881	1886	1888	rBV2	175	137	0.01%	0.002%
58	7.427	1890	1893	1897	rVB2	239	181	0.02%	0.002%
59	7.481	1907	1910	1912	rBV2	147	100	0.01%	0.001%
60	7.565	1924	1936	1952	rBV	127561	220273	21.90%	2.797%
61	7.690	1968	1975	1978	rBV4	1240	1594	0.16%	0.020%
62	7.896	2025	2039	2056	rBV	429084	734872	73.07%	9.330%
63	8.128	2109	2111	2114	rBV	178	95	0.01%	0.001%
64	8.179	2116	2127	2145	rVV2	91472	151985	15.11%	1.930%
65	8.452	2209	2212	2213	rBV	269	180	0.02%	0.002%
66	8.504	2225	2228	2231	rBV2	232	170	0.02%	0.002%
67	8.558	2244	2245	2246	rBV	260	84	0.01%	0.001%
68	8.632	2256	2268	2304	rBV2	350649	669832	66.60%	8.504%
69	9.060	2397	2401	2408	rBV	298	359	0.04%	0.005%
70	9.095	2410	2412	2418	rVV2	127	105	0.01%	0.001%
71	9.259	2461	2463	2465	rBV	176	92	0.01%	0.001%
72	9.292	2471	2473	2476	rVB2	285	120	0.01%	0.002%
73	9.333	2483	2486	2488	rBV2	280	171	0.02%	0.002%
74	9.417	2499	2512	2546	rBV	475996	797158	79.26%	10.121%
75	9.558	2553	2556	2557	rBV2	338	191	0.02%	0.002%
76	9.816	2635	2636	2639	rBV	180	89	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049010.D
 Acq On : 10 Jun 2022 20:35
 Operator : SY/MD
 Sample : N3254-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.829	2639	2640	2642	rBV	210	121	0.01%	0.002%
78	9.896	2658	2661	2665	rBV2	181	147	0.01%	0.002%
79	10.038	2702	2705	2708	rBV2	240	188	0.02%	0.002%
80	10.314	2788	2791	2792	rBV	180	103	0.01%	0.001%
81	10.353	2800	2803	2805	rBV2	236	175	0.02%	0.002%
82	10.459	2831	2836	2841	rBV2	344	344	0.03%	0.004%
83	10.491	2843	2846	2852	rVB2	351	350	0.03%	0.004%
84	10.574	2869	2872	2875	rBV2	300	206	0.02%	0.003%
85	10.639	2890	2892	2894	rBV	195	94	0.01%	0.001%
86	10.671	2894	2902	2907	rVV3	994	1220	0.12%	0.015%
87	10.713	2911	2915	2916	rBV	311	190	0.02%	0.002%
88	10.758	2916	2929	2950	rVV	369230	602045	59.86%	7.644%
89	11.031	3007	3014	3017	rBV2	452	577	0.06%	0.007%
90	11.111	3036	3039	3041	rBV2	306	203	0.02%	0.003%
91	11.124	3041	3043	3045	rVV	296	133	0.01%	0.002%
92	11.169	3055	3057	3059	rBV	276	159	0.02%	0.002%
93	11.510	3159	3163	3164	rBV2	345	243	0.02%	0.003%
94	11.812	3244	3257	3279	rBV	366681	588761	58.54%	7.475%
95	12.195	3363	3376	3396	rBV	366868	601079	59.77%	7.631%
96	12.372	3426	3431	3438	rVB2	505	594	0.06%	0.008%
97	12.401	3438	3440	3443	rBV2	291	195	0.02%	0.002%
98	12.439	3449	3452	3455	rBV	512	389	0.04%	0.005%
99	13.986	3930	3933	3936	rBV2	509	423	0.04%	0.005%
100	14.089	3962	3965	3966	rBV	628	389	0.04%	0.005%




Sum of corrected areas: 7876362

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049010.D
Acq On : 10 Jun 2022 20:35
Operator : SY/MD
Sample : N3254-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

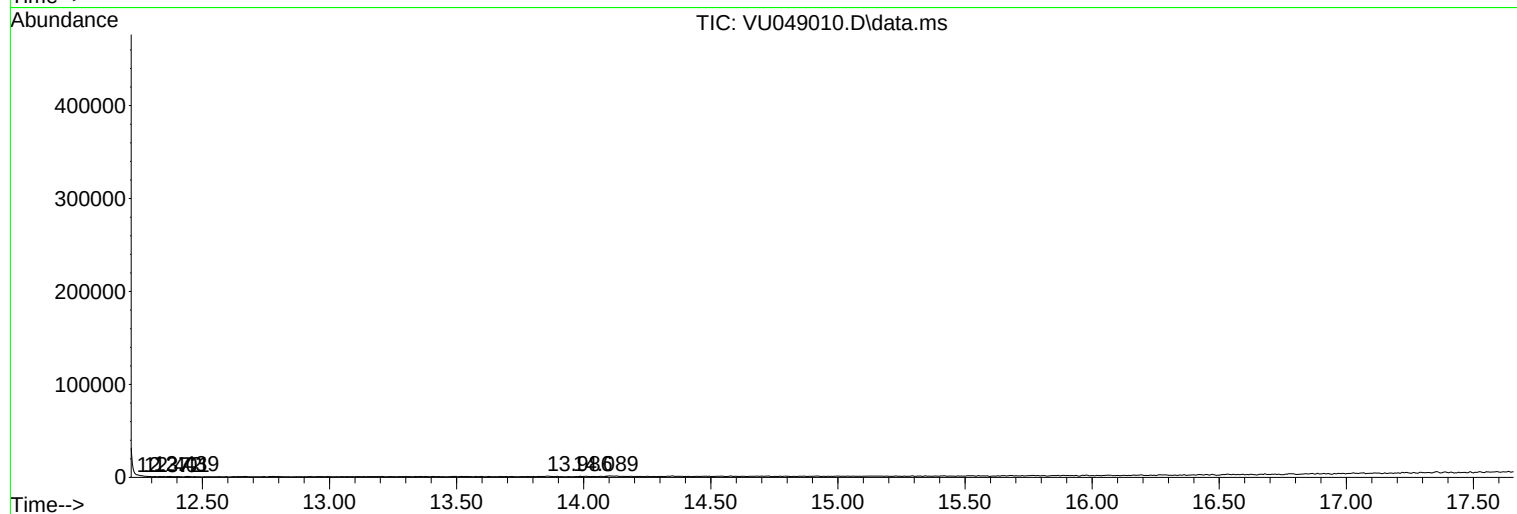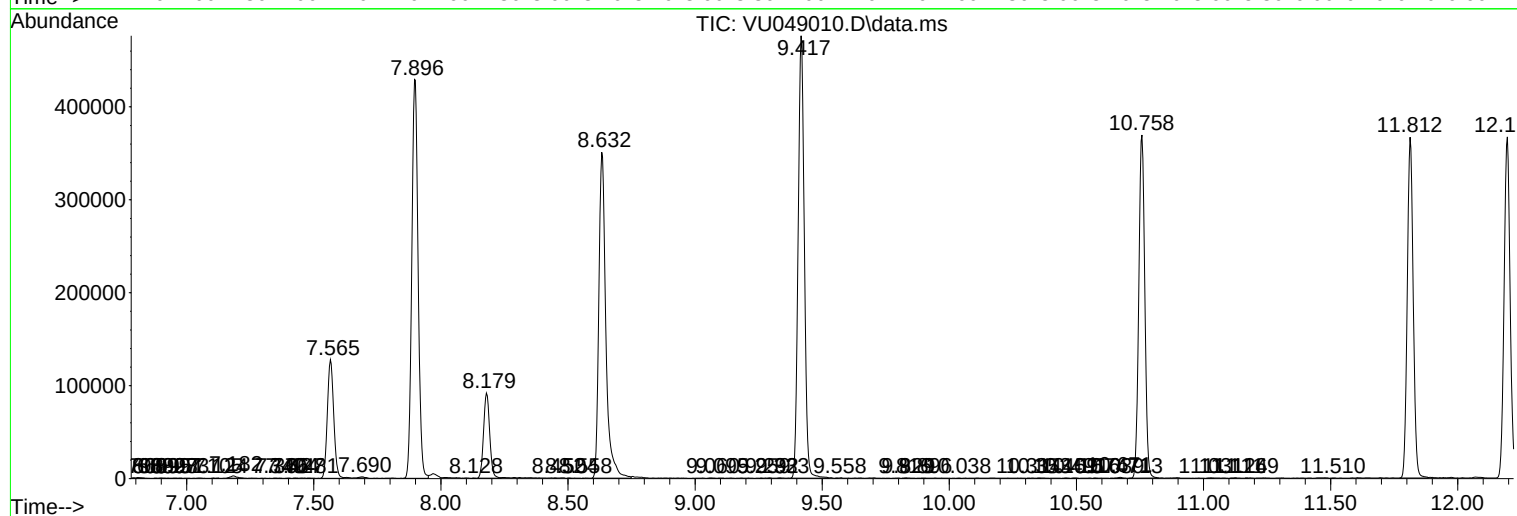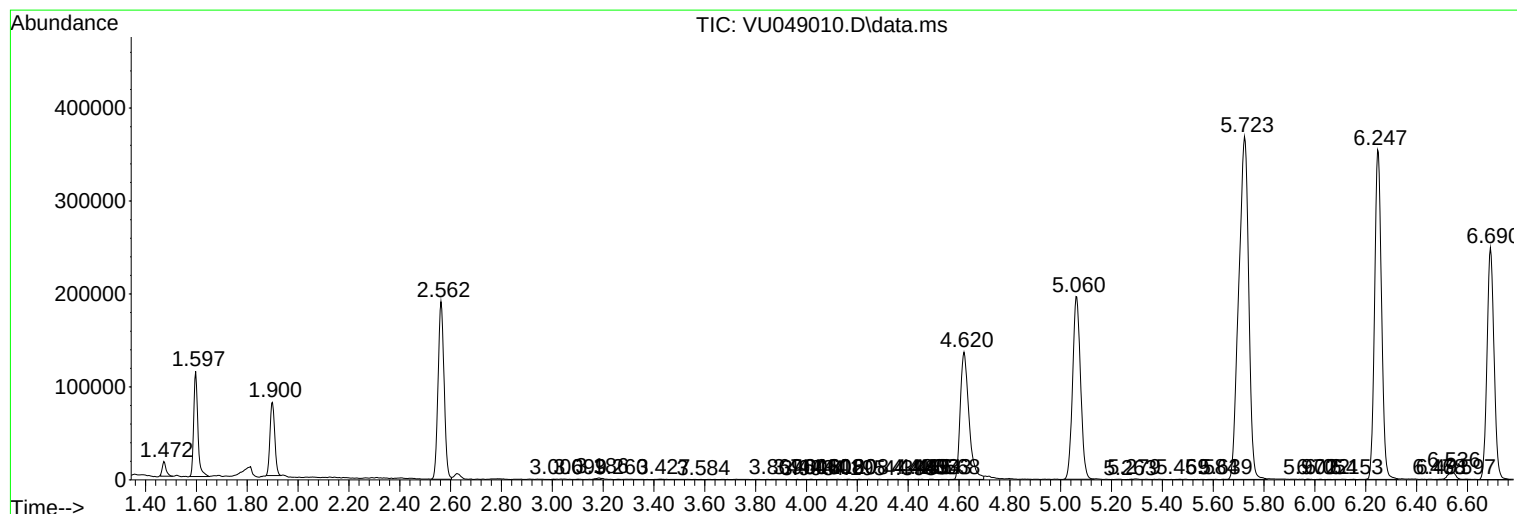

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049010.D
Acq On : 10 Jun 2022 20:35
Operator : SY/MD
Sample : N3254-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049010.D
Acq On : 10 Jun 2022 20:35
Operator : SY/MD
Sample : N3254-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc