

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049011.D
 Acq On : 10 Jun 2022 20:59
 Operator : SY/MD
 Sample : N3254-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	40	46	52	rBV3	3063	3611	0.36%	0.045%
2	1.597	73	80	95	rVB	112245	122458	12.34%	1.522%
3	1.906	167	176	191	rVB	82525	108848	10.97%	1.353%
4	2.565	369	381	392	rVV	189542	308934	31.14%	3.840%
5	2.623	393	399	413	rVB2	25310	39002	3.93%	0.485%
6	2.761	430	442	453	rBV5	1646	3545	0.36%	0.044%
7	2.880	476	479	484	rVB2	354	287	0.03%	0.004%
8	2.915	487	490	494	rVB	456	283	0.03%	0.004%
9	2.944	496	499	502	rBV3	361	295	0.03%	0.004%
10	3.028	523	525	529	rVB3	256	204	0.02%	0.003%
11	3.186	563	574	585	rBV3	1953	4195	0.42%	0.052%
12	3.356	622	627	630	rBV	363	297	0.03%	0.004%
13	3.491	666	669	675	rVB	247	214	0.02%	0.003%
14	3.948	807	811	814	rBV2	430	300	0.03%	0.004%
15	4.015	830	832	837	rVB2	304	230	0.02%	0.003%
16	4.054	840	844	847	rBV	330	335	0.03%	0.004%
17	4.166	875	879	884	rBV2	213	190	0.02%	0.002%
18	4.620	1007	1020	1044	rBV	129087	311077	31.36%	3.867%
19	4.829	1084	1085	1092	rVB3	668	307	0.03%	0.004%
20	4.899	1104	1107	1109	rBV2	340	232	0.02%	0.003%
21	4.948	1116	1122	1126	rBV3	321	452	0.05%	0.006%
22	5.005	1137	1140	1141	rBV2	325	211	0.02%	0.003%
23	5.063	1141	1158	1179	rVV	191345	421056	42.44%	5.234%
24	5.247	1212	1215	1219	rBV2	361	248	0.02%	0.003%
25	5.282	1221	1226	1228	rBV2	640	619	0.06%	0.008%
26	5.378	1252	1256	1259	rBV3	418	284	0.03%	0.004%
27	5.571	1314	1316	1323	rBV2	352	247	0.02%	0.003%
28	5.726	1341	1364	1387	rBV2	363554	992091	100.00%	12.333%
29	5.915	1420	1423	1427	rBV2	306	332	0.03%	0.004%
30	5.951	1432	1434	1436	rVV	350	219	0.02%	0.003%
31	5.964	1436	1438	1444	rVB3	561	504	0.05%	0.006%
32	6.009	1449	1452	1456	rVV	300	208	0.02%	0.003%
33	6.250	1507	1527	1546	rBV	347785	666092	67.14%	8.280%
34	6.539	1603	1617	1632	rBV5	29191	55802	5.62%	0.694%
35	6.597	1632	1635	1639	rVB2	459	386	0.04%	0.005%
36	6.626	1639	1644	1649	rBV	338	374	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049011.D
 Acq On : 10 Jun 2022 20:59
 Operator : SY/MD
 Sample : N3254-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.690	1649	1664	1685	rBV	241686	470300	47.40%	5.847%
38	6.838	1708	1710	1715	rVB2	273	210	0.02%	0.003%
39	6.883	1720	1724	1727	rBV	369	278	0.03%	0.003%
40	7.021	1763	1767	1771	rBV2	219	237	0.02%	0.003%
41	7.044	1771	1774	1783	rVB3	462	520	0.05%	0.006%
42	7.082	1783	1786	1790	rBV2	254	240	0.02%	0.003%
43	7.182	1806	1817	1827	rBV6	2199	4208	0.42%	0.052%
44	7.246	1832	1837	1841	rVV2	194	202	0.02%	0.003%
45	7.330	1860	1863	1869	rVB2	269	287	0.03%	0.004%
46	7.565	1922	1936	1956	rBV	122503	215859	21.76%	2.683%
47	7.639	1956	1959	1964	rVB4	663	561	0.06%	0.007%
48	7.681	1964	1972	1975	rBV5	1322	1422	0.14%	0.018%
49	7.787	2002	2005	2009	rBV2	421	369	0.04%	0.005%
50	7.899	2026	2040	2056	rBV	423515	739085	74.50%	9.188%
51	8.044	2082	2085	2087	rBV2	491	278	0.03%	0.003%
52	8.053	2087	2088	2092	rVB2	530	260	0.03%	0.003%
53	8.073	2092	2094	2097	rVB2	405	203	0.02%	0.003%
54	8.121	2106	2109	2113	rBV	273	271	0.03%	0.003%
55	8.179	2116	2127	2146	rVV	88830	147740	14.89%	1.837%
56	8.304	2163	2166	2171	rVB3	705	590	0.06%	0.007%
57	8.420	2199	2202	2206	rBV2	466	327	0.03%	0.004%
58	8.481	2218	2221	2224	rVB3	628	357	0.04%	0.004%
59	8.542	2235	2240	2243	rBV2	406	362	0.04%	0.005%
60	8.632	2255	2268	2303	rBV2	345962	658344	66.36%	8.184%
61	8.902	2349	2352	2356	rVB2	300	215	0.02%	0.003%
62	9.150	2426	2429	2433	rVB2	545	364	0.04%	0.005%
63	9.417	2499	2512	2537	rBV	494406	822206	82.88%	10.221%
64	9.693	2593	2598	2601	rBV2	568	577	0.06%	0.007%
65	9.828	2637	2640	2644	rVB2	321	197	0.02%	0.002%
66	9.854	2644	2648	2653	rBV2	365	405	0.04%	0.005%
67	9.883	2653	2657	2662	rBV	337	416	0.04%	0.005%
68	10.201	2747	2756	2759	rBV	242	337	0.03%	0.004%
69	10.307	2787	2789	2794	rVV2	324	200	0.02%	0.002%
70	10.362	2803	2806	2815	rVB2	260	361	0.04%	0.004%
71	10.401	2815	2818	2822	rVB2	309	237	0.02%	0.003%
72	10.430	2822	2827	2831	rBV2	304	404	0.04%	0.005%
73	10.674	2896	2903	2910	rVB5	1021	1598	0.16%	0.020%
74	10.758	2915	2929	2950	rBV	369211	599425	60.42%	7.452%
75	10.893	2968	2971	2974	rVB	410	243	0.02%	0.003%
76	11.182	3058	3061	3066	rVB2	287	225	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049011.D
 Acq On : 10 Jun 2022 20:59
 Operator : SY/MD
 Sample : N3254-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.433	3135	3139	3141	rBV	363	286	0.03%	0.004%
78	11.487	3154	3156	3160	rVB2	354	220	0.02%	0.003%
79	11.738	3232	3234	3239	rVB	338	194	0.02%	0.002%
80	11.812	3244	3257	3278	rBV	421040	667817	67.31%	8.302%
81	12.092	3341	3344	3349	rVB	477	355	0.04%	0.004%
82	12.118	3349	3352	3359	rVB	299	257	0.03%	0.003%
83	12.195	3360	3376	3396	rBV	395561	655301	66.05%	8.146%
84	12.693	3528	3531	3536	rVB2	375	296	0.03%	0.004%
85	12.738	3541	3545	3547	rBV	303	250	0.03%	0.003%
86	12.873	3584	3587	3590	rBV	532	371	0.04%	0.005%
87	12.909	3595	3598	3600	rVB2	399	232	0.02%	0.003%
88	13.105	3656	3659	3664	rVB2	330	232	0.02%	0.003%
89	13.156	3672	3675	3677	rBV2	369	227	0.02%	0.003%
90	13.269	3707	3710	3713	rBV	375	275	0.03%	0.003%
91	13.323	3724	3727	3730	rBV2	349	237	0.02%	0.003%
92	13.372	3739	3742	3745	rBV2	293	245	0.02%	0.003%
93	13.452	3763	3767	3770	rBV2	469	393	0.04%	0.005%
94	13.847	3888	3890	3896	rBV3	294	237	0.02%	0.003%
95	13.963	3923	3926	3928	rBV	365	220	0.02%	0.003%
96	14.150	3981	3984	3990	rVB3	1005	959	0.10%	0.012%
97	14.185	3990	3995	4000	rBV2	618	764	0.08%	0.009%
98	14.253	4012	4016	4023	rBB3	335	392	0.04%	0.005%
99	14.542	4103	4106	4108	rBV2	400	262	0.03%	0.003%
100	15.465	4391	4393	4396	rBV2	358	207	0.02%	0.003%




Sum of corrected areas: 8044118

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049011.D
Acq On : 10 Jun 2022 20:59
Operator : SY/MD
Sample : N3254-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

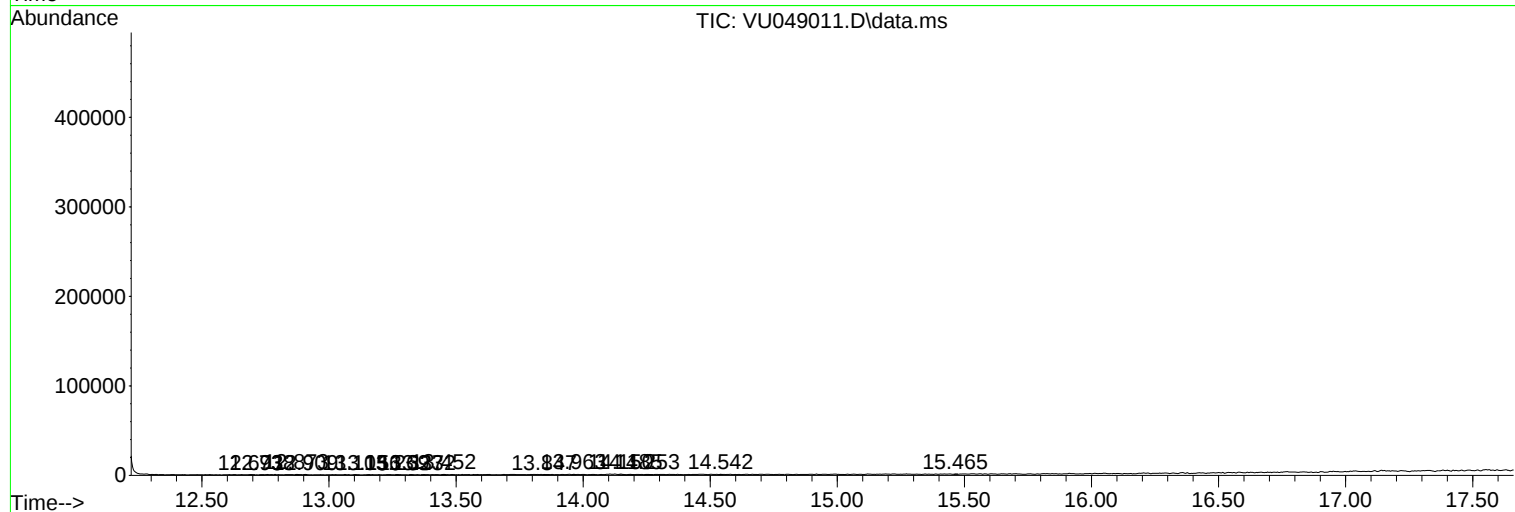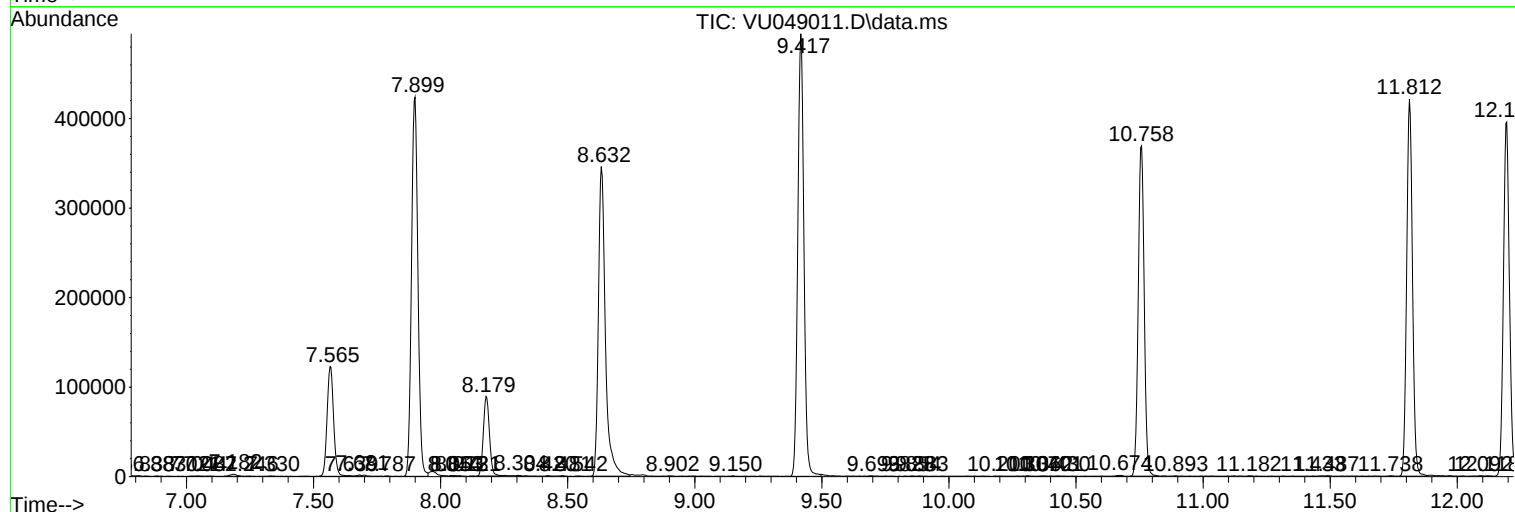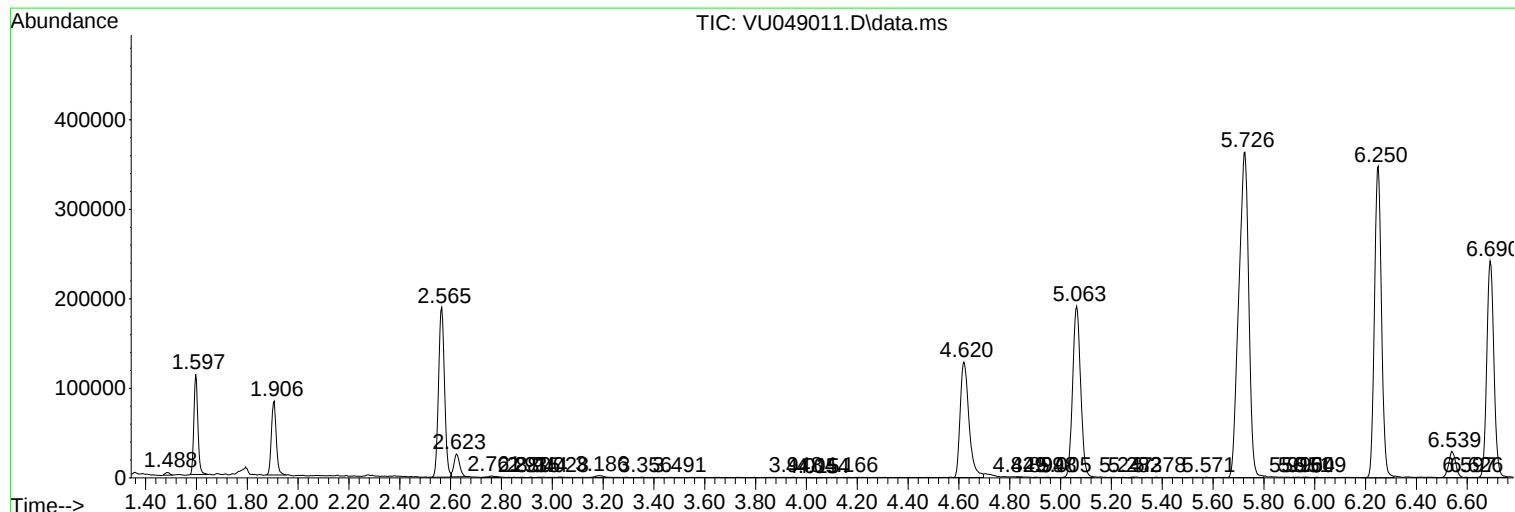

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049011.D
Acq On : 10 Jun 2022 20:59
Operator : SY/MD
Sample : N3254-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049011.D
Acq On : 10 Jun 2022 20:59
Operator : SY/MD
Sample : N3254-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc