

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049013.D
 Acq On : 10 Jun 2022 21:46
 Operator : SY/MD
 Sample : N3254-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049013.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	106515	120822	12.44%	1.385%
2	1.899	167	174	191	rVB	79280	107686	11.09%	1.234%
3	2.562	368	380	391	rBV	183709	304257	31.33%	3.487%
4	2.623	392	399	422	rVB	54008	90997	9.37%	1.043%
5	2.922	489	492	495	rBV	278	255	0.03%	0.003%
6	2.973	505	508	513	rVB3	384	278	0.03%	0.003%
7	3.015	519	521	524	rBV2	179	104	0.01%	0.001%
8	3.041	526	529	531	rBV	497	269	0.03%	0.003%
9	3.153	560	564	565	rBV2	341	268	0.03%	0.003%
10	3.269	597	600	603	rBV2	213	129	0.01%	0.001%
11	3.356	617	627	635	rVB3	2426	4269	0.44%	0.049%
12	3.423	642	648	651	rBV2	408	334	0.03%	0.004%
13	3.485	665	667	668	rBV	244	109	0.01%	0.001%
14	3.594	698	701	703	rBV	199	137	0.01%	0.002%
15	3.809	766	768	770	rBV	158	91	0.01%	0.001%
16	3.919	800	802	803	rBV	201	81	0.01%	0.001%
17	3.928	803	805	807	rVV	124	70	0.01%	0.001%
18	4.005	825	829	831	rBV2	179	153	0.02%	0.002%
19	4.247	902	904	905	rBV	173	81	0.01%	0.001%
20	4.407	951	954	961	rVB	304	225	0.02%	0.003%
21	4.478	974	976	979	rVB2	253	105	0.01%	0.001%
22	4.497	979	982	984	rBV	140	103	0.01%	0.001%
23	4.620	1007	1020	1037	rBV	124798	321453	33.10%	3.684%
24	4.970	1127	1129	1132	rBV2	254	144	0.01%	0.002%
25	5.057	1140	1156	1181	rBV2	305256	743821	76.60%	8.526%
26	5.314	1221	1236	1248	rBV4	8378	19594	2.02%	0.225%
27	5.443	1272	1276	1278	rBV	257	157	0.02%	0.002%
28	5.462	1278	1282	1284	rBV	265	202	0.02%	0.002%
29	5.501	1291	1294	1298	rBV2	162	148	0.02%	0.002%
30	5.610	1324	1328	1330	rBV	215	186	0.02%	0.002%
31	5.639	1334	1337	1339	rBV	191	136	0.01%	0.002%
32	5.722	1342	1363	1394	rVV2	351137	971012	100.00%	11.130%
33	5.890	1413	1415	1417	rBV2	307	146	0.02%	0.002%
34	6.034	1458	1460	1462	rBV	353	94	0.01%	0.001%
35	6.124	1481	1488	1490	rBV2	342	412	0.04%	0.005%
36	6.173	1500	1503	1508	rVB	310	240	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049013.D
 Acq On : 10 Jun 2022 21:46
 Operator : SY/MD
 Sample : N3254-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.247	1508	1526	1547	rBV	346750	656221	67.58%	7.522%
38	6.542	1603	1618	1639	rBV	321510	610030	62.82%	6.992%
39	6.690	1650	1664	1690	rVB	233500	459005	47.27%	5.261%
40	6.877	1720	1722	1725	rBV	212	98	0.01%	0.001%
41	6.925	1733	1737	1740	rBV	200	211	0.02%	0.002%
42	6.986	1754	1756	1757	rBV	177	86	0.01%	0.001%
43	7.095	1788	1790	1794	rVB2	185	104	0.01%	0.001%
44	7.144	1801	1805	1807	rBV	175	133	0.01%	0.002%
45	7.182	1809	1817	1827	rVV5	2212	3864	0.40%	0.044%
46	7.272	1843	1845	1848	rBV2	211	115	0.01%	0.001%
47	7.349	1866	1869	1870	rBV	153	80	0.01%	0.001%
48	7.433	1891	1895	1897	rBV2	183	156	0.02%	0.002%
49	7.468	1901	1906	1908	rBV	189	206	0.02%	0.002%
50	7.510	1916	1919	1922	rBV2	150	159	0.02%	0.002%
51	7.565	1923	1936	1954	rVV2	117401	206994	21.32%	2.373%
52	7.697	1967	1977	1982	rBV6	1231	2113	0.22%	0.024%
53	7.735	1986	1989	1991	rBV2	154	98	0.01%	0.001%
54	7.748	1991	1993	1996	rVB2	314	195	0.02%	0.002%
55	7.800	2006	2009	2012	rBV2	276	220	0.02%	0.003%
56	7.832	2016	2019	2021	rBV2	318	202	0.02%	0.002%
57	7.899	2026	2040	2057	rBV	410488	704341	72.54%	8.073%
58	8.121	2108	2109	2110	rVB	147	28	0.00%	0.000%
59	8.179	2115	2127	2146	rBV2	84654	140628	14.48%	1.612%
60	8.398	2193	2195	2196	rBV	301	145	0.01%	0.002%
61	8.439	2204	2208	2210	rVB3	381	262	0.03%	0.003%
62	8.552	2240	2243	2246	rBV2	247	169	0.02%	0.002%
63	8.632	2255	2268	2301	rBV2	324129	615780	63.42%	7.058%
64	8.799	2318	2320	2323	rBV2	472	324	0.03%	0.004%
65	8.854	2334	2337	2338	rBV2	275	116	0.01%	0.001%
66	8.902	2349	2352	2353	rBV2	200	102	0.01%	0.001%
67	9.053	2396	2399	2400	rBV	162	96	0.01%	0.001%
68	9.314	2478	2480	2482	rBV	186	106	0.01%	0.001%
69	9.417	2499	2512	2534	rBV	471715	787088	81.06%	9.022%
70	9.722	2604	2607	2614	rBV2	290	320	0.03%	0.004%
71	9.806	2630	2633	2637	rVB2	312	194	0.02%	0.002%
72	9.828	2637	2640	2642	rVB	393	181	0.02%	0.002%
73	9.844	2642	2645	2647	rBV	107	54	0.01%	0.001%
74	10.288	2778	2783	2787	rBV2	346	391	0.04%	0.004%
75	10.324	2791	2794	2799	rVV2	311	270	0.03%	0.003%
76	10.523	2852	2856	2859	rBV	345	322	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049013.D
 Acq On : 10 Jun 2022 21:46
 Operator : SY/MD
 Sample : N3254-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	10.578	2867	2873	2877	rBV2	456	627	0.06%	0.007%
78	10.671	2897	2902	2909	rVB4	842	987	0.10%	0.011%
79	10.754	2914	2928	2950	rBV	343468	564142	58.10%	6.466%
80	10.909	2970	2976	2978	rBV2	568	577	0.06%	0.007%
81	10.970	2993	2995	3000	rBV2	254	135	0.01%	0.002%
82	11.163	3046	3055	3057	rBV2	468	649	0.07%	0.007%
83	11.446	3141	3143	3144	rBV	310	112	0.01%	0.001%
84	11.709	3221	3225	3228	rBV2	355	290	0.03%	0.003%
85	11.812	3244	3257	3275	rBV	402549	649842	66.92%	7.448%
86	11.934	3292	3295	3297	rBV	568	372	0.04%	0.004%
87	12.086	3339	3342	3348	rVB	458	425	0.04%	0.005%
88	12.195	3363	3376	3394	rBV	387172	625236	64.39%	7.166%
89	12.442	3450	3453	3455	rBV	314	227	0.02%	0.003%
90	12.481	3462	3465	3467	rBV	350	199	0.02%	0.002%
91	13.131	3665	3667	3670	rBV	237	145	0.01%	0.002%
92	13.600	3808	3813	3817	rBV2	605	752	0.08%	0.009%


Sum of corrected areas: 8724492

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049013.D
Acq On : 10 Jun 2022 21:46
Operator : SY/MD
Sample : N3254-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

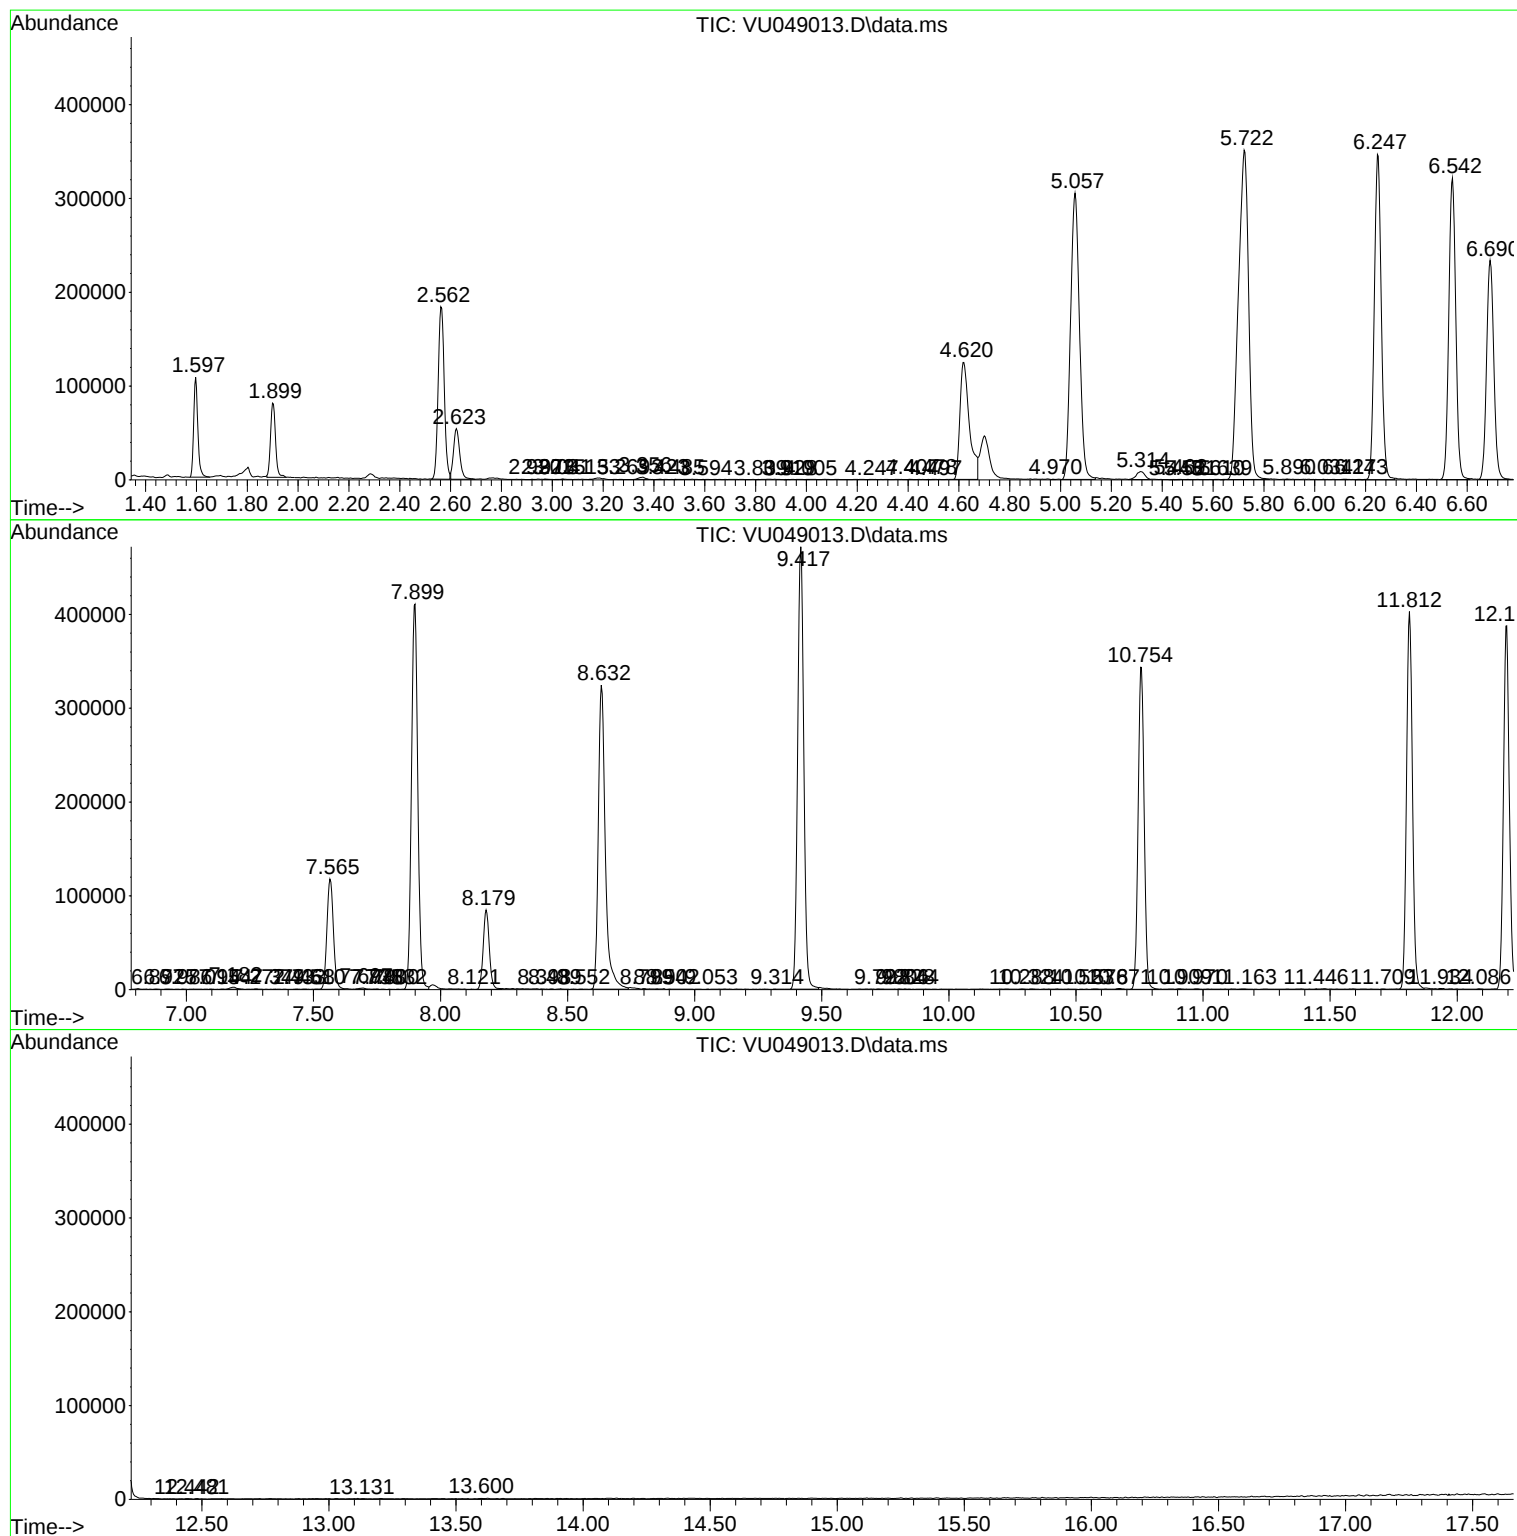

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049013.D
Acq On : 10 Jun 2022 21:46
Operator : SY/MD
Sample : N3254-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049013.D
Acq On : 10 Jun 2022 21:46
Operator : SY/MD
Sample : N3254-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------