

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049015.D
 Acq On : 10 Jun 2022 22:33
 Operator : SY/MD
 Sample : N3254-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	51	rVB6	2142	2510	0.26%	0.033%
2	1.597	73	80	94	rBV	100619	112760	11.83%	1.493%
3	1.899	165	174	186	rBV	74790	99661	10.46%	1.320%
4	2.562	368	380	393	rBV	172436	280572	29.44%	3.716%
5	2.623	394	399	415	rVB	8214	13507	1.42%	0.179%
6	2.710	423	426	430	rVB2	500	315	0.03%	0.004%
7	2.742	430	436	438	rBV2	616	528	0.06%	0.007%
8	2.896	480	484	488	rBV	413	415	0.04%	0.005%
9	2.957	499	503	507	rVB2	369	320	0.03%	0.004%
10	3.009	517	519	526	rBV	399	253	0.03%	0.003%
11	3.176	565	571	572	rBV2	662	582	0.06%	0.008%
12	3.427	643	649	654	rBV2	382	534	0.06%	0.007%
13	3.784	754	760	763	rVV2	278	317	0.03%	0.004%
14	3.816	766	770	773	rBV2	298	238	0.02%	0.003%
15	3.928	800	805	810	rBV2	266	276	0.03%	0.004%
16	3.960	811	815	818	rVB2	350	253	0.03%	0.003%
17	4.237	896	901	904	rBV	268	244	0.03%	0.003%
18	4.259	904	908	914	rBV	216	347	0.04%	0.005%
19	4.620	1005	1020	1041	rBV	123736	300102	31.49%	3.974%
20	4.919	1109	1113	1115	rBV2	278	240	0.03%	0.003%
21	5.060	1137	1157	1176	rBV	198246	445351	46.74%	5.898%
22	5.185	1194	1196	1202	rVB3	318	274	0.03%	0.004%
23	5.288	1224	1228	1229	rBV2	590	426	0.04%	0.006%
24	5.375	1252	1255	1258	rBV	418	284	0.03%	0.004%
25	5.452	1275	1279	1282	rVV2	229	209	0.02%	0.003%
26	5.568	1312	1315	1320	rBV2	191	239	0.03%	0.003%
27	5.722	1341	1363	1387	rBV2	343976	952889	100.00%	12.619%
28	5.967	1436	1439	1440	rBV3	341	203	0.02%	0.003%
29	6.041	1459	1462	1467	rVV3	263	265	0.03%	0.004%
30	6.250	1512	1527	1548	rBV	326529	622331	65.31%	8.241%
31	6.484	1598	1600	1605	rVB2	375	268	0.03%	0.004%
32	6.536	1605	1616	1628	rVB5	5940	12819	1.35%	0.170%
33	6.584	1628	1631	1633	rBV2	558	362	0.04%	0.005%
34	6.610	1636	1639	1642	rVB2	444	333	0.03%	0.004%
35	6.632	1642	1646	1649	rBV2	253	205	0.02%	0.003%
36	6.690	1649	1664	1686	rBV	230092	445301	46.73%	5.897%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049015.D
 Acq On : 10 Jun 2022 22:33
 Operator : SY/MD
 Sample : N3254-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CODH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.880	1720	1723	1727	rVB2	353	244	0.03%	0.003%
38	7.083	1781	1786	1790	rBV2	229	263	0.03%	0.003%
39	7.108	1790	1794	1798	rBV2	243	273	0.03%	0.004%
40	7.179	1806	1816	1817	rBV3	2200	2533	0.27%	0.034%
41	7.510	1916	1919	1922	rBV	450	316	0.03%	0.004%
42	7.565	1923	1936	1955	rVV	117625	202590	21.26%	2.683%
43	7.674	1966	1970	1971	rBV2	406	318	0.03%	0.004%
44	7.690	1971	1975	1977	rVV3	608	499	0.05%	0.007%
45	7.726	1983	1986	1990	rBV	349	279	0.03%	0.004%
46	7.899	2022	2040	2057	rBV	397561	685279	71.92%	9.075%
47	8.034	2077	2082	2086	rVB3	645	549	0.06%	0.007%
48	8.179	2114	2127	2146	rBV	83311	138394	14.52%	1.833%
49	8.263	2150	2153	2155	rBV2	398	234	0.02%	0.003%
50	8.304	2162	2166	2170	rVB2	485	402	0.04%	0.005%
51	8.346	2175	2179	2182	rBV2	455	347	0.04%	0.005%
52	8.388	2189	2192	2194	rBV3	474	304	0.03%	0.004%
53	8.472	2213	2218	2223	rVB3	374	389	0.04%	0.005%
54	8.632	2255	2268	2298	rBV2	322697	619183	64.98%	8.200%
55	8.828	2325	2329	2333	rBV3	351	284	0.03%	0.004%
56	8.883	2342	2346	2350	rBV3	405	458	0.05%	0.006%
57	9.012	2382	2386	2387	rBV	553	352	0.04%	0.005%
58	9.417	2498	2512	2532	rBV	462237	763867	80.16%	10.116%
59	9.562	2553	2557	2559	rBV2	278	265	0.03%	0.004%
60	9.687	2586	2596	2597	rBV	497	498	0.05%	0.007%
61	9.976	2683	2686	2691	rBV2	273	219	0.02%	0.003%
62	10.192	2749	2753	2758	rBV2	219	215	0.02%	0.003%
63	10.259	2768	2774	2776	rBV2	225	242	0.03%	0.003%
64	10.455	2827	2835	2836	rBV	196	249	0.03%	0.003%
65	10.565	2866	2869	2871	rBV	311	230	0.02%	0.003%
66	10.661	2895	2899	2903	rBV4	734	834	0.09%	0.011%
67	10.754	2916	2928	2951	rVB	352498	572670	60.10%	7.584%
68	10.899	2970	2973	2979	rBV4	482	442	0.05%	0.006%
69	11.012	3005	3008	3013	rVB3	349	341	0.04%	0.005%
70	11.047	3013	3019	3022	rBV2	408	456	0.05%	0.006%
71	11.121	3039	3042	3045	rBV	448	231	0.02%	0.003%
72	11.266	3084	3087	3091	rVB2	232	214	0.02%	0.003%
73	11.288	3091	3094	3099	rBV2	450	378	0.04%	0.005%
74	11.314	3099	3102	3108	rVV2	256	232	0.02%	0.003%
75	11.471	3147	3151	3154	rVB	404	333	0.03%	0.004%
76	11.745	3234	3236	3239	rBV2	268	205	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049015.D
 Acq On : 10 Jun 2022 22:33
 Operator : SY/MD
 Sample : N3254-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.812	3245	3257	3275	rBV	403559	635631	66.71%	8.418%
78	11.967	3302	3305	3312	rVB3	744	804	0.08%	0.011%
79	12.031	3322	3325	3329	rBV3	445	316	0.03%	0.004%
80	12.195	3363	3376	3397	rBV	372934	615194	64.56%	8.147%
81	12.317	3412	3414	3416	rBV3	545	272	0.03%	0.004%
82	12.333	3416	3419	3423	rVB3	410	297	0.03%	0.004%
83	12.378	3427	3433	3435	rBV2	302	250	0.03%	0.003%
84	13.095	3653	3656	3661	rBV3	422	368	0.04%	0.005%
85	13.323	3725	3727	3732	rVB2	382	271	0.03%	0.004%
86	13.436	3759	3762	3765	rBV	319	227	0.02%	0.003%
87	13.648	3825	3828	3832	rBV2	330	393	0.04%	0.005%
88	14.028	3943	3946	3947	rBV2	329	208	0.02%	0.003%
89	14.050	3951	3953	3956	rVV	340	214	0.02%	0.003%
90	14.259	4015	4018	4027	rBV3	399	552	0.06%	0.007%
91	14.638	4132	4136	4138	rBV3	462	389	0.04%	0.005%
92	14.732	4161	4165	4168	rBV2	402	370	0.04%	0.005%
93	14.751	4168	4171	4173	rBV3	423	286	0.03%	0.004%
94	14.806	4186	4188	4192	rVB2	543	333	0.03%	0.004%
95	15.272	4330	4333	4337	rBV3	542	422	0.04%	0.006%
96	15.635	4443	4446	4449	rBV3	585	365	0.04%	0.005%
97	15.677	4456	4459	4464	rBV3	620	486	0.05%	0.006%
98	15.828	4504	4506	4509	rBV3	651	505	0.05%	0.007%
99	16.265	4638	4642	4645	rBV5	1100	901	0.09%	0.012%
100	16.571	4734	4737	4740	rBV3	1077	832	0.09%	0.011%




Sum of corrected areas: 7551230

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049015.D
Acq On : 10 Jun 2022 22:33
Operator : SY/MD
Sample : N3254-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

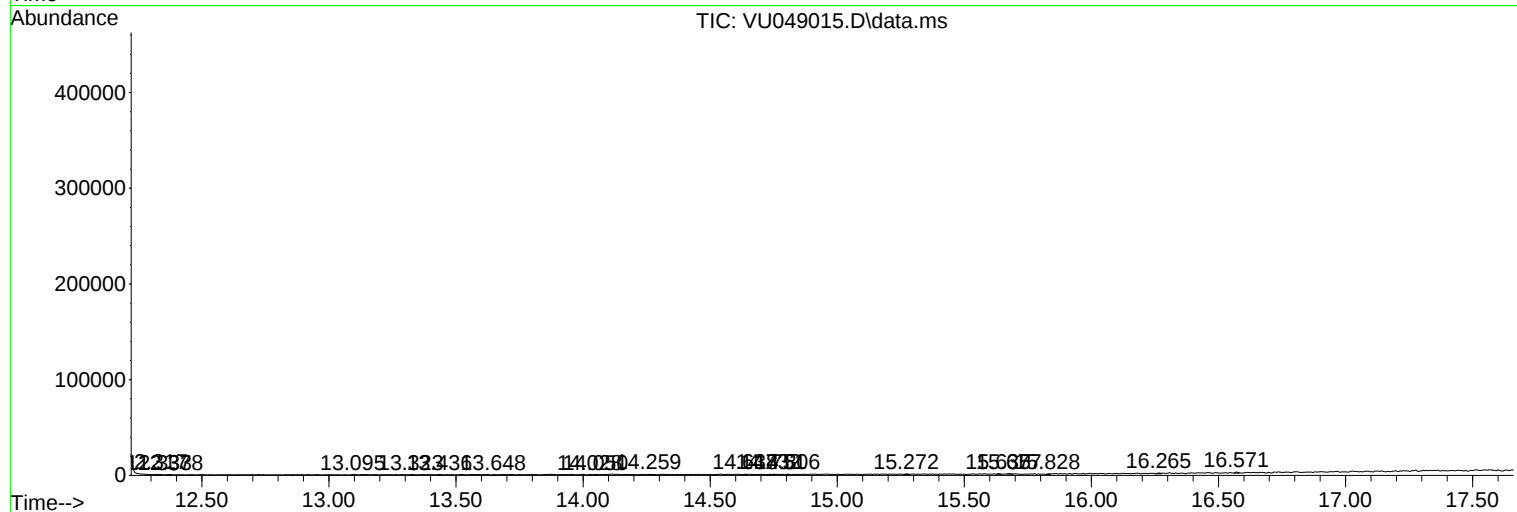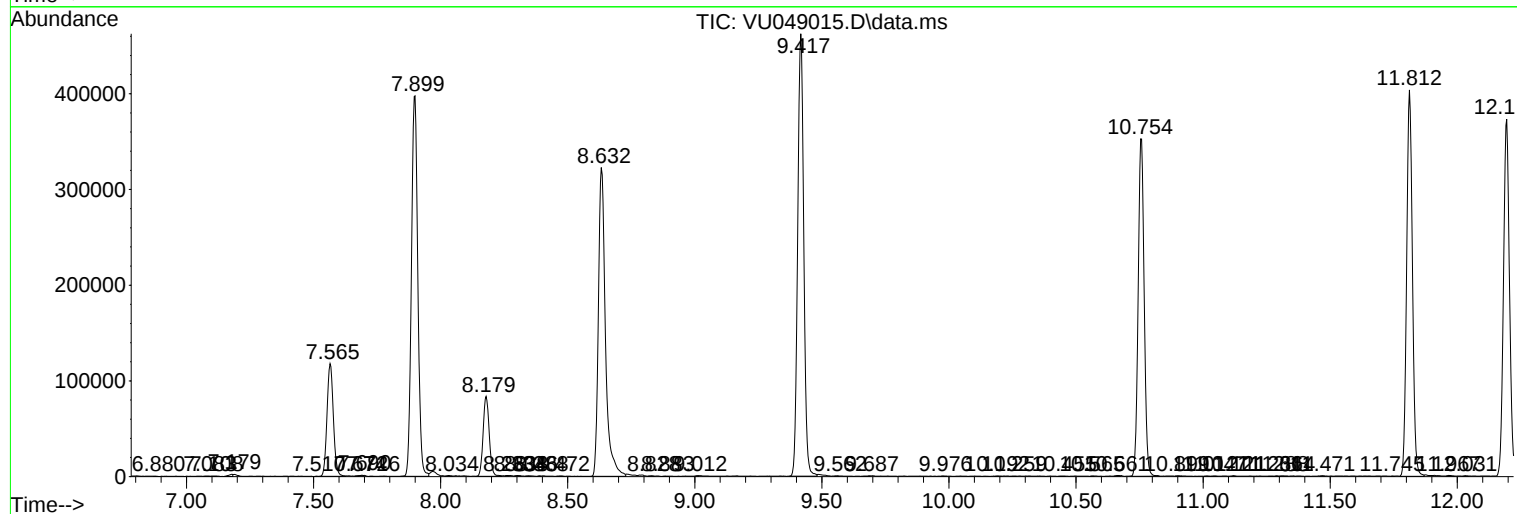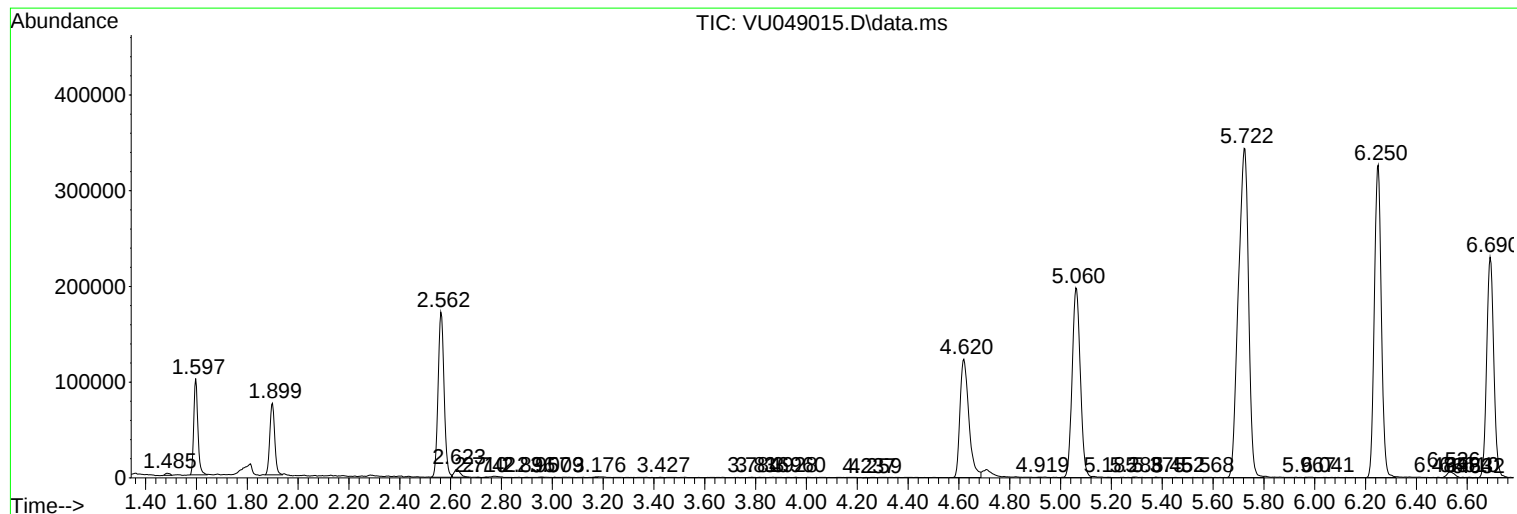

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049015.D
Acq On : 10 Jun 2022 22:33
Operator : SY/MD
Sample : N3254-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049015.D
Acq On : 10 Jun 2022 22:33
Operator : SY/MD
Sample : N3254-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------