

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049018.D
 Acq On : 10 Jun 2022 23:44
 Operator : SY/MD
 Sample : N3254-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	107604	119483	12.32%	1.521%
2	1.893	164	172	185	rVB	75202	98469	10.15%	1.253%
3	2.562	367	380	393	rBV	179336	299352	30.87%	3.810%
4	2.845	464	468	470	rBV	406	354	0.04%	0.005%
5	2.948	497	500	503	rBV2	320	264	0.03%	0.003%
6	3.041	525	529	531	rBV2	492	400	0.04%	0.005%
7	3.514	674	676	677	rBV	286	114	0.01%	0.001%
8	3.568	690	693	694	rBV	267	157	0.02%	0.002%
9	3.671	722	725	727	rBV2	294	202	0.02%	0.003%
10	4.022	829	834	837	rBV	365	325	0.03%	0.004%
11	4.346	932	935	937	rBV2	248	146	0.02%	0.002%
12	4.617	1006	1019	1039	rBV	126616	306236	31.58%	3.897%
13	4.851	1089	1092	1094	rBV3	434	272	0.03%	0.003%
14	4.896	1103	1106	1109	rVB2	371	237	0.02%	0.003%
15	4.912	1109	1111	1113	rBV3	209	130	0.01%	0.002%
16	5.060	1142	1157	1181	rBV2	216668	488338	50.36%	6.215%
17	5.205	1199	1202	1204	rBV	356	263	0.03%	0.003%
18	5.285	1222	1227	1230	rBV4	758	826	0.09%	0.011%
19	5.317	1235	1237	1238	rBV	132	31	0.00%	0.000%
20	5.366	1250	1252	1253	rBV	157	64	0.01%	0.001%
21	5.375	1253	1255	1257	rBV	172	75	0.01%	0.001%
22	5.507	1293	1296	1299	rBV2	185	159	0.02%	0.002%
23	5.723	1341	1363	1385	rBV2	351933	969747	100.00%	12.342%
24	6.041	1460	1462	1465	rBV	198	98	0.01%	0.001%
25	6.173	1498	1503	1508	rBV2	540	532	0.05%	0.007%
26	6.247	1513	1526	1545	rVV	334347	628570	64.82%	8.000%
27	6.469	1591	1595	1598	rBV3	317	342	0.04%	0.004%
28	6.526	1604	1613	1624	rBV3	3272	6398	0.66%	0.081%
29	6.690	1650	1664	1684	rBV2	233213	458633	47.29%	5.837%
30	6.809	1697	1701	1707	rVB3	659	754	0.08%	0.010%
31	6.896	1725	1728	1730	rBV2	207	151	0.02%	0.002%
32	6.996	1756	1759	1760	rBV	249	137	0.01%	0.002%
33	7.176	1807	1815	1831	rBV8	2617	5534	0.57%	0.070%
34	7.272	1842	1845	1849	rBV2	274	292	0.03%	0.004%
35	7.417	1887	1890	1892	rBV	211	145	0.01%	0.002%
36	7.565	1924	1936	1954	rBV	117370	205209	21.16%	2.612%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049018.D
 Acq On : 10 Jun 2022 23:44
 Operator : SY/MD
 Sample : N3254-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	7.690	1968	1975	1976	rBV2	1399	1375	0.14%	0.017%
38	7.896	2027	2039	2056	rBV	408356	710147	73.23%	9.038%
39	8.179	2116	2127	2142	rBV2	84318	141467	14.59%	1.800%
40	8.562	2243	2246	2250	rVB	301	171	0.02%	0.002%
41	8.632	2256	2268	2301	rBV2	340233	655911	67.64%	8.348%
42	9.089	2407	2410	2415	rBB2	250	232	0.02%	0.003%
43	9.115	2415	2418	2419	rBV	186	120	0.01%	0.002%
44	9.144	2424	2427	2429	rBV	303	206	0.02%	0.003%
45	9.189	2438	2441	2445	rBV2	259	201	0.02%	0.003%
46	9.272	2464	2467	2469	rBV2	393	289	0.03%	0.004%
47	9.366	2493	2496	2498	rBV	270	194	0.02%	0.002%
48	9.417	2498	2512	2532	rVV	479825	790995	81.57%	10.067%
49	9.578	2561	2562	2565	rBV	162	91	0.01%	0.001%
50	9.758	2615	2618	2625	rBV2	189	249	0.03%	0.003%
51	9.793	2627	2629	2630	rBV	172	70	0.01%	0.001%
52	10.494	2843	2847	2848	rBV2	163	131	0.01%	0.002%
53	10.594	2875	2878	2881	rBV2	269	237	0.02%	0.003%
54	10.758	2916	2929	2948	rBV	380702	617898	63.72%	7.864%
55	11.034	3012	3015	3019	rVB2	419	331	0.03%	0.004%
56	11.057	3019	3022	3025	rVB	260	183	0.02%	0.002%
57	11.083	3025	3030	3034	rBV2	346	414	0.04%	0.005%
58	11.118	3039	3041	3042	rBV	297	74	0.01%	0.001%
59	11.812	3244	3257	3272	rBV	419251	669556	69.04%	8.521%
60	12.195	3362	3376	3401	rBV	408230	673882	69.49%	8.576%
61	13.713	3844	3848	3852	rBV3	544	485	0.05%	0.006%




Sum of corrected areas: 7857348

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049018.D
Acq On : 10 Jun 2022 23:44
Operator : SY/MD
Sample : N3254-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

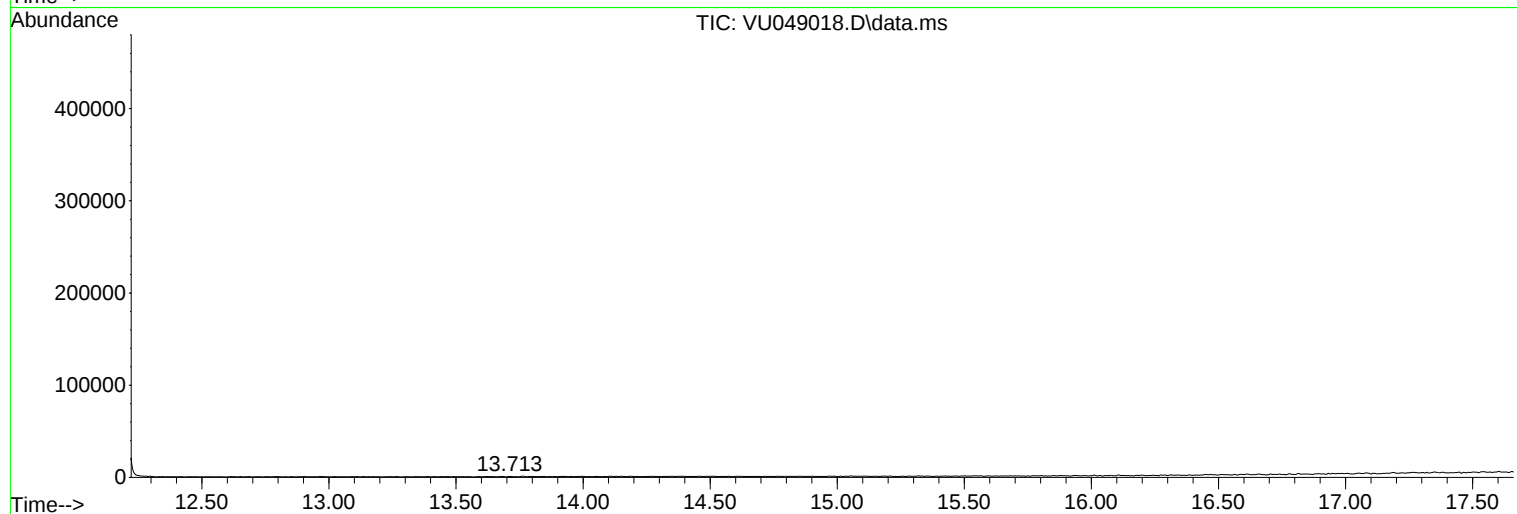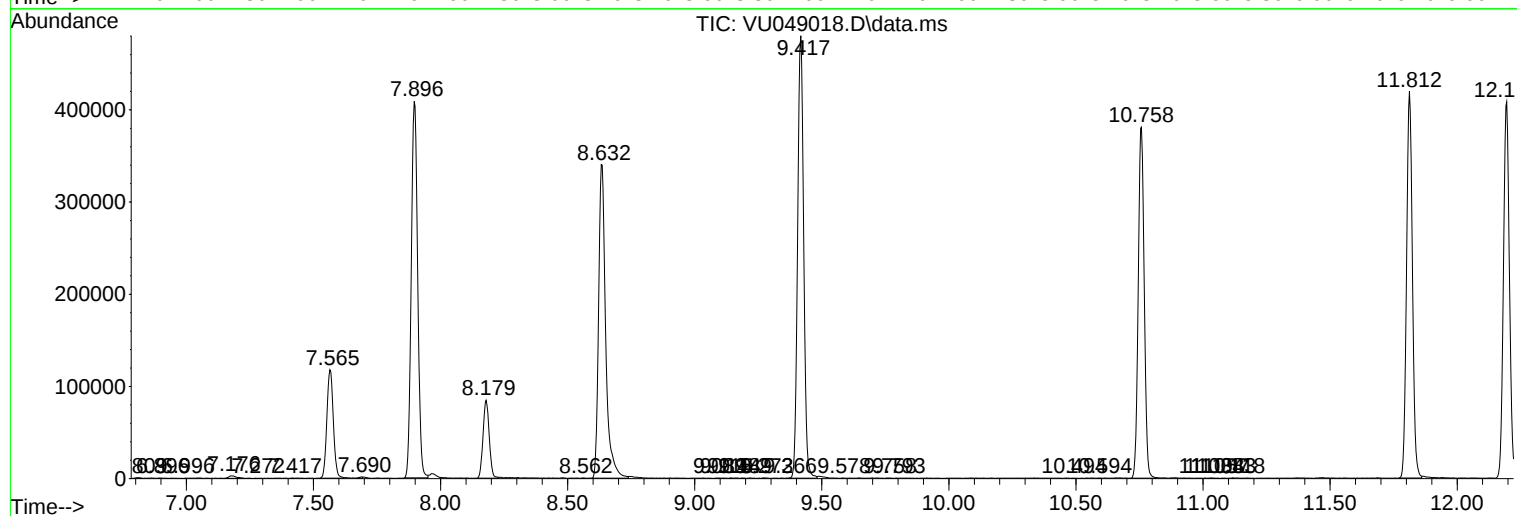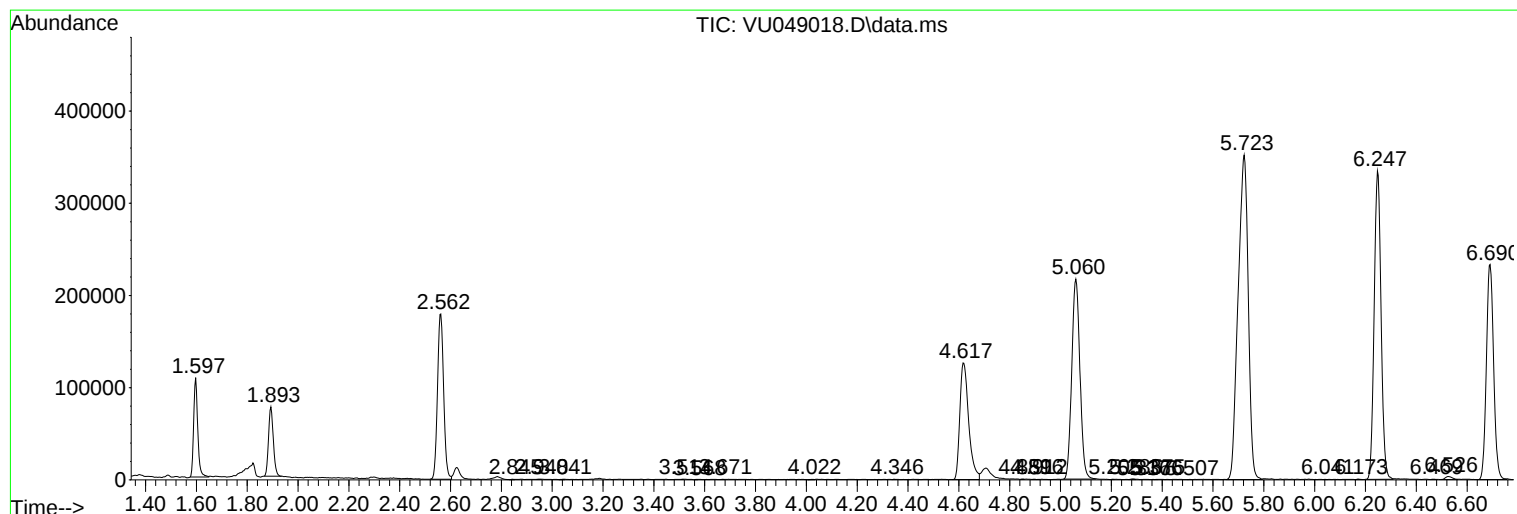

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049018.D
Acq On : 10 Jun 2022 23:44
Operator : SY/MD
Sample : N3254-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049018.D
Acq On : 10 Jun 2022 23:44
Operator : SY/MD
Sample : N3254-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------