

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049019.D
 Acq On : 11 Jun 2022 00:07
 Operator : SY/MD
 Sample : N3291-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	97	rBV	107984	123015	12.75%	1.549%
2	1.806	136	145	146	rBB8	608	2236	0.23%	0.028%
3	1.893	164	172	186	rBV	75889	101743	10.55%	1.281%
4	2.340	309	311	314	rBV	677	369	0.04%	0.005%
5	2.359	315	317	322	rVV4	733	668	0.07%	0.008%
6	2.391	325	327	331	rVV2	927	632	0.07%	0.008%
7	2.424	334	337	340	rVB3	581	361	0.04%	0.005%
8	2.498	357	360	361	rBV2	404	226	0.02%	0.003%
9	2.562	368	380	395	rBV	182834	300837	31.19%	3.787%
10	2.755	436	440	442	rBV2	240	217	0.02%	0.003%
11	2.944	495	499	503	rBV2	330	280	0.03%	0.004%
12	2.970	503	507	510	rBV2	350	292	0.03%	0.004%
13	3.044	524	530	534	rBV2	578	622	0.06%	0.008%
14	3.173	566	570	573	rBV	578	461	0.05%	0.006%
15	3.192	574	576	585	rVB3	656	654	0.07%	0.008%
16	3.266	594	599	602	rVB2	277	279	0.03%	0.004%
17	3.565	686	692	695	rBV2	203	258	0.03%	0.003%
18	3.645	711	717	719	rBV2	233	272	0.03%	0.003%
19	3.896	792	795	802	rBV	183	214	0.02%	0.003%
20	3.932	803	806	810	rVB	280	207	0.02%	0.003%
21	4.031	833	837	840	rBV2	286	232	0.02%	0.003%
22	4.054	841	844	847	rVV2	289	218	0.02%	0.003%
23	4.182	881	884	890	rBV	240	203	0.02%	0.003%
24	4.263	905	909	911	rBV	267	237	0.02%	0.003%
25	4.301	918	921	923	rBV2	302	233	0.02%	0.003%
26	4.510	980	986	988	rBV	253	242	0.03%	0.003%
27	4.620	1007	1020	1044	rBV	120449	293998	30.48%	3.701%
28	4.922	1109	1114	1117	rBV3	265	265	0.03%	0.003%
29	4.964	1122	1127	1131	rBV3	297	340	0.04%	0.004%
30	5.060	1141	1157	1183	rVB	182064	398327	41.29%	5.015%
31	5.292	1217	1229	1235	rBV2	714	1207	0.13%	0.015%
32	5.333	1240	1242	1248	rBV2	284	300	0.03%	0.004%
33	5.501	1289	1294	1297	rBV2	174	191	0.02%	0.002%
34	5.722	1342	1363	1381	rBV2	353813	964603	100.00%	12.144%
35	5.819	1391	1393	1398	rVB4	547	363	0.04%	0.005%
36	5.922	1422	1425	1428	rBV2	450	298	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049019.D
 Acq On : 11 Jun 2022 00:07
 Operator : SY/MD
 Sample : N3291-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.970	1435	1440	1442	rBV3	657	564	0.06%	0.007%
38	6.041	1459	1462	1463	rBV	398	228	0.02%	0.003%
39	6.112	1479	1484	1486	rBV3	304	258	0.03%	0.003%
40	6.147	1492	1495	1500	rVB	384	243	0.03%	0.003%
41	6.247	1510	1526	1544	rBV	355511	667672	69.22%	8.406%
42	6.353	1557	1559	1563	rVB2	597	312	0.03%	0.004%
43	6.436	1582	1585	1589	rVB2	309	217	0.02%	0.003%
44	6.465	1592	1594	1598	rVB2	396	258	0.03%	0.003%
45	6.539	1604	1617	1632	rBV3	44241	86283	8.94%	1.086%
46	6.690	1650	1664	1688	rBV	238245	469401	48.66%	5.910%
47	6.777	1688	1691	1695	rVB2	431	331	0.03%	0.004%
48	6.800	1695	1698	1701	rBV3	352	341	0.04%	0.004%
49	6.902	1724	1730	1735	rBV2	258	308	0.03%	0.004%
50	7.015	1760	1765	1766	rBV	230	200	0.02%	0.003%
51	7.182	1808	1817	1830	rBV7	2454	5416	0.56%	0.068%
52	7.311	1851	1857	1860	rBV2	288	297	0.03%	0.004%
53	7.394	1877	1883	1886	rBV2	259	295	0.03%	0.004%
54	7.565	1923	1936	1955	rBV	116398	205165	21.27%	2.583%
55	7.690	1968	1975	1982	rBV3	1261	1568	0.16%	0.020%
56	7.790	2003	2006	2010	rVB3	235	190	0.02%	0.002%
57	7.829	2014	2018	2022	rBV	224	227	0.02%	0.003%
58	7.896	2026	2039	2056	rBV	411979	709325	73.54%	8.930%
59	8.179	2115	2127	2143	rBV	83289	137922	14.30%	1.736%
60	8.266	2150	2154	2157	rBV3	523	361	0.04%	0.005%
61	8.523	2231	2234	2238	rVV2	321	198	0.02%	0.002%
62	8.632	2256	2268	2304	rBV2	330142	641948	66.55%	8.082%
63	8.893	2346	2349	2351	rBV	372	237	0.02%	0.003%
64	8.970	2368	2373	2377	rBV	267	334	0.03%	0.004%
65	9.018	2385	2388	2391	rVB	405	286	0.03%	0.004%
66	9.041	2391	2395	2397	rBV	360	335	0.03%	0.004%
67	9.166	2426	2434	2436	rBV	402	476	0.05%	0.006%
68	9.417	2499	2512	2534	rBV	508912	827233	85.76%	10.415%
69	9.681	2592	2594	2596	rBV2	391	215	0.02%	0.003%
70	9.857	2644	2649	2652	rBV2	331	250	0.03%	0.003%
71	10.115	2724	2729	2733	rBV	274	268	0.03%	0.003%
72	10.584	2868	2875	2877	rBV	426	383	0.04%	0.005%
73	10.668	2897	2901	2911	rVB4	520	753	0.08%	0.009%
74	10.758	2915	2929	2947	rBV	381945	608888	63.12%	7.666%
75	11.356	3112	3115	3119	rVB2	408	272	0.03%	0.003%
76	11.378	3119	3122	3128	rBV2	309	378	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049019.D
 Acq On : 11 Jun 2022 00:07
 Operator : SY/MD
 Sample : N3291-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.404	3128	3130	3134	rVB2	307	207	0.02%	0.003%
78	11.446	3140	3143	3146	rBV2	361	291	0.03%	0.004%
79	11.597	3188	3190	3195	rVB2	296	201	0.02%	0.003%
80	11.700	3220	3222	3227	rVB2	572	283	0.03%	0.004%
81	11.812	3245	3257	3277	rBV	443012	707080	73.30%	8.902%
82	12.028	3318	3324	3326	rBV2	407	367	0.04%	0.005%
83	12.195	3363	3376	3404	rBV	400970	663280	68.76%	8.351%
84	12.629	3508	3511	3516	rVB2	338	285	0.03%	0.004%
85	13.188	3682	3685	3687	rBV3	445	341	0.04%	0.004%
86	13.295	3715	3718	3721	rVV2	302	234	0.02%	0.003%
87	13.375	3741	3743	3747	rBV	302	196	0.02%	0.002%
88	13.446	3762	3765	3768	rBV3	285	227	0.02%	0.003%
89	13.500	3779	3782	3784	rBV2	252	195	0.02%	0.002%
90	13.536	3790	3793	3798	rBV3	287	279	0.03%	0.004%
91	14.085	3961	3964	3967	rBV3	408	304	0.03%	0.004%
92	14.420	4063	4068	4071	rBV3	543	558	0.06%	0.007%
93	14.693	4148	4153	4157	rBV3	663	684	0.07%	0.009%
94	14.764	4172	4175	4179	rBV3	430	354	0.04%	0.004%
95	15.150	4293	4295	4299	rBV2	425	330	0.03%	0.004%
96	15.169	4299	4301	4304	rVB2	480	189	0.02%	0.002%
97	15.336	4351	4353	4357	rBV	467	401	0.04%	0.005%
98	15.876	4519	4521	4525	rBV4	748	575	0.06%	0.007%
99	15.950	4542	4544	4546	rBV	636	324	0.03%	0.004%
100	15.999	4556	4559	4565	rBV3	960	830	0.09%	0.010%




Sum of corrected areas: 7942951

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049019.D
Acq On : 11 Jun 2022 00:07
Operator : SY/MD
Sample : N3291-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

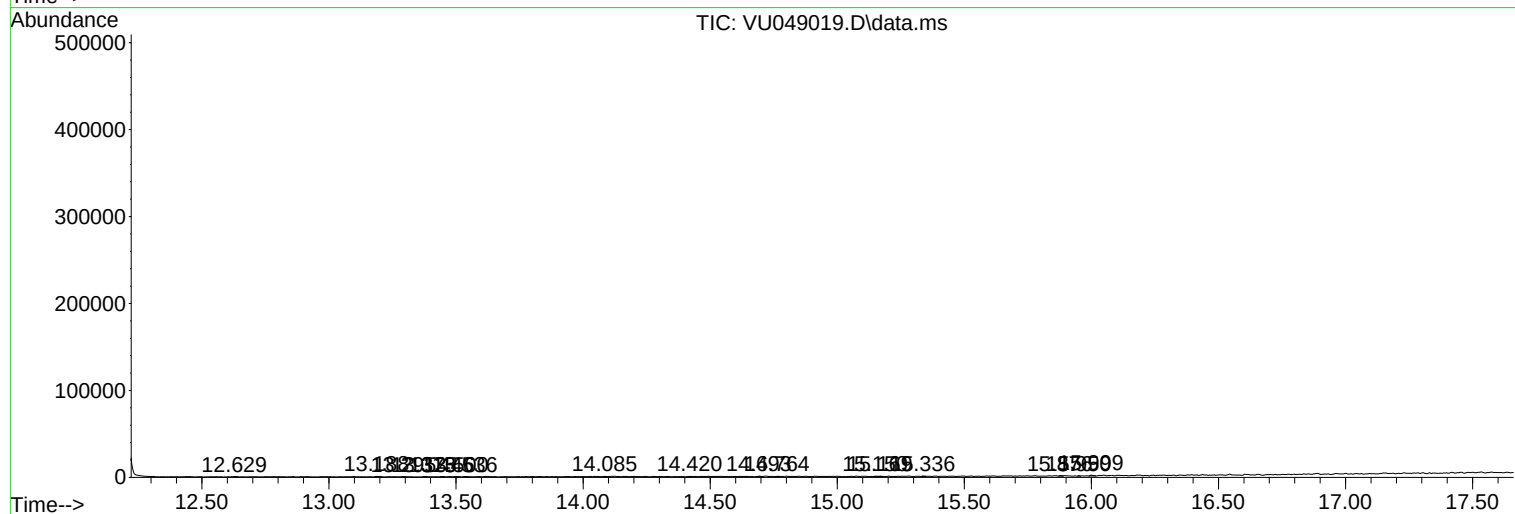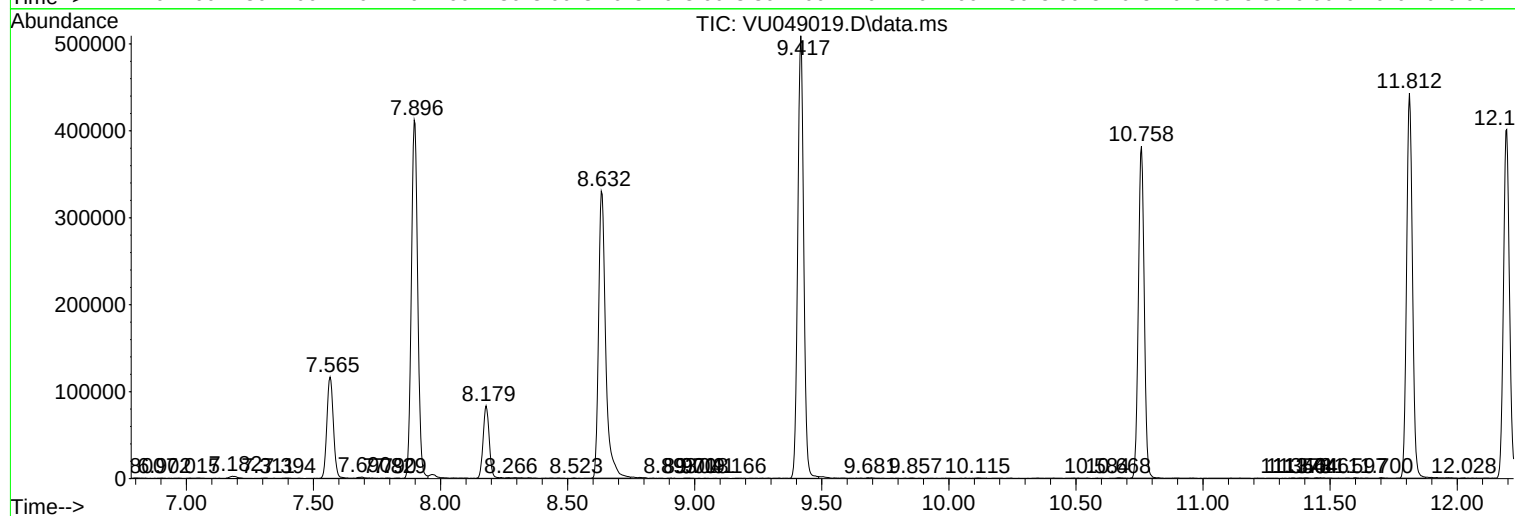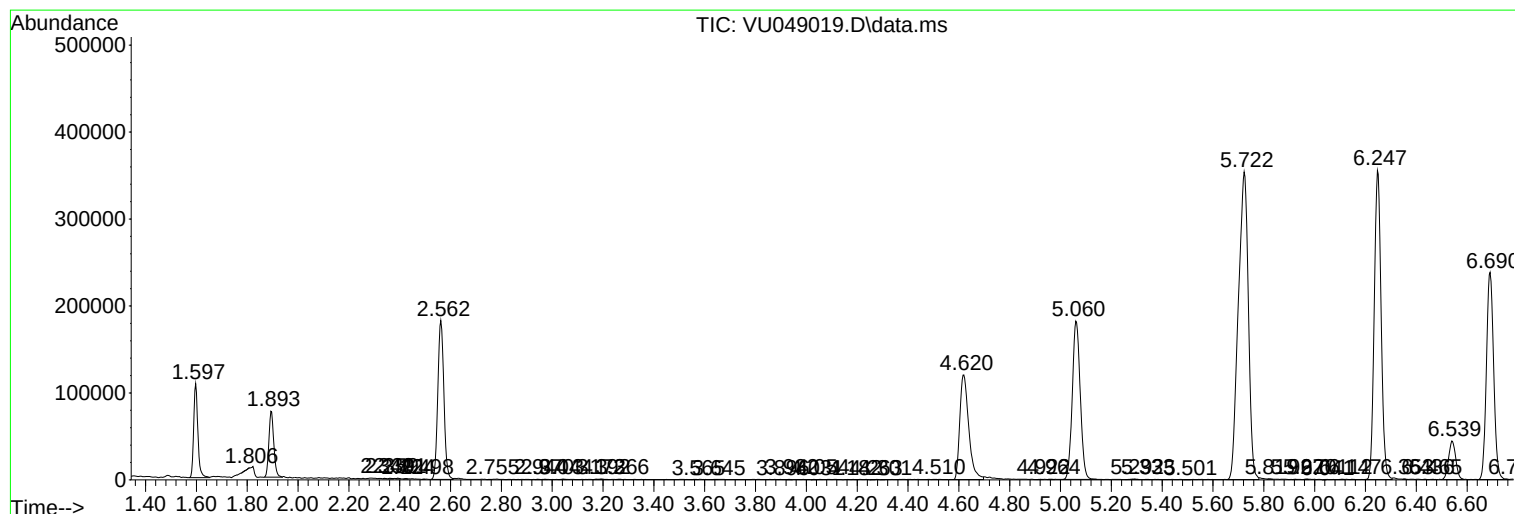

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049019.D
Acq On : 11 Jun 2022 00:07
Operator : SY/MD
Sample : N3291-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049019.D
Acq On : 11 Jun 2022 00:07
Operator : SY/MD
Sample : N3291-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------