

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049020.D
 Acq On : 11 Jun 2022 00:31
 Operator : SY/MD
 Sample : N3291-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

Signal : TIC: VU049020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	107307	120712	12.12%	1.537%
2	1.896	165	173	188	rVB	75971	99121	9.95%	1.262%
3	2.562	368	380	395	rBV	182445	299256	30.04%	3.811%
4	2.777	440	447	453	rBV3	611	1017	0.10%	0.013%
5	2.932	492	495	497	rBV	220	130	0.01%	0.002%
6	3.009	516	519	522	rBV	324	214	0.02%	0.003%
7	3.028	523	525	528	rVV2	317	210	0.02%	0.003%
8	3.115	548	552	553	rBV	171	113	0.01%	0.001%
9	3.169	566	569	571	rBV3	483	331	0.03%	0.004%
10	3.311	610	613	618	rBV	191	194	0.02%	0.002%
11	3.356	623	627	628	rBV	234	168	0.02%	0.002%
12	3.372	628	632	635	rBV2	381	335	0.03%	0.004%
13	3.443	652	654	658	rBV	193	145	0.01%	0.002%
14	3.504	672	673	676	rBV	207	80	0.01%	0.001%
15	3.716	737	739	742	rBV2	172	101	0.01%	0.001%
16	3.748	747	749	751	rVB2	224	96	0.01%	0.001%
17	3.803	763	766	768	rBV2	212	148	0.01%	0.002%
18	3.938	806	808	813	rVB2	197	107	0.01%	0.001%
19	3.983	819	822	826	rBV2	150	127	0.01%	0.002%
20	4.192	885	887	890	rBV	142	118	0.01%	0.002%
21	4.298	917	920	923	rBV2	222	188	0.02%	0.002%
22	4.349	933	936	940	rBV2	135	108	0.01%	0.001%
23	4.440	961	964	969	rVB	342	257	0.03%	0.003%
24	4.459	969	970	971	rBV	143	47	0.00%	0.001%
25	4.526	988	991	993	rBV	115	86	0.01%	0.001%
26	4.542	993	996	998	rBV2	159	125	0.01%	0.002%
27	4.620	1006	1020	1047	rBV	124691	301513	30.27%	3.839%
28	4.886	1100	1103	1105	rBV	317	163	0.02%	0.002%
29	5.060	1142	1157	1176	rBV	186980	413443	41.50%	5.265%
30	5.227	1205	1209	1213	rVB2	408	337	0.03%	0.004%
31	5.292	1223	1229	1236	rVB3	557	831	0.08%	0.011%
32	5.321	1236	1238	1241	rBV	153	53	0.01%	0.001%
33	5.388	1254	1259	1266	rVB3	217	253	0.03%	0.003%
34	5.472	1281	1285	1291	rBV2	165	183	0.02%	0.002%
35	5.578	1315	1318	1320	rBV	237	176	0.02%	0.002%
36	5.722	1341	1363	1388	rBV3	362144	996240	100.00%	12.686%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049020.D
 Acq On : 11 Jun 2022 00:31
 Operator : SY/MD
 Sample : N3291-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.970	1435	1440	1446	rBV3	952	1139	0.11%	0.015%
38	6.015	1451	1454	1456	rBV2	157	105	0.01%	0.001%
39	6.060	1465	1468	1475	rBV2	314	359	0.04%	0.005%
40	6.247	1511	1526	1552	rBV	352304	673423	67.60%	8.575%
41	6.529	1606	1614	1624	rVB5	4089	7151	0.72%	0.091%
42	6.574	1627	1628	1630	rBV	143	64	0.01%	0.001%
43	6.603	1635	1637	1639	rBV	289	137	0.01%	0.002%
44	6.690	1649	1664	1685	rBV	243781	471848	47.36%	6.008%
45	6.777	1689	1691	1693	rBV2	226	107	0.01%	0.001%
46	6.803	1696	1699	1702	rBV3	655	532	0.05%	0.007%
47	6.841	1709	1711	1714	rVB	281	110	0.01%	0.001%
48	6.861	1714	1717	1719	rBV	256	158	0.02%	0.002%
49	6.912	1731	1733	1736	rBV	114	82	0.01%	0.001%
50	7.025	1765	1768	1770	rBV	213	132	0.01%	0.002%
51	7.079	1783	1785	1788	rBV2	186	102	0.01%	0.001%
52	7.144	1802	1805	1806	rBV2	162	72	0.01%	0.001%
53	7.179	1806	1816	1827	rVV7	2287	4393	0.44%	0.056%
54	7.263	1839	1842	1845	rVB2	383	223	0.02%	0.003%
55	7.378	1877	1878	1880	rVB	243	48	0.00%	0.001%
56	7.439	1892	1897	1901	rBV2	240	269	0.03%	0.003%
57	7.565	1924	1936	1954	rBV	115753	202312	20.31%	2.576%
58	7.687	1968	1974	1983	rBV4	1374	2089	0.21%	0.027%
59	7.755	1994	1995	2000	rVB	464	264	0.03%	0.003%
60	7.793	2000	2007	2010	rBV3	414	543	0.05%	0.007%
61	7.822	2013	2016	2020	rBV2	234	128	0.01%	0.002%
62	7.838	2020	2021	2023	rVB	118	23	0.00%	0.000%
63	7.899	2026	2040	2055	rBV	417635	720415	72.31%	9.174%
64	8.179	2116	2127	2141	rBV	87158	143592	14.41%	1.828%
65	8.340	2174	2177	2180	rBV3	503	354	0.04%	0.005%
66	8.520	2230	2233	2236	rBV2	286	183	0.02%	0.002%
67	8.536	2236	2238	2239	rVB	129	32	0.00%	0.000%
68	8.555	2239	2244	2247	rBV2	209	223	0.02%	0.003%
69	8.632	2256	2268	2300	rBV2	324437	612629	61.49%	7.801%
70	8.906	2350	2353	2355	rVB2	253	138	0.01%	0.002%
71	8.925	2355	2359	2362	rBV2	478	333	0.03%	0.004%
72	9.147	2424	2428	2433	rVB	396	369	0.04%	0.005%
73	9.266	2459	2465	2466	rBV2	277	281	0.03%	0.004%
74	9.327	2481	2484	2488	rBV2	284	297	0.03%	0.004%
75	9.417	2498	2512	2531	rBV	489164	803756	80.68%	10.235%
76	9.565	2556	2558	2560	rBV	199	117	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049020.D
 Acq On : 11 Jun 2022 00:31
 Operator : SY/MD
 Sample : N3291-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.652	2584	2585	2587	rVB	245	48	0.00%	0.001%
78	9.783	2623	2626	2628	rBV	288	200	0.02%	0.003%
79	9.970	2680	2684	2689	rBV2	325	375	0.04%	0.005%
80	10.150	2738	2740	2745	rBV2	249	236	0.02%	0.003%
81	10.552	2862	2865	2868	rBV	260	171	0.02%	0.002%
82	10.677	2897	2904	2911	rBV3	677	979	0.10%	0.012%
83	10.758	2916	2929	2948	rVV	375945	600250	60.25%	7.643%
84	11.246	3078	3081	3083	rBV2	309	230	0.02%	0.003%
85	11.619	3193	3197	3199	rBV2	261	225	0.02%	0.003%
86	11.812	3245	3257	3280	rBV	437566	698194	70.08%	8.891%
87	12.192	3363	3375	3397	rBV	397896	665762	66.83%	8.478%
88	12.352	3422	3425	3427	rVB	416	214	0.02%	0.003%
89	12.385	3432	3435	3437	rBV	511	288	0.03%	0.004%
90	12.664	3519	3522	3525	rBV2	384	338	0.03%	0.004%
91	12.851	3576	3580	3582	rBV	376	337	0.03%	0.004%




Sum of corrected areas: 7853105

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049020.D
Acq On : 11 Jun 2022 00:31
Operator : SY/MD
Sample : N3291-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

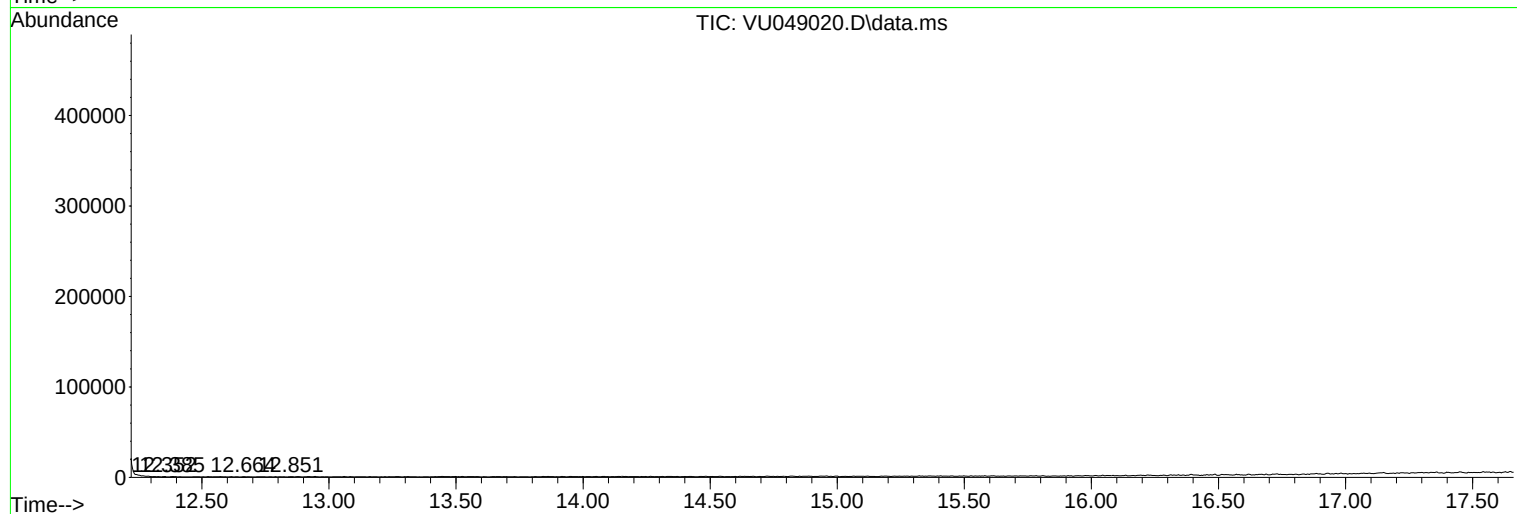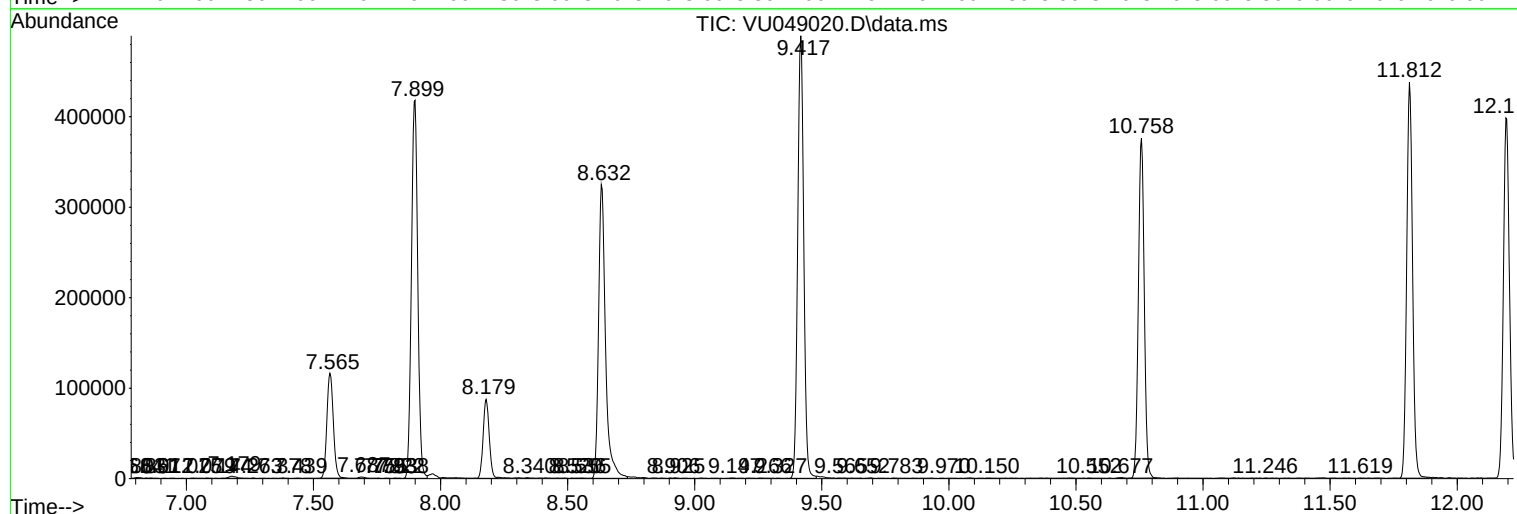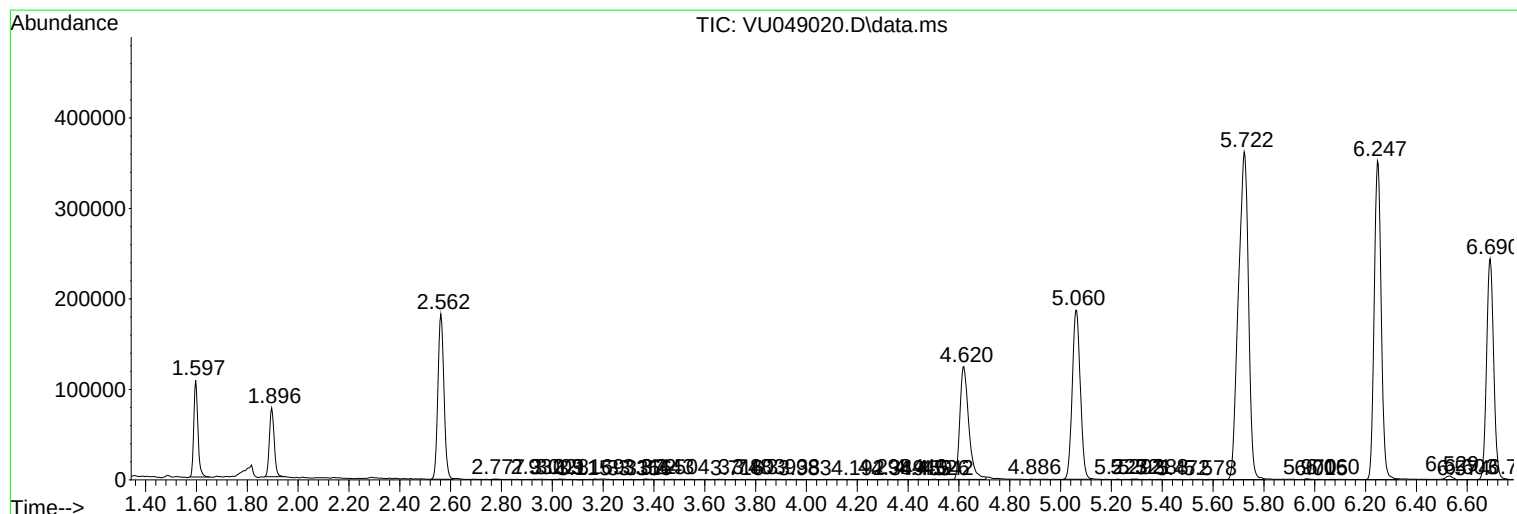

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049020.D
Acq On : 11 Jun 2022 00:31
Operator : SY/MD
Sample : N3291-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049020.D
Acq On : 11 Jun 2022 00:31
Operator : SY/MD
Sample : N3291-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc