

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049021.D
 Acq On : 11 Jun 2022 00:54
 Operator : SY/MD
 Sample : N3291-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049021.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	95	rBV	99648	115126	12.21%	1.508%
2	1.893	164	172	189	rVB	74649	101084	10.72%	1.324%
3	2.514	362	365	368	rVB2	357	204	0.02%	0.003%
4	2.562	368	380	394	rBV	178219	288394	30.59%	3.778%
5	2.787	447	450	454	rVB2	530	462	0.05%	0.006%
6	2.909	485	488	495	rBV2	331	357	0.04%	0.005%
7	2.954	499	502	506	rVB2	275	200	0.02%	0.003%
8	3.163	564	567	568	rVV2	374	215	0.02%	0.003%
9	3.186	569	574	583	rVB2	1040	1496	0.16%	0.020%
10	3.266	596	599	602	rBV2	376	235	0.02%	0.003%
11	3.369	628	631	634	rVB2	306	226	0.02%	0.003%
12	3.388	634	637	639	rBV	338	245	0.03%	0.003%
13	3.404	639	642	645	rVB	231	188	0.02%	0.002%
14	3.453	653	657	664	rBV2	299	296	0.03%	0.004%
15	3.549	681	687	689	rBV2	336	317	0.03%	0.004%
16	3.610	702	706	710	rVB2	292	253	0.03%	0.003%
17	3.713	734	738	741	rBV2	372	271	0.03%	0.004%
18	3.864	781	785	790	rBV	326	298	0.03%	0.004%
19	3.941	805	809	814	rVV2	268	255	0.03%	0.003%
20	4.623	1008	1021	1046	rBV	115899	289124	30.66%	3.788%
21	4.816	1079	1081	1086	rVB2	429	333	0.04%	0.004%
22	5.060	1140	1157	1179	rBV2	178395	390684	41.43%	5.118%
23	5.182	1190	1195	1198	rBV2	488	434	0.05%	0.006%
24	5.298	1226	1231	1239	rVB3	555	616	0.07%	0.008%
25	5.514	1295	1298	1300	rVV	313	259	0.03%	0.003%
26	5.723	1342	1363	1389	rBV2	343993	942894	100.00%	12.353%
27	5.861	1402	1406	1408	rVB2	439	320	0.03%	0.004%
28	5.877	1408	1411	1416	rVB3	355	398	0.04%	0.005%
29	5.977	1439	1442	1451	rVB6	627	721	0.08%	0.009%
30	6.108	1480	1483	1486	rBV2	246	182	0.02%	0.002%
31	6.247	1511	1526	1544	rBV	337196	644248	68.33%	8.440%
32	6.456	1587	1591	1592	rBV	264	190	0.02%	0.002%
33	6.530	1605	1614	1624	rVB8	4242	7930	0.84%	0.104%
34	6.597	1631	1635	1637	rBV2	291	197	0.02%	0.003%
35	6.690	1650	1664	1688	rBV2	228491	448847	47.60%	5.880%
36	6.771	1688	1689	1693	rVB2	513	214	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049021.D
 Acq On : 11 Jun 2022 00:54
 Operator : SY/MD
 Sample : N3291-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.793	1693	1696	1698	rBV	349	216	0.02%	0.003%
38	6.809	1699	1701	1704	rVB	459	230	0.02%	0.003%
39	7.015	1763	1765	1770	rVB2	290	267	0.03%	0.003%
40	7.041	1770	1773	1774	rBV2	444	245	0.03%	0.003%
41	7.051	1774	1776	1780	rVB2	393	270	0.03%	0.004%
42	7.099	1789	1791	1797	rVB	402	268	0.03%	0.004%
43	7.141	1797	1804	1807	rBV2	270	289	0.03%	0.004%
44	7.179	1809	1816	1831	rVB6	2706	5236	0.56%	0.069%
45	7.282	1843	1848	1851	rVV	300	274	0.03%	0.004%
46	7.472	1904	1907	1913	rVB2	435	429	0.05%	0.006%
47	7.497	1913	1915	1917	rBV	272	182	0.02%	0.002%
48	7.565	1923	1936	1954	rBV2	114988	199734	21.18%	2.617%
49	7.687	1968	1974	1985	rVB4	1512	2461	0.26%	0.032%
50	7.729	1985	1987	1990	rVB	477	241	0.03%	0.003%
51	7.748	1990	1993	1997	rBV2	309	295	0.03%	0.004%
52	7.793	2004	2007	2011	rVV2	276	225	0.02%	0.003%
53	7.813	2011	2013	2020	rVB2	279	194	0.02%	0.003%
54	7.896	2026	2039	2055	rBV	400803	697141	73.94%	9.133%
55	8.060	2085	2090	2093	rBV3	505	445	0.05%	0.006%
56	8.099	2099	2102	2109	rVB3	274	267	0.03%	0.003%
57	8.179	2115	2127	2144	rBV	81391	136465	14.47%	1.788%
58	8.240	2144	2146	2149	rBV3	478	287	0.03%	0.004%
59	8.301	2163	2165	2166	rBV	515	203	0.02%	0.003%
60	8.459	2211	2214	2217	rBV2	355	241	0.03%	0.003%
61	8.555	2241	2244	2251	rVB2	487	455	0.05%	0.006%
62	8.636	2251	2269	2300	rBV2	342162	645636	68.47%	8.458%
63	8.832	2325	2330	2333	rBV3	345	287	0.03%	0.004%
64	8.925	2357	2359	2365	rVB	395	338	0.04%	0.004%
65	8.954	2365	2368	2371	rBV3	395	292	0.03%	0.004%
66	9.301	2473	2476	2483	rVB2	293	334	0.04%	0.004%
67	9.417	2498	2512	2537	rVV	477597	790858	83.88%	10.361%
68	9.684	2591	2595	2597	rBV2	301	236	0.03%	0.003%
69	9.742	2611	2613	2617	rBV	260	225	0.02%	0.003%
70	10.067	2711	2714	2718	rVV2	246	199	0.02%	0.003%
71	10.105	2724	2726	2732	rVB2	358	282	0.03%	0.004%
72	10.214	2756	2760	2762	rBV	287	197	0.02%	0.003%
73	10.591	2875	2877	2881	rVB2	300	184	0.02%	0.002%
74	10.668	2896	2901	2906	rVB3	537	630	0.07%	0.008%
75	10.694	2906	2909	2912	rBV2	250	201	0.02%	0.003%
76	10.758	2916	2929	2946	rBV	355737	578022	61.30%	7.573%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049021.D
 Acq On : 11 Jun 2022 00:54
 Operator : SY/MD
 Sample : N3291-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	10.893	2967	2971	2972	rBV2	400	307	0.03%	0.004%
78	11.166	3052	3056	3059	rBV2	304	251	0.03%	0.003%
79	11.269	3086	3088	3092	rVB2	334	213	0.02%	0.003%
80	11.301	3092	3098	3100	rBV2	226	246	0.03%	0.003%
81	11.452	3142	3145	3148	rBV3	320	239	0.03%	0.003%
82	11.812	3245	3257	3280	rBV	436759	685317	72.68%	8.978%
83	11.941	3295	3297	3302	rVB2	523	272	0.03%	0.004%
84	11.970	3302	3306	3309	rBV3	511	478	0.05%	0.006%
85	12.050	3330	3331	3335	rVB	541	252	0.03%	0.003%
86	12.079	3337	3340	3346	rBV2	197	267	0.03%	0.003%
87	12.192	3362	3375	3393	rBV	392075	638314	67.70%	8.363%
88	12.748	3543	3548	3550	rVV2	318	317	0.03%	0.004%
89	12.835	3572	3575	3581	rVB	355	226	0.02%	0.003%
90	12.967	3613	3616	3620	rVB2	285	233	0.02%	0.003%
91	13.600	3810	3813	3816	rBV2	434	255	0.03%	0.003%
92	13.832	3883	3885	3889	rBV	310	225	0.02%	0.003%
93	13.928	3912	3915	3919	rVB3	618	466	0.05%	0.006%
94	13.954	3919	3923	3925	rBV2	487	402	0.04%	0.005%
95	14.025	3938	3945	3947	rBV3	466	493	0.05%	0.006%
96	14.108	3968	3971	3973	rBV2	451	347	0.04%	0.005%
97	14.211	4000	4003	4004	rBV	357	226	0.02%	0.003%
98	14.726	4161	4163	4169	rVB2	336	302	0.03%	0.004%
99	15.256	4324	4328	4330	rBV	707	548	0.06%	0.007%
100	16.504	4713	4716	4718	rBV2	1152	629	0.07%	0.008%




Sum of corrected areas: 7633019

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049021.D
Acq On : 11 Jun 2022 00:54
Operator : SY/MD
Sample : N3291-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

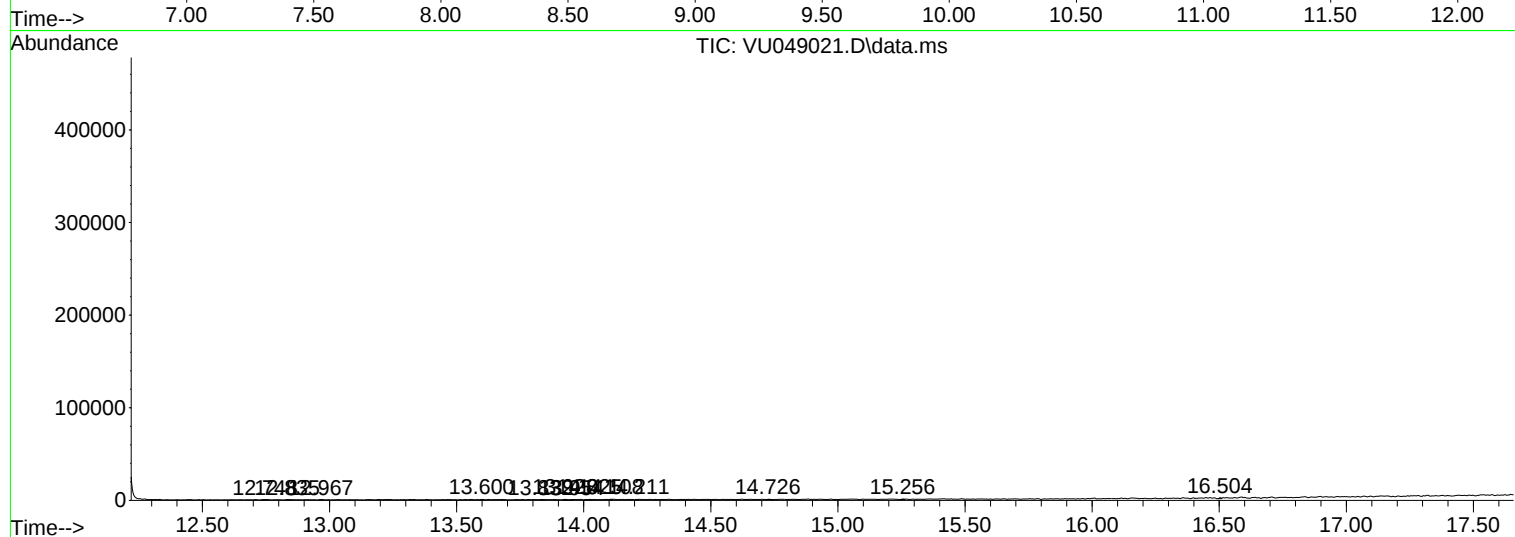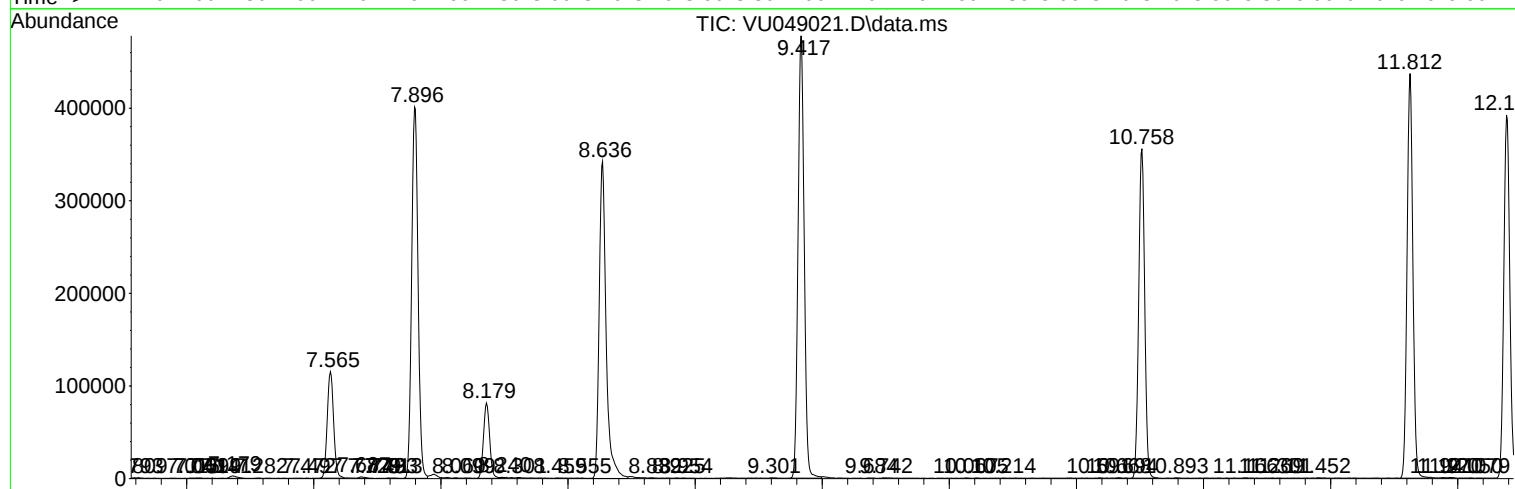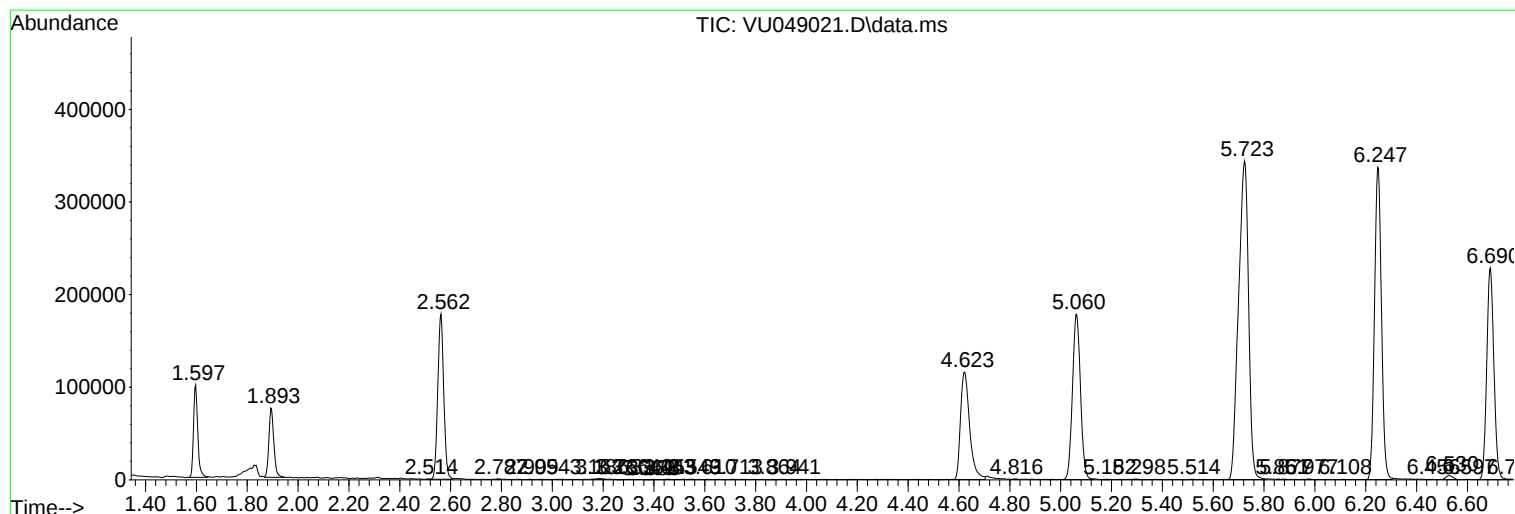

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049021.D
Acq On : 11 Jun 2022 00:54
Operator : SY/MD
Sample : N3291-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049021.D
Acq On : 11 Jun 2022 00:54
Operator : SY/MD
Sample : N3291-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc