

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049023.D
 Acq On : 11 Jun 2022 01:41
 Operator : SY/MD
 Sample : N3291-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	104057	116561	12.18%	1.517%
2	1.900	166	174	185	rBV	76061	97912	10.23%	1.274%
3	2.289	285	295	304	rBV2	4778	8363	0.87%	0.109%
4	2.427	335	338	342	rBV3	625	493	0.05%	0.006%
5	2.565	367	381	393	rBV	176065	286314	29.93%	3.727%
6	2.626	394	400	416	rVB	9662	16313	1.71%	0.212%
7	2.713	424	427	431	rBV2	257	216	0.02%	0.003%
8	2.748	436	438	439	rBV2	453	215	0.02%	0.003%
9	2.899	480	485	489	rBV2	331	330	0.03%	0.004%
10	2.941	495	498	500	rBV	269	198	0.02%	0.003%
11	2.954	500	502	505	rVV	396	240	0.03%	0.003%
12	3.173	566	570	571	rBV2	533	381	0.04%	0.005%
13	3.182	571	573	577	rVB2	514	335	0.04%	0.004%
14	3.546	683	686	692	rBV2	343	391	0.04%	0.005%
15	3.584	696	698	704	rVB2	324	239	0.02%	0.003%
16	3.777	756	758	761	rBV2	309	209	0.02%	0.003%
17	4.038	835	839	841	rBV	316	260	0.03%	0.003%
18	4.176	878	882	883	rBV2	274	224	0.02%	0.003%
19	4.391	945	949	954	rBV2	179	216	0.02%	0.003%
20	4.440	962	964	969	rVV2	258	250	0.03%	0.003%
21	4.520	984	989	993	rBV2	188	209	0.02%	0.003%
22	4.620	1007	1020	1041	rBV	118072	282365	29.51%	3.675%
23	5.063	1139	1158	1183	rBV	190276	427433	44.67%	5.564%
24	5.166	1187	1190	1193	rVB2	367	197	0.02%	0.003%
25	5.295	1223	1230	1237	rVB2	602	870	0.09%	0.011%
26	5.378	1254	1256	1259	rVB2	398	236	0.02%	0.003%
27	5.440	1268	1275	1276	rBV	224	223	0.02%	0.003%
28	5.536	1299	1305	1307	rBV2	232	228	0.02%	0.003%
29	5.726	1342	1364	1387	rBV2	343127	956771	100.00%	12.454%
30	5.890	1412	1415	1423	rVB2	583	441	0.05%	0.006%
31	5.932	1426	1428	1432	rVB2	322	216	0.02%	0.003%
32	5.964	1436	1438	1442	rBV	551	394	0.04%	0.005%
33	6.086	1472	1476	1479	rBV	225	221	0.02%	0.003%
34	6.247	1512	1526	1549	rBV2	350828	662478	69.24%	8.623%
35	6.539	1605	1617	1628	rVB8	7020	14218	1.49%	0.185%
36	6.690	1650	1664	1686	rBV	235694	457912	47.86%	5.960%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049023.D
 Acq On : 11 Jun 2022 01:41
 Operator : SY/MD
 Sample : N3291-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.800	1695	1698	1705	rBV4	522	547	0.06%	0.007%
38	6.935	1737	1740	1747	rVV2	172	199	0.02%	0.003%
39	7.185	1807	1818	1828	rVB4	2135	4200	0.44%	0.055%
40	7.288	1847	1850	1857	rVB2	264	259	0.03%	0.003%
41	7.321	1857	1860	1865	rVB2	337	376	0.04%	0.005%
42	7.353	1865	1870	1873	rBV2	430	485	0.05%	0.006%
43	7.565	1924	1936	1952	rBV	113694	198968	20.80%	2.590%
44	7.687	1968	1974	1979	rBV4	1087	1255	0.13%	0.016%
45	7.793	2003	2007	2010	rBV2	304	247	0.03%	0.003%
46	7.896	2025	2039	2057	rBV	406086	700383	73.20%	9.117%
47	8.118	2105	2108	2111	rVB2	536	356	0.04%	0.005%
48	8.140	2111	2115	2116	rBV2	413	264	0.03%	0.003%
49	8.179	2116	2127	2141	rBV2	81845	135493	14.16%	1.764%
50	8.462	2211	2215	2218	rVV3	319	344	0.04%	0.004%
51	8.632	2253	2268	2299	rBV2	316666	609470	63.70%	7.933%
52	8.793	2312	2318	2328	rVB6	1779	2786	0.29%	0.036%
53	8.919	2351	2357	2360	rBV2	437	447	0.05%	0.006%
54	8.983	2371	2377	2380	rBV	374	393	0.04%	0.005%
55	9.028	2387	2391	2394	rBV2	308	295	0.03%	0.004%
56	9.189	2436	2441	2445	rBV	278	289	0.03%	0.004%
57	9.279	2465	2469	2474	rBV2	254	250	0.03%	0.003%
58	9.417	2499	2512	2533	rBV	484585	802937	83.92%	10.452%
59	9.877	2648	2655	2658	rBV2	350	439	0.05%	0.006%
60	9.980	2683	2687	2690	rBV	270	220	0.02%	0.003%
61	9.996	2690	2692	2696	rVB2	361	237	0.02%	0.003%
62	10.034	2696	2704	2706	rBV2	464	525	0.05%	0.007%
63	10.111	2723	2728	2730	rBV2	598	474	0.05%	0.006%
64	10.214	2756	2760	2765	rBV2	315	421	0.04%	0.005%
65	10.237	2765	2767	2771	rVB	302	195	0.02%	0.003%
66	10.343	2794	2800	2803	rVV2	279	272	0.03%	0.004%
67	10.404	2816	2819	2823	rVB2	276	209	0.02%	0.003%
68	10.491	2842	2846	2848	rBV	355	240	0.03%	0.003%
69	10.661	2894	2899	2900	rBV2	588	420	0.04%	0.005%
70	10.674	2900	2903	2907	rVB2	1469	1205	0.13%	0.016%
71	10.758	2913	2929	2945	rBV	368677	588861	61.55%	7.665%
72	10.906	2972	2975	2978	rVB2	551	330	0.03%	0.004%
73	11.343	3107	3111	3114	rBV	360	351	0.04%	0.005%
74	11.449	3140	3144	3155	rVB5	790	1488	0.16%	0.019%
75	11.697	3215	3221	3222	rBV2	717	495	0.05%	0.006%
76	11.812	3244	3257	3277	rBV	409912	653923	68.35%	8.512%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049023.D
 Acq On : 11 Jun 2022 01:41
 Operator : SY/MD
 Sample : N3291-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	12.047	3327	3330	3333	rBV	226	201	0.02%	0.003%
78	12.192	3362	3375	3400	rBV	383088	630615	65.91%	8.208%
79	12.279	3400	3402	3404	rVB3	510	245	0.03%	0.003%
80	12.330	3415	3418	3422	rBV2	389	359	0.04%	0.005%
81	12.639	3510	3514	3519	rVB3	503	454	0.05%	0.006%
82	12.703	3531	3534	3537	rBV	242	195	0.02%	0.003%
83	12.944	3607	3609	3612	rVB	576	319	0.03%	0.004%
84	12.963	3612	3615	3618	rBV	303	245	0.03%	0.003%
85	13.150	3669	3673	3675	rVB2	375	293	0.03%	0.004%
86	13.201	3686	3689	3690	rBV2	415	211	0.02%	0.003%
87	13.356	3735	3737	3742	rVB	335	261	0.03%	0.003%
88	13.430	3757	3760	3763	rBV	400	278	0.03%	0.004%
89	13.526	3785	3790	3793	rBV2	281	317	0.03%	0.004%
90	13.758	3859	3862	3864	rBV	303	206	0.02%	0.003%
91	13.870	3894	3897	3900	rBV2	306	256	0.03%	0.003%
92	14.124	3971	3976	3979	rVV4	505	503	0.05%	0.007%
93	14.336	4040	4042	4045	rVB3	389	196	0.02%	0.003%
94	14.603	4123	4125	4129	rBV2	283	225	0.02%	0.003%
95	14.729	4161	4164	4167	rBV	468	261	0.03%	0.003%
96	14.831	4194	4196	4198	rBV2	415	213	0.02%	0.003%
97	14.995	4244	4247	4251	rBV2	402	350	0.04%	0.005%
98	15.552	4416	4420	4425	rBV4	775	871	0.09%	0.011%
99	15.905	4528	4530	4533	rBV2	584	385	0.04%	0.005%
100	16.098	4587	4590	4592	rBV2	765	422	0.04%	0.005%




Sum of corrected areas: 7682501

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049023.D
Acq On : 11 Jun 2022 01:41
Operator : SY/MD
Sample : N3291-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

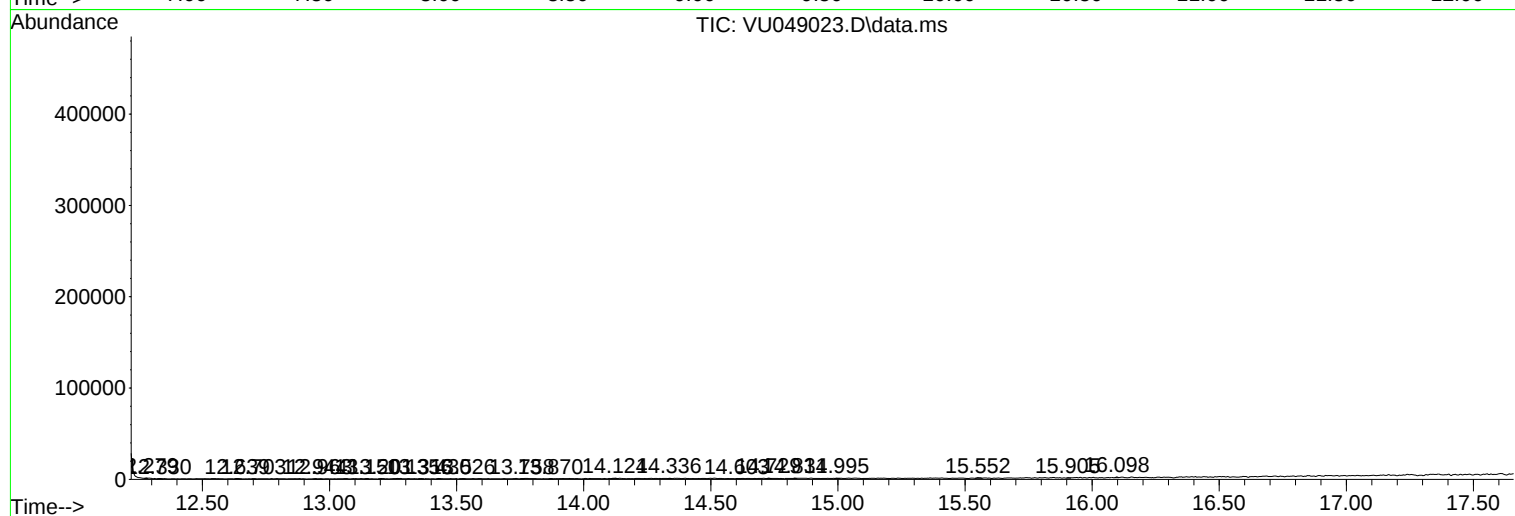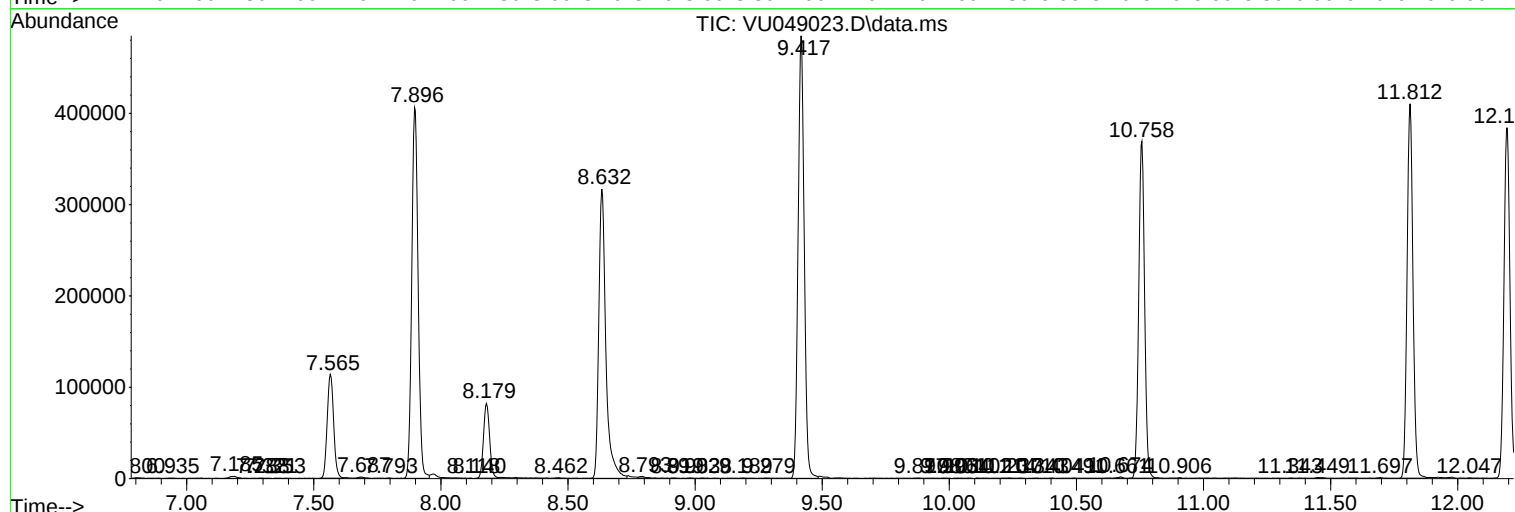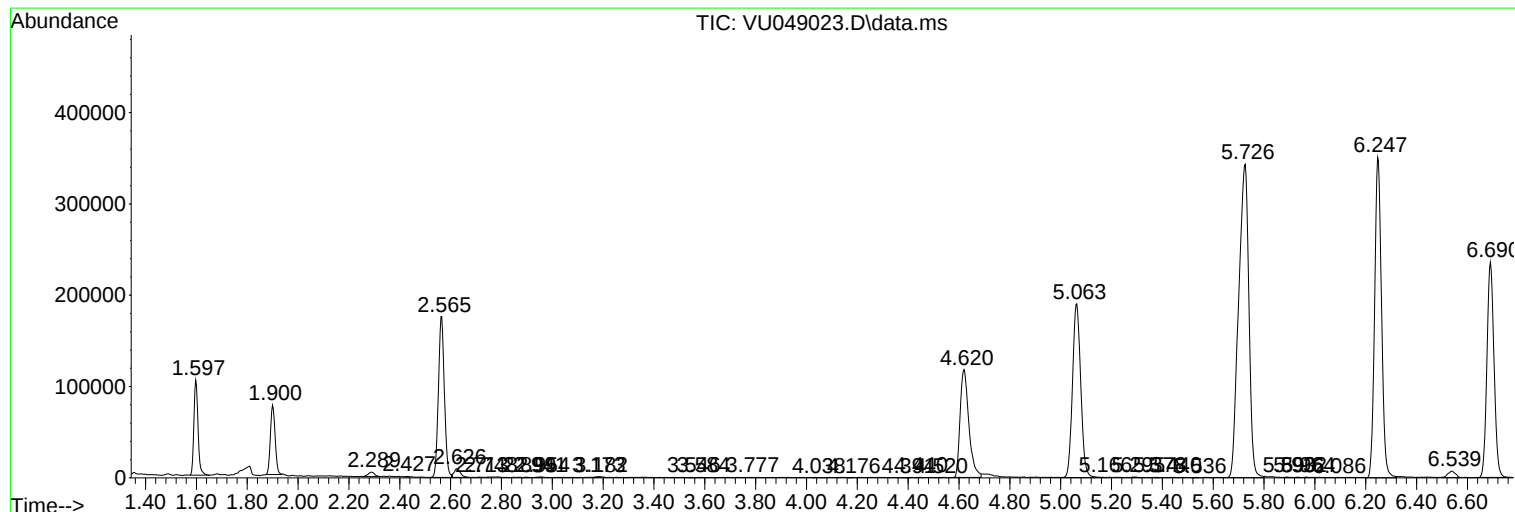

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049023.D
Acq On : 11 Jun 2022 01:41
Operator : SY/MD
Sample : N3291-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049023.D
Acq On : 11 Jun 2022 01:41
Operator : SY/MD
Sample : N3291-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------