

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049024.D
 Acq On : 11 Jun 2022 02:05
 Operator : SY/MD
 Sample : N3291-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	52	rBV4	2347	2457	0.25%	0.032%
2	1.597	73	80	95	rBV	104379	117621	12.14%	1.512%
3	1.896	164	173	191	rVB	77014	105423	10.88%	1.356%
4	2.289	291	295	304	rVB4	1859	2844	0.29%	0.037%
5	2.562	367	380	396	rBV	178754	293293	30.27%	3.771%
6	2.729	429	432	434	rBV	285	205	0.02%	0.003%
7	3.041	526	529	534	rVB2	384	362	0.04%	0.005%
8	3.112	546	551	553	rBV2	246	213	0.02%	0.003%
9	3.186	569	574	578	rBV3	502	648	0.07%	0.008%
10	3.263	595	598	602	rBV	257	217	0.02%	0.003%
11	3.359	625	628	630	rBV	518	317	0.03%	0.004%
12	3.832	772	775	781	rVB2	239	189	0.02%	0.002%
13	4.105	857	860	863	rBV2	167	137	0.01%	0.002%
14	4.620	1007	1020	1043	rBV	122691	297500	30.71%	3.825%
15	4.973	1126	1130	1135	rVB2	319	318	0.03%	0.004%
16	5.063	1141	1158	1181	rBV2	186994	417830	43.13%	5.373%
17	5.195	1196	1199	1206	rBV3	435	533	0.06%	0.007%
18	5.263	1216	1220	1222	rBV2	212	176	0.02%	0.002%
19	5.497	1290	1293	1295	rBV2	351	310	0.03%	0.004%
20	5.723	1341	1363	1382	rBV3	355647	968858	100.00%	12.458%
21	5.874	1405	1410	1416	rBV3	395	610	0.06%	0.008%
22	5.954	1433	1435	1438	rBV2	248	167	0.02%	0.002%
23	5.970	1438	1440	1446	rVB3	459	452	0.05%	0.006%
24	6.034	1458	1460	1463	rVB	336	196	0.02%	0.003%
25	6.247	1512	1526	1548	rBV	343000	651396	67.23%	8.376%
26	6.372	1562	1565	1567	rBV2	408	210	0.02%	0.003%
27	6.462	1591	1593	1598	rBV2	283	251	0.03%	0.003%
28	6.501	1602	1605	1607	rVV2	575	439	0.05%	0.006%
29	6.539	1607	1617	1629	rVB7	8726	18353	1.89%	0.236%
30	6.610	1636	1639	1642	rVB2	339	297	0.03%	0.004%
31	6.629	1642	1645	1647	rBV	314	203	0.02%	0.003%
32	6.690	1650	1664	1683	rBV	238325	456572	47.12%	5.871%
33	6.793	1693	1696	1698	rBV2	314	211	0.02%	0.003%
34	6.809	1698	1701	1704	rBV2	798	663	0.07%	0.009%
35	6.890	1722	1726	1727	rBV2	233	171	0.02%	0.002%
36	6.996	1756	1759	1763	rBV	288	201	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049024.D
 Acq On : 11 Jun 2022 02:05
 Operator : SY/MD
 Sample : N3291-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	7.038	1770	1772	1774	rBV	274	150	0.02%	0.002%
38	7.176	1805	1815	1818	rBV4	2093	2998	0.31%	0.039%
39	7.565	1923	1936	1958	rVB	116168	202637	20.92%	2.606%
40	7.642	1958	1960	1964	rBV3	408	303	0.03%	0.004%
41	7.687	1967	1974	1977	rBV3	1150	1415	0.15%	0.018%
42	7.771	1995	2000	2006	rVB2	296	355	0.04%	0.005%
43	7.896	2026	2039	2057	rBV	405012	698094	72.05%	8.976%
44	8.140	2112	2115	2116	rBV	255	138	0.01%	0.002%
45	8.179	2116	2127	2144	rVV2	81246	136370	14.08%	1.753%
46	8.462	2211	2215	2216	rBV2	650	407	0.04%	0.005%
47	8.632	2256	2268	2295	rBV2	324622	631873	65.22%	8.125%
48	8.838	2329	2332	2333	rBV	318	171	0.02%	0.002%
49	8.992	2373	2380	2387	rVB3	388	570	0.06%	0.007%
50	9.037	2391	2394	2397	rBV2	212	157	0.02%	0.002%
51	9.324	2477	2483	2488	rBV2	406	409	0.04%	0.005%
52	9.417	2499	2512	2545	rBV	485800	803927	82.98%	10.337%
53	9.716	2603	2605	2608	rBV	273	186	0.02%	0.002%
54	9.780	2622	2625	2628	rBV2	281	179	0.02%	0.002%
55	9.954	2676	2679	2681	rBV	241	163	0.02%	0.002%
56	10.018	2696	2699	2702	rVB	418	253	0.03%	0.003%
57	10.041	2702	2706	2712	rBV2	286	354	0.04%	0.005%
58	10.089	2718	2721	2723	rBV	281	202	0.02%	0.003%
59	10.156	2739	2742	2745	rBV2	338	228	0.02%	0.003%
60	10.526	2855	2857	2860	rBV2	194	135	0.01%	0.002%
61	10.571	2868	2871	2875	rBV2	215	185	0.02%	0.002%
62	10.758	2915	2929	2957	rBV	369774	596317	61.55%	7.668%
63	10.854	2957	2959	2961	rVB2	320	144	0.01%	0.002%
64	10.890	2965	2970	2975	rBV3	853	1266	0.13%	0.016%
65	10.944	2984	2987	2993	rBV2	412	420	0.04%	0.005%
66	11.111	3036	3039	3041	rVV2	343	198	0.02%	0.003%
67	11.124	3041	3043	3046	rVB	363	200	0.02%	0.003%
68	11.240	3075	3079	3082	rBV2	395	286	0.03%	0.004%
69	11.410	3129	3132	3136	rBV2	235	239	0.02%	0.003%
70	11.523	3163	3167	3169	rVB	379	227	0.02%	0.003%
71	11.674	3212	3214	3218	rVB	276	146	0.02%	0.002%
72	11.700	3219	3222	3224	rBV2	280	191	0.02%	0.002%
73	11.742	3230	3235	3238	rBV	486	442	0.05%	0.006%
74	11.812	3244	3257	3275	rBV	432738	688851	71.10%	8.858%
75	11.944	3295	3298	3302	rVB3	642	397	0.04%	0.005%
76	12.047	3324	3330	3335	rBV2	363	526	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049024.D
 Acq On : 11 Jun 2022 02:05
 Operator : SY/MD
 Sample : N3291-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	12.118	3347	3352	3355	rBV	353	416	0.04%	0.005%
78	12.195	3362	3376	3397	rBV	396918	656525	67.76%	8.442%
79	12.545	3483	3485	3488	rBV	340	193	0.02%	0.002%
80	12.597	3498	3501	3503	rBV2	303	153	0.02%	0.002%
81	12.658	3517	3520	3526	rVB2	411	303	0.03%	0.004%
82	12.928	3600	3604	3610	rBV2	490	564	0.06%	0.007%
83	13.069	3645	3648	3651	rBV2	290	240	0.02%	0.003%
84	13.086	3651	3653	3656	rVB	441	254	0.03%	0.003%
85	13.214	3690	3693	3696	rBV	306	253	0.03%	0.003%
86	13.259	3704	3707	3712	rBV	266	281	0.03%	0.004%
87	13.523	3787	3789	3791	rBV	252	140	0.01%	0.002%
88	13.639	3822	3825	3826	rBV	371	199	0.02%	0.003%
89	13.770	3863	3866	3870	rBV3	469	437	0.05%	0.006%
90	13.928	3912	3915	3920	rVB2	404	295	0.03%	0.004%
91	13.970	3925	3928	3929	rBV	334	195	0.02%	0.003%
92	14.256	4014	4017	4020	rBV2	469	327	0.03%	0.004%
93	14.581	4114	4118	4124	rVB3	586	614	0.06%	0.008%
94	15.060	4264	4267	4272	rBV3	470	343	0.04%	0.004%
95	15.401	4371	4373	4375	rBV2	499	270	0.03%	0.003%
96	15.548	4414	4419	4422	rBV4	886	847	0.09%	0.011%
97	15.648	4446	4450	4453	rVB2	635	499	0.05%	0.006%
98	15.667	4453	4456	4459	rBV	713	503	0.05%	0.006%
99	15.764	4482	4486	4488	rBV3	1109	965	0.10%	0.012%
100	15.915	4531	4533	4538	rVB2	1083	661	0.07%	0.008%




Sum of corrected areas: 7777029

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049024.D
Acq On : 11 Jun 2022 02:05
Operator : SY/MD
Sample : N3291-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

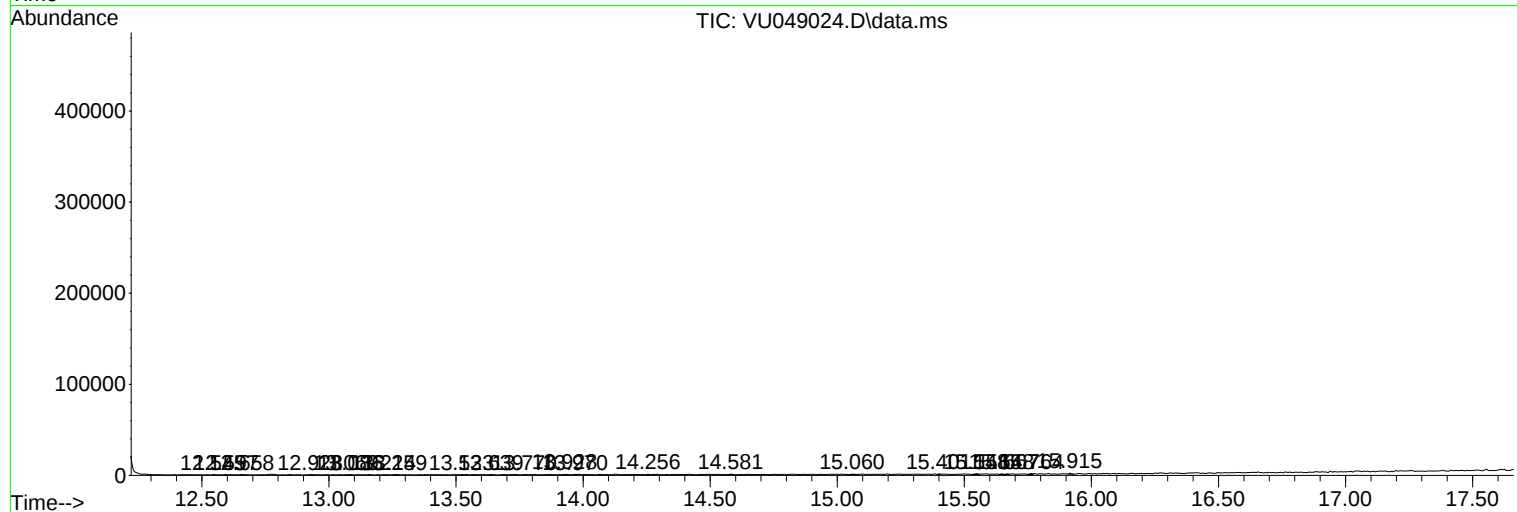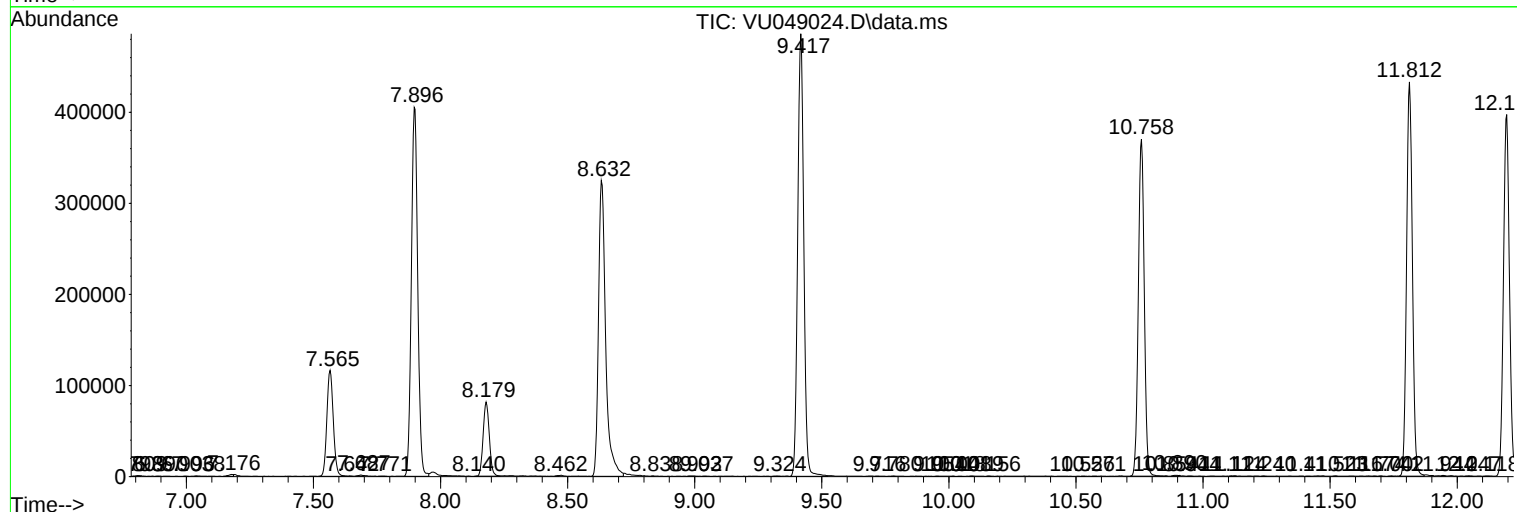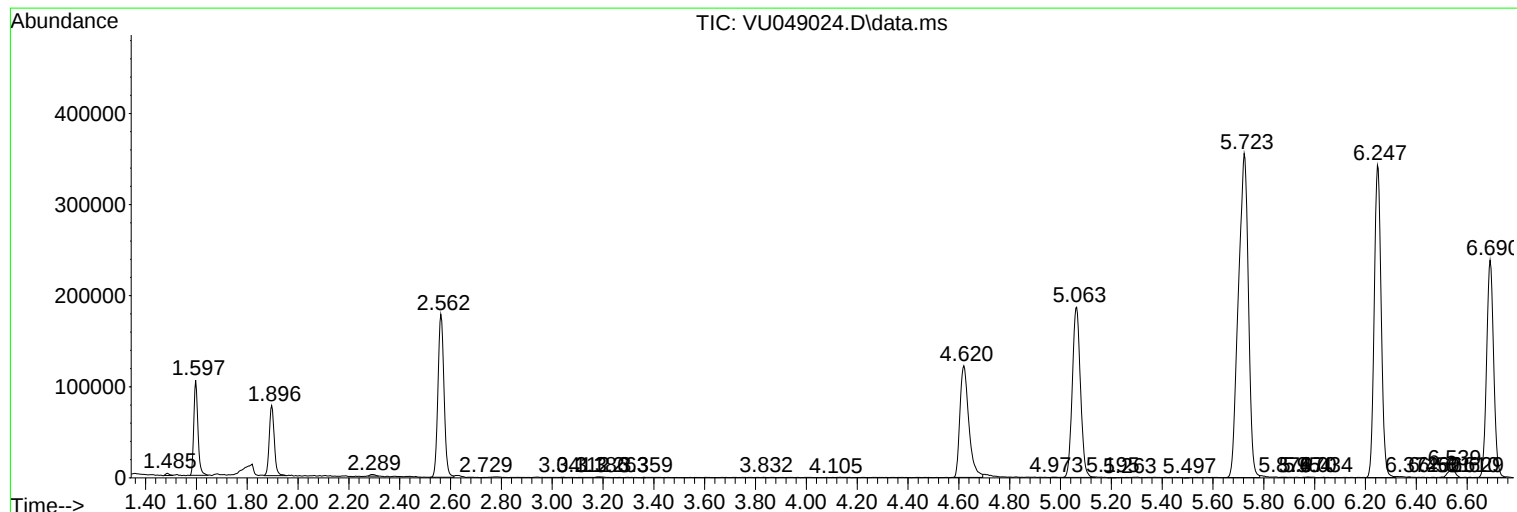

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049024.D
Acq On : 11 Jun 2022 02:05
Operator : SY/MD
Sample : N3291-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049024.D
Acq On : 11 Jun 2022 02:05
Operator : SY/MD
Sample : N3291-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc