

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049026.D
 Acq On : 11 Jun 2022 03:15
 Operator : SY/MD
 Sample : VU0610WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK141

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	40	46	52	rBV5	2259	2692	0.25%	0.032%
2	1.597	72	80	97	rBV	121241	137615	13.01%	1.661%
3	1.903	167	175	192	rVB	87998	117959	11.15%	1.424%
4	2.565	369	381	395	rBV	202746	330844	31.28%	3.994%
5	2.931	492	495	496	rBV	413	236	0.02%	0.003%
6	2.944	497	499	506	rVV2	579	694	0.07%	0.008%
7	3.041	522	529	539	rVB5	1171	2022	0.19%	0.024%
8	3.185	558	574	588	rBV2	9199	19241	1.82%	0.232%
9	3.285	601	605	611	rVB2	362	451	0.04%	0.005%
10	3.401	638	641	646	rVB2	358	327	0.03%	0.004%
11	3.485	663	667	674	rBV2	219	260	0.02%	0.003%
12	3.565	686	692	695	rBV2	200	232	0.02%	0.003%
13	3.751	746	750	753	rBV	330	261	0.02%	0.003%
14	3.777	753	758	760	rBV	297	235	0.02%	0.003%
15	4.620	1007	1020	1051	rBV	130811	316931	29.97%	3.826%
16	4.957	1121	1125	1129	rBV3	402	321	0.03%	0.004%
17	5.063	1140	1158	1177	rBV	197427	429298	40.59%	5.182%
18	5.176	1190	1193	1200	rVB4	412	343	0.03%	0.004%
19	5.214	1201	1205	1208	rVB2	576	462	0.04%	0.006%
20	5.578	1314	1318	1322	rVB2	276	245	0.02%	0.003%
21	5.722	1342	1363	1387	rBV2	387145	1057532	100.00%	12.766%
22	5.970	1439	1440	1444	rVB2	378	225	0.02%	0.003%
23	6.169	1499	1502	1506	rBV	237	256	0.02%	0.003%
24	6.250	1511	1527	1549	rBV	358493	681302	64.42%	8.225%
25	6.455	1588	1591	1597	rVB3	478	464	0.04%	0.006%
26	6.529	1604	1614	1624	rBV5	4639	7945	0.75%	0.096%
27	6.690	1650	1664	1681	rVV	253527	492363	46.56%	5.944%
28	6.800	1694	1698	1699	rBV3	470	264	0.02%	0.003%
29	6.992	1755	1758	1761	rVB2	407	256	0.02%	0.003%
30	7.012	1761	1764	1767	rBV	271	258	0.02%	0.003%
31	7.054	1773	1777	1781	rVV3	364	377	0.04%	0.005%
32	7.182	1807	1817	1821	rBV5	2007	3015	0.29%	0.036%
33	7.362	1869	1873	1876	rBV2	398	294	0.03%	0.004%
34	7.565	1923	1936	1955	rBV2	122903	215341	20.36%	2.600%
35	7.697	1967	1977	1984	rVB4	1311	2227	0.21%	0.027%
36	7.787	2002	2005	2006	rBV2	450	256	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049026.D
 Acq On : 11 Jun 2022 03:15
 Operator : SY/MD
 Sample : VU0610WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK141

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	7.899	2025	2040	2055	rBV	448518	775468	73.33%	9.361%
38	8.047	2084	2086	2097	rVB2	637	696	0.07%	0.008%
39	8.089	2097	2099	2103	rVB2	563	373	0.04%	0.005%
40	8.179	2113	2127	2145	rBV2	86450	146905	13.89%	1.773%
41	8.478	2217	2220	2222	rVB3	394	231	0.02%	0.003%
42	8.520	2230	2233	2237	rVB	376	300	0.03%	0.004%
43	8.552	2237	2243	2246	rBV3	626	492	0.05%	0.006%
44	8.632	2254	2268	2305	rBV2	342237	664491	62.83%	8.022%
45	8.951	2364	2367	2370	rBV2	324	251	0.02%	0.003%
46	9.002	2377	2383	2385	rBV	215	224	0.02%	0.003%
47	9.063	2399	2402	2406	rVB	358	262	0.02%	0.003%
48	9.163	2430	2433	2437	rVB2	351	279	0.03%	0.003%
49	9.208	2444	2447	2453	rVB	381	272	0.03%	0.003%
50	9.417	2498	2512	2536	rBV	505918	835601	79.01%	10.087%
51	9.561	2554	2557	2562	rBV5	590	559	0.05%	0.007%
52	9.651	2581	2585	2589	rVV2	335	376	0.04%	0.005%
53	9.693	2594	2598	2607	rVB3	902	1083	0.10%	0.013%
54	9.954	2676	2679	2684	rVV2	289	300	0.03%	0.004%
55	9.983	2685	2688	2695	rVB2	286	263	0.02%	0.003%
56	10.034	2701	2704	2706	rBV	280	225	0.02%	0.003%
57	10.095	2718	2723	2725	rBV2	384	321	0.03%	0.004%
58	10.356	2801	2804	2808	rVB	387	254	0.02%	0.003%
59	10.484	2833	2844	2849	rBV4	735	1080	0.10%	0.013%
60	10.561	2865	2868	2875	rBV	340	329	0.03%	0.004%
61	10.674	2895	2903	2904	rBV	897	841	0.08%	0.010%
62	10.758	2915	2929	2947	rBV	372706	615728	58.22%	7.433%
63	10.877	2960	2966	2973	rBV3	363	531	0.05%	0.006%
64	11.066	3022	3025	3027	rVV	300	227	0.02%	0.003%
65	11.089	3029	3032	3034	rVV3	595	408	0.04%	0.005%
66	11.114	3038	3040	3045	rVB3	477	466	0.04%	0.006%
67	11.147	3045	3050	3053	rBV2	398	463	0.04%	0.006%
68	11.237	3075	3078	3086	rVB2	330	455	0.04%	0.005%
69	11.275	3086	3090	3093	rBV	356	296	0.03%	0.004%
70	11.330	3102	3107	3109	rBV2	270	230	0.02%	0.003%
71	11.568	3176	3181	3184	rBV2	311	370	0.03%	0.004%
72	11.748	3231	3237	3245	rVB5	1512	1835	0.17%	0.022%
73	11.812	3245	3257	3282	rBV	430051	694518	65.67%	8.384%
74	11.970	3303	3306	3309	rBV2	489	368	0.03%	0.004%
75	12.044	3324	3329	3332	rBV2	348	361	0.03%	0.004%
76	12.192	3362	3375	3393	rBV	412602	678052	64.12%	8.185%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049026.D
 Acq On : 11 Jun 2022 03:15
 Operator : SY/MD
 Sample : VU0610WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK141

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	12.356	3424	3426	3431	rBV	347	289	0.03%	0.003%
78	12.555	3485	3488	3490	rBV2	329	241	0.02%	0.003%
79	12.638	3510	3514	3518	rVB2	472	366	0.03%	0.004%
80	12.671	3518	3524	3527	rBV2	434	485	0.05%	0.006%
81	12.716	3532	3538	3539	rBV2	311	279	0.03%	0.003%
82	12.979	3616	3620	3623	rBV	293	312	0.03%	0.004%
83	13.002	3623	3627	3635	rVB6	577	771	0.07%	0.009%
84	13.111	3658	3661	3663	rVB	424	252	0.02%	0.003%
85	13.134	3663	3668	3670	rBV	290	284	0.03%	0.003%
86	13.217	3690	3694	3696	rBV2	784	647	0.06%	0.008%
87	13.230	3696	3698	3705	rVB4	1037	1046	0.10%	0.013%
88	13.439	3759	3763	3766	rBV2	485	398	0.04%	0.005%
89	13.847	3884	3890	3900	rVB5	3810	5282	0.50%	0.064%
90	13.886	3900	3902	3906	rBV3	354	340	0.03%	0.004%
91	13.995	3934	3936	3940	rBV	363	284	0.03%	0.003%
92	14.095	3958	3967	3982	rBV2	7193	13931	1.32%	0.168%
93	14.336	4032	4042	4054	rBV6	4443	6996	0.66%	0.084%
94	14.873	4204	4209	4213	rBV3	476	565	0.05%	0.007%
95	15.002	4246	4249	4252	rBV2	437	305	0.03%	0.004%
96	15.220	4315	4317	4320	rVV2	506	287	0.03%	0.003%
97	15.384	4365	4368	4369	rBV	698	402	0.04%	0.005%
98	15.835	4506	4508	4511	rBV4	765	509	0.05%	0.006%
99	16.008	4560	4562	4565	rBV2	503	249	0.02%	0.003%
100	16.162	4607	4610	4612	rBV3	733	428	0.04%	0.005%




Sum of corrected areas: 8283776

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049026.D
Acq On : 11 Jun 2022 03:15
Operator : SY/MD
Sample : VU0610WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK141

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

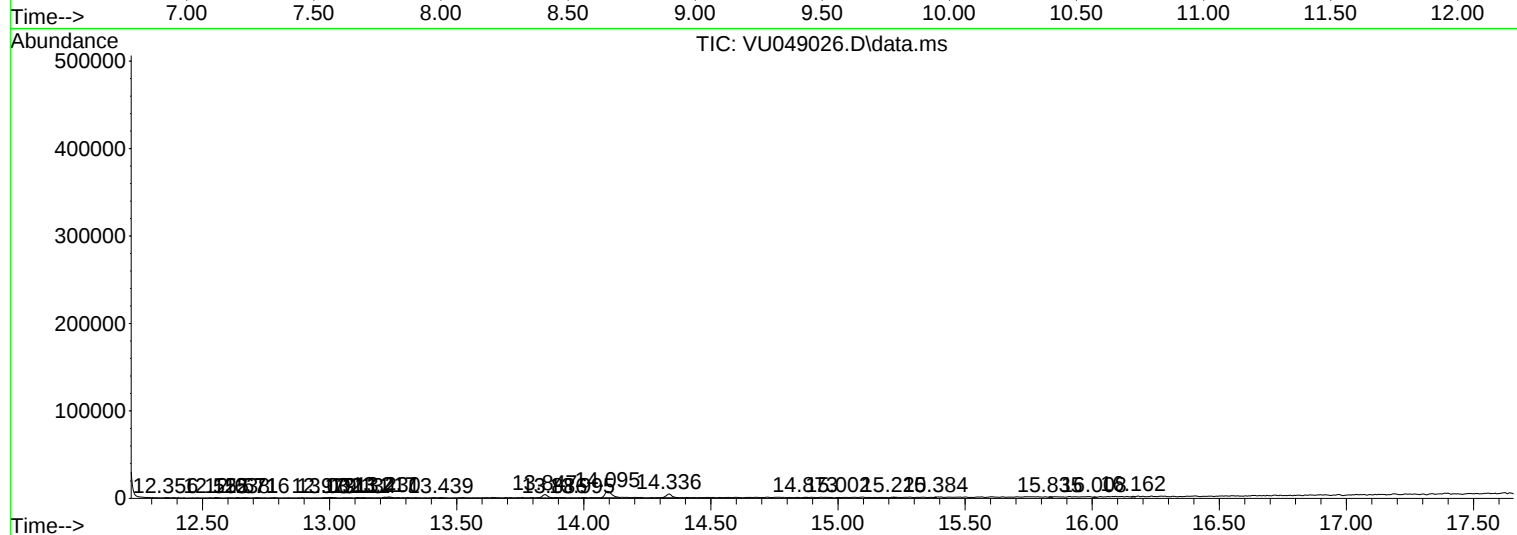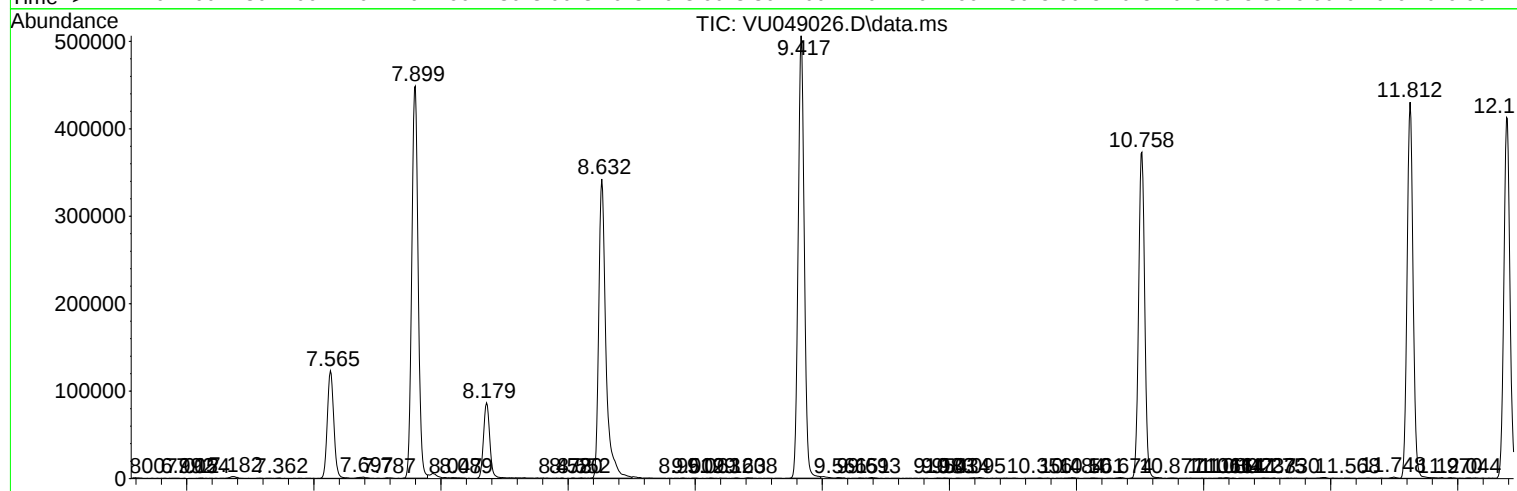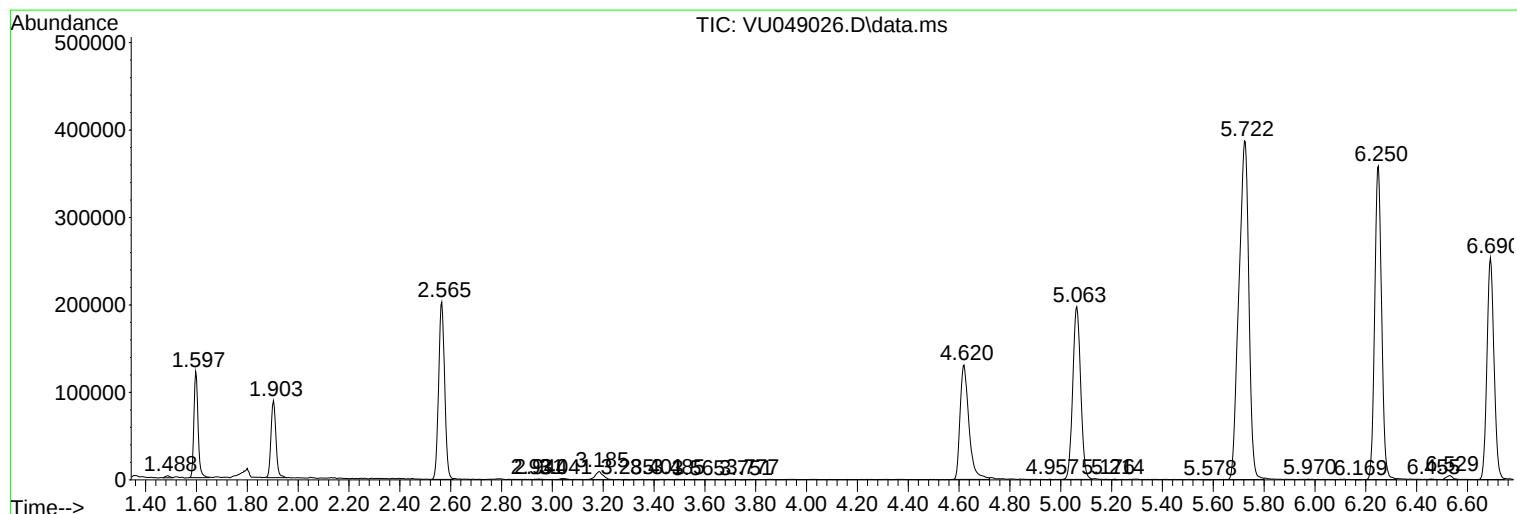

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049026.D
Acq On : 11 Jun 2022 03:15
Operator : SY/MD
Sample : VU0610WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK141

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049026.D
Acq On : 11 Jun 2022 03:15
Operator : SY/MD
Sample : VU0610WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK141

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------