

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049027.D
 Acq On : 11 Jun 2022 03:39
 Operator : SY/MD
 Sample : N3249-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	100	rBV2	113770	132202	13.69%	1.709%
2	1.906	169	176	191	rVB	77316	100698	10.42%	1.302%
3	2.565	369	381	396	rBV	174253	281184	29.11%	3.635%
4	2.781	445	448	449	rBV	353	160	0.02%	0.002%
5	2.867	474	475	477	rBV	133	47	0.00%	0.001%
6	2.945	497	499	500	rBV	156	61	0.01%	0.001%
7	3.051	530	532	536	rVB3	522	299	0.03%	0.004%
8	3.183	563	573	584	rVB2	2670	5359	0.55%	0.069%
9	3.237	589	590	591	rBV	120	35	0.00%	0.000%
10	3.298	604	609	611	rBV	227	245	0.03%	0.003%
11	3.353	616	626	642	rVB4	6289	12561	1.30%	0.162%
12	3.440	651	653	655	rVB	161	40	0.00%	0.001%
13	3.475	663	664	666	rBV	137	67	0.01%	0.001%
14	3.584	694	698	702	rVB2	268	175	0.02%	0.002%
15	3.732	742	744	746	rBV2	126	63	0.01%	0.001%
16	3.867	769	786	808	rBV	119829	282164	29.21%	3.648%
17	4.054	840	844	849	rBV	350	315	0.03%	0.004%
18	4.102	856	859	862	rVB	247	152	0.02%	0.002%
19	4.125	862	866	869	rBV2	135	103	0.01%	0.001%
20	4.144	869	872	877	rBV2	144	150	0.02%	0.002%
21	4.234	897	900	903	rBV	158	123	0.01%	0.002%
22	4.314	922	925	928	rBV	236	164	0.02%	0.002%
23	4.427	953	960	965	rBV	274	418	0.04%	0.005%
24	4.449	965	967	970	rBV2	141	90	0.01%	0.001%
25	4.572	1003	1005	1007	rBV	183	98	0.01%	0.001%
26	4.620	1007	1020	1026	rBV	120013	251168	26.00%	3.247%
27	4.993	1133	1136	1137	rBV	185	91	0.01%	0.001%
28	5.063	1142	1158	1178	rBV	188575	409873	42.43%	5.299%
29	5.317	1219	1237	1254	rBV	64054	143992	14.91%	1.861%
30	5.604	1323	1326	1327	rBV	226	122	0.01%	0.002%
31	5.649	1336	1340	1341	rBV	230	151	0.02%	0.002%
32	5.726	1342	1364	1382	rBV2	350553	965956	100.00%	12.487%
33	6.125	1486	1488	1490	rBV	192	104	0.01%	0.001%
34	6.250	1512	1527	1551	rBV	295887	563461	58.33%	7.284%
35	6.543	1607	1618	1632	rVB4	19691	39001	4.04%	0.504%
36	6.594	1632	1634	1636	rVB4	334	120	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049027.D
 Acq On : 11 Jun 2022 03:39
 Operator : SY/MD
 Sample : N3249-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.690	1650	1664	1685	rBV	235259	456296	47.24%	5.899%
38	6.803	1698	1699	1701	rBV3	696	306	0.03%	0.004%
39	6.861	1714	1717	1718	rBV2	235	159	0.02%	0.002%
40	6.870	1718	1720	1725	rVB2	371	251	0.03%	0.003%
41	6.970	1742	1751	1752	rBV4	1602	1774	0.18%	0.023%
42	7.108	1790	1794	1796	rBV	362	299	0.03%	0.004%
43	7.182	1808	1817	1819	rBV3	703	948	0.10%	0.012%
44	7.227	1827	1831	1836	rVB2	288	376	0.04%	0.005%
45	7.250	1836	1838	1839	rBV2	125	61	0.01%	0.001%
46	7.260	1839	1841	1842	rBV	179	47	0.00%	0.001%
47	7.276	1842	1846	1848	rBV2	176	145	0.02%	0.002%
48	7.288	1848	1850	1852	rVB	188	65	0.01%	0.001%
49	7.350	1866	1869	1870	rBV	393	164	0.02%	0.002%
50	7.420	1889	1891	1893	rBV2	231	120	0.01%	0.002%
51	7.443	1893	1898	1899	rVV	126	119	0.01%	0.002%
52	7.472	1906	1907	1908	rBB	66	25	0.00%	0.000%
53	7.565	1923	1936	1957	rBV	101460	179911	18.63%	2.326%
54	7.716	1979	1983	1985	rBV	426	322	0.03%	0.004%
55	7.732	1985	1988	1993	rVV	257	199	0.02%	0.003%
56	7.774	1998	2001	2003	rBV2	358	240	0.02%	0.003%
57	7.899	2025	2040	2063	rBV	398276	696572	72.11%	9.005%
58	8.179	2115	2127	2141	rBV	72022	123390	12.77%	1.595%
59	8.398	2191	2195	2206	rVB5	1181	1649	0.17%	0.021%
60	8.440	2206	2208	2210	rVB	173	79	0.01%	0.001%
61	8.472	2210	2218	2230	rBV4	2213	3854	0.40%	0.050%
62	8.552	2235	2243	2255	rVB3	11911	19876	2.06%	0.257%
63	8.632	2255	2268	2299	rBV3	297389	603042	62.43%	7.796%
64	8.935	2360	2362	2364	rBV	254	101	0.01%	0.001%
65	8.983	2375	2377	2378	rBV	280	67	0.01%	0.001%
66	9.124	2418	2421	2426	rBV2	224	156	0.02%	0.002%
67	9.166	2431	2434	2436	rBV	391	254	0.03%	0.003%
68	9.227	2448	2453	2456	rBV2	332	316	0.03%	0.004%
69	9.417	2499	2512	2535	rBV	415914	696823	72.14%	9.008%
70	9.597	2566	2568	2571	rBV2	175	130	0.01%	0.002%
71	9.677	2591	2593	2595	rBV	315	142	0.01%	0.002%
72	9.700	2595	2600	2606	rVB2	923	1037	0.11%	0.013%
73	9.729	2606	2609	2612	rBV2	470	224	0.02%	0.003%
74	9.938	2672	2674	2676	rBV	322	114	0.01%	0.001%
75	10.070	2712	2715	2718	rBV2	220	151	0.02%	0.002%
76	10.227	2763	2764	2769	rBV2	231	121	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049027.D
 Acq On : 11 Jun 2022 03:39
 Operator : SY/MD
 Sample : N3249-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

77	10.484	2840	2844	2848	rBV3	522	492	0.05%	0.006%
78	10.607	2881	2882	2883	rBV	153	48	0.00%	0.001%
79	10.706	2910	2913	2916	rBV	341	356	0.04%	0.005%
80	10.755	2916	2928	2949	rVV	338443	560355	58.01%	7.244%
81	10.890	2961	2970	2981	rBV3	3721	5995	0.62%	0.077%
82	11.343	3107	3111	3114	rBV	541	427	0.04%	0.006%
83	11.812	3244	3257	3281	rBV	354095	568797	58.88%	7.353%
84	12.076	3337	3339	3342	rBV2	292	161	0.02%	0.002%
85	12.192	3362	3375	3394	rBV	374763	617059	63.88%	7.977%
86	12.629	3509	3511	3514	rBV	285	145	0.02%	0.002%
87	12.986	3619	3622	3629	rBV2	371	490	0.05%	0.006%
88	13.510	3784	3785	3789	rBV	312	113	0.01%	0.001%
89	13.533	3790	3792	3795	rVV	370	138	0.01%	0.002%




Sum of corrected areas: 7735513

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049027.D
Acq On : 11 Jun 2022 03:39
Operator : SY/MD
Sample : N3249-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

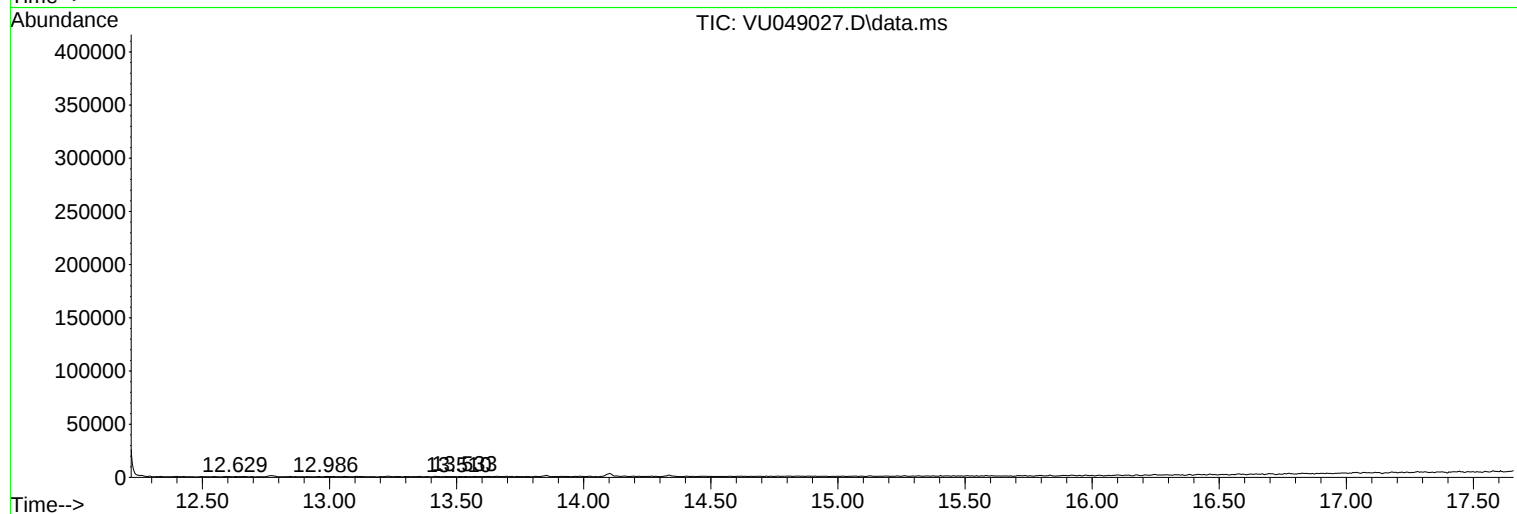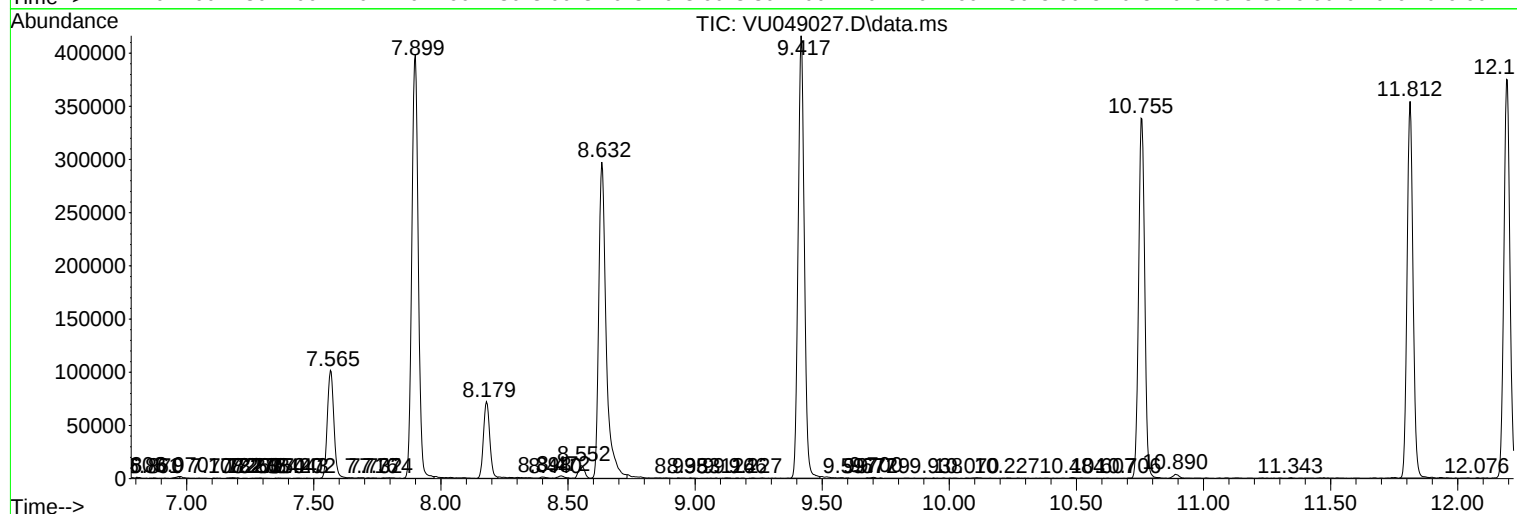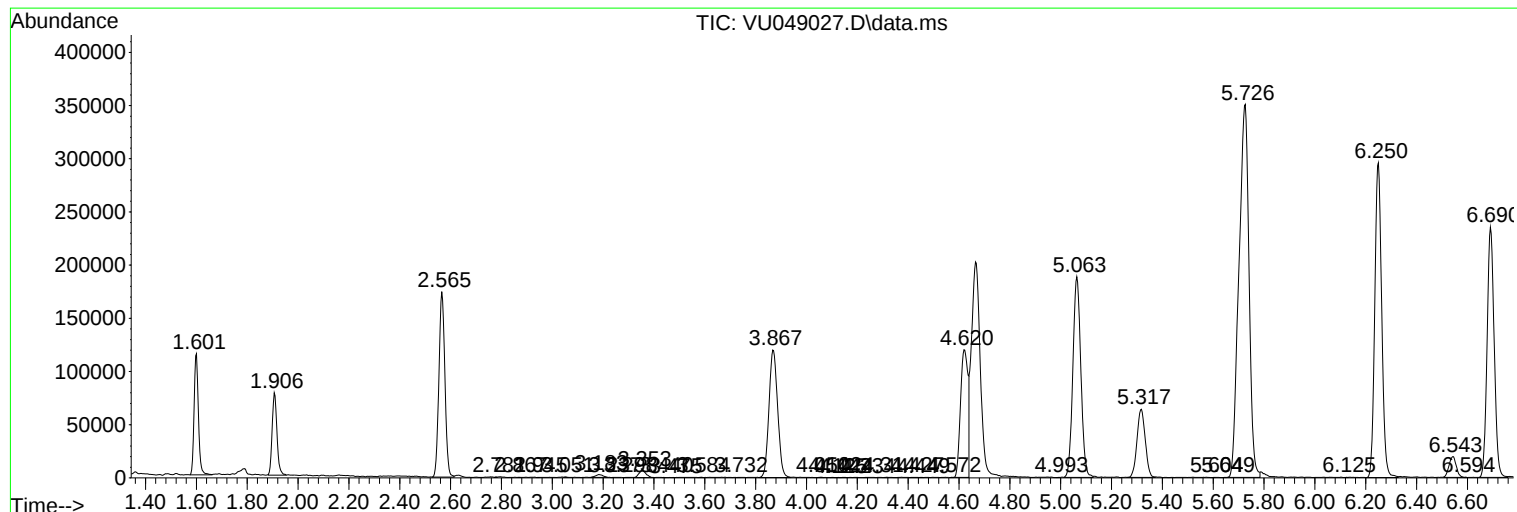

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049027.D
Acq On : 11 Jun 2022 03:39
Operator : SY/MD
Sample : N3249-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049027.D
Acq On : 11 Jun 2022 03:39
Operator : SY/MD
Sample : N3249-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc