

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049030.D
 Acq On : 11 Jun 2022 04:49
 Operator : SY/MD
 Sample : N3249-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	103736	116788	12.86%	1.664%
2	1.899	166	174	186	rBV	73135	95839	10.55%	1.366%
3	2.485	352	356	359	rBV3	386	337	0.04%	0.005%
4	2.565	369	381	393	rBV	165264	270593	29.79%	3.855%
5	2.623	395	399	412	rVV2	3772	5967	0.66%	0.085%
6	2.723	427	430	432	rBV2	359	189	0.02%	0.003%
7	2.761	438	442	445	rBV2	359	367	0.04%	0.005%
8	2.842	464	467	475	rVB2	378	492	0.05%	0.007%
9	2.877	475	478	479	rBV	356	210	0.02%	0.003%
10	2.944	493	499	503	rBV2	281	368	0.04%	0.005%
11	3.041	526	529	532	rBV2	347	271	0.03%	0.004%
12	3.189	561	575	587	rVV3	1614	3443	0.38%	0.049%
13	3.411	640	644	648	rBV2	260	214	0.02%	0.003%
14	3.755	747	751	757	rBV	260	289	0.03%	0.004%
15	3.867	779	786	794	rBV4	746	1518	0.17%	0.022%
16	4.208	888	892	897	rBV2	159	209	0.02%	0.003%
17	4.382	942	946	951	rBV2	260	339	0.04%	0.005%
18	4.404	951	953	959	rVV2	283	251	0.03%	0.004%
19	4.620	1007	1020	1049	rBV	111524	280707	30.90%	4.000%
20	4.832	1083	1086	1091	rVB3	309	279	0.03%	0.004%
21	5.063	1139	1158	1182	rBV	175012	382672	42.13%	5.452%
22	5.317	1222	1237	1252	rVV4	30396	69842	7.69%	0.995%
23	5.449	1276	1278	1281	rVB	311	185	0.02%	0.003%
24	5.526	1299	1302	1303	rBV2	406	242	0.03%	0.003%
25	5.722	1342	1363	1387	rBV2	325650	908292	100.00%	12.941%
26	5.848	1400	1402	1408	rVB4	481	411	0.05%	0.006%
27	5.980	1435	1443	1445	rBV3	428	507	0.06%	0.007%
28	6.063	1466	1469	1473	rBV2	248	269	0.03%	0.004%
29	6.118	1484	1486	1493	rVB2	307	251	0.03%	0.004%
30	6.247	1511	1526	1545	rBV	279565	533144	58.70%	7.596%
31	6.385	1564	1569	1571	rBV2	208	197	0.02%	0.003%
32	6.539	1607	1617	1625	rVB6	3257	6140	0.68%	0.087%
33	6.690	1649	1664	1680	rBV	224393	432871	47.66%	6.168%
34	6.784	1691	1693	1696	rVB3	351	189	0.02%	0.003%
35	6.812	1696	1702	1705	rBV3	415	381	0.04%	0.005%
36	7.079	1777	1785	1789	rBV3	327	411	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049030.D
 Acq On : 11 Jun 2022 04:49
 Operator : SY/MD
 Sample : N3249-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	7.163	1807	1811	1813	rBV2	497	353	0.04%	0.005%
38	7.185	1813	1818	1823	rVV3	1233	1285	0.14%	0.018%
39	7.349	1867	1869	1876	rBV2	273	371	0.04%	0.005%
40	7.382	1876	1879	1884	rVB	318	227	0.02%	0.003%
41	7.565	1924	1936	1956	rVV	90678	158770	17.48%	2.262%
42	7.693	1968	1976	1983	rVB4	529	1010	0.11%	0.014%
43	7.793	2003	2007	2008	rBV2	336	242	0.03%	0.003%
44	7.851	2020	2025	2026	rBV	448	328	0.04%	0.005%
45	7.899	2026	2040	2058	rVV	384688	660979	72.77%	9.418%
46	8.099	2100	2102	2108	rVB3	619	380	0.04%	0.005%
47	8.179	2115	2127	2144	rBV	68815	115321	12.70%	1.643%
48	8.246	2144	2148	2150	rVB3	503	406	0.04%	0.006%
49	8.468	2214	2217	2220	rBV2	525	422	0.05%	0.006%
50	8.552	2234	2243	2251	rBV5	5521	8638	0.95%	0.123%
51	8.632	2256	2268	2297	rBV3	302071	597743	65.81%	8.517%
52	8.915	2351	2356	2357	rBV3	354	218	0.02%	0.003%
53	9.127	2419	2422	2426	rBV2	366	224	0.02%	0.003%
54	9.259	2459	2463	2468	rBV2	170	200	0.02%	0.003%
55	9.417	2499	2512	2530	rBV	392707	647789	71.32%	9.230%
56	9.568	2553	2559	2561	rBV3	478	502	0.06%	0.007%
57	9.619	2571	2575	2581	rBV2	266	335	0.04%	0.005%
58	9.726	2604	2608	2611	rBV2	204	200	0.02%	0.003%
59	9.960	2676	2681	2685	rBV2	380	356	0.04%	0.005%
60	10.105	2723	2726	2728	rBV	358	259	0.03%	0.004%
61	10.291	2779	2784	2787	rBV2	408	414	0.05%	0.006%
62	10.311	2787	2790	2795	rVV2	195	195	0.02%	0.003%
63	10.488	2842	2845	2849	rVB3	367	265	0.03%	0.004%
64	10.754	2915	2928	2949	rVB	339640	550516	60.61%	7.844%
65	10.893	2963	2971	2980	rVB3	1725	2621	0.29%	0.037%
66	11.015	3006	3009	3014	rVB2	241	222	0.02%	0.003%
67	11.047	3014	3019	3023	rBV2	216	219	0.02%	0.003%
68	11.086	3027	3031	3039	rVB4	483	572	0.06%	0.008%
69	11.140	3045	3048	3054	rBV2	204	263	0.03%	0.004%
70	11.372	3117	3120	3129	rVB2	362	537	0.06%	0.008%
71	11.414	3129	3133	3136	rBV2	196	208	0.02%	0.003%
72	11.475	3147	3152	3156	rBV2	426	470	0.05%	0.007%
73	11.587	3184	3187	3190	rVB	291	206	0.02%	0.003%
74	11.648	3204	3206	3211	rVB2	344	213	0.02%	0.003%
75	11.751	3233	3238	3241	rBV2	546	515	0.06%	0.007%
76	11.812	3245	3257	3280	rBV	341749	542989	59.78%	7.737%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049030.D
 Acq On : 11 Jun 2022 04:49
 Operator : SY/MD
 Sample : N3249-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	12.008	3314	3318	3320	rBV2	303	235	0.03%	0.003%
78	12.192	3362	3375	3397	rBV	364779	598354	65.88%	8.525%
79	12.439	3447	3452	3456	rBV2	276	300	0.03%	0.004%
80	12.629	3508	3511	3513	rBV	343	189	0.02%	0.003%
81	12.761	3548	3552	3553	rBV2	465	339	0.04%	0.005%
82	13.063	3643	3646	3650	rBV	267	266	0.03%	0.004%
83	13.230	3695	3698	3700	rBV	373	204	0.02%	0.003%
84	13.288	3712	3716	3723	rBV3	494	495	0.05%	0.007%
85	13.381	3742	3745	3748	rBV2	409	271	0.03%	0.004%
86	13.529	3788	3791	3793	rBV	526	397	0.04%	0.006%
87	13.568	3801	3803	3808	rVB3	269	185	0.02%	0.003%
88	13.677	3834	3837	3841	rBV2	406	380	0.04%	0.005%
89	13.790	3869	3872	3875	rVB2	470	296	0.03%	0.004%
90	13.928	3912	3915	3918	rBV	376	258	0.03%	0.004%
91	13.963	3923	3926	3929	rBV2	271	223	0.02%	0.003%
92	14.066	3953	3958	3961	rBV3	439	394	0.04%	0.006%
93	14.095	3961	3967	3968	rBV	1100	1061	0.12%	0.015%
94	14.333	4037	4041	4043	rBV2	663	474	0.05%	0.007%
95	14.407	4061	4064	4067	rBV	429	312	0.03%	0.004%
96	14.471	4081	4084	4088	rVB2	405	254	0.03%	0.004%
97	15.674	4455	4458	4461	rVB2	695	375	0.04%	0.005%
98	15.844	4509	4511	4513	rBV2	723	361	0.04%	0.005%
99	16.011	4560	4563	4565	rBV	714	422	0.05%	0.006%
100	16.028	4566	4568	4573	rVB4	1317	792	0.09%	0.011%




Sum of corrected areas: 7018494

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049030.D
Acq On : 11 Jun 2022 04:49
Operator : SY/MD
Sample : N3249-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

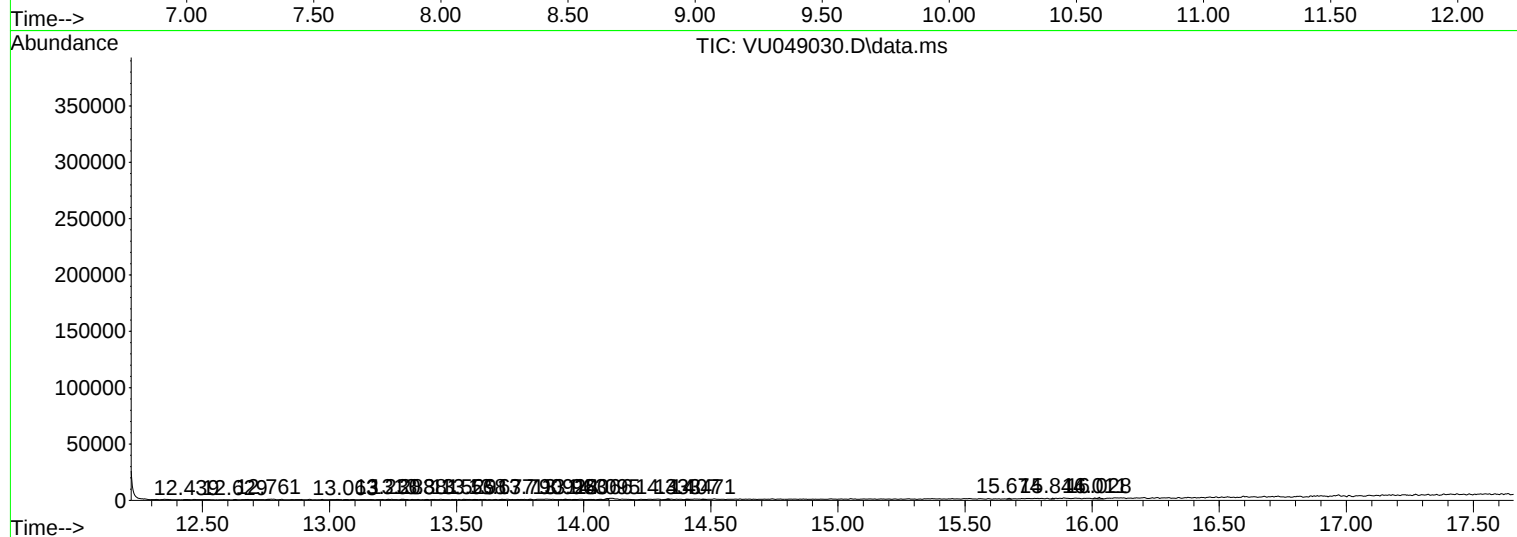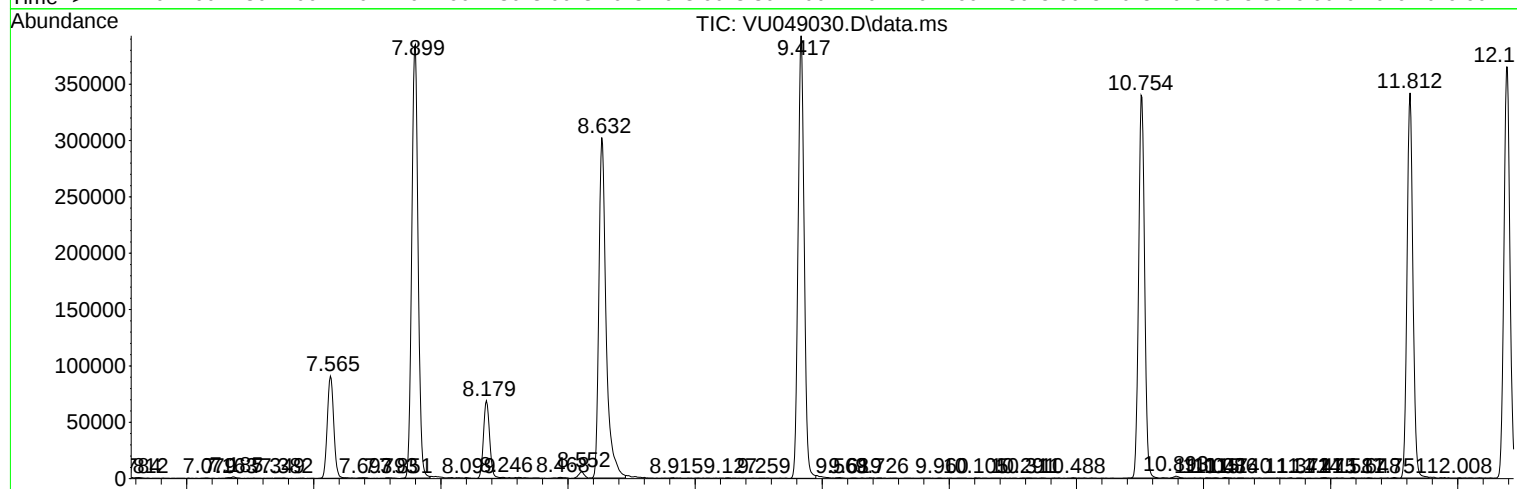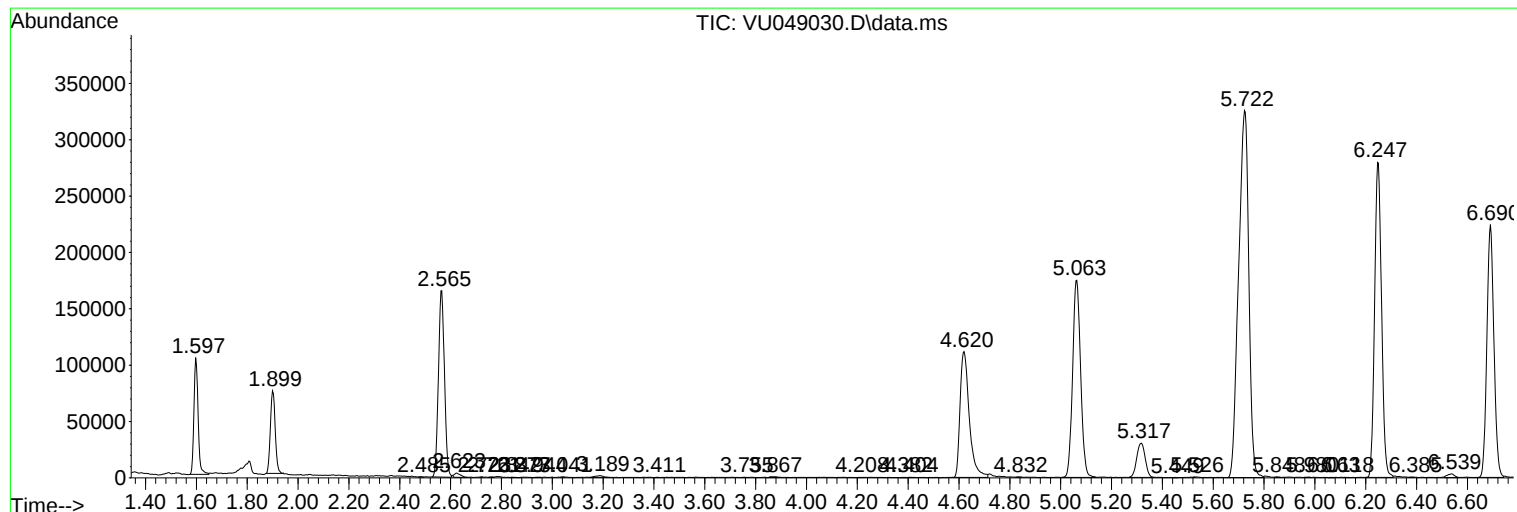

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049030.D
Acq On : 11 Jun 2022 04:49
Operator : SY/MD
Sample : N3249-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049030.D
Acq On : 11 Jun 2022 04:49
Operator : SY/MD
Sample : N3249-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------