

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049031.D
 Acq On : 11 Jun 2022 05:12
 Operator : SY/MD
 Sample : N3249-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	96649	111468	12.46%	1.516%
2	1.890	163	171	187	rVB	70246	93949	10.50%	1.277%
3	2.562	367	380	394	rBV2	163719	270813	30.27%	3.682%
4	2.761	436	442	443	rBV2	760	782	0.09%	0.011%
5	2.919	483	491	495	rBV2	291	449	0.05%	0.006%
6	3.031	521	526	527	rBV2	464	255	0.03%	0.003%
7	3.044	527	530	534	rVV2	490	463	0.05%	0.006%
8	3.173	561	570	577	rBV3	1583	3045	0.34%	0.041%
9	3.317	611	615	621	rBV2	302	339	0.04%	0.005%
10	3.443	651	654	661	rVB2	356	420	0.05%	0.006%
11	3.597	696	702	706	rBV	340	427	0.05%	0.006%
12	3.623	706	710	712	rBV	269	239	0.03%	0.003%
13	3.642	712	716	719	rVV2	324	276	0.03%	0.004%
14	3.867	773	786	800	rBV4	4138	9219	1.03%	0.125%
15	3.986	820	823	832	rVB2	371	491	0.05%	0.007%
16	4.108	857	861	863	rBV	304	260	0.03%	0.004%
17	4.150	868	874	878	rVB2	196	236	0.03%	0.003%
18	4.388	940	948	951	rBV2	186	258	0.03%	0.004%
19	4.420	951	958	961	rBV	291	291	0.03%	0.004%
20	4.465	967	972	975	rBV2	286	317	0.04%	0.004%
21	4.539	987	995	997	rBV	365	482	0.05%	0.007%
22	4.620	1006	1020	1046	rBV	111248	284591	31.81%	3.870%
23	4.851	1087	1092	1095	rBV2	512	359	0.04%	0.005%
24	5.060	1140	1157	1177	rBV	168632	372546	41.64%	5.065%
25	5.153	1182	1186	1190	rVB3	374	370	0.04%	0.005%
26	5.179	1190	1194	1202	rVB3	403	410	0.05%	0.006%
27	5.314	1219	1236	1259	rBV	122010	273096	30.52%	3.713%
28	5.722	1341	1363	1390	rBV2	328635	894707	100.00%	12.165%
29	5.967	1433	1439	1445	rBV5	628	700	0.08%	0.010%
30	6.157	1495	1498	1502	rVB	430	256	0.03%	0.003%
31	6.247	1512	1526	1554	rBV	272046	518357	57.94%	7.048%
32	6.430	1581	1583	1589	rVB2	349	237	0.03%	0.003%
33	6.533	1606	1615	1626	rBV10	4044	8754	0.98%	0.119%
34	6.690	1649	1664	1685	rBV	220584	429930	48.05%	5.846%
35	6.800	1694	1698	1700	rBV2	659	403	0.05%	0.005%
36	7.173	1803	1814	1816	rBV4	1395	1846	0.21%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049031.D
 Acq On : 11 Jun 2022 05:12
 Operator : SY/MD
 Sample : N3249-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	7.507	1914	1918	1924	rBV2	390	377	0.04%	0.005%
38	7.565	1924	1936	1954	rBV	93350	163453	18.27%	2.222%
39	7.697	1973	1977	1980	rBV2	450	387	0.04%	0.005%
40	7.896	2025	2039	2058	rBV	385406	661111	73.89%	8.989%
41	8.079	2092	2096	2103	rVB3	571	585	0.07%	0.008%
42	8.179	2115	2127	2142	rBV	68051	114051	12.75%	1.551%
43	8.320	2168	2171	2173	rBV3	462	286	0.03%	0.004%
44	8.410	2196	2199	2203	rVB3	421	266	0.03%	0.004%
45	8.439	2203	2208	2211	rBV2	387	424	0.05%	0.006%
46	8.462	2211	2215	2216	rBV	550	390	0.04%	0.005%
47	8.555	2233	2244	2254	rVB4	13245	22033	2.46%	0.300%
48	8.636	2255	2269	2302	rBV2	327293	660296	73.80%	8.978%
49	8.796	2317	2319	2321	rBV3	485	264	0.03%	0.004%
50	8.838	2330	2332	2340	rVB3	679	568	0.06%	0.008%
51	8.873	2340	2343	2346	rBV	473	294	0.03%	0.004%
52	8.893	2346	2349	2352	rVV2	343	252	0.03%	0.003%
53	8.909	2352	2354	2358	rVV	329	229	0.03%	0.003%
54	9.217	2444	2450	2455	rBV2	271	342	0.04%	0.005%
55	9.417	2498	2512	2534	rBV	384857	635773	71.06%	8.644%
56	9.568	2555	2559	2563	rVV2	400	373	0.04%	0.005%
57	9.687	2593	2596	2607	rVB5	879	1297	0.14%	0.018%
58	9.783	2623	2626	2630	rBV2	467	415	0.05%	0.006%
59	9.825	2634	2639	2643	rVB2	240	236	0.03%	0.003%
60	9.928	2666	2671	2673	rBV	284	230	0.03%	0.003%
61	10.098	2722	2724	2727	rBV	399	310	0.03%	0.004%
62	10.115	2727	2729	2731	rVV	578	276	0.03%	0.004%
63	10.150	2737	2740	2743	rVB	312	245	0.03%	0.003%
64	10.205	2747	2757	2760	rBV2	362	601	0.07%	0.008%
65	10.481	2837	2843	2848	rVB3	286	416	0.05%	0.006%
66	10.510	2848	2852	2856	rBV2	249	265	0.03%	0.004%
67	10.632	2887	2890	2898	rVB	383	377	0.04%	0.005%
68	10.758	2915	2929	2946	rBV	370777	593423	66.33%	8.069%
69	10.893	2963	2971	2981	rVB3	1557	2672	0.30%	0.036%
70	10.951	2981	2989	2993	rBV2	412	668	0.07%	0.009%
71	11.272	3085	3089	3094	rBV2	307	271	0.03%	0.004%
72	11.578	3180	3184	3189	rVB2	280	290	0.03%	0.004%
73	11.658	3207	3209	3212	rBV2	392	261	0.03%	0.004%
74	11.812	3245	3257	3282	rVV	363537	576203	64.40%	7.835%
75	11.899	3282	3284	3285	rBV	538	242	0.03%	0.003%
76	12.192	3362	3375	3402	rBV	373178	624853	69.84%	8.496%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049031.D
 Acq On : 11 Jun 2022 05:12
 Operator : SY/MD
 Sample : N3249-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	12.378	3431	3433	3440	rVB4	374	363	0.04%	0.005%
78	12.413	3440	3444	3446	rBV2	380	273	0.03%	0.004%
79	12.597	3495	3501	3502	rBV	356	374	0.04%	0.005%
80	12.764	3548	3553	3554	rBV2	512	445	0.05%	0.006%
81	12.835	3571	3575	3578	rBV2	309	259	0.03%	0.004%
82	12.909	3594	3598	3603	rVV2	290	370	0.04%	0.005%
83	12.986	3618	3622	3624	rBV	440	361	0.04%	0.005%
84	13.005	3624	3628	3633	rVV2	349	401	0.04%	0.005%
85	13.034	3635	3637	3640	rVB	458	251	0.03%	0.003%
86	13.131	3664	3667	3671	rBV	445	395	0.04%	0.005%
87	13.481	3773	3776	3778	rBV	440	267	0.03%	0.004%
88	13.516	3782	3787	3790	rBV2	417	401	0.04%	0.005%
89	13.645	3823	3827	3830	rBV2	350	320	0.04%	0.004%
90	13.690	3839	3841	3844	rBV2	392	255	0.03%	0.003%
91	13.812	3876	3879	3882	rBV	350	264	0.03%	0.004%
92	13.886	3899	3902	3903	rBV	400	245	0.03%	0.003%
93	14.311	4028	4034	4037	rBV3	468	585	0.07%	0.008%
94	14.500	4090	4093	4098	rVB2	574	433	0.05%	0.006%
95	14.539	4103	4105	4108	rBV3	385	282	0.03%	0.004%
96	14.626	4129	4132	4135	rBV2	322	279	0.03%	0.004%
97	15.153	4293	4296	4300	rBV2	573	426	0.05%	0.006%
98	15.346	4353	4356	4359	rBV2	498	366	0.04%	0.005%
99	15.619	4438	4441	4444	rBV2	510	415	0.05%	0.006%
100	15.918	4532	4534	4537	rBV2	679	308	0.03%	0.004%




Sum of corrected areas: 7354684

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049031.D
Acq On : 11 Jun 2022 05:12
Operator : SY/MD
Sample : N3249-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

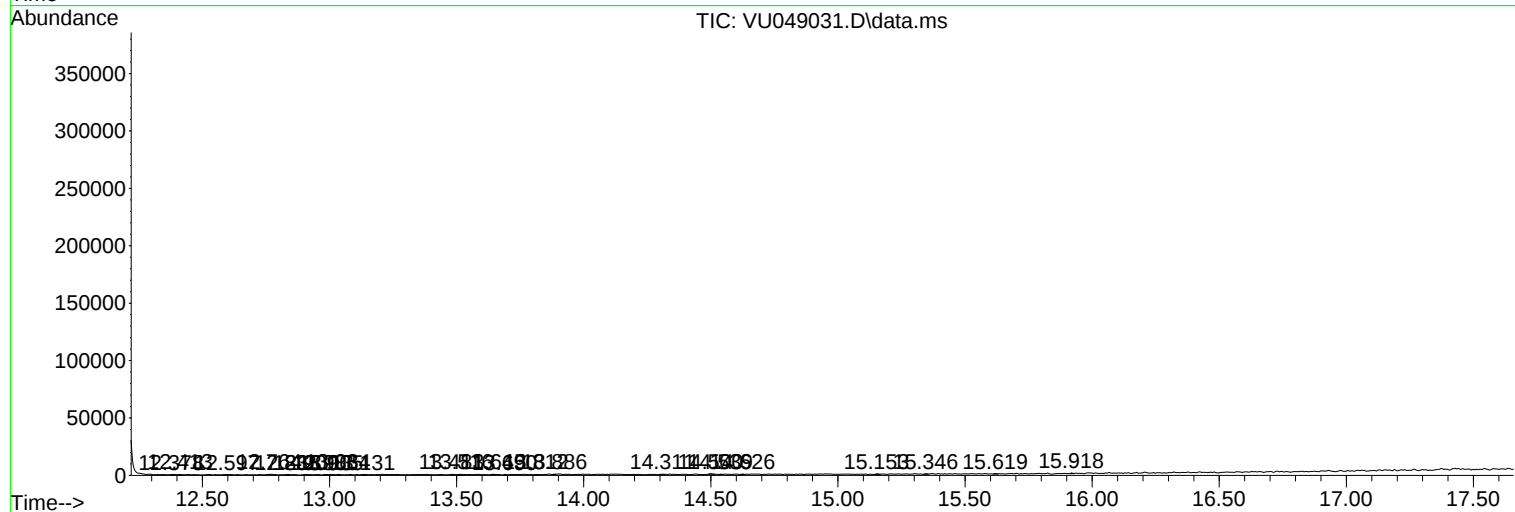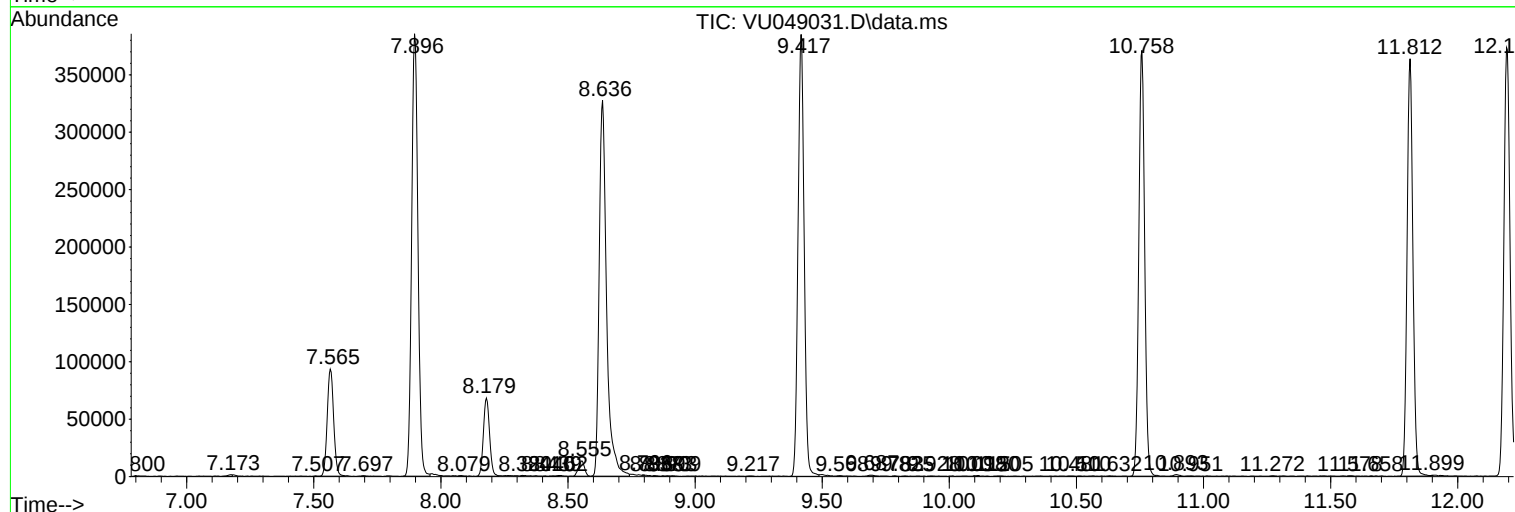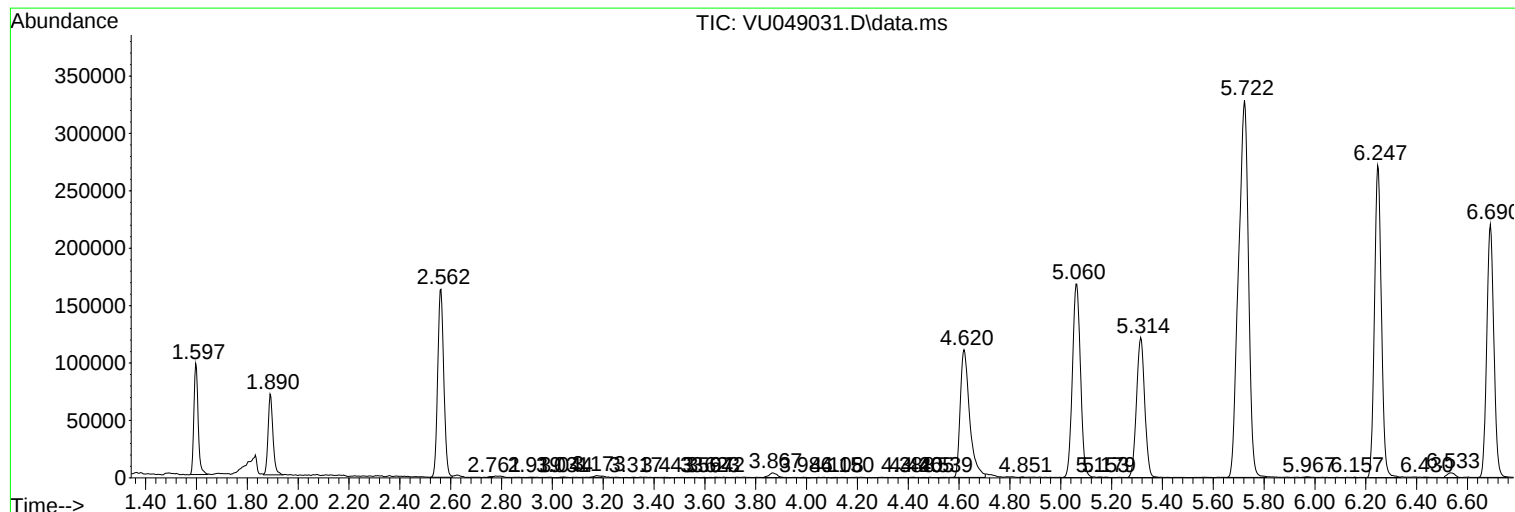

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049031.D
Acq On : 11 Jun 2022 05:12
Operator : SY/MD
Sample : N3249-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049031.D
Acq On : 11 Jun 2022 05:12
Operator : SY/MD
Sample : N3249-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------