

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049040.D
 Acq On : 11 Jun 2022 08:43
 Operator : SY/MD
 Sample : N3248-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rBV	110938	126266	12.66%	1.477%
2	1.906	168	176	197	rVB	82884	112436	11.28%	1.315%
3	2.131	244	246	249	rBV3	975	686	0.07%	0.008%
4	2.565	369	381	397	rBV2	187752	320313	32.13%	3.746%
5	2.687	415	419	422	rBV2	368	304	0.03%	0.004%
6	2.777	444	447	449	rBV3	495	284	0.03%	0.003%
7	2.851	467	470	473	rVB2	475	317	0.03%	0.004%
8	2.951	497	501	503	rBV2	304	273	0.03%	0.003%
9	3.048	527	531	537	rVB4	841	881	0.09%	0.010%
10	3.186	564	574	584	rVV3	1699	3272	0.33%	0.038%
11	3.285	601	605	607	rBV2	394	294	0.03%	0.003%
12	3.353	617	626	638	rBV5	3153	5775	0.58%	0.068%
13	3.430	646	650	655	rBV2	346	338	0.03%	0.004%
14	3.552	684	688	690	rBV2	429	304	0.03%	0.004%
15	3.867	770	786	804	rBV2	39305	90982	9.13%	1.064%
16	4.183	881	884	888	rBV	275	257	0.03%	0.003%
17	4.208	888	892	899	rBV2	227	374	0.04%	0.004%
18	4.346	932	935	939	rBV	308	337	0.03%	0.004%
19	4.420	955	958	965	rVB2	341	355	0.04%	0.004%
20	4.620	1006	1020	1030	rBV	116352	277610	27.84%	3.246%
21	5.064	1139	1158	1178	rBV	182562	399310	40.05%	4.670%
22	5.318	1216	1237	1259	rBV	441749	997058	100.00%	11.660%
23	5.395	1259	1261	1264	rVB3	528	345	0.03%	0.004%
24	5.469	1281	1284	1290	rVB3	423	348	0.03%	0.004%
25	5.530	1301	1303	1307	rVB2	462	303	0.03%	0.004%
26	5.726	1342	1364	1397	rBV2	342323	950598	95.34%	11.117%
27	5.871	1406	1409	1411	rVB2	502	273	0.03%	0.003%
28	5.890	1411	1415	1419	rBV3	393	283	0.03%	0.003%
29	5.970	1438	1440	1445	rVB3	376	331	0.03%	0.004%
30	6.250	1511	1527	1545	rBV	290024	550384	55.20%	6.436%
31	6.543	1605	1618	1634	rVV5	30895	59685	5.99%	0.698%
32	6.690	1649	1664	1689	rBV	231729	450934	45.23%	5.273%
33	6.787	1692	1694	1697	rVV2	612	412	0.04%	0.005%
34	6.803	1697	1699	1707	rVV4	563	662	0.07%	0.008%
35	6.922	1732	1736	1741	rVB	390	383	0.04%	0.004%
36	7.012	1758	1764	1769	rBV	360	426	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049040.D
 Acq On : 11 Jun 2022 08:43
 Operator : SY/MD
 Sample : N3248-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	7.182	1813	1817	1820	rVV3	670	499	0.05%	0.006%
38	7.282	1840	1848	1851	rBV2	243	326	0.03%	0.004%
39	7.311	1855	1857	1862	rBV2	284	339	0.03%	0.004%
40	7.443	1894	1898	1902	rBV2	307	291	0.03%	0.003%
41	7.462	1902	1904	1911	rVB	310	269	0.03%	0.003%
42	7.523	1916	1923	1925	rBV2	487	534	0.05%	0.006%
43	7.565	1925	1936	1951	rBV2	94227	168395	16.89%	1.969%
44	7.703	1974	1979	1982	rVB4	546	429	0.04%	0.005%
45	7.723	1982	1985	1990	rVB3	405	393	0.04%	0.005%
46	7.790	2004	2006	2014	rVB4	724	813	0.08%	0.010%
47	7.899	2026	2040	2056	rBV	399506	695020	69.71%	8.128%
48	8.118	2104	2108	2110	rBV	359	294	0.03%	0.003%
49	8.134	2110	2113	2116	rVB3	419	285	0.03%	0.003%
50	8.179	2116	2127	2143	rBV	70230	118732	11.91%	1.389%
51	8.401	2192	2196	2199	rVB5	667	610	0.06%	0.007%
52	8.472	2214	2218	2219	rVV	414	311	0.03%	0.004%
53	8.552	2232	2243	2256	rBV2	84797	141120	14.15%	1.650%
54	8.632	2256	2268	2305	rBV2	301614	598233	60.00%	6.996%
55	8.780	2312	2314	2317	rBV2	569	265	0.03%	0.003%
56	9.317	2475	2481	2485	rVB2	243	265	0.03%	0.003%
57	9.417	2499	2512	2534	rBV	405845	672089	67.41%	7.860%
58	9.562	2554	2557	2569	rVB4	1108	1913	0.19%	0.022%
59	9.649	2582	2584	2589	rVB2	419	323	0.03%	0.004%
60	9.690	2589	2597	2609	rBV4	1755	3251	0.33%	0.038%
61	10.057	2709	2711	2718	rVB	444	318	0.03%	0.004%
62	10.105	2718	2726	2735	rBV3	1307	2613	0.26%	0.031%
63	10.272	2776	2778	2783	rVB	335	267	0.03%	0.003%
64	10.301	2783	2787	2790	rBV2	354	289	0.03%	0.003%
65	10.488	2838	2845	2851	rVB4	734	879	0.09%	0.010%
66	10.755	2915	2928	2947	rBV	336247	550573	55.22%	6.439%
67	10.903	2966	2974	2984	rVV4	1001	1980	0.20%	0.023%
68	10.999	2998	3004	3007	rBV3	1179	1288	0.13%	0.015%
69	11.089	3024	3032	3040	rBV5	1479	2378	0.24%	0.028%
70	11.185	3059	3062	3068	rVB	467	396	0.04%	0.005%
71	11.295	3090	3096	3102	rBV4	1589	2133	0.21%	0.025%
72	11.468	3142	3150	3160	rVB3	5802	8323	0.83%	0.097%
73	11.616	3192	3196	3200	rBV2	337	332	0.03%	0.004%
74	11.648	3202	3206	3207	rBV	411	279	0.03%	0.003%
75	11.745	3233	3236	3237	rBV2	746	439	0.04%	0.005%
76	11.812	3245	3257	3278	rVV	358135	577655	57.94%	6.755%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049040.D
 Acq On : 11 Jun 2022 08:43
 Operator : SY/MD
 Sample : N3248-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.893	3278	3282	3288	rVB4	2187	2359	0.24%	0.028%
78	12.089	3336	3343	3345	rBV7	540	609	0.06%	0.007%
79	12.118	3349	3352	3355	rBV3	372	292	0.03%	0.003%
80	12.192	3363	3375	3395	rBV	382207	626990	62.88%	7.332%
81	12.320	3411	3415	3417	rBV2	318	274	0.03%	0.003%
82	12.571	3489	3493	3496	rBV2	655	675	0.07%	0.008%
83	12.777	3555	3557	3561	rVB2	487	322	0.03%	0.004%
84	12.899	3591	3595	3600	rBV2	337	418	0.04%	0.005%
85	13.028	3633	3635	3641	rVB3	664	634	0.06%	0.007%
86	13.105	3656	3659	3661	rBV2	425	282	0.03%	0.003%
87	13.127	3664	3666	3669	rVB2	490	292	0.03%	0.003%
88	13.410	3751	3754	3758	rBV3	327	313	0.03%	0.004%
89	13.449	3761	3766	3777	rBV3	1038	1528	0.15%	0.018%
90	13.854	3889	3892	3895	rVV2	370	327	0.03%	0.004%
91	13.902	3902	3907	3909	rBV	404	384	0.04%	0.004%
92	13.989	3931	3934	3939	rBV3	478	455	0.05%	0.005%
93	14.102	3962	3969	3974	rBV4	2295	2881	0.29%	0.034%
94	14.336	4036	4042	4045	rVB2	784	636	0.06%	0.007%
95	14.484	4084	4088	4092	rBV3	435	457	0.05%	0.005%
96	14.725	4160	4163	4165	rBV	421	267	0.03%	0.003%
97	15.565	4422	4424	4426	rBV	443	266	0.03%	0.003%
98	15.909	4529	4531	4534	rVB2	1069	524	0.05%	0.006%
99	16.185	4615	4617	4620	rBV4	839	534	0.05%	0.006%
100	16.394	4677	4682	4683	rBV3	1236	835	0.08%	0.010%




Sum of corrected areas: 8551088

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049040.D
Acq On : 11 Jun 2022 08:43
Operator : SY/MD
Sample : N3248-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

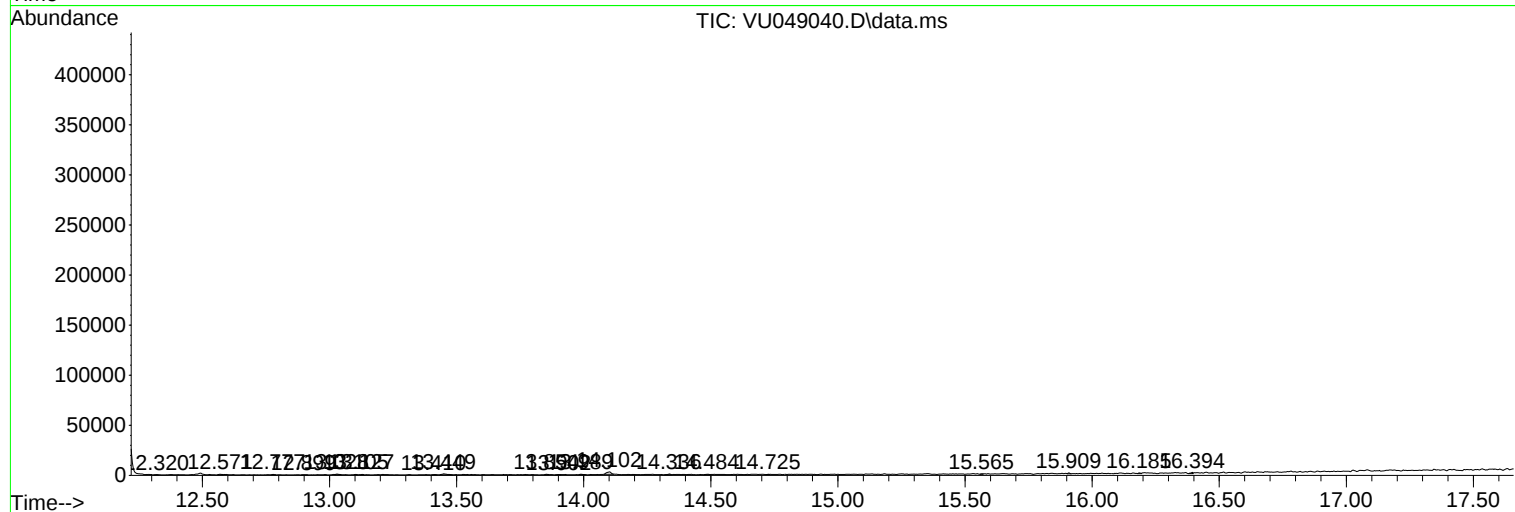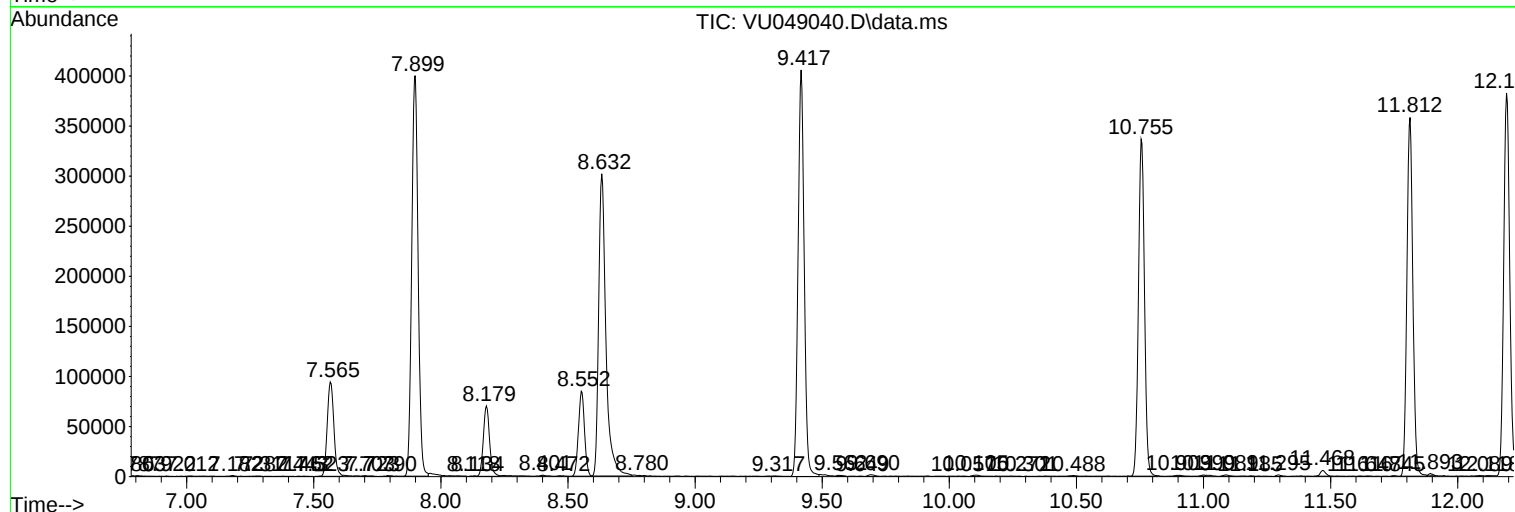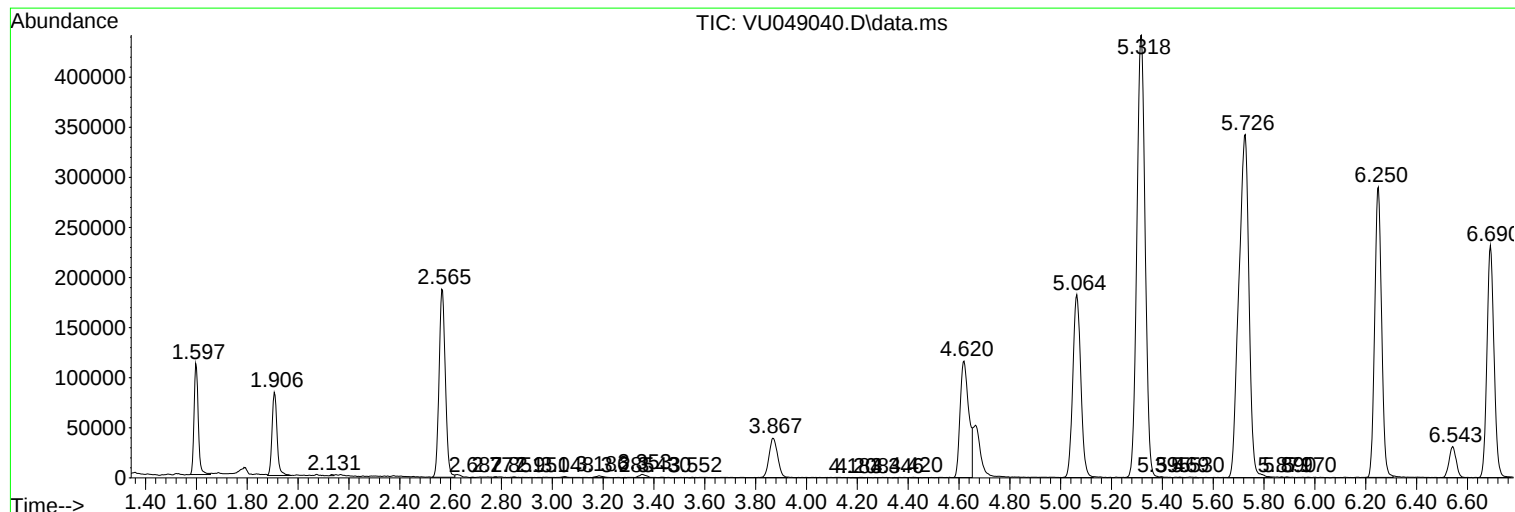

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049040.D
Acq On : 11 Jun 2022 08:43
Operator : SY/MD
Sample : N3248-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049040.D
Acq On : 11 Jun 2022 08:43
Operator : SY/MD
Sample : N3248-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------