

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049043.D
 Acq On : 11 Jun 2022 09:54
 Operator : SY/MD
 Sample : N3249-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049043.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	104483	117049	13.04%	1.632%
2	1.900	166	174	187	rBV	72371	95276	10.61%	1.329%
3	2.298	296	298	300	rBV4	683	341	0.04%	0.005%
4	2.517	363	366	369	rBV2	593	469	0.05%	0.007%
5	2.562	369	380	394	rBV	168012	275101	30.64%	3.836%
6	2.675	411	415	419	rVV2	336	268	0.03%	0.004%
7	2.723	427	430	433	rVB2	358	248	0.03%	0.003%
8	2.765	438	443	447	rBV2	409	449	0.05%	0.006%
9	2.842	464	467	471	rBV3	317	257	0.03%	0.004%
10	2.967	503	506	510	rVB3	367	248	0.03%	0.003%
11	2.993	510	514	518	rVB2	312	299	0.03%	0.004%
12	3.044	526	530	535	rVB2	660	603	0.07%	0.008%
13	3.125	551	555	558	rVB2	392	335	0.04%	0.005%
14	3.183	558	573	590	rBV5	3223	8274	0.92%	0.115%
15	3.302	607	610	614	rVB3	484	368	0.04%	0.005%
16	3.871	774	787	789	rBV3	2123	3074	0.34%	0.043%
17	4.321	920	927	930	rBV2	351	481	0.05%	0.007%
18	4.433	958	962	971	rVB2	267	377	0.04%	0.005%
19	4.620	1007	1020	1054	rBV	112811	314418	35.02%	4.384%
20	4.903	1103	1108	1112	rBV3	319	291	0.03%	0.004%
21	4.961	1124	1126	1132	rVB2	478	381	0.04%	0.005%
22	5.060	1141	1157	1178	rBV	175110	384829	42.86%	5.366%
23	5.279	1221	1225	1226	rBV	300	234	0.03%	0.003%
24	5.317	1226	1237	1248	rVV5	3973	8460	0.94%	0.118%
25	5.501	1289	1294	1295	rBV2	377	267	0.03%	0.004%
26	5.568	1311	1315	1321	rBV2	352	489	0.05%	0.007%
27	5.723	1341	1363	1381	rBV2	328234	897912	100.00%	12.521%
28	5.829	1394	1396	1400	rVB2	557	368	0.04%	0.005%
29	5.967	1435	1439	1445	rBV5	804	727	0.08%	0.010%
30	6.247	1512	1526	1547	rBV	296067	564935	62.92%	7.878%
31	6.356	1558	1560	1563	rVB3	582	272	0.03%	0.004%
32	6.456	1586	1591	1595	rVB2	330	326	0.04%	0.005%
33	6.533	1603	1615	1622	rBV8	2326	4765	0.53%	0.066%
34	6.690	1649	1664	1688	rVV	227384	441580	49.18%	6.158%
35	6.790	1691	1695	1698	rVV3	446	427	0.05%	0.006%
36	7.018	1760	1766	1769	rBV2	342	243	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049043.D
 Acq On : 11 Jun 2022 09:54
 Operator : SY/MD
 Sample : N3249-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	7.170	1808	1813	1814	rBV	855	632	0.07%	0.009%
38	7.501	1910	1916	1920	rBV2	411	400	0.04%	0.006%
39	7.565	1923	1936	1957	rVV	93937	164289	18.30%	2.291%
40	7.639	1957	1959	1963	rVV2	451	248	0.03%	0.003%
41	7.687	1970	1974	1985	rVB4	836	901	0.10%	0.013%
42	7.800	2005	2009	2016	rVB3	902	829	0.09%	0.012%
43	7.896	2025	2039	2058	rBV	389385	674431	75.11%	9.404%
44	8.070	2091	2093	2098	rVB4	395	292	0.03%	0.004%
45	8.179	2115	2127	2141	rBV	69194	119129	13.27%	1.661%
46	8.452	2208	2212	2213	rBV2	619	458	0.05%	0.006%
47	8.465	2213	2216	2217	rVV2	1048	688	0.08%	0.010%
48	8.475	2217	2219	2224	rVB4	1467	1197	0.13%	0.017%
49	8.552	2236	2243	2251	rBV6	1301	1850	0.21%	0.026%
50	8.632	2256	2268	2303	rBV2	300762	599548	66.77%	8.360%
51	9.153	2424	2430	2435	rBV2	311	456	0.05%	0.006%
52	9.182	2436	2439	2445	rVB	538	478	0.05%	0.007%
53	9.214	2445	2449	2454	rBV	403	404	0.04%	0.006%
54	9.247	2454	2459	2462	rVB2	307	266	0.03%	0.004%
55	9.417	2498	2512	2536	rBV	410967	686061	76.41%	9.567%
56	9.568	2555	2559	2560	rBV2	371	285	0.03%	0.004%
57	9.578	2560	2562	2567	rVB	605	439	0.05%	0.006%
58	9.690	2592	2597	2599	rBV3	622	576	0.06%	0.008%
59	9.886	2654	2658	2662	rBV2	296	274	0.03%	0.004%
60	10.105	2718	2726	2729	rVV3	638	717	0.08%	0.010%
61	10.488	2842	2845	2848	rBV2	310	289	0.03%	0.004%
62	10.758	2914	2929	2944	rBV	337472	543838	60.57%	7.583%
63	10.893	2963	2971	2981	rBV4	2568	4064	0.45%	0.057%
64	10.996	3000	3003	3005	rVV2	362	238	0.03%	0.003%
65	11.086	3026	3031	3041	rBV3	809	1433	0.16%	0.020%
66	11.295	3089	3096	3097	rBV2	738	754	0.08%	0.011%
67	11.468	3143	3150	3158	rVB2	2098	2595	0.29%	0.036%
68	11.517	3161	3165	3168	rBV2	361	340	0.04%	0.005%
69	11.748	3234	3237	3240	rVB2	514	290	0.03%	0.004%
70	11.812	3245	3257	3277	rVV	370103	591460	65.87%	8.248%
71	11.896	3277	3283	3289	rVB5	2003	2816	0.31%	0.039%
72	11.944	3295	3298	3301	rBV2	563	475	0.05%	0.007%
73	11.986	3308	3311	3317	rBV	196	239	0.03%	0.003%
74	12.057	3328	3333	3336	rVB2	482	406	0.05%	0.006%
75	12.089	3340	3343	3345	rBV2	728	548	0.06%	0.008%
76	12.195	3362	3376	3393	rBV	371644	624413	69.54%	8.707%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049043.D
 Acq On : 11 Jun 2022 09:54
 Operator : SY/MD
 Sample : N3249-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	12.378	3430	3433	3440	rVB3	487	568	0.06%	0.008%
78	12.439	3450	3452	3457	rVB3	397	263	0.03%	0.004%
79	12.488	3457	3467	3477	rBV7	2280	3925	0.44%	0.055%
80	12.581	3490	3496	3499	rBV2	392	475	0.05%	0.007%
81	12.774	3547	3556	3566	rBV4	1506	2536	0.28%	0.035%
82	12.861	3578	3583	3584	rBV	334	275	0.03%	0.004%
83	12.890	3589	3592	3599	rBV2	301	304	0.03%	0.004%
84	13.028	3630	3635	3636	rBV2	499	423	0.05%	0.006%
85	13.179	3679	3682	3686	rVB2	350	265	0.03%	0.004%
86	13.227	3692	3697	3700	rBV2	253	312	0.03%	0.004%
87	13.388	3740	3747	3752	rBV3	433	686	0.08%	0.010%
88	13.459	3765	3769	3774	rVB3	1082	955	0.11%	0.013%
89	13.597	3809	3812	3816	rVB3	381	272	0.03%	0.004%
90	13.915	3908	3911	3913	rBV	418	294	0.03%	0.004%
91	14.063	3952	3957	3961	rVB3	395	347	0.04%	0.005%
92	14.095	3961	3967	3974	rBV5	1872	3095	0.34%	0.043%
93	14.176	3989	3992	3995	rBV2	379	320	0.04%	0.004%
94	14.693	4151	4153	4158	rVB2	463	259	0.03%	0.004%
95	14.722	4159	4162	4166	rBV	451	288	0.03%	0.004%
96	15.279	4333	4335	4340	rBV3	373	285	0.03%	0.004%
97	15.320	4344	4348	4350	rBV3	535	429	0.05%	0.006%
98	15.417	4376	4378	4380	rBV	538	346	0.04%	0.005%
99	15.803	4496	4498	4502	rVB2	911	438	0.05%	0.006%
100	16.340	4663	4665	4668	rBV	880	531	0.06%	0.007%




Sum of corrected areas: 7171378

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049043.D
Acq On : 11 Jun 2022 09:54
Operator : SY/MD
Sample : N3249-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 57 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

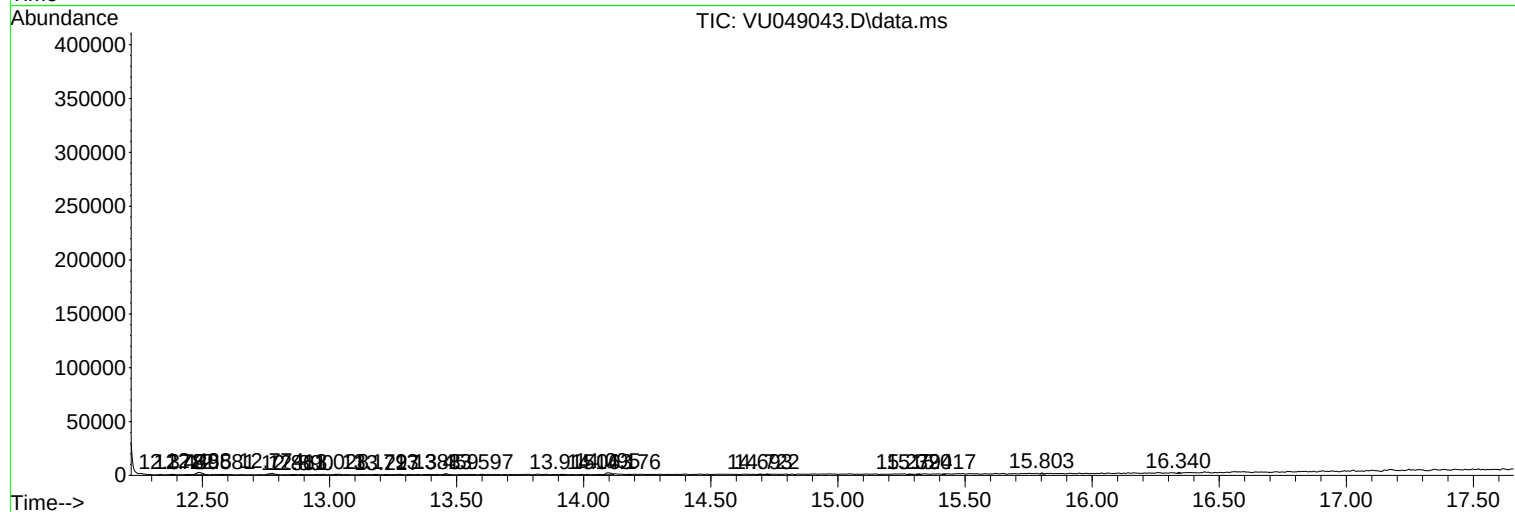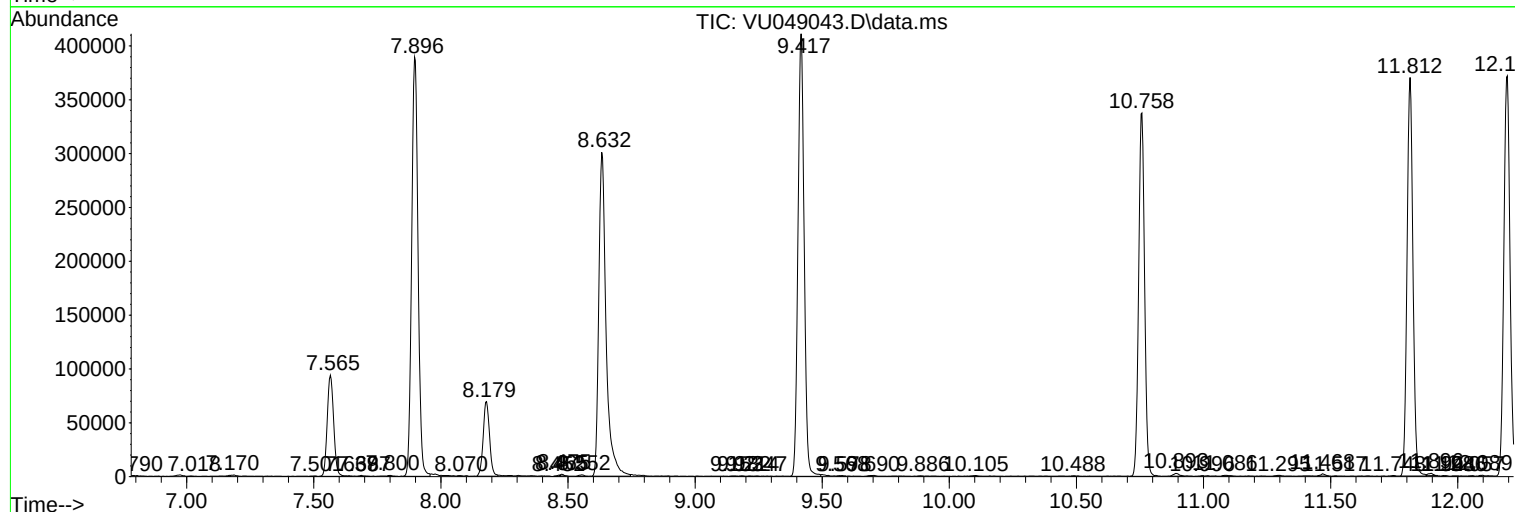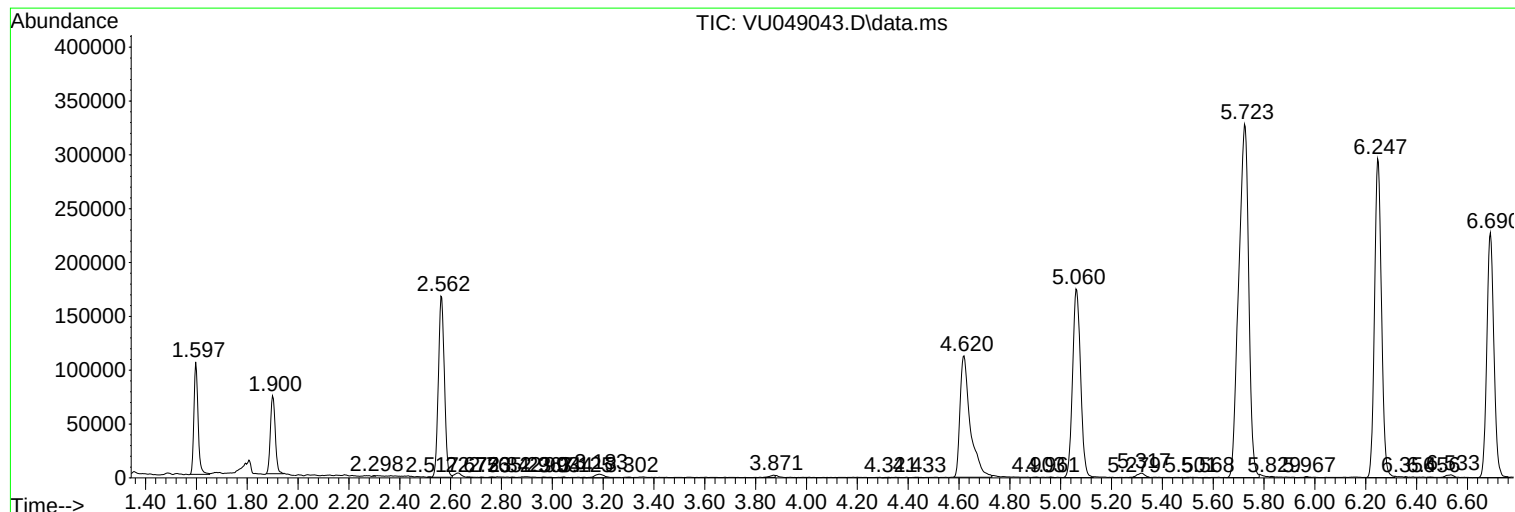

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049043.D
Acq On : 11 Jun 2022 09:54
Operator : SY/MD
Sample : N3249-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 57 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049043.D
Acq On : 11 Jun 2022 09:54
Operator : SY/MD
Sample : N3249-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 57 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------