

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049044.D
 Acq On : 11 Jun 2022 10:17
 Operator : SY/MD
 Sample : N3249-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

Signal : TIC: VU049044.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	106460	120304	12.96%	1.496%
2	1.900	167	174	192	rVB	75292	102300	11.02%	1.272%
3	2.565	368	381	394	rBV2	177680	300458	32.38%	3.737%
4	2.790	446	451	454	rBV2	438	592	0.06%	0.007%
5	2.948	496	500	503	rBV3	382	269	0.03%	0.003%
6	3.141	557	560	561	rBV	102	55	0.01%	0.001%
7	3.182	562	573	586	rVV3	2839	6159	0.66%	0.077%
8	3.350	617	625	627	rBV3	2694	2747	0.30%	0.034%
9	3.726	740	742	746	rVB2	341	168	0.02%	0.002%
10	3.867	766	786	809	rBV	65350	157204	16.94%	1.955%
11	3.957	811	814	818	rBV	294	205	0.02%	0.003%
12	4.022	833	834	835	rBV	115	32	0.00%	0.000%
13	4.031	835	837	838	rVV	174	57	0.01%	0.001%
14	4.067	846	848	851	rBV	227	125	0.01%	0.002%
15	4.108	858	861	866	rBV2	190	184	0.02%	0.002%
16	4.160	873	877	880	rBV2	228	183	0.02%	0.002%
17	4.179	880	883	885	rBV	169	125	0.01%	0.002%
18	4.443	962	965	968	rBV	126	75	0.01%	0.001%
19	4.497	980	982	985	rBV	115	70	0.01%	0.001%
20	4.517	985	988	993	rVB	282	203	0.02%	0.003%
21	4.546	993	997	1000	rBV	162	170	0.02%	0.002%
22	4.571	1002	1005	1007	rBV2	200	138	0.01%	0.002%
23	4.620	1007	1020	1028	rBV	113181	255319	27.51%	3.175%
24	4.932	1114	1117	1120	rBV2	322	222	0.02%	0.003%
25	5.063	1140	1158	1181	rBV	177400	394159	42.48%	4.902%
26	5.314	1219	1236	1260	rBV2	274566	626770	67.54%	7.795%
27	5.407	1262	1265	1268	rVB2	547	302	0.03%	0.004%
28	5.430	1268	1272	1276	rVB2	374	313	0.03%	0.004%
29	5.449	1276	1278	1281	rBV2	229	152	0.02%	0.002%
30	5.491	1289	1291	1292	rBV	124	40	0.00%	0.000%
31	5.604	1323	1326	1327	rBV	172	105	0.01%	0.001%
32	5.723	1342	1363	1388	rBV2	336729	927971	100.00%	11.541%
33	5.964	1432	1438	1441	rBV2	390	456	0.05%	0.006%
34	5.999	1447	1449	1452	rBV	155	78	0.01%	0.001%
35	6.034	1459	1460	1461	rVB	195	38	0.00%	0.000%
36	6.112	1480	1484	1489	rBV3	330	407	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049044.D
 Acq On : 11 Jun 2022 10:17
 Operator : SY/MD
 Sample : N3249-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.166	1498	1501	1505	rBV	233	190	0.02%	0.002%
38	6.192	1507	1509	1512	rBV	239	90	0.01%	0.001%
39	6.247	1512	1526	1542	rBV	294534	557883	60.12%	6.938%
40	6.542	1605	1618	1633	rVB5	21177	42057	4.53%	0.523%
41	6.604	1633	1637	1641	rBV3	443	363	0.04%	0.005%
42	6.629	1642	1645	1646	rVB	261	115	0.01%	0.001%
43	6.690	1649	1664	1683	rBV	222266	431029	46.45%	5.360%
44	6.796	1694	1697	1699	rBV3	553	346	0.04%	0.004%
45	6.861	1715	1717	1718	rBV	190	64	0.01%	0.001%
46	6.906	1729	1731	1736	rVB2	235	156	0.02%	0.002%
47	6.970	1750	1751	1754	rVB	312	94	0.01%	0.001%
48	6.986	1754	1756	1757	rVB2	129	29	0.00%	0.000%
49	7.157	1805	1809	1810	rBV	388	210	0.02%	0.003%
50	7.343	1865	1867	1868	rBV	336	159	0.02%	0.002%
51	7.510	1917	1919	1920	rBV	150	49	0.01%	0.001%
52	7.565	1923	1936	1955	rVV	94476	163978	17.67%	2.039%
53	7.742	1988	1991	1997	rBV2	339	402	0.04%	0.005%
54	7.803	2007	2010	2014	rBV2	642	505	0.05%	0.006%
55	7.896	2025	2039	2058	rBV	386983	675739	72.82%	8.404%
56	8.179	2116	2127	2142	rBV	69084	113545	12.24%	1.412%
57	8.552	2232	2243	2256	rBV2	55602	92521	9.97%	1.151%
58	8.632	2256	2268	2305	rBV3	310992	607165	65.43%	7.551%
59	9.060	2397	2401	2403	rBV	176	145	0.02%	0.002%
60	9.340	2486	2488	2494	rVB2	405	311	0.03%	0.004%
61	9.372	2494	2498	2499	rBV	266	185	0.02%	0.002%
62	9.417	2499	2512	2533	rBV	413453	690549	74.41%	8.588%
63	9.767	2616	2621	2622	rVB	258	162	0.02%	0.002%
64	9.787	2622	2627	2630	rBV	296	344	0.04%	0.004%
65	9.896	2658	2661	2662	rBV	219	117	0.01%	0.001%
66	10.005	2691	2695	2696	rBV2	124	82	0.01%	0.001%
67	10.208	2755	2758	2760	rBV	172	108	0.01%	0.001%
68	10.584	2872	2875	2877	rBV	188	156	0.02%	0.002%
69	10.758	2915	2929	2948	rBV	335141	546808	58.93%	6.800%
70	10.896	2962	2972	2980	rVB5	1308	2282	0.25%	0.028%
71	10.931	2980	2983	2989	rBV2	211	283	0.03%	0.004%
72	11.005	3000	3006	3007	rBV2	402	444	0.05%	0.006%
73	11.066	3023	3025	3028	rBV2	284	215	0.02%	0.003%
74	11.381	3120	3123	3125	rBV2	263	161	0.02%	0.002%
75	11.465	3145	3149	3150	rBV2	776	514	0.06%	0.006%
76	11.504	3159	3161	3164	rBV2	294	212	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
 Data File : VU049044.D
 Acq On : 11 Jun 2022 10:17
 Operator : SY/MD
 Sample : N3249-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

77	11.555	3175	3177	3180	rBV2	317	180	0.02%	0.002%
78	11.587	3185	3187	3189	rVV	172	70	0.01%	0.001%
79	11.613	3193	3195	3198	rBV2	341	224	0.02%	0.003%
80	11.812	3245	3257	3277	rBV	370650	596441	64.27%	7.418%
81	12.121	3350	3353	3357	rVB2	379	296	0.03%	0.004%
82	12.192	3363	3375	3397	rBV	365411	614018	66.17%	7.636%
83	12.523	3475	3478	3482	rBV2	301	331	0.04%	0.004%
84	12.764	3546	3553	3554	rBV3	803	670	0.07%	0.008%
85	12.825	3569	3572	3575	rBV4	428	311	0.03%	0.004%
86	12.877	3585	3588	3590	rBV	302	166	0.02%	0.002%
87	13.266	3707	3709	3712	rBV	387	291	0.03%	0.004%




Sum of corrected areas: 8040920

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049044.D
Acq On : 11 Jun 2022 10:17
Operator : SY/MD
Sample : N3249-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

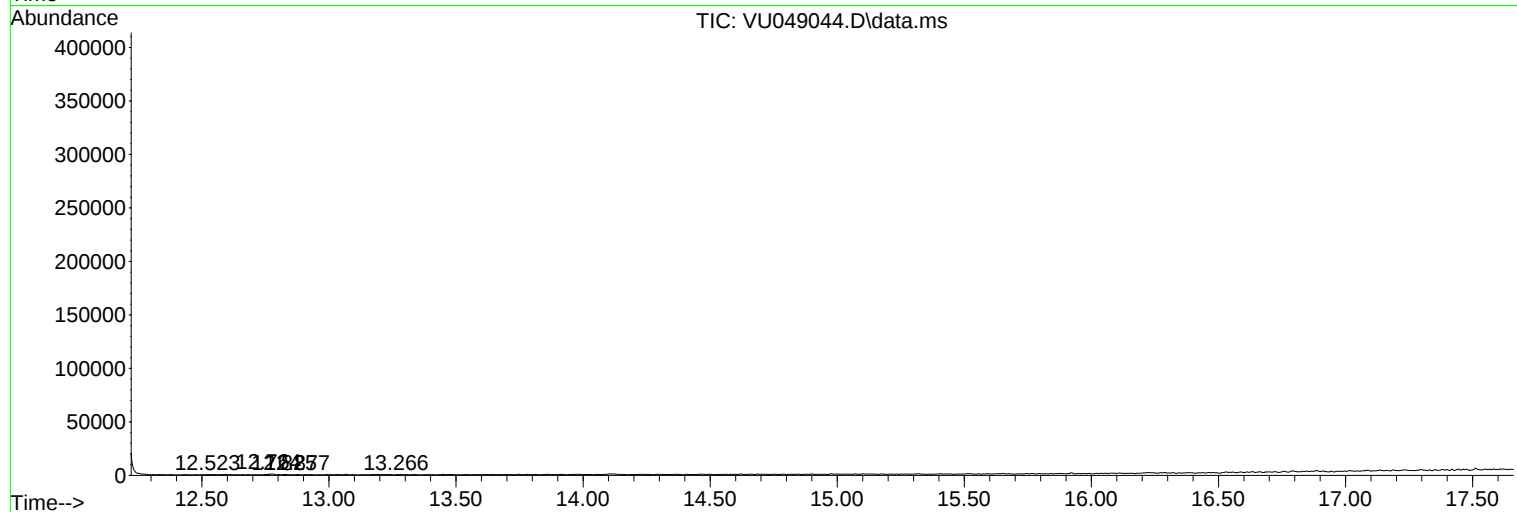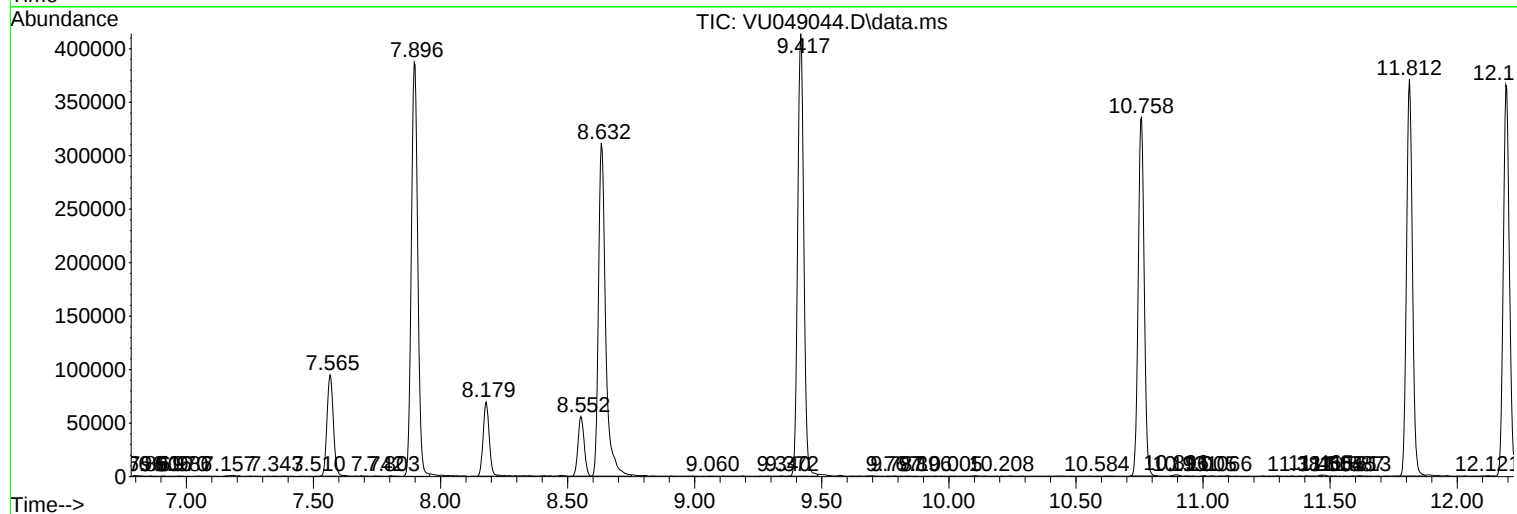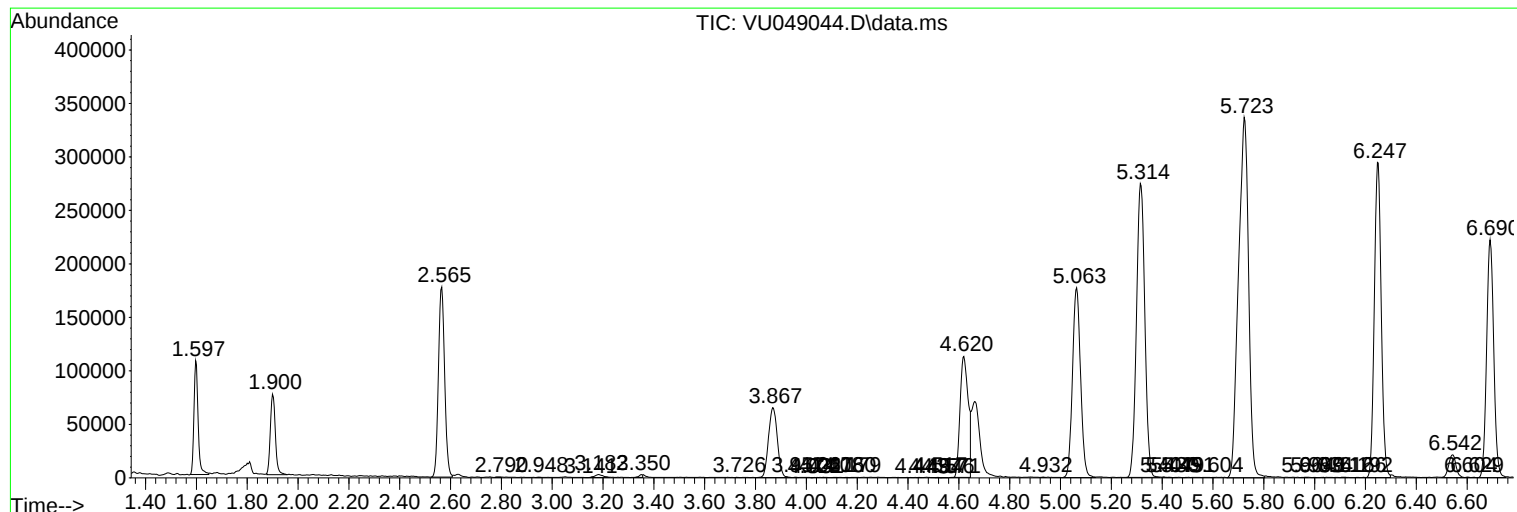

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049044.D
Acq On : 11 Jun 2022 10:17
Operator : SY/MD
Sample : N3249-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061022\
Data File : VU049044.D
Acq On : 11 Jun 2022 10:17
Operator : SY/MD
Sample : N3249-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------